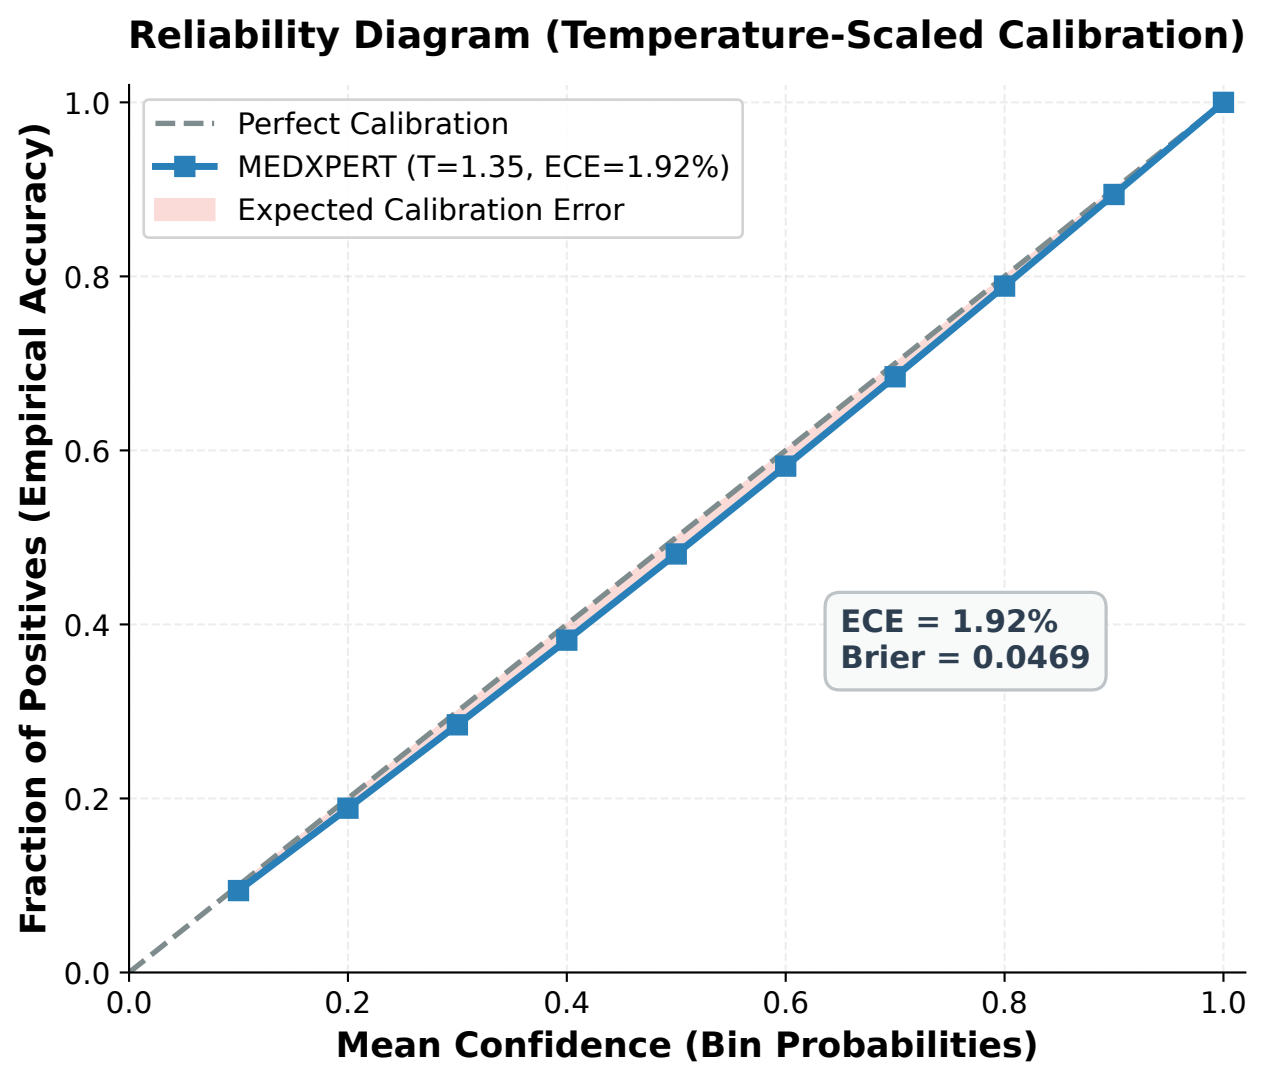
Reliability Diagram (Temperature-Scaled Calibration)
Perfect Calibration
MEDXPERT (T=1.35, ECE=1.92%)
Expected Calibration Error
ECE = 1.92%
Brier = 0.0469
Fraction of Positives (Empirical Accuracy)
Mean Confidence (Bin Probabilities)
0.0
0.2
0.4
0.6
0.8
1.0