



eleration of the z-axis of the left shank with synchronisation lines and red marker when the patient steps with the left

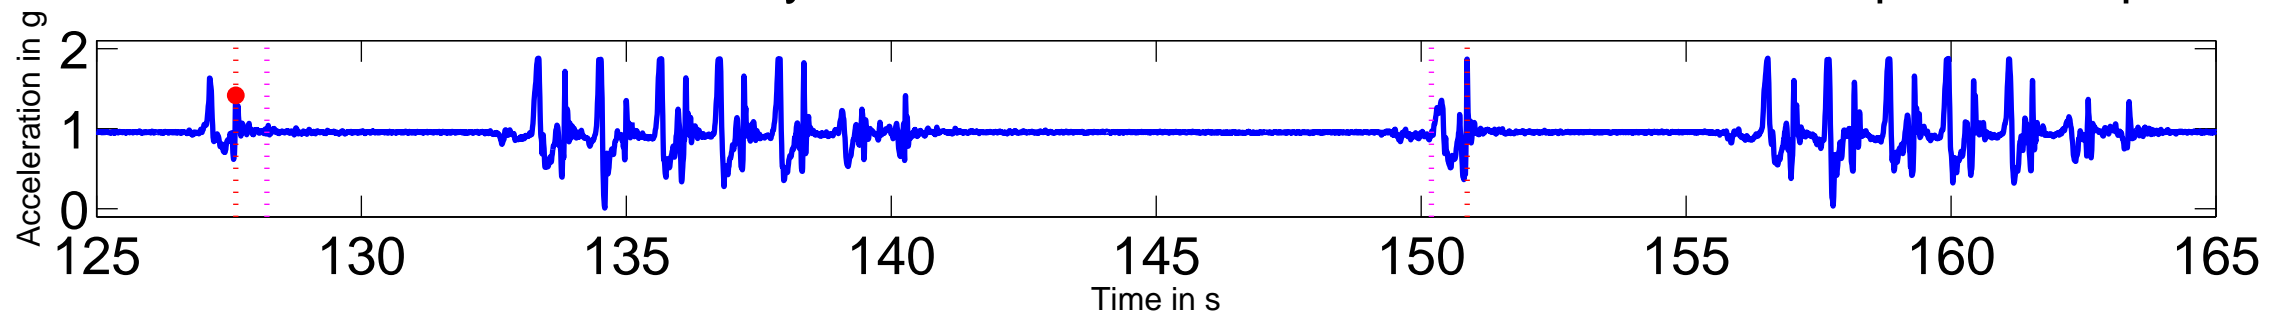

eleration of the z-axis of the right shank with synchronisation lines and red marker when the patient steps with the left

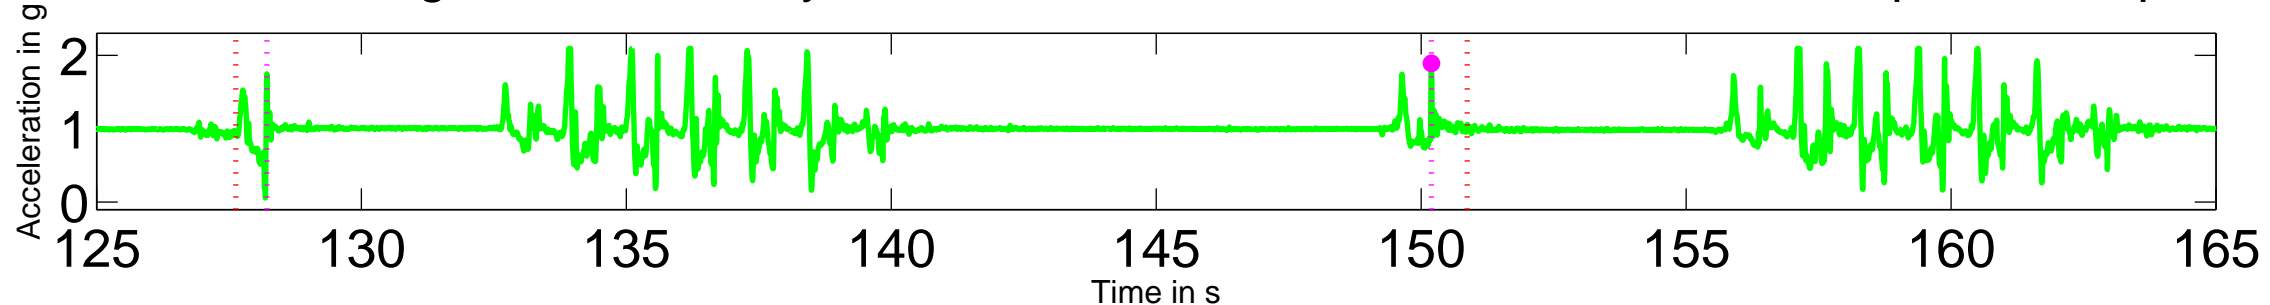

Exemplary the course of the synchronised signals of the four force sensors.

