




pH Isolated measuring part - I2C 0x49

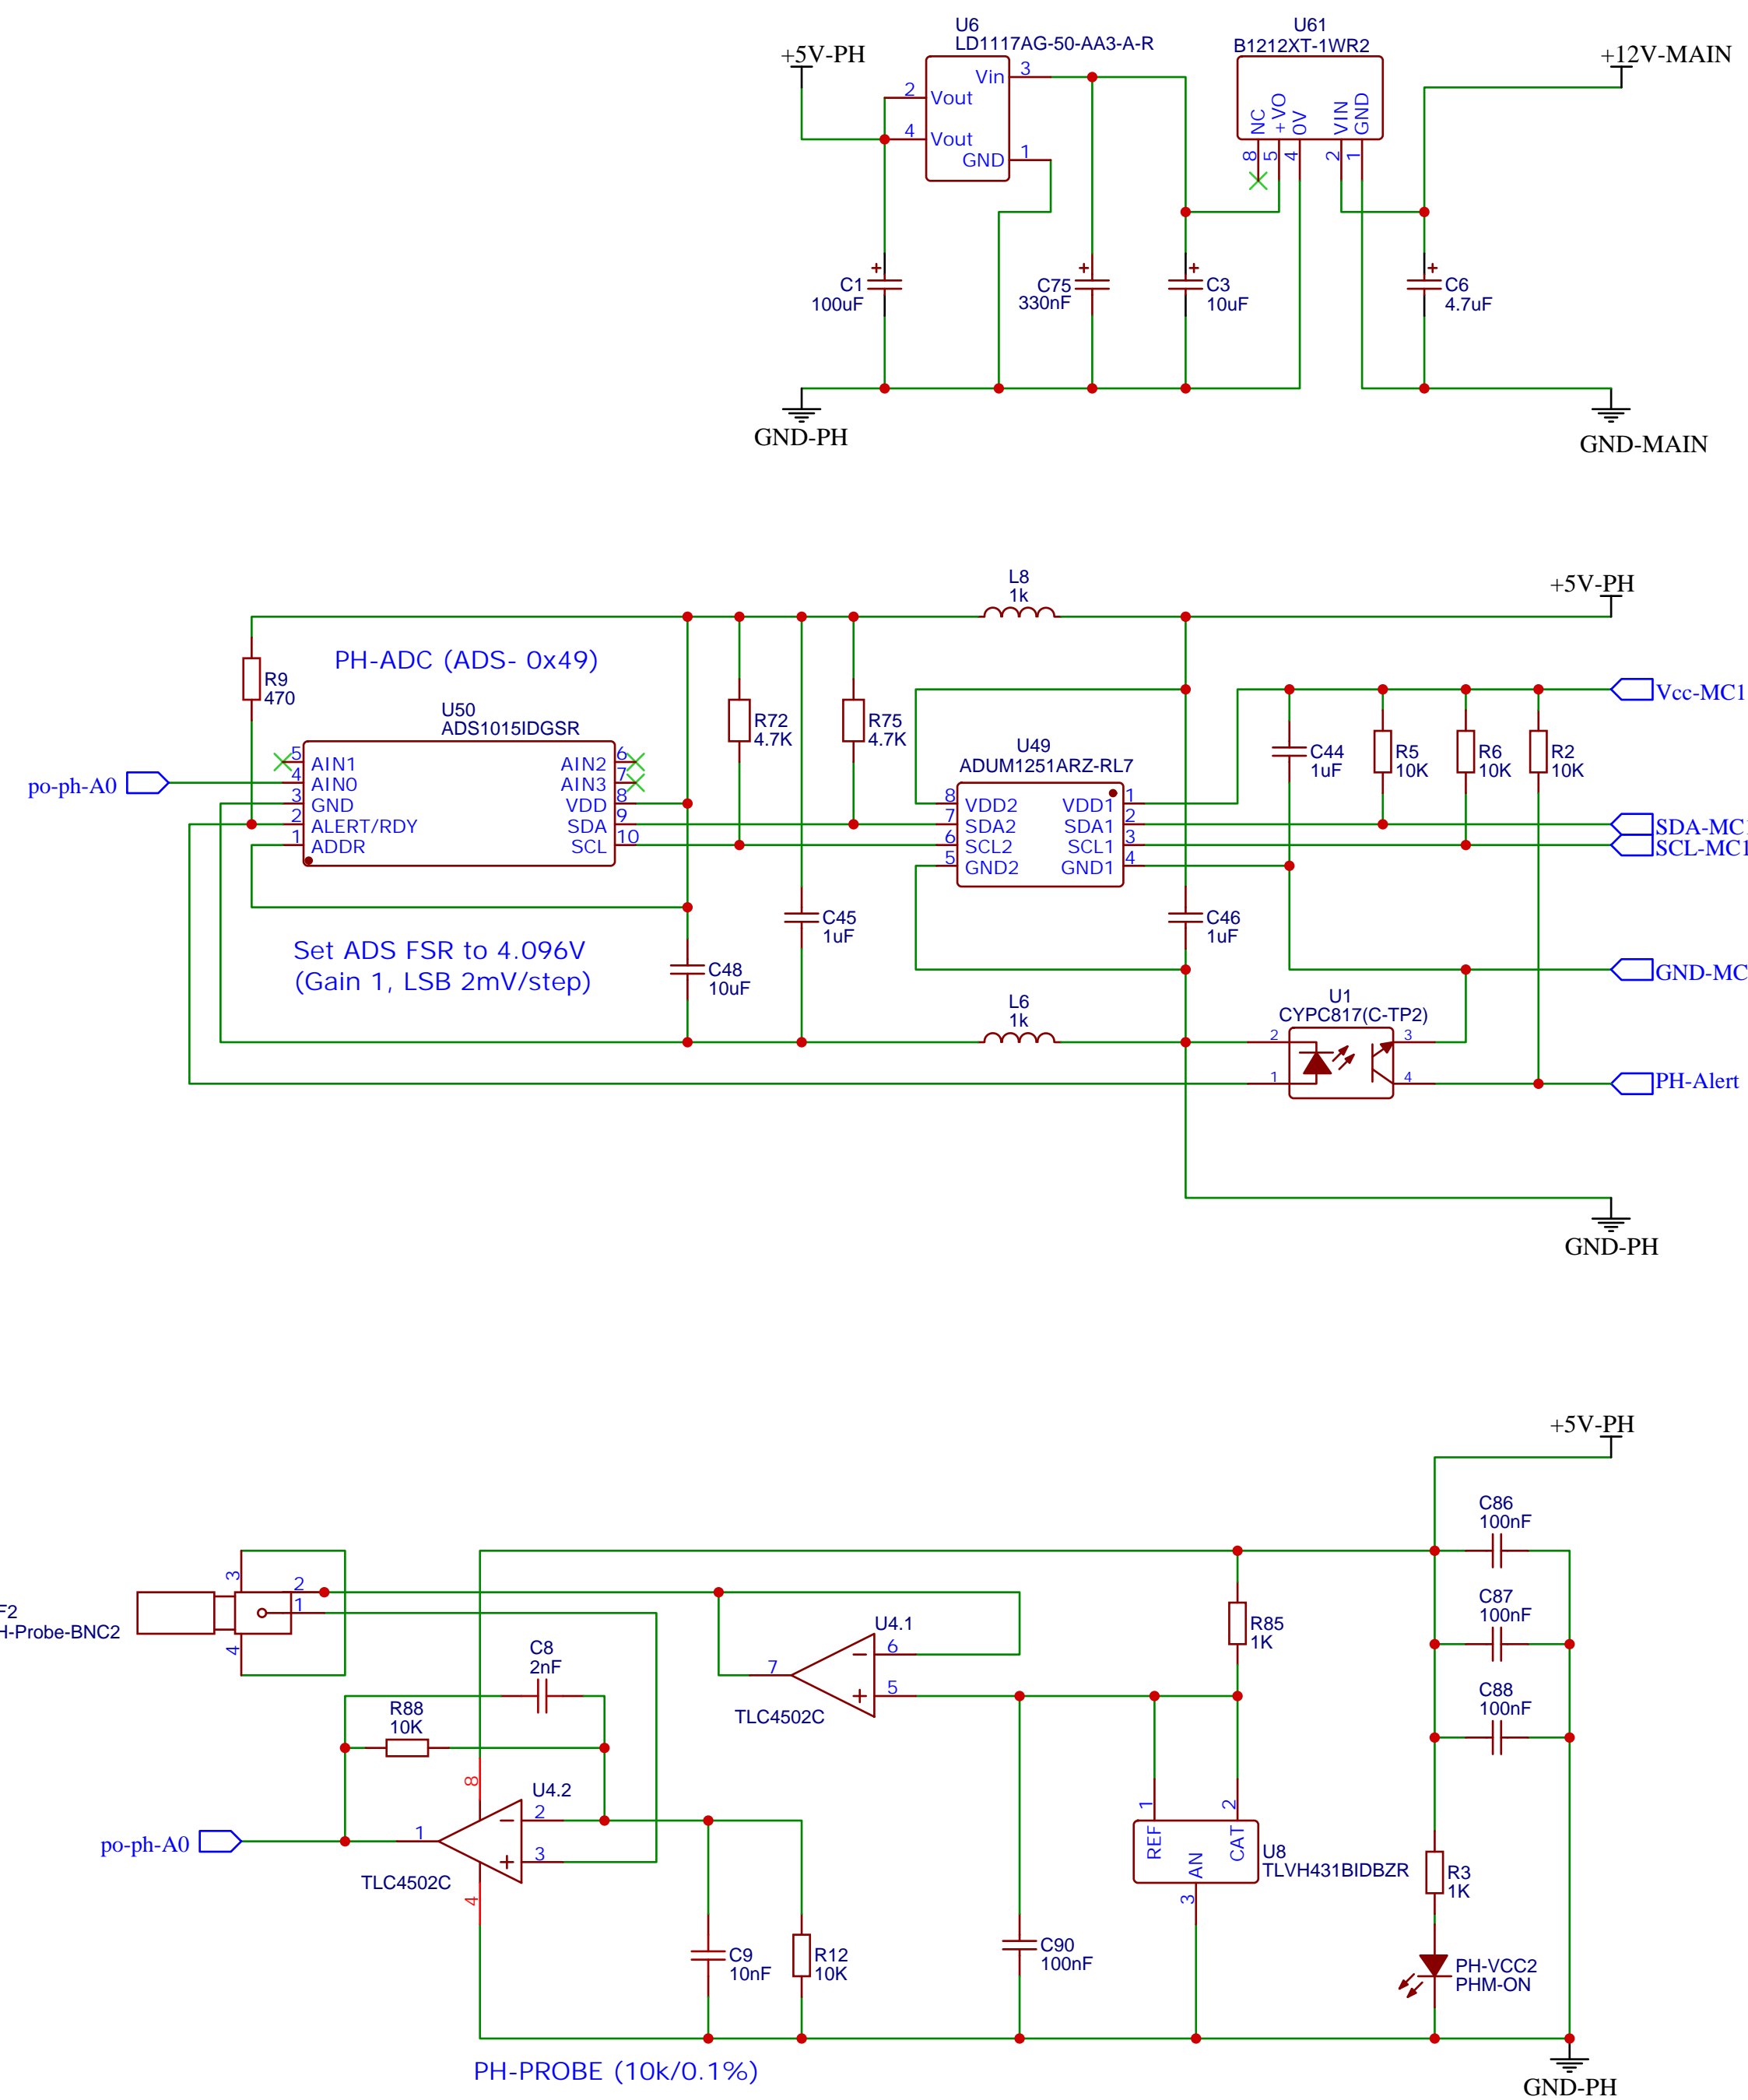

ORP Isolated measuring part - I2C 0x48

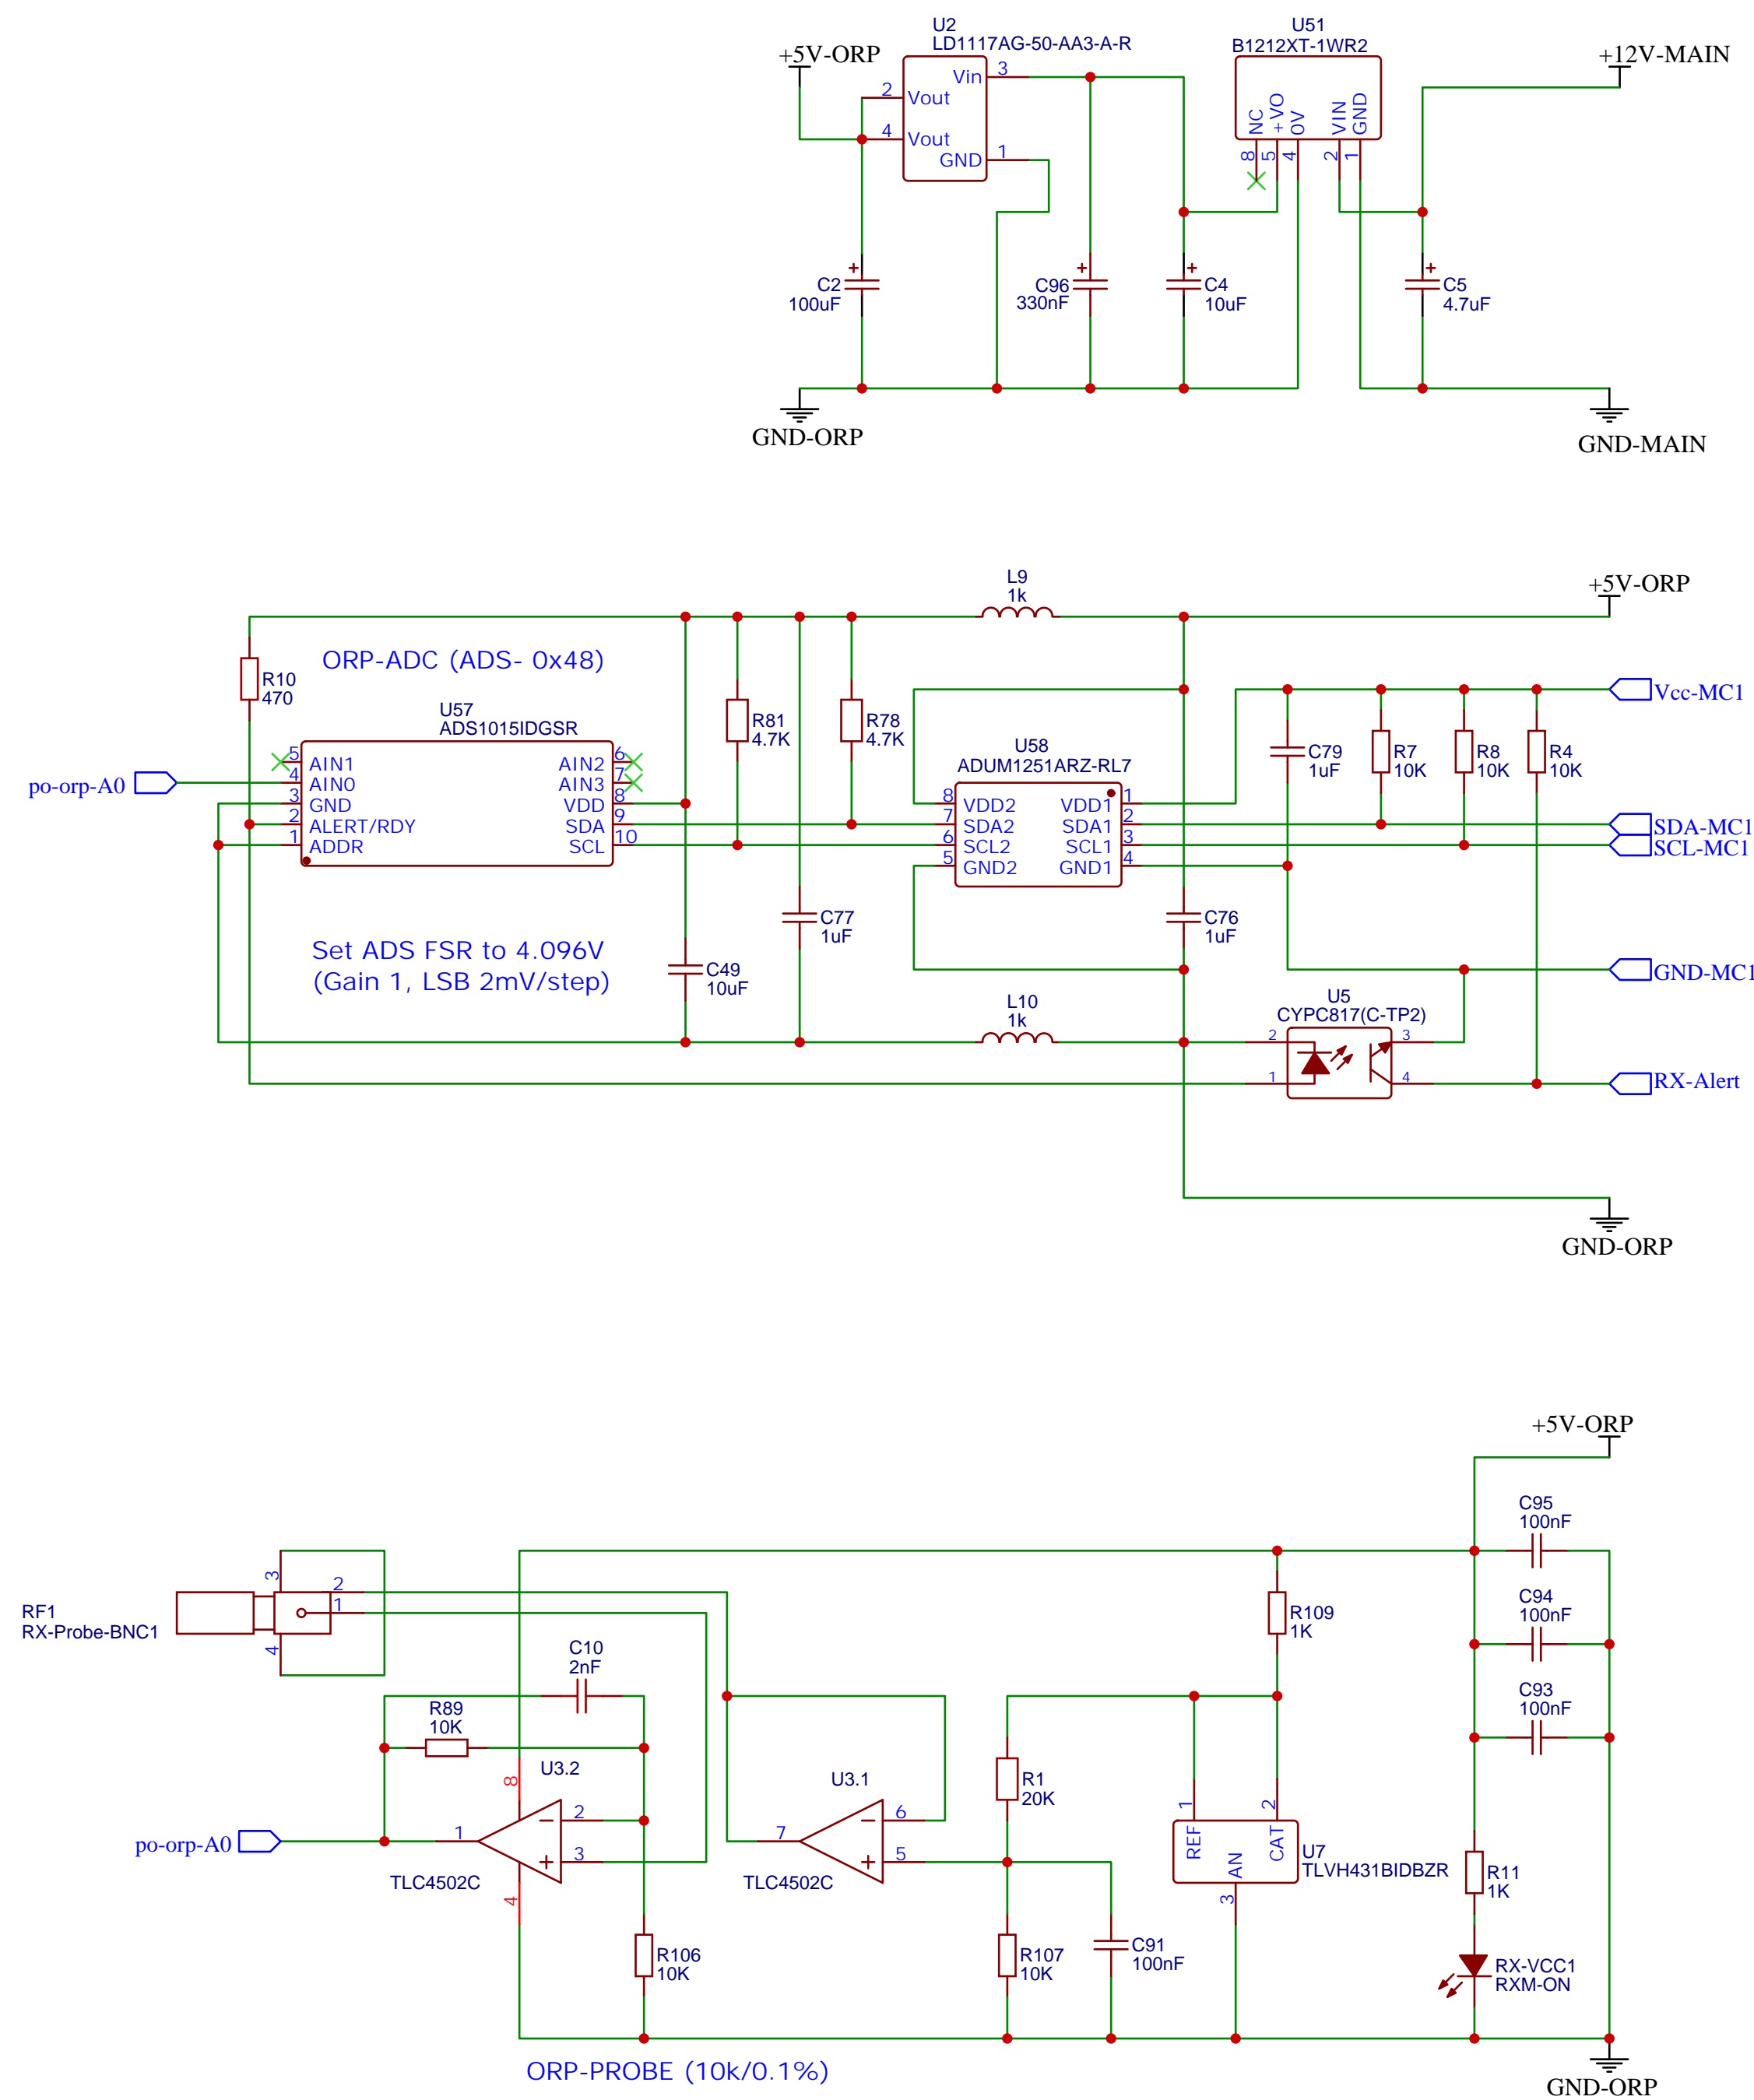

Connections

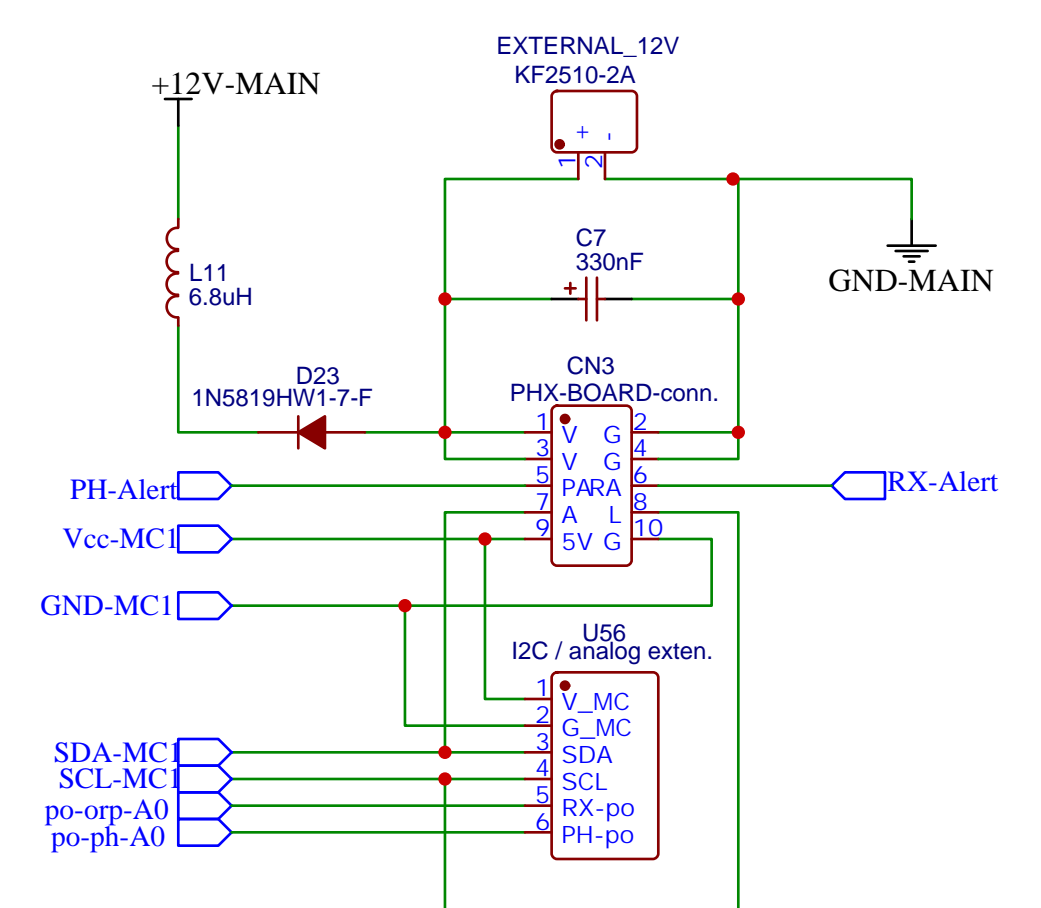

BETTER OPAMP ALTERNATIVE:

<https://www.ti.com/lit/ds/snosai9h/snosai9h.pdf?ts=1633703026230>
<https://e2e.ti.com/support/amplifiers-group/amplifiers/f/amplifiers-forum/954653/imp7721-confusion-about-example-schematics>

