




PRODUCT IDENTIFICATION		HPLC-UV coupled with LC-MS/MS, standard laboratory conditions	
Compound Name	Glutathione	CAS No.	70-18-8
Molecular Formula	C10H17N3O6S	Molecular Weight	307.32 g/mol
Appearance	White Lyophilized Powder	Compound Concentration	1500mg
Sequence:	gamma-Glu-Cys-Gly		
SAMPLE IDENTIFICATION		Client-supplied, verified at intake	
Container Size	10ml Glass Vial	Cap Color	Purple
Crimp / Seal Color	Silver		
Product Company	APEXX BIOLABS LLC		



MOLECULAR STRUCTURE



CLIENT SAMPLE PHOTO

ANALYTICAL RESULTS			
Test	Specification	Result	Status
Purity (HPLC)	$\geq 90.0\%$	99.91%	PASS
Mass Identification (LC-MS/MS)	Conforms to declared compound	Glutathione	PASS
Net Peptide Content	$\geq 90\%$ of 1500 mg	1657.83 mg	PASS
Water Content (Karl Fischer)	$\leq 10.0\%$	4.01%	PASS
Acetate Content (HPLC)	$< 12.0\%$	3.99%	PASS
Heavy Metals (ICP-MS)	< 10 ppm	Not Detected	PASS
Bacterial Endotoxins (LAL)	< 5 EU/mg	Not Detected	PASS
Sterility (RMM)	USP <71>	Not Tested	-
Mass Balance	95.0 – 105.0%	Conforms	PASS

ANALYST NOTES

The submitted RUO sample was received in an amber 10 mL vial with a nominal label claim of 1,500 mg Glutathione. Quantitative analysis determined a net Glutathione content of 1,657.83 mg, equivalent to 110.52% of the stated label claim. The reported result reflects the measured content of the submitted sample under the applied analytical conditions.

INSTRUMENT DATA

Traces behind the results above

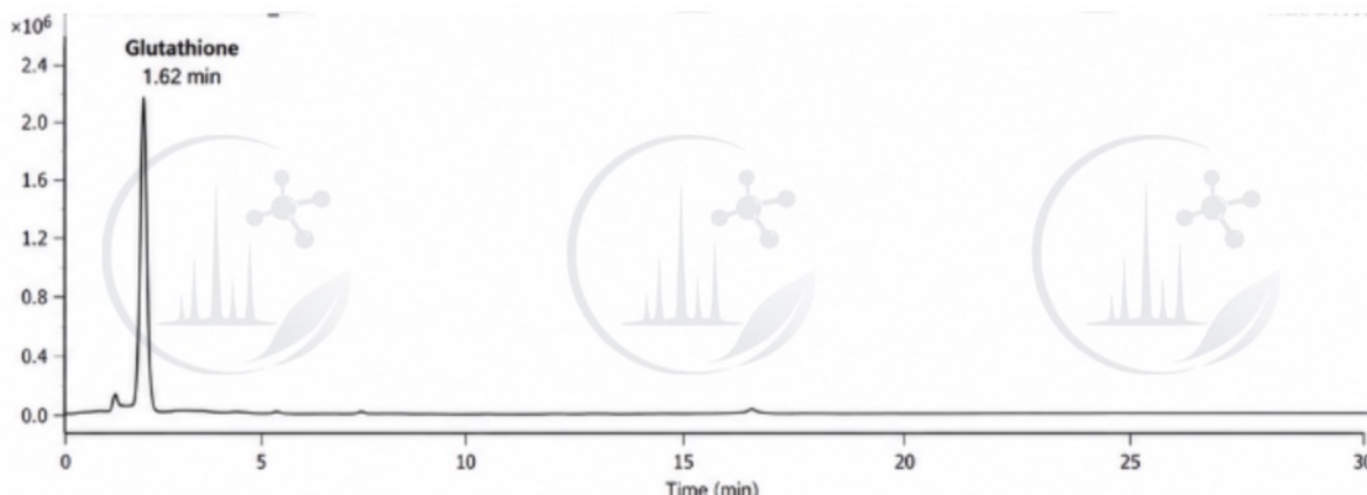


FIGURE 1 — CHROMATOGRAPHIC DATA (HPLC-UV)

Lee Adams

Lee Adams
Lab Director

COA: PMS-9741064507

The analysis reported herein was conducted using HPLC-UV and LC-MS/MS under standard laboratory conditions. This analysis is intended for informational purposes only and is specific to the sample(s) provided. The compounds tested are intended for research use only and are not approved for human or veterinary use, diagnostic, therapeutic, or clinical applications. Results should be interpreted by qualified professionals within the scope of the intended research. The accuracy and reliability of the test may be influenced by sample integrity, handling, and other experimental variables. The sample image included in this Certificate of Analysis was provided by the client during intake. For research use only.



SCAN FOR THE COA LIBRARY
testwithprecision.com/coa-library