




PRODUCT IDENTIFICATION

HPLC-UV coupled with LC-MS/MS, standard laboratory conditions

Compound Name	CJC-1295 w/ Ipamorelin	CAS No.	170851-70-4
Molecular Formula	Not applicable to blend	Molecular Weight	
Appearance	White Lyophilized Powder	Compound Concentration	10mg



MOLECULAR STRUCTURE



CLIENT SAMPLE PHOTO

SAMPLE IDENTIFICATION

Client-supplied, verified at intake

Container Size	3ml Glass Vial	Cap Color	Purple
Crimp / Seal Color	Red		
Product Company	APEXX BIOLABS LLC		

ANALYTICAL RESULTS

Test	Specification	Result	Status
Purity (HPLC)	$\geq 90.0\%$	99.74%	PASS
Mass Identification (LC-MS/MS)	Conforms to declared compound	CJC-1295 w/ Ipamorelin	PASS
Net Peptide Content	$\geq 90\%$ of 10 mg	10.58 mg	PASS
Water Content (Karl Fischer)	$\leq 10.0\%$	4.91%	PASS
Acetate Content (HPLC)	$< 12.0\%$	4.01%	PASS
Heavy Metals (ICP-MS)	< 10 ppm	Not Detected	PASS
Bacterial Endotoxins (LAL)	< 5 EU/mg	Not Detected	PASS
Sterility (RMM)	USP <71>	Not Tested	-
Mass Balance	95.0 – 105.0%	Conforms	PASS

ANALYST NOTES

The submitted RUO sample was identified as a blended preparation containing CJC 1295 and Ipamorelin. Quantitative analysis determined the CJC 1295 content to be 5.31 mg and the Ipamorelin content to be 5.27 mg, for a combined peptide content of 10.58 mg in the tested sample.

INSTRUMENT DATA

Traces behind the results above

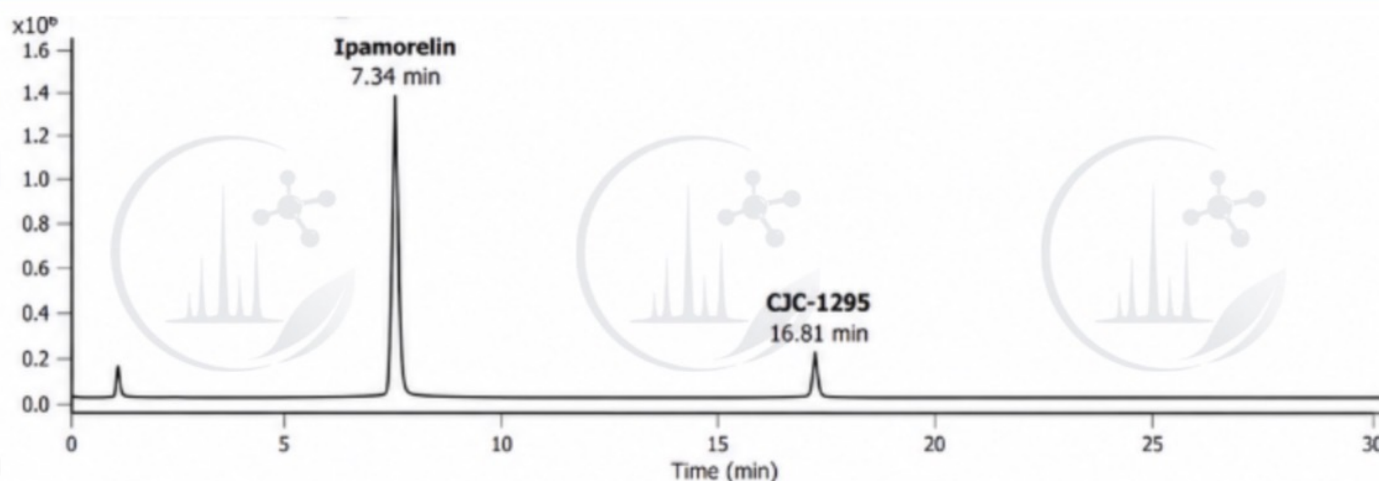


FIGURE 1 — CHROMATOGRAPHIC DATA (HPLC-UV)

Lee Adams

Lee Adams
Lab Director

COA: PMS-9742635981

The analysis reported herein was conducted using HPLC-UV and LC-MS/MS under standard laboratory conditions. This analysis is intended for informational purposes only and is specific to the sample(s) provided. The compounds tested are intended for research use only and are not approved for human or veterinary use, diagnostic, therapeutic, or clinical applications. Results should be interpreted by qualified professionals within the scope of the intended research. The accuracy and reliability of the test may be influenced by sample integrity, handling, and other experimental variables. The sample image included in this Certificate of Analysis was provided by the client during intake. For research use only.



SCAN FOR THE COA LIBRARY
testwithprecision.com/coa-library