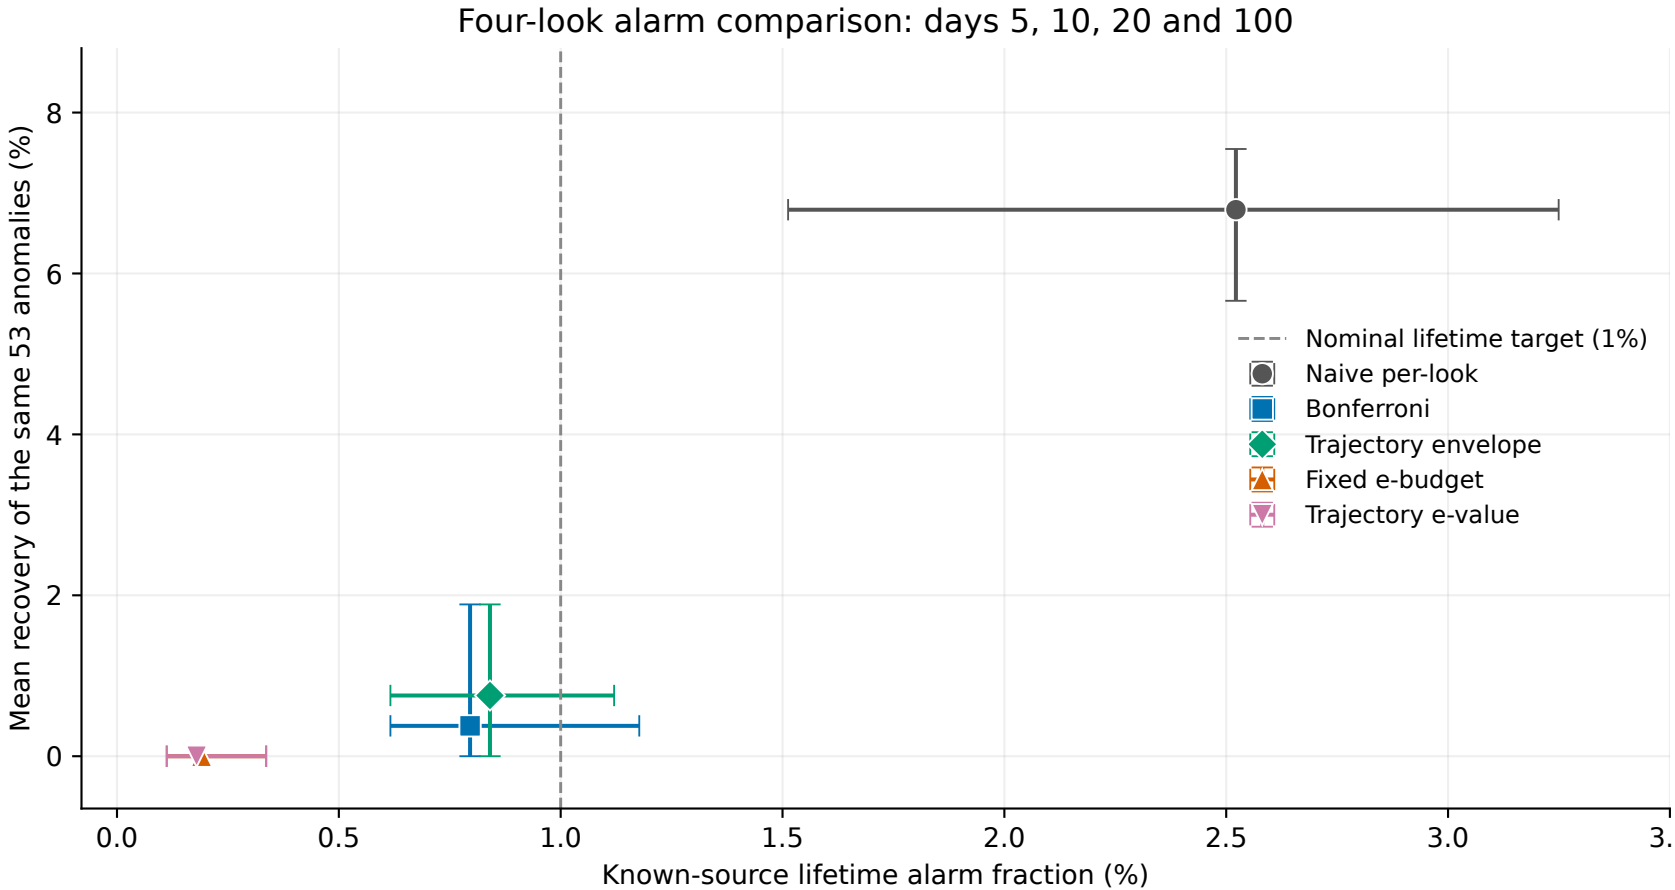


Points: pooled rates for 8,922 held-out known objects; mean anomaly recovery over five refits.
Bars: descriptive fold minima–maxima, not confidence intervals; refits share training/calibration data.
Same 53 anomalies reused. Nominal 1% thresholds; achieved FARs are not matched. Naive: 1% per look.