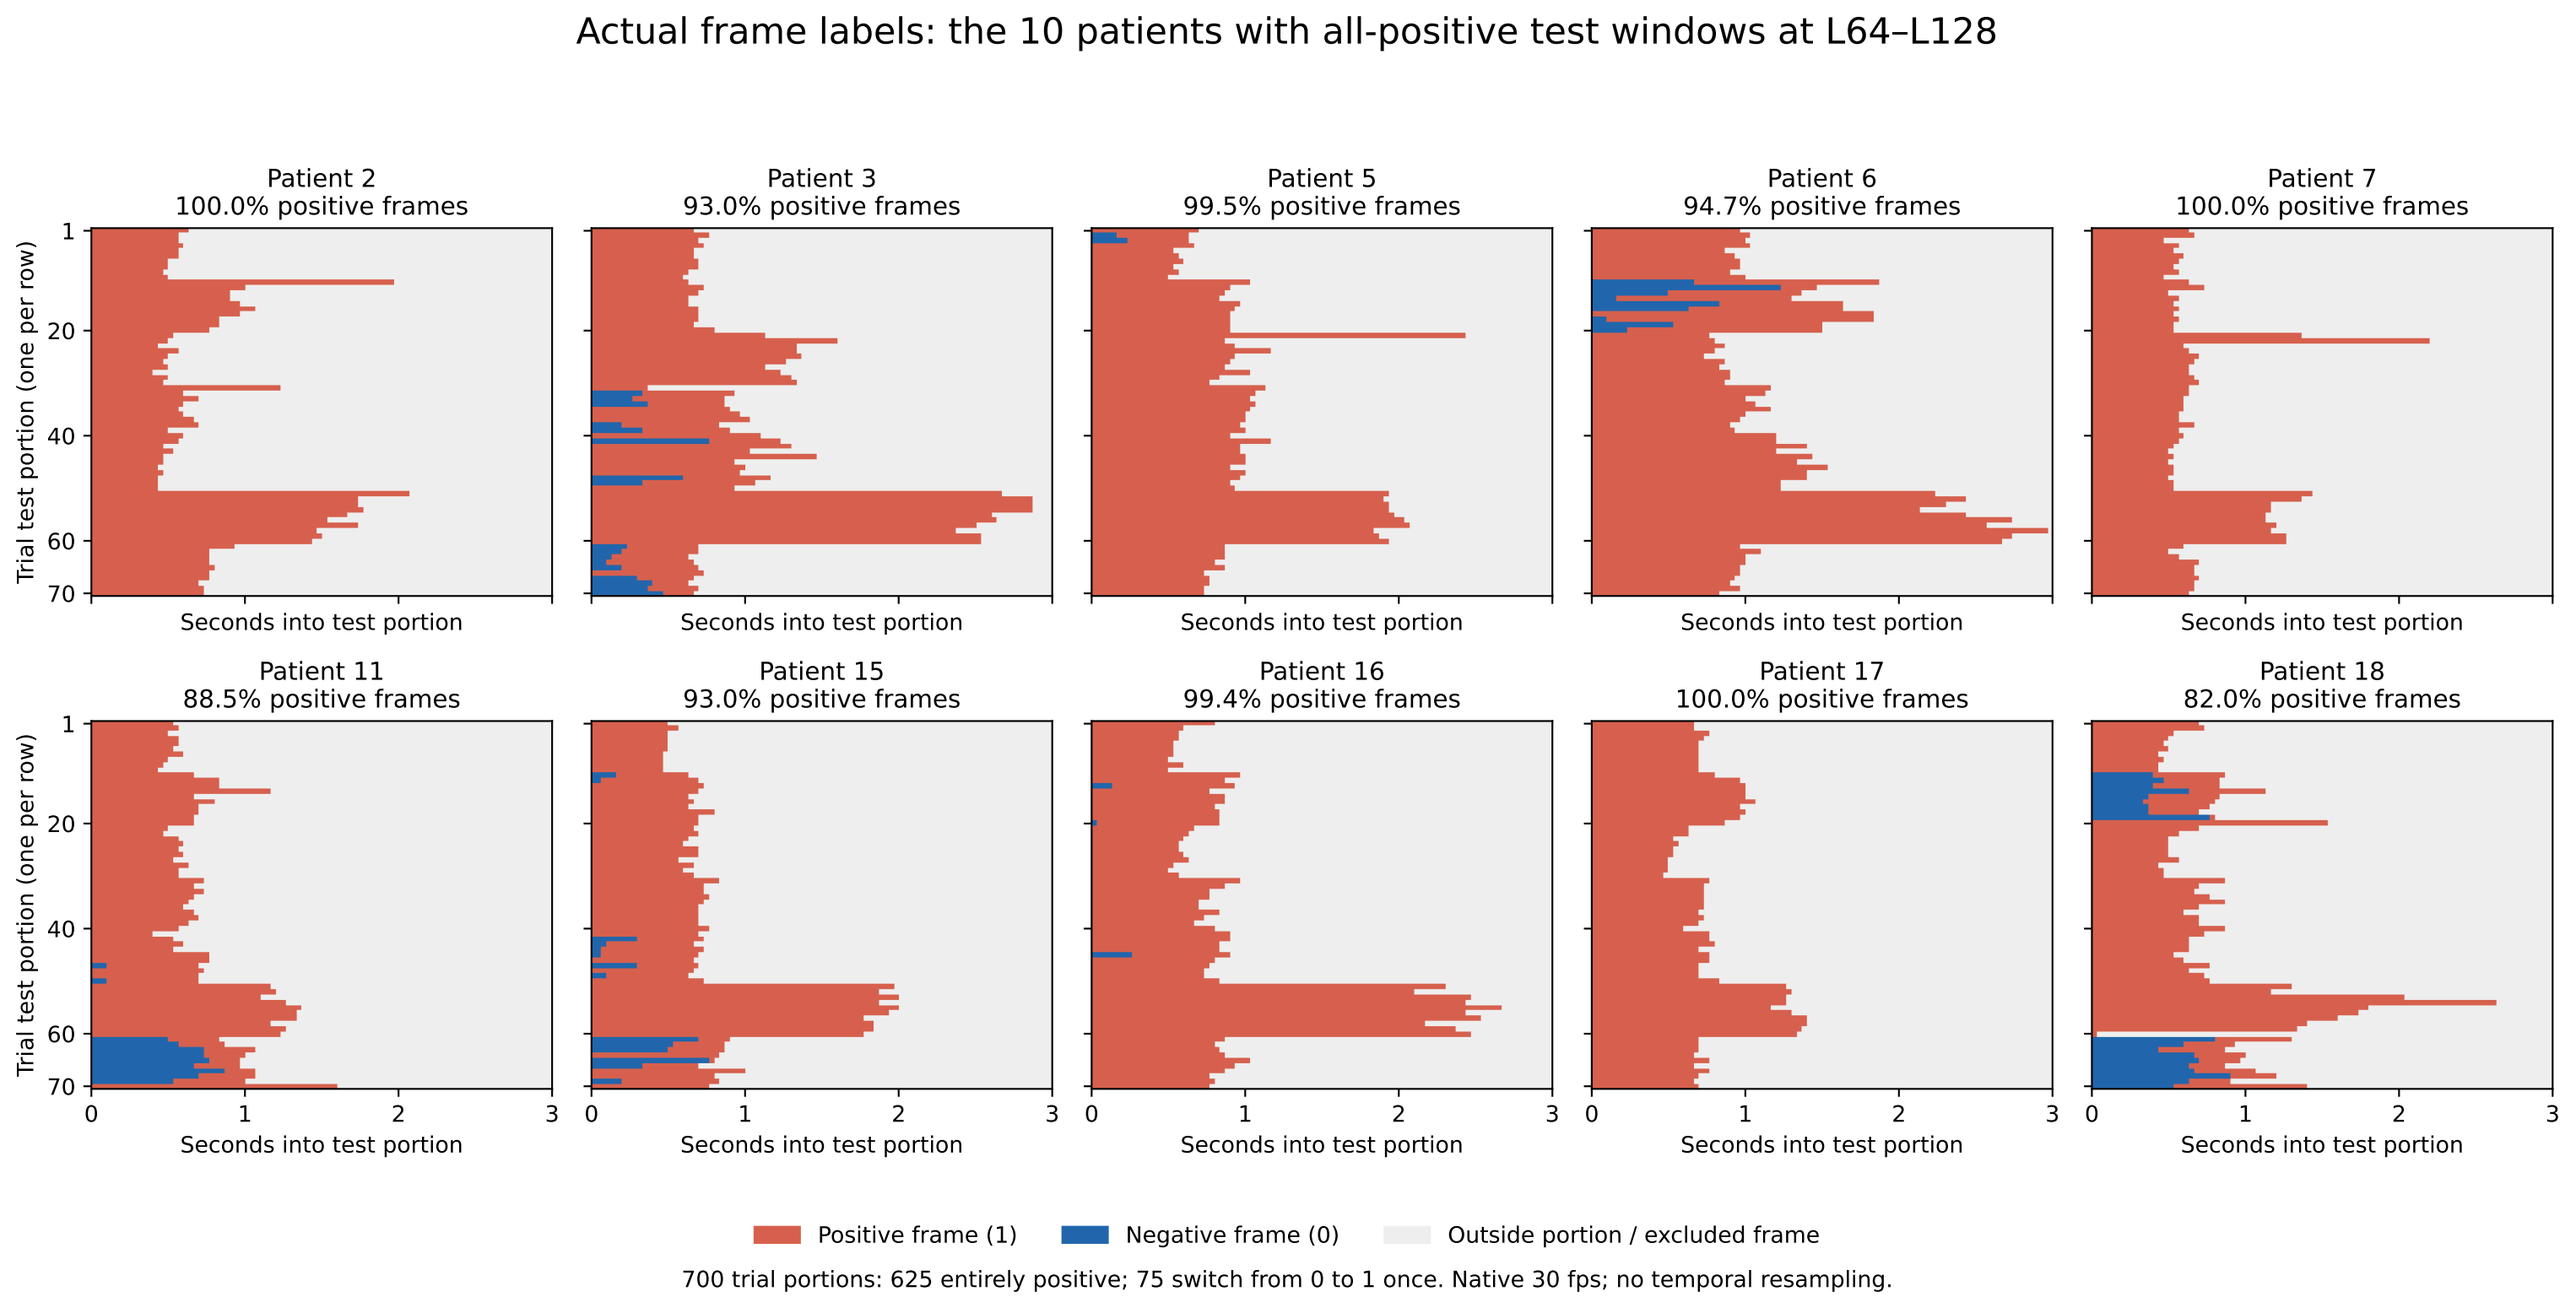
Actual frame labels: the 10 patients with all-positive test windows at L64–L128
Patient 2
100.0% positive frames
Patient 3
93.0% positive frames
Patient 5
99.5% positive frames
Patient 6
94.7% positive frames
Patient 7
100.0% positive frames
Patient 11
88.5% positive frames
Patient 15
93.0% positive frames
Patient 16
99.4% positive frames
Patient 17
100.0% positive frames
Patient 18
82.0% positive frames
Trial test portion (one per row)
1
20
40
60
70
0
1
2
3
Seconds into test portion
Positive frame (1)
Negative frame (0)
Outside portion / excluded frame
700 trial portions: 625 entirely positive; 75 switch from 0 to 1 once. Native 30 fps; no temporal resampling.