

SCPM-Net: An Anchor-Free 3D Lung Nodule Detection Network using Sphere Representation and Center Points Matching

Xiangde Luo^{a,b,*}, Tao Song^{b,*}, Guotai Wang^{a,**}, Jieneng Chen^c, Yinan Chen^{b,d}, Kang Li^d, Dimitris N. Metaxas^e, Shaoting Zhang^{a,b}

^a*School of Mechanical and Electrical Engineering, University of Electronic Science and Technology of China, Chengdu, China*

^b*SenseTime Research, Shanghai, China*

^c*College of Electronics and Information Engineering, Tongji University, Shanghai, China.*

^d*West China Biomedical Big Data Center, Sichuan University West China Hospital, Chengdu, China.*

^e*Department of Computer Science, Rutgers University, Piscataway, NJ 08854 USA*

Abstract

Automatic and accurate lung nodule detection from 3D Computed Tomography (CT) scans plays a vital role in efficient lung cancer screening. Despite the state-of-the-art performance obtained by recent anchor-based detectors using Convolutional Neural Networks (CNNs) for this task, they require predetermined anchor parameters such as the size, number, and aspect ratio of anchors, and have limited robustness when dealing with lung nodules with a massive variety of sizes. To overcome these problems, we propose a 3D sphere representation-based center-points matching detection network (SCPM-Net) that is anchor-free and automatically predicts the position, radius, and offset of nodules without manual design of nodule/anchor parameters. The SCPM-Net consists of two novel components: sphere representation and center points matching. First, to match the nodule annotation in clinical practice, we replace the commonly used bounding box with our proposed bounding sphere to represent nodules with the centroid, radius, and local offset in 3D space. A compatible sphere-based intersection over-union loss function is introduced to train the lung nodule detection network stably and efficiently. Second, we empower the network anchor-free by designing a positive center-points selection and matching (CPM) process, which naturally discards pre-determined anchor boxes. An online hard example mining and re-focal loss subsequently enable the CPM process to be more robust, resulting in more accurate point assignment and mitigation of class imbalance. In addition, to better capture spatial information and 3D context for the detection, we propose to fuse multi-level spatial coordinate maps with the feature extractor and combine them with 3D squeeze-and-excitation attention modules. Experimental results on the LUNA16 dataset showed that our proposed SCPM-Net framework achieves superior performance compared with existing anchor-based and anchor-free methods for lung nodule detection with the sensitivity of 1 FP/Scan, 2 FPs/Scan, and 8 FPs/Scan being 92.2%, 93.9%, and 96.4%, respectively. Moreover, our sphere representation is verified to achieve higher detection accuracy than the traditional bounding box representation of lung nodules. Code will be available at: <https://github.com/HiLab-git/SCPM-Net>.

Keywords: Lung nodule detection, anchor-free detection, sphere representation, center points matching

1. Introduction

Lung cancer is one of the leading life-threatening cancer around the world, and the diagnosis at an early stage is crucial for the best prognosis (Siegel et al., 2015). As

*Equal Contribution, X. Luo did this work during his internship at SenseTime.

**Corresponding author

Email address: guotai.wang@uestc.edu.cn (Guotai Wang)

one of the essential computer-aided diagnosis technologies, lung nodule detection from medical images such as Computed Tomography (CT) has been increasingly studied for automatic screening and diagnosis of lung cancer. Detecting pulmonary nodules is very challenging due to the large variation of nodule size, location, and appearance. With the success of Convolutional Neural Networks (CNN) for object detection, CNN-based algorithms have been widely used for detecting pulmonary nodules from CT scans (Ding et al., 2017; Dou et al., 2017; Zhu et al., 2018; Zheng et al., 2019; Wang et al., 2020; Mei et al., 2021; Tang et al., 2019).

Current automatic CNN-based 2D object detection approaches are often based on pre-defined anchors and can be mainly summarized into two categories. The first uses a two-stage strategy, where the first stage obtains a set of region proposals and the second stage classifies each proposal and regresses the bounding box of the associated instance of that proposal. For example, Faster RCNN (Ren et al., 2015) and its variants (Ding et al., 2017; Dou et al., 2017) use a network to obtain the region proposals following a feature extractor in the first stage and employ a regression head and a classification head in the second stage. The second category only uses one stage to achieve a trade-off between inference speed and accuracy, like SSD (Liu et al., 2016), YOLO (Redmon and Farhadi, 2017). Compared with one-stage detectors, the two-stage detectors use a more complex region proposal network and achieve better performance but also require more inference time. Although these anchor-based methods such as Faster RCNN (Ren et al., 2015), RetinaNet (Lin et al., 2017b), SSD (Liu et al., 2016) and YOLO (Redmon and Farhadi, 2017) have achieved promising results in object detection from 2D natural images, they are faced with several limitations when applied to 3D medical images. First, they typically need a very large set of anchor boxes, e.g. more than 100k in 2D RetinaNet (Lin et al., 2017b), resulting in huge computational and memory consumption for 3D medical images. Second, the use of anchor boxes introduces many hyper-parameters and design choices, including the number, size, and aspect ratio of the anchor boxes. Manual design of these hyper-parameters is not only time-consuming but also subject to human experience, which may limit the detection performance. It was indicated in (Ding et al., 2017) that detection of small objects is sensitive to the manual design of anchors. More-

over, the default anchor configuration is ineffective for detecting lesions with a small size and large aspect ratio (Zlocha et al., 2019), let alone the more complex pulmonary nodules, of which the size can vary by as much as ten times. Therefore, a novel detection framework for objects in 3D medical images with higher efficiency and less manual configuring is highly desirable.

Recently, anchor-free one-stage detection methods have attracted many researcher’s attention and achieved tremendous success in natural image detection (Tian et al., 2019; Duan et al., 2019; Zhou et al., 2019b). These anchor-free detectors use key points (i.e., center points or corner points) and offset in different directions to represent the object. However, they may have limited performance when dealing with complex cases. For example, the center point may not be inside the target object, and corner points may be insufficient to represent objects with irregular shapes. These challenges limit the performance of detector to predict the target’s location. Meanwhile, there is a lack of existing works on using 3D anchor-free detectors to boost the accuracy and efficiency of object detection from volumetric images.

Besides, almost all existing objection detection methods aim to predict or regress the bounding box location and size directly, because all objects are annotated with dense bounding boxes in natural images (Lin et al., 2014; Everingham et al., 2010). However, in clinical pulmonary nodule diagnosis, clinicians pay more attention to the location and diameter of a nodule (MacMahon et al., 2017). Therefore, a 3D lung nodule is often represented by a sphere by specifying its location and radius (Setio et al., 2017), rather than a 3D bounding box. Motivated by these observations, we investigate using sphere (parameterized by the central coordinate and radius) to precisely represent lung nodule in 3D space. However, to the best of our knowledge, there have been no studies on using bounding sphere for 3D nodule representation and detection.

Based on these observations, we propose a novel 3D Sphere Representation-based Center-Points Matching Network (SCPM-Net) for pulmonary nodule detection in 3D CT scans. The SCPM-Net is a one-stage anchor-free detection method, which predicts the probability of a pixel i in a coordinate grid being around the center of a nodule, and simultaneously regresses the radius and offset from pixel i to the real nodule center. It is worth mentioning that few works focus on 3D anchor-free detection in med-

ical images, and unlike recent anchor-free methods (Law and Deng, 2018; Duan et al., 2019) for 2D natural images, we don’t need a key points estimation network to generate a heatmap. Due to the huge variations of size, shape, and location of lung nodules, using a single centroid to represent the lung nodule may lead to a low sensitivity and further limit the potential for clinical application (Song et al., 2020). In addition, we proposed a novel center points matching strategy, which uses K points near the centroid to represent a nodule to improve the sensitivity of detectors. Another highlight of our work is that we introduce a sphere representation for lung nodules in 3D space, and further derive an effective sphere-based loss function (L_{SIOU++}) to train our anchor-free detector. Compared to the traditional Intersection-over-Union loss (Zhou et al., 2019a) that is based on bounding boxes, the L_{SIOU++} here is closer to clinical scene, since a nodule’s geometry structure is similar to a sphere or an ellipsoid in most situations. Moreover, our SCPM-Net is a one-stage end-to-end network without additional false positive reduction module adopted in (Ding et al., 2017; Dou et al., 2017; Mei et al., 2021; Tang et al., 2019), so that it has a higher efficiency and lower memory cost.

A preliminary version of this work was published in MICCAI2020 (Song et al., 2020), where we first introduced a center-points-matching-based anchor-free detection network for lung nodule detection in 3D CT scans. In this extend version, we provide more details of our proposed method and describe this work more precisely. Additionally, we introduce a novel sphere representation-based intersection-over-union loss (L_{SIOU++}) and provide more experiments to better demonstrate the effectiveness of L_{SIOU++} for lung nodule detection. Meanwhile, we provide a deeper analysis and discussion of this work. Our main contributions are summarized as follows:

- 1) We mitigate the ineffectiveness of current anchor-based detectors (Ren et al., 2015; Lin et al., 2017b) by discarding pre-determined anchor boxes, as we instead predict a center-point map directly via a points matching strategy. To this end, we propose an anchor-free center-points matching network named as SCPM-Net with novel attentive modules (Hu et al., 2018), online hard example mining (Shrivastava et al., 2016), and re-focal loss (Lin et al., 2017b).
- 2) We present the first attempt to represent the pul-

monary nodule as a bounding sphere in 3D space. Based on sphere representation, we further derive an effective sphere-based intersection-over-union loss function (L_{SIOU++}) to train SCPM-Net for pulmonary nodule detection.

- 3) We evaluate our approach on LUNA16 dataset (Setio et al., 2017), and experimental results showed that the proposed SCPM-Net with L_{SIOU++} achieved superior performance compared with anchor-based and existing anchor-free methods for lung nodule detection from 3D CT scans.

2. Related works

2.1. Anchor-Free Model for Object Detection

Object detection is a fundamental task in the computer vision community and has been studied for many years (Zhao et al., 2019). In the past few years, many anchor-based frameworks have achieved good performance in natural image detection (Ren et al., 2015; Lin et al., 2017b; Redmon and Farhadi, 2017; Liu et al., 2016), but they are also limited by computational and inference time cost. Recently, anchor-free detectors are widely used in image detection to boost inference speed and alleviate computing cost (Law and Deng, 2018; Duan et al., 2019; Zhou et al., 2019c; Tian et al., 2019). Differently from anchor-based detection frameworks, anchor-free methods do not use predefined anchor boxes to predict bounding boxes. Instead, they locate target objects by predicting the central points, size and offsets directly.

2.2. Loss function for Object Detection

Many detection methods used $L1$ or $L2$ distance loss functions for bounding box regression (Zhou et al., 2019a), but they are sensitive to various scales. As a popular evaluation metric, the Intersection-over-Union (IoU) has been used to train various detectors, as it is invariant to the scale. For two bounding boxes B^a and B^b , the IoU loss (L_{IoU}) is defined as:

$$L_{IoU} = 1.0 - \frac{|B^a \cap B^b|}{|B^a \cup B^b|} \quad (1)$$

After that, many extensions are proposed to boost the detector’s performance by adopting the classical L_{IoU} . For

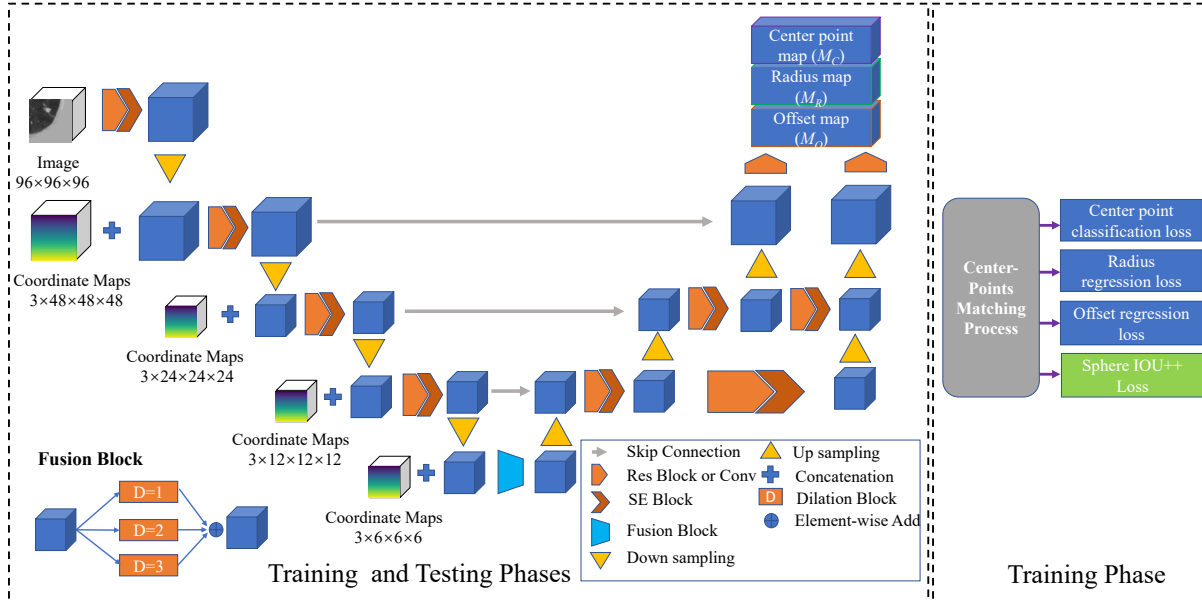


Figure 1: Overview of the proposed SCPM-Net. It consists of an encoder-decoder network with some fusion and attention blocks. The SCPM-Net predicts a center point map M_C , a radius map M_R and an offset map M_O to locate target objects without any predefined anchor boxes. In the training stage, a novel center points matching strategy is used to mining hard example for better performance. A geometric-aware sphere representation is proposed to represent the nodule and a sphere-based IoU loss function (L_{SIOU++}) is proposed to combine geometric measures with CNN for lung nodule detection.

example, GIoU (Rezatofighi et al., 2019) loss was proposed to deal with gradient vanishing in non-overlapping cases. To further improve models’ ability of bounding box regression, DIOU (Zheng et al., 2020) loss modified L_{IoU} by bringing in the normalized distance between a predicted box and the target box. All of these losses have achieved promising performance in 2D nature image detection tasks. Meanwhile, L_{IoU} is also used in 3D medical image analysis as a powerful and efficient loss function to train 3D detectors (Li et al., 2019; Wang et al., 2020; Tang et al., 2019; Mei et al., 2021).

2.3. 3D Pulmonary Nodule Detection

Pulmonary nodule detection plays an essential role in lung cancer diagnosis and treatment. Thus, automated Computer-Aided Diagnosis (CAD) for pulmonary nodule detection has been an active research field. Most of the CAD systems include two stages: nodule candidate detection and false positive reduction. In order to detect nodules at different scales, most previous works extended 2D anchor-based detectors to handle 3D nodule detection,

such as using Faster R-CNN (Ren et al., 2015), FPN (Lin et al., 2017a). Even so, how to guarantee a high sensitivity with a lower false positive rate is a challenging problem. Hence, False Positive Reduction (FPR) models (Ding et al., 2017; Dou et al., 2017) were adopted in pulmonary nodule CAD systems as a second stage to reduce false positives. To alleviate foreground-background class imbalance, focal loss (Lin et al., 2017b) was used to train anchor-based detectors (Wang et al., 2020). These methods have largely improved the performance of pulmonary nodule detection (Ding et al., 2017; Zheng et al., 2019; Wang et al., 2020). However, suffered by the pre-defined anchor boxes and multiple stages, these methods need to carefully design many hyper parameters manually to obtain a good performance. In addition, anchor-based multi-stages detectors require higher computational cost and time than anchor-free detectors (Tian et al., 2019).

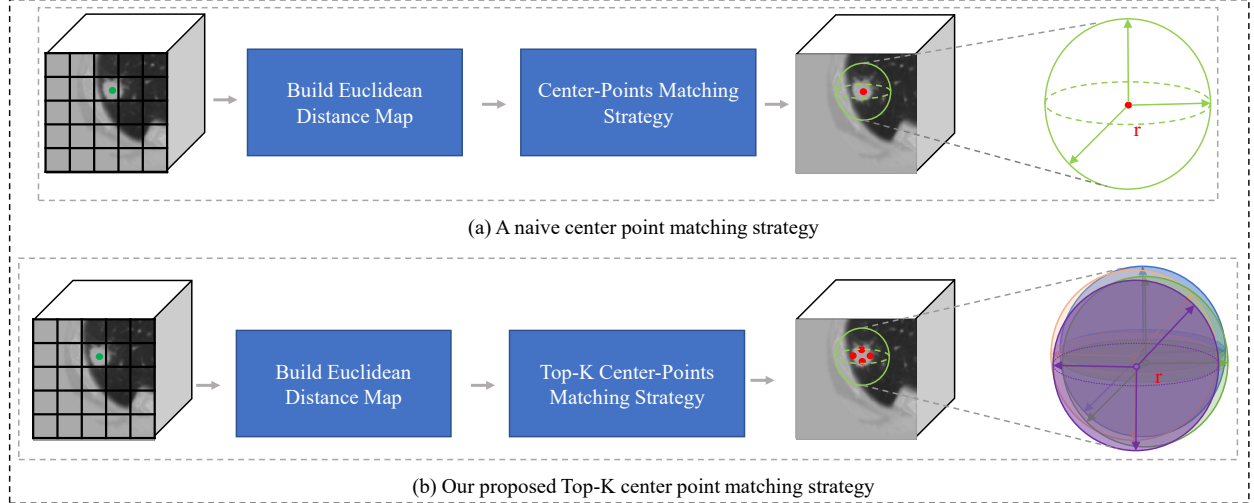


Figure 2: Illustration of center-point matching used for training. (a) is a simple center point matching strategy, where a nodule is only associated with a single centroid. (b) is our proposed top- K center points matching strategy, where we find K points around the centroid of the nodule.

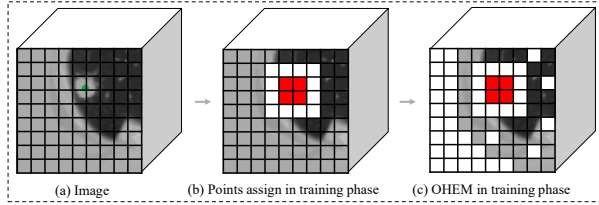


Figure 3: The points assigning process in the training phase. Red, white and the others grids mean positive, ignored and negative points respectively.

3. Method

The overall structure of the proposed SCPM-Net is illustrated in Fig. 1. It consists of a feature extractor that takes advantage of multi-level spatial coordinate maps and Squeeze-and-Excitation (SE)-based channel attention for better feature extraction, and a head that predicts the existence of a nodule and its radius and offset simultaneously at two resolution levels. To assist the training process, we propose a center points matching strategy to predict K points that are nearest to the center of a nodule. Inspired by clinical guidance (MacMahon et al., 2017), we use a novel sphere representation of nodules to improve the detection accuracy. We represent the network’s 3D input as $I \in \mathbb{R}^{D \times H \times W}$, where D , H and W denote depth,

height and width of the input image, respectively. The predicted feature map with the size of $\frac{D}{R} \times \frac{H}{R} \times \frac{W}{R} \times C$ can be obtained by forward process of the SCPM-Net, where R denotes down-sampling ratio and C denotes channel number. Let M_C represent the center point map with one channel indicating the probability of each pixel (i.e., point), being close to the center of a nodule, M_R represent the radius map with one channel where each element gives the radius of the nodule centered at that pixel, and M_O represent the offset map with three channels indicating offsets of the center point in the directions of x , y , and z , respectively.

3.1. Architecture of the SCPM-Net

The architecture of our detection backbone follows an encoder-decoder flowchart as shown in Fig. 1. It has a series of convolutional layers to learn 3D patterns. Each convolution uses $3 \times 3 \times 3$ kernels with 1 as stride, and each down-sampling and up-sampling is implemented by max-pooling and deconvolution, respectively. Skip connections are used to link low-level features and high-level features. Each of the last two decoder blocks in our SCPM-Net obtains three prediction maps, i.e. center point map M_C , radius map M_R , and offset map M_O , respectively. To be clear, the center point map (M_C) is a pixel-wise binary classification map, where each element gives the probabil-

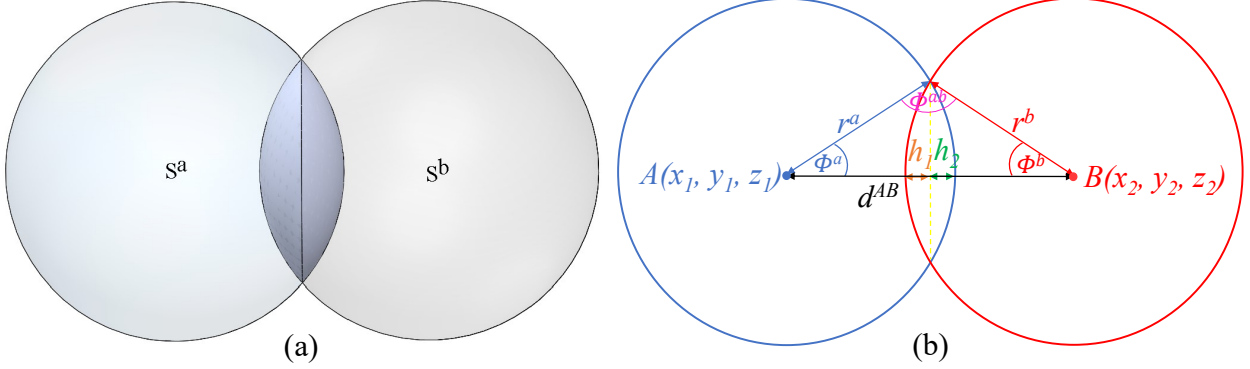


Figure 4: Illustration of SIoU calculation. (a) An example of intersection between two spheres; (b) A projection view of the intersection area between two spheres.

ity of the corresponding pixel being a center point. Following (Zhao et al., 2019), an offset map (M_O) is used to represent the offset from the current point to the real centroid of a nodule and a radius map (M_R) is used to represent the predicted radii of the bounding spheres. In particular, we introduce multi-path normalized coordinate map fusion blocks to generate attentive features for being aware of spatial position. These coordinate maps are generated by using three channels to encode the spatial coordinates along x, y, and z directions, respectively. We obtain a pyramid of the coordinate map by downscaling it into four resolution levels, with the size of 48^3 , 24^3 , 12^3 , and 6^3 respectively. At each resolution level of the pyramid, we concatenate the coordinate map with the image features. Following (Hu et al., 2018), SE-blocks are adopted to learn spatial and channel-wise attentions to enhance more discriminative features. In the last block of the encoder, we utilize a dilated fusion block, consisting of three dilated convolutions with dilation rates of 1, 2, 3 respectively. In the training phase, we use a proposed center-points matching procedure as mentioned in Sec. 3.2 and a combination loss as described in Sec. 3.4. In the testing phase, a bounding sphere of detection result can be constructed by the position of predicted centroids, radius, and offset as clarified in Sec. 3.5.

3.2. Center-Points Matching

Anchor-based methods assign positive and negative anchors according to the threshold of overlap between anchor boxes and ground-truth for training. In contrast,

without any anchor prior, a novel center-points matching strategy for training is proposed in this work to assign positive, negative, and ignored labels to make the network predict whether a point belongs to center points of lung nodules. In short, this center-points matching process is to generate classification labels in the training phase on the fly. Fig. 2 shows two different point matching strategies in the training phase: (a) a simple center point matching strategy, where the nodule is only associated with one centroid. (b) our proposed top- K points matching strategy, which uses K points near the centroid to represent a nodule.

The whole strategy can be divided into four steps: 1) calculating the distance between each point to the ground truth centroid and using the distance map as a prior to assigning positive, negative, and ignored points; 2) selecting top- K points that are nearest to a centroid as the positive point set \mathcal{P} ; 3) to reduce the false positive, a certain amount of points around positive points are put into the set of ignored points \mathcal{I} . The remaining points are treated as a temporary negative points-set \mathcal{N} ; 4) using online hard example mining (OHEM (Shrivastava et al., 2016), detailed in Sec. 3.4) to further sample hard negative points as point set $\mathcal{N}' \subset \mathcal{N}$, while points in $\mathcal{N} - \mathcal{N}'$ are reset to the ignored points, and therefore we can obtain an ignored point set $\mathcal{I}' = \mathcal{I} + \mathcal{N} - \mathcal{N}'$. The points assigning process in the training phase is shown in Fig. 3. It is worth mentioning that this matching strategy can be used to train any center points-based anchor-free detector. But in this paper, we pay more attention to training a detector to predict the

bounding sphere. We loop all the annotations in the image using the above steps. Note that the top- K positive points are selected according to the lowest distance values sorted in the distance map, and ignored points do not participate in training.

3.3. Sphere Representation and Sphere-Based Loss Functions

3.3.1. Similarity based on Sphere Representation

Due to the ellipsoid-like shape, lung nodules can be better represented by the bounding sphere than the bounding box (Sladoje et al., 2005). In clinical pulmonary nodule diagnosis, it is a common practice that using the coordinate and diameter to represent the nodule in 3D space (Setio et al., 2017; MacMahon et al., 2017). Based on these observations, we use the sphere representation for nodules in 3D space. First, we introduce a sphere-based intersection-over-union (SIoU) to measure the similarity between a predicted nodule and the ground truth nodule. The SIoU similarity is defined as:

$$SIoU = \frac{|S^a \cap S^b|}{|S^a \cup S^b|} \quad (2)$$

where S^a and S^b denote the predicted bounding sphere and the ground truth bounding sphere respectively as shown in Fig. 4 (a). To better formulate this method, we use a projection view to illustrate calculations details in Fig. 4 (b). The centroids of sphere A and sphere B are defined as $A(x_1, y_1, z_1)$ and $B(x_2, y_2, z_2)$ in image space respectively. r^a and r^b denote the radius of sphere A and sphere B respectively. The distance of between the central coordinates of sphere A and B is defined as:

$$d^{AB} = \|A - B\|_2 \quad (3)$$

When S^a and S^b are intersected, i.e., $r^a + r^b > d^{AB}$, let ϕ^a and ϕ^b denote the central angles of the two spheres, respectively, and let ϕ^{ab} denote the intersection angle. h_1 and h_2 represent the distance between the intersected chord to the arcs, respectively, as shown in Fig. 4(b). These values and the intersection between A and B can be obtained by:

$$\cos(\phi^a) = \frac{(r^a)^2 + (d^{AB})^2 - (r^b)^2}{2r^a d^{AB}} \quad (4)$$

$$\cos(\phi^b) = \frac{(r^b)^2 + (d^{AB})^2 - (r^a)^2}{2r^b d^{AB}} \quad (5)$$

$$\cos(\phi^{ab}) = \frac{(r^b)^2 + (r^a)^2 - (d^{AB})^2}{2r^a r^b} \quad (6)$$

$$h_1 = r^b(1 - \cos(\phi^b)) \quad (7)$$

$$h_2 = r^a(1 - \cos(\phi^a)) \quad (8)$$

$$|S^a \cap S^b| = \pi r^a h_2^2 - \frac{\pi h_2^3}{3} + \pi r^b h_1^2 - \frac{\pi h_1^3}{3} \quad (9)$$

When S^a and S^b are not intersected, i.e., $r^a + r^b \leq d^{AB}$, $|S^a \cap S^b|$ is 0. The union between S^a and S^b is defined as:

$$|S^a \cup S^b| = \frac{4\pi((r^a)^3 + (r^b)^3)}{3} - |S^a \cap S^b| \quad (10)$$

Based on these sub-modules, we can calculate the SIoU similarity of two spheres using Eq. (2).

3.3.2. Sphere-Based Intersection-over-Union Loss Function

The effectiveness of IoU-based loss function has been well proved for 2D detection tasks (Rezatofghi et al., 2019; Zhou et al., 2019a; Zheng et al., 2020). However, there are few works that focus on designing loss function for 3D object detection, especially in 3D medical images. Based on our proposed sphere representation, we introduce a Sphere Intersection-over-Union (SIoU) loss for 3D nodule detector training which is inspired by (Zhou et al., 2019a; Rezatofghi et al., 2019; Zheng et al., 2020):

$$L_{SIoU} = 1 - SIoU \quad (11)$$

where $SIoU$ is defined in Eq. (2). Similarly with traditional Intersection over Union loss function L_{IoU} (Zhou et al., 2019a), L_{SIoU} only works when the predicted sphere and the ground truth have overlap, and would not provide any moving gradient for non-overlapping cases. To deal with the cases where S^a and S^b are not intersected, we additionally use distance and radius ratio (R_{DR}) for optimization.

$$R_{DR} = \frac{d^{AB}}{d^{AB} + r^a + r^b} \quad (12)$$

Then, we integrate the R_{DR} into L_{SIoU} :

$$L_{SDIoU} = 1.0 + R_{DR} - SIoU \quad (13)$$

In addition, we found that the angle of intersection ϕ^{ab} between the two spheres can also be used to better describe the regression of the sphere. We therefore define a angle score η as follows:

$$\eta = \begin{cases} 0, & \text{if } d^{AB} > (r^a + r^b) \\ \frac{\arccos(\phi^{ab})}{\pi}, & \text{otherwise} \end{cases} \quad (14)$$

Finally, we integrated all geometric measures (sphere iou, distance and radius ratio, angle of intersection) into a unified loss, which is referred to as L_{SIoU++} :

$$L_{SIoU++} = \begin{cases} R_{DR}, & \text{if } d^{AB} > (r^a + r^b) \\ 1.0 + R_{DR} - SIoU + \eta, & \text{otherwise} \end{cases} \quad (15)$$

It can be observed that the sphere representation considers many geometric measures, i.e., overlap area ($S^a \cap S^b$), central point distance (d^{AB}) and angle of intersection (η), which have been ignored in the other representations. The pseudo-code for L_{SIoU++} computation with two spheres is given in Alg. (1). The properties of L_{SIoU++} function can be summarized as follows:

- 1) Like the genral L_{IoU} , our L_{SIoU++} is invariant to the scale of regression problem.
- 2) L_{SIoU++} can alleviate the gradient vanishing problem when there is not overlap between prediction and the ground truth.
- 3) L_{SIoU++} converges much faster than L_{IoU} , since L_{SIoU++} minimizes the overlap, distance, radius ratio and angle of intersection directly.

3.4. The Overall Loss Function

The imbalance of positive and negative samples in 3D point classification is more severe than that in 2D point classification. A hybrid method of Online Hard Example Mining (OHEM) (Shrivastava et al., 2016) and re-focal loss (Lin et al., 2017b) are used in our SCPM-Net to deal with such a huge imbalance. In OHEM, we select some hardest negative point samples for training. Specifically, all the negative points are sorted in the descending order

Algorithm 1: Pseudocode of L_{SIoU++} for 3D Lung Nodules Detector Training.

Input: Central coordinates $A(x_1, y_1, z_1)$ and $B(x_2, y_2, z_2)$ and radii r^a and r^b of two spheres in image space respectively.

Output: L_{SIoU++} ;

Initialization: $d^{AB} = \|A - B\|_2$; $R_{DR} = \frac{d^{AB}}{d^{AB} + r^a + r^b}$;

if ($r^a + r^b > d^{AB}$) **then**

Calculate $|S^a \cap S^b|$ according to Eq. (9);

Calculate $|S^a \cup S^b|$ according to Eq. (10);

Calculate the $SIoU$ according to Eq. (2);

Calculate the angle score η using Eq. (14);

Calculate $L_{SIoU++} = 1.0 + R_{DR} - SIoU + \eta$;

end

else

$L_{SIoU++} = R_{DR}$;

end

return L_{SIoU++} ;

of the center point classification loss, and we select the first N points of them after the sorting. N is set to $100M$ if $M > 0$ and 100 otherwise, where M is the number of positive points in the input image. In the end, negative points those are not selected are reset as ignored points. A re-focal loss is shown as Eq. (16), which can improve the sensitivity and further balance the gradient of the positives and the negatives.

$$L_{cls} = \sum_{j=0}^J -w_j \alpha (1 - p_j)^\gamma \log(p_j) \quad (16)$$

The weight of re-focal loss is defined as:

$$w_j = \begin{cases} 1, & \text{if } j \in \mathcal{P} \text{ and } p_j > t \text{ or } j \in \mathcal{N} \\ 0, & \text{if } j \in \mathcal{I} \\ w, & \text{if } j \in \mathcal{P} \text{ and } p_j < t \end{cases} \quad (17)$$

where p_j denotes the probability of point j being the centroid of a nodule. $J = \frac{D}{R} \times \frac{H}{R} \times \frac{W}{R}$ is the total number of points. t is a threshold to filter unqualified points, and w is a weight to balance the re-focal loss. A smooth L1 loss (Ren et al., 2015) is also used to regress the normalized radius of bounding sphere:

$$L_{radius}(r, r^*) = \begin{cases} \frac{0.5(r-r^*)^2}{\beta}, & \text{if } |r - r^*| < \beta \\ |r - r^*|, & \text{otherwise} \end{cases} \quad (18)$$

where r denotes predicted radius value, and r^* is the ground truth radius value. To obtain more accurate locations of small objects, we use $L2$ loss to regress the offset between the center points ground truth and the predicted positive points.

$$L_{offset}(f, f^*) = \|f - f^*\|_2 \quad (19)$$

where f and f^* are 3D vectors and denote the predicted and ground truth offsets, respectively. The total loss is expressed by the following equation:

$$L_{total} = L_{cls} + \alpha(L_{radius} + L_{offset} + \lambda_s L_{SIoU++}) \quad (20)$$

where L_{radius} , L_{offset} and L_{SIoU++} are only meaningful for positive points, thus we define $\alpha = 1$ for points in \mathcal{P} and 0 for points in \mathcal{I} and \mathcal{N} . λ_s represents the weight factor of L_{SIoU++} .

3.5. Implementation Details

We used PyTorch (Paszke et al., 2019) to implement our SCPM-Net. The training and testing process were done via SenseCare (Duan et al., 2020) platform with one 8-core Intel E5-2650 CPUs, 8 NVIDIA 1080Ti GPUs and 2T memory. During pre-processing, we resampled all images to the isotropic resolution of $1.0 \times 1.0 \times 1.0 \text{ mm}^3$ to reduce the spatial variation among images and normalized them to zero mean and unit variance. In the training phase, following (Song et al., 2020; Wang et al., 2020), we randomly cropped a patch with a size of $96 \times 96 \times 96$ as the input of SCPM-Net. For each model, we used 170 epochs in total with stochastic gradient descent optimization, momentum 0.9, and weight decay 10^{-4} . The batch size was 24. The initial learning rate was 10^{-4} in the first 20 epochs for warm up training, and then set as 10^{-2} , 10^{-3} and 10^{-4} after 20, 80 and 150 epochs, respectively.

In the inference phase, we used sliding window with a stride of $24 \times 24 \times 24$ to obtain the whole scan’s prediction. Then, we picked up top- n candidate predicted points $[p_0, p_1, \dots, p_{n-1}]$ in a classification map with a size of $D \times H \times W \times 1$ by sorting the probabilities. Each predicted candidate point has a probability p_j in a 3D integer location $\mathbf{x}_j \in \mathbb{Z}^3$. In the same integer location, we can get an offset prediction $\mathbf{v}_j \in \mathbb{R}^3$ and a radius prediction r_j , respectively. Then a detected bounding sphere will be located at $\mathbf{x}_j + \mathbf{v}_j$ with a radius of r_j . Finally, all the detected spheres will pass a 3D SIoU++ based non-maxima

suppression (NMS) (Ren et al., 2015; Zheng et al., 2020) to filter overlapping spheres. Compared with IoU-based NMS, the SIoU++ based NMS uses SIoU and distance and radius ratio of two spheres as the measures to filter redundant spheres. Parameter setting was $K = 7$, $\lambda_s = 2$, $t = 0.9$, $w = 4$, $\beta = \frac{1}{9}$, $\alpha = 0.375$, $\gamma = 2$ and $n = 100$ based on a grid search with the validation data.

4. Experimental Results

4.1. Dataset and Evaluation Metrics

In this work, we validated the proposed framework on the large-scale public challenge dataset of LUNA16 (Setio et al., 2017), which contains 888 low-dose CT scans with the centroids and diameters of the pulmonary nodules annotated. In the LUNA16 challenge, performances of detection systems are evaluated using the Free-Response Receiver Operating Characteristic (FROC) (Setio et al., 2017). The sensitivity and the average number of false positives per scan (FPs/Scan) are used to measure the detector’s performance. In this work, we used the first nine subsets (includes 800 scans) for training and validation and the last subset (includes 88 scans) for testing. Ablation study and efficiency evaluation are presented in Sec. 4.2, 4.3, 4.4, 4.5.1. We further compare the proposed with state-of-the-art methods using 10-fold cross-validation in Sec. 4.5.2.

4.2. Analysis of SCPM-Net

The attentive module with Coordinate Attention (CA) and Squeeze-and-Excitation (SE) attention is a crucial component of our SCPM-Net. To understand each component’s contribution to performance, we perform an ablation study firstly. Following (Song et al., 2020), λ_s in Eq. (20) was set as 0 to investigate the effectiveness of SCPM-Net without any extra effects. In addition, the OHem and the center-points matching strategy are used to train detectors stably and efficiently, and K is set to 7. Then, we trained three models: 1) SCPM-Net without both CA and SE attentions; 2) SCPM-Net without CA but with SE attention module; 3) SCPM-Net with both CA and SE attentions. A quantitative evaluation of this ablation study is listed in Table 1. It shows that adding SE and CA improves the sensitivity by 4.4% at 1 FPs/Scan, by 3% at 2 FPs/Scan and by 2.1% at 8 FPs/Scan, respectively.

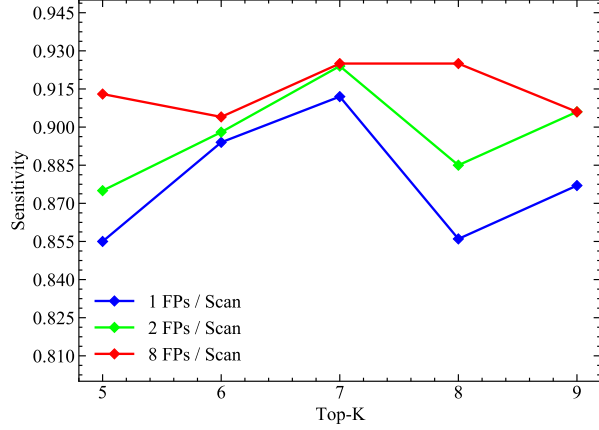


Figure 5: Detection performance of SCPM-Net with center points matching strategy with different values of K .

Module	Sensitivity		
	FPs/Scan=1	FPs/Scan=2	FPs/Scan=8
w/o SE and CA	86.8%	89.4%	90.4%
w/o CA	90.5%	90.8%	91.5%
SCPM-Net	91.2%	92.4%	92.5%

Table 1: Ablation study of SCPM-Net. SE and CA represent squeeze-and-excitation attention and coordinate attention respectively. (FPs/Scan: the false positives per scan)

4.3. Effect of Center-Points Matching Strategy

To investigate the effect of our center-points matching strategy, we set λ_s in Eq. (20) to 0 without any additional efforts, and compared the performance at different K values for selecting the top- K positive center points of each nodule during training, as mentioned in Sec.3.2. Fig. 5 shows evolution of the detector’s performance on the testing subset when K changes from 5 to 9. It can be found that when K is greater or smaller than 7, the sensitivity goes down significantly. This is because too many positive points during training will bring in false positives while few positive points weaken the model’s ability to locate the nodules. Therefore, we set $K = 7$ for our center-points matching strategy in the following experiments.

4.4. Effects of Sphere-Based Intersection-over-Union Loss

We first analyzed the difference of gradient between L_{IoU} , L_{SIoU} and L_{SIoU++} by simulating the procedure of

Method	Sensitivity		
	FPs/Scan=1	FPs/Scan=2	FPs/Scan=8
IoU	90.4%	91.3%	94.2%
SIoU	90.0%	92.4%	93.5%
SIoU with R_{RD}	90.5%	92.1%	93.0%
SIoU++	92.3%	92.7%	94.8%

Table 2: Ablation study of L_{SIoU++} function. The L_{SIoU++} consists of sphere IoU term (SIoU), angle of intersection and distance-radius-ratio term (R_{RD}). (FPs/Scan: the false positives per scan)

sphere regression using gradient descent algorithm. To better formulate this study, we suppose that the predicted sphere S^a is at $(0, 0, -8)$ and the ground truth sphere S^b is at the origin of 3D coordinate. Assume both of them have a radius of 1.5. Then, we calculate the partial derivatives: $\frac{\partial L_{IoU}}{\partial z}$, $\frac{\partial L_{SIoU}}{\partial z}$, $\frac{\partial L_{SIoU++}}{\partial z}$ when S^a gradually moves to S^b along the z -axis. Fig. 6 shows evolution of these gradient values with different d^{AB} . Compared with L_{IoU} and L_{SIoU} , L_{SIoU++} can provide optimization directions for non-overlapping cases (i.e., $d^{AB} > 3$). In addition, L_{SIoU++} has higher gradient values than L_{IoU} and L_{SIoU} , since L_{SIoU++} is a joint optimization loss which considers more geometric measures (overlap, distance, radius ratio and angle of intersection).

We further analyzed the ability of convergence between L_{SIoU++} , L_{SIoU} and L_{IoU} . We combined L_{SIoU++} , L_{SIoU} and L_{IoU} with L_{cls} , L_{radius} and L_{offset} to train our proposed SCPM-Net respectively. The evolution of mean FROC curve on the testing data is present in Fig. 7. It shows that L_{SIoU++} accelerates the convergence of SCPM-Net and leads to better performance than L_{SIoU} and L_{IoU} . Note that there exists a sudden drop of mean FROC at the 20th epoch, which is because we used learning rate warm up strategy (Gotmare et al., 2019) to boost the network’s performance. Fig. 7 also shows that L_{SIoU++} is more stable than L_{IoU} and L_{SIoU} when the learning rate changed.

Finally, we investigated the contribution of each submodule in L_{SIoU++} function and also compared L_{SIoU++} with L_{IoU} with the same experimental setting. A quantitative evaluation of these methods is listed in Table 2. It shows that using L_{IoU} to train a strong network (SCPM-Net) leads to worse results in 1 and 2 FPs/Scan than using L_{SIoU} with R_{RD} . In contrast, L_{SIoU++} has the ability to boost the network’s performance. Meanwhile, and both the distance term R_{RD} and angle of intersection term η improved the performance, since geometric measures can

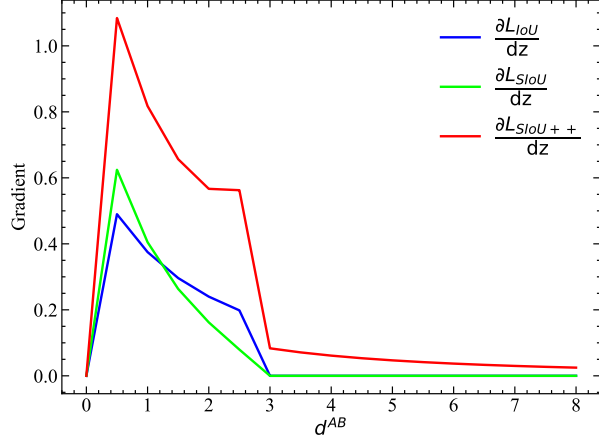


Figure 6: Comparison of the gradients of different loss functions with respect to z when S^a gradually moves to S^b along the z -axis (d^{AB} changes from 8 to 0).

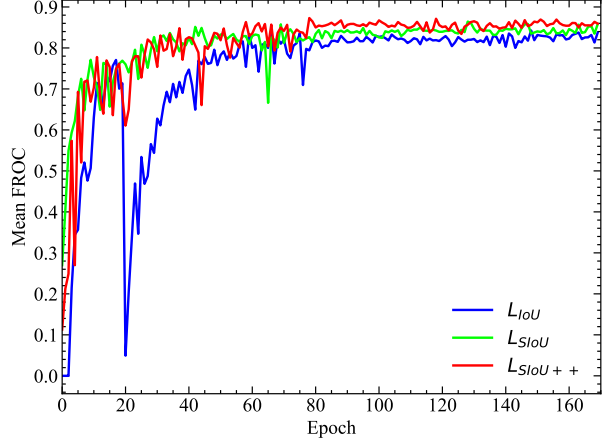


Figure 7: The evolution curve of mean FROC on the testing data. The blue, lime and red curves show the performance of the network trained using the L_{IoU} , L_{SIoU} and L_{SIoU++} respectively.

boost the model to capture more geometric information rather than just focus on reducing regression error.

4.5. Comparison with Existing Methods

4.5.1. Comparison with Different Detectors

We compared our method with some powerful anchor-based detectors including Deeplung (Zhu et al., 2018), 3D RetinaNet (Lin et al., 2017b) and 3D RetinaNet++ (Lin et al., 2017b), and also with several existing anchor-free-based detectors including 3D CenterNet (Duan et al., 2019) and CPM-Net (Song et al., 2020). In this study, we re-implemented the 3D version of CenterNet (Duan et al., 2019) and RetinaNet (Lin et al., 2017b) following the original works’ descriptions. It should be noted that 3D RetinaNet++ is an enhanced version of 3D RetinaNet, adopting the same OHEM and re-focal loss as our SCPM-Net and using an online anchors’ matching strategy instead of offline pre-determining strategy in (Lin et al., 2017b). We drew the FROC curve in Fig. 8 demonstrating the sensitivities at seven predefined FPs/Scan rates: 1/8, 1/4, 1/2, 1, 2, 4 and 8. A quantitative evaluation of these methods at 1, 2 and 8 FPs/Scan are listed in Table 3. Our SCPM-Net achieved sensitivities of 92.3% at 1 FPs/Scan and 92.7% at 2 FPs/Scan. The anchor-free 3D CenterNet obtained the lowest performance, which is due to that it uses a single centroid to represent a nodule, resulting in

location failure and false negatives. In contrary to CenterNet (Duan et al., 2019), our SCPM-Net uses multi-point matching to reduce the false negatives, and thus increases the sensitivity. Compared with CPM-Net (Song et al., 2020), SCPM-Net outperformed CPM-Net in terms of all the three evaluation metrics, since it used L_{SIoU++} for model training which takes many geometric properties into account, i.e., sphere overlap, center point distance and angle of intersection of two spheres. In addition, we also investigated the inference time of each detector with the same experimental settings and hardware. For all one-stage detectors (3D CenterNet, 3D RetinaNet, 3D RetinaNet++, CPM-Net, and SCPM-Net) based on the same backbone, they spend very close inference time (8.37s per scan), but SCPM-Net achieves a better sensitivity than the others. Compared with multi-stage detectors, SCPM-Net requires less inference time and also obtains a better result, such as DeepLung requires more than 11.00s per scan. Fig. 9 shows some visualization results of different detectors. It can be observed that SCPM-Net is able to capture small nodules that would be missed by the other detectors.

4.5.2. Comparison with State-of-the-Art Lung Nodule Detectors

We further compared our method with several published state-of-the-art lung nodule detection methods on

Method	Sensitivity		
	FPs/Scan=1	FPs/Scan=2	FPs/Scan=8
3D CenterNet (Duan et al., 2019)	71.4%	75.8%	77.5%
DeepLung (Zhu et al., 2018)	85.8%	86.9%	87.5%
3D RetinaNet (Lin et al., 2017b)	83.6%	86.8%	88.7%
3D RetinaNet++ (Lin et al., 2017b)	88.8%	91.3%	91.4%
CPM-Net (Song et al., 2020)	91.2%	92.4%	92.5%
Ours	92.3%	92.7%	94.8%

Table 3: Comparison of different detectors on LUNA16 dataset. (FPs/Scan: the false positives per scan)

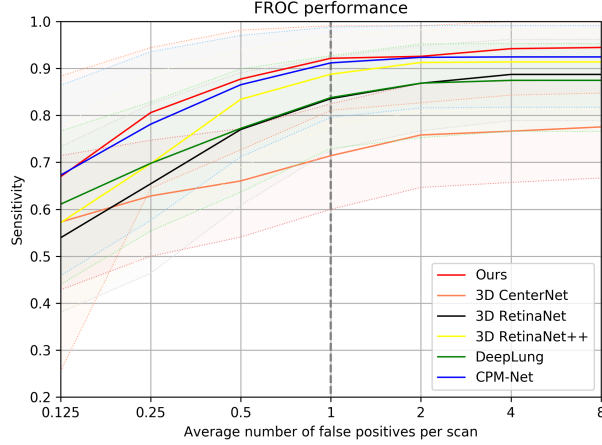


Figure 8: Comparison of FROC curves using different network configurations, with shaded areas presenting the 95% confidence interval.

the LUNA16 dataset (Setio et al., 2017): Dou et al. (2017) employed a two-stage framework which consists of a candidate screening stage and false positive reduction stage. Ding et al. (2017) used a Faster R-CNN for candidate detection and a 3D CNN to reduce false positives. Zhu et al. (2018) used a three-stage framework consisting of candidate generation, feature extraction and classification. Tang et al. (2019) proposed a multi-task framework to solve nodule detection, false-positive reduction, and nodule segmentation jointly. Song et al. (2020) developed an anchor-free detector which obtains the detection results by regressing the bounding box size of the nodule and local offset of the center points. Mei et al. (2021) proposed a slice-aware network to capture long-range dependencies among any positions and any channels of one slice group in the feature map. The quantitative comparison of these methods based on a 10-fold cross validation is presented in Table 4. Compared with

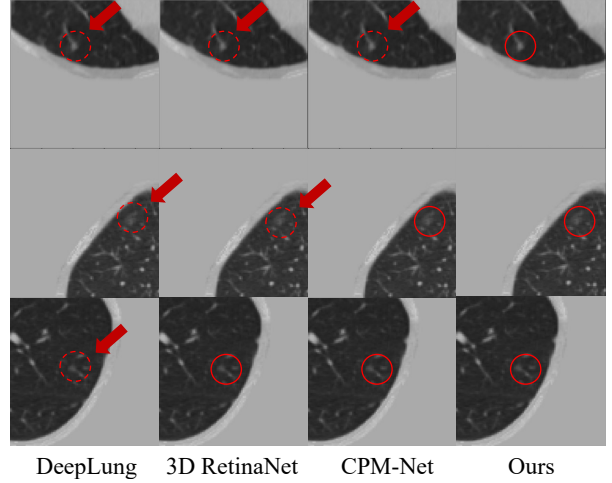


Figure 9: Visualizations of detection results obtained by different methods, where dotted circles represent missed cases and solid circles represent correct detection.

these state-of-the-art detection frameworks, our SCPM-Net achieves better performance and shows an advantage over the others as it's an efficient end-to-end single-stage detection network.

5. Discussion and Conclusion

We have successfully evaluated the proposed SCPM-Net and L_{Stou++} on a large lung nodule detection dataset (Setio et al., 2017). To overcome the drawbacks of anchor-based approaches, we propose an anchor-free framework to detect lung nodules in 3D CT scans. To capture context efficiently, we integrate Squeeze-and-Excitation modules (Hu et al., 2018) and multi-level spatial coordinate maps into an encoder-decoder structure for better performance. Inspired by anchor-matching methods (Zhang et al., 2019; Ren et al., 2015), we propose a

Method	Sensitivity			FPR	Stages
	FPs/Scan=1	FPs/Scan=2	FPs/Scan=8		
Dou et al. (2017)	86.5%	90.6%	94.6%	w	2
Ding et al. (2017)	92.8%	93.1%	94.6%	w	2
Zhu et al. (2018)*	86.5%	89.3%	93.3%	w	3
Tang et al. (2019)*	87.5%	91.1%	93.8%	w	2
Song et al. (2020)	91.1%	92.8%	94.8%	w/o	1
Mei et al. (2021)*	90.1%	93.7%	95.5%	w	2
Ours	92.2%	93.9%	96.4%	w/o	1

Table 4: Comparison between our method and state-of-the-art methods on LUNA16 dataset using a 10-fold cross validation. * denotes results borrowed from SANet (Mei et al., 2021) (FPs/Scan: False positives per scan, FPR: False positive reduction)

center points matching method to train the detector more efficiently. Based on the fact of annotating nodules as spheres in clinical practice (MacMahon et al., 2017), we use bounding spheres to represent nodules rather than bounding boxes, and further combine geometric measures to propose a sphere-based intersection-over-union loss function (L_{SIoU++}) to train the detector. All these sub-modules and loss functions constitute a powerful and efficient detector for lung nodule detection. In this work, we just used the L_{SIoU++} function to train our proposed anchor-free detectors for lung nodules detection, it may also be extended to train anchor-based detectors.

Recently, Yang et al. (2020) proposed an anchor-free detection method with circle representation (i.e., CircleNet), and the main differences between SCPM-Net and CircleNet are: 1) CircleNet uses 2D circles to represent the glomerulus in 2D pathology images, while our method uses spheres to represent lung nodules in 3D space, which is inspired by clinical practice of lung nodule diagnosis and measurement; 2) For detector optimization, our SCPM-Net uses a sphere-based loss function, and CircleNet just uses circle IoU as a metric for loss calculation. 3) To accelerate the convergence, SCPM-Net introduces many geometric metrics to L_{SIoU++} , which was not considered in CircleNet. Note that our framework can be easily extended to other detection tasks, such as lesion detection, as the SCPM-Net is a general anchor-free framework and does not rely on any specific task, and the L_{SIoU++} considers many geometric metrics that may be applied to other structures as well. In the future, we will investigate further improving the efficiency of the anchor-free detector, and validate it with other clinical applications.

In conclusion, we propose a novel 3D sphere representation-based center-points matching detection

network (SCPM-Net) for pulmonary nodule detection from volumetric CT images. Meanwhile, we use an attentive module consisting of coordinate attention and squeeze-and-excitation attention to capturing spatial position. Besides, we adopt a hybrid method of online hard example mining (OHEM) and re-focal loss to solve the imbalance between positive points and negative points. In addition, we introduce a novel sphere representation for lung nodules detection in 3D space and propose a novel loss function L_{SIoU++} that considers geometric measures for training. Experimental results on the LUNA16 nodule detection dataset show that the proposed SCPM-Net achieves a better or comparable performance with a simpler architecture compared with several state-of-the-art single-stage and multi-stage approaches. The high sensitivities in single-stage inference demonstrate promising potential for further clinical use.

6. Acknowledgment

This work was supported by the National Natural Science Foundations of China [81771921, 61901084], and also by key research and development project of Sichuan province, China [20ZDYF2817]. We would like to thank Mr. Yechong Huang from SenseTime Research for constructive discussions, suggestion and manuscript proof-read and also thank the organization teams of LUNA16 challenge for the publicly available datasets.

References

- Ding, J., Li, A., Hu, Z., Wang, L., 2017. Accurate pulmonary nodule detection in computed tomography images using deep convolutional neural networks, in: International Conference on Medical Image Computing and Computer-Assisted Intervention, Springer. pp. 559–567.
- Dou, Q., Chen, H., Jin, Y., Lin, H., Qin, J., Heng, P.A., 2017. Automated pulmonary nodule detection via 3d convnets with online sample filtering and hybrid-loss residual learning, in: International Conference on Medical Image Computing and Computer-Assisted Intervention, Springer. pp. 630–638.

- Duan, K., Bai, S., Xie, L., Qi, H., Huang, Q., Tian, Q., 2019. Centernet: Keypoint triplets for object detection, in: The IEEE International Conference on Computer Vision, pp. 6569–6578.
- Duan, Q., Wang, G., Wang, R., Fu, C., Li, X., Gong, M., Liu, X., Xia, Q., Huang, X., Hu, Z., et al., 2020. SenseCare: A research platform for medical image informatics and interactive 3d visualization. *arXiv preprint arXiv:2004.07031*.
- Everingham, M., Van Gool, L., Williams, C.K., Winn, J., Zisserman, A., 2010. The pascal visual object classes (VOC) challenge. *International journal of computer vision* 88, 303–338.
- Gotmare, A., Keskar, N.S., Xiong, C., Socher, R., 2019. A closer look at deep learning heuristics: Learning rate restarts, warmup and distillation. *International Conference on Learning Representations*.
- Hu, J., Shen, L., Sun, G., 2018. Squeeze-and-excitation networks, in: the IEEE Conference on Computer Vision and Pattern Recognition, pp. 7132–7141.
- Law, H., Deng, J., 2018. Cornernet: Detecting objects as paired keypoints, in: European conference on computer vision, pp. 734–750.
- Li, F., Huang, H., Wu, Y., Cai, C., Huang, Y., Ding, X., 2019. Lung nodule detection with a 3d convnet via iou self-normalization and maxout unit, in: IEEE International Conference on Acoustics, Speech and Signal Processing, pp. 1214–1218.
- Lin, T.Y., Dollár, P., Girshick, R., He, K., Hariharan, B., Belongie, S., 2017a. Feature pyramid networks for object detection, in: the IEEE conference on computer vision and pattern recognition, pp. 2117–2125.
- Lin, T.Y., Goyal, P., Girshick, R., He, K., Dollár, P., 2017b. Focal loss for dense object detection, in: The IEEE International Conference on Computer Vision, pp. 2980–2988.
- Lin, T.Y., Maire, M., Belongie, S., Hays, J., Perona, P., Ramanan, D., Dollár, P., Zitnick, C.L., 2014. Microsoft COCO: Common objects in context, in: European conference on computer vision, Springer. pp. 740–755.
- Liu, W., Anguelov, D., Erhan, D., Szegedy, C., Berg, A.C., 2016. SSD: Single shot multibox detector, in: European conference on computer vision.
- MacMahon, H., Naidich, D.P., Goo, J.M., Lee, K.S., Leung, A.N., Mayo, J.R., Mehta, A.C., Ohno, Y., Powell, C.A., Prokop, M., et al., 2017. Guidelines for management of incidental pulmonary nodules detected on CT images: from the fleischner society 2017. *Radiology* 284, 228–243.
- Mei, J., Cheng, M.M., Xu, G., Wan, L.R., Zhang, H., 2021. SANet: A slice-aware network for pulmonary nodule detection. *IEEE transactions on pattern analysis and machine intelligence*.
- Paszke, A., Gross, S., Massa, F., Lerer, A., Bradbury, J., Chanan, G., Killeen, T., Lin, Z., Gimelshein, N., Antiga, L., et al., 2019. Pytorch: An imperative style, high-performance deep learning library, in: Advances in neural information processing systems, pp. 8026–8037.
- Redmon, J., Farhadi, A., 2017. YOLO9000: better, faster, stronger, in: the IEEE conference on computer vision and pattern recognition, pp. 7263–7271.
- Ren, S., He, K., Girshick, R., Sun, J., 2015. Faster R-CNN: Towards real-time object detection with region proposal networks, in: Advances in neural information processing systems, pp. 91–99.
- Rezatofighi, H., Tsoi, N., Gwak, J., Sadeghian, A., Reid, I., Savarese, S., 2019. Generalized intersection over union: A metric and a loss for bounding box regression, in: the IEEE Conference on Computer Vision and Pattern Recognition, pp. 658–666.
- Setio, A.A.A., Traverso, A., De Bel, T., Berens, M.S., van den Bogaard, C., Cerello, P., Chen, H., Dou, Q., Fantacci, M.E., Geurts, B., et al., 2017. Validation, comparison, and combination of algorithms for automatic detection of pulmonary nodules in computed tomography images: the LUNA16 challenge. *Medical image analysis* 42, 1–13.
- Shrivastava, A., Gupta, A., Girshick, R., 2016. Training region-based object detectors with online hard example mining, in: Proceedings of the IEEE conference on computer vision and pattern recognition, pp. 761–769.

- Siegel, R.L., Miller, K.D., Jemal, A., 2015. Cancer statistics, 2015. *CA: a cancer journal for clinicians* 65, 5.
- Sladoje, N., Nyström, I., Saha, P.K., 2005. Measurements of digitized objects with fuzzy borders in 2d and 3d. *Image and Vision Computing* 23, 123–132.
- Song, T., Cheng, J., Luo, X., Huang, Y., Chen, Y., Liu, X., Huang, N., Ye, Z., Sheng, H., Zhang, S., Wang, G., 2020. CPM-Net: A 3d center-points matching network for pulmonary nodule detection in CT, in: *International Conference on Medical Image Computing and Computer-Assisted Intervention*.
- Tang, H., Zhang, C., Xie, X., 2019. Nodulenet: Decoupled false positive reduction for pulmonary nodule detection and segmentation, in: *International Conference on Medical Image Computing and Computer-Assisted Intervention*, Springer. pp. 266–274.
- Tian, Z., Shen, C., Chen, H., He, T., 2019. FCOS: Fully convolutional one-stage object detection, in: *the IEEE international conference on computer vision*, pp. 9627–9636.
- Wang, D., Zhang, Y., Zhang, K., Wang, L., 2020. FocalMix: Semi-supervised learning for 3D medical image detection, in: *the IEEE Conference on Computer Vision and Pattern Recognition*, pp. 3951–3960.
- Yang, H., Deng, R., Lu, Y., Zhu, Z., Chen, Y., Roland, J.T., Lu, L., Landman, B.A., Fogo, A.B., Huo, Y., 2020. Circlenet: Anchor-free detection with circle representation. *arXiv preprint arXiv:2006.02474*.
- Zhang, X., Wan, F., Liu, C., Ji, R., Ye, Q., 2019. FreeAnchor: Learning to match anchors for visual object detection, in: *Advances in Neural Information Processing Systems*, pp. 147–155.
- Zhao, Z.Q., Zheng, P., Xu, S.t., Wu, X., 2019. Object detection with deep learning: A review. *IEEE transactions on neural networks and learning systems* 30, 3212–3232.
- Zheng, S., Guo, J., Cui, X., Veldhuis, R.N., Oudkerk, M., Van Ooijen, P.M., 2019. Automatic pulmonary nodule detection in CT scans using convolutional neural networks based on maximum intensity projection. *IEEE transactions on medical imaging* 39, 797–805.
- Zheng, Z., Wang, P., Liu, W., Li, J., Ye, R., Ren, D., 2020. Distance-IoU Loss: Faster and better learning for bounding box regression., in: *AAAI*, pp. 12993–13000.
- Zhou, D., Fang, J., Song, X., Guan, C., Yin, J., Dai, Y., Yang, R., 2019a. IoU loss for 2D/3D object detection, in: *2019 International Conference on 3D Vision*, IEEE. pp. 85–94.
- Zhou, X., Wang, D., Krähenbühl, P., 2019b. Objects as points. *arXiv preprint arXiv:1904.07850*.
- Zhou, X., Zhuo, J., Krahenbuhl, P., 2019c. Bottom-up object detection by grouping extreme and center points, in: *the IEEE Conference on Computer Vision and Pattern Recognition*, pp. 850–859.
- Zhu, W., Liu, C., Fan, W., Xie, X., 2018. Deeplung: Deep 3D dual path nets for automated pulmonary nodule detection and classification, in: *The IEEE Winter Conference on Applications of Computer Vision*, pp. 673–681.
- Zlocha, M., Dou, Q., Glocker, B., 2019. Improving retinanet for CT lesion detection with dense masks from weak recist labels, in: *International Conference on Medical Image Computing and Computer-Assisted Intervention*, Springer. pp. 402–410.