


General Information

Instrument	R&S©RTO2044 S/N 300235
Firmware version	5.10.1.0
Selfalignment	Passed 2022-03-24 23:48:56
User	
Comment	

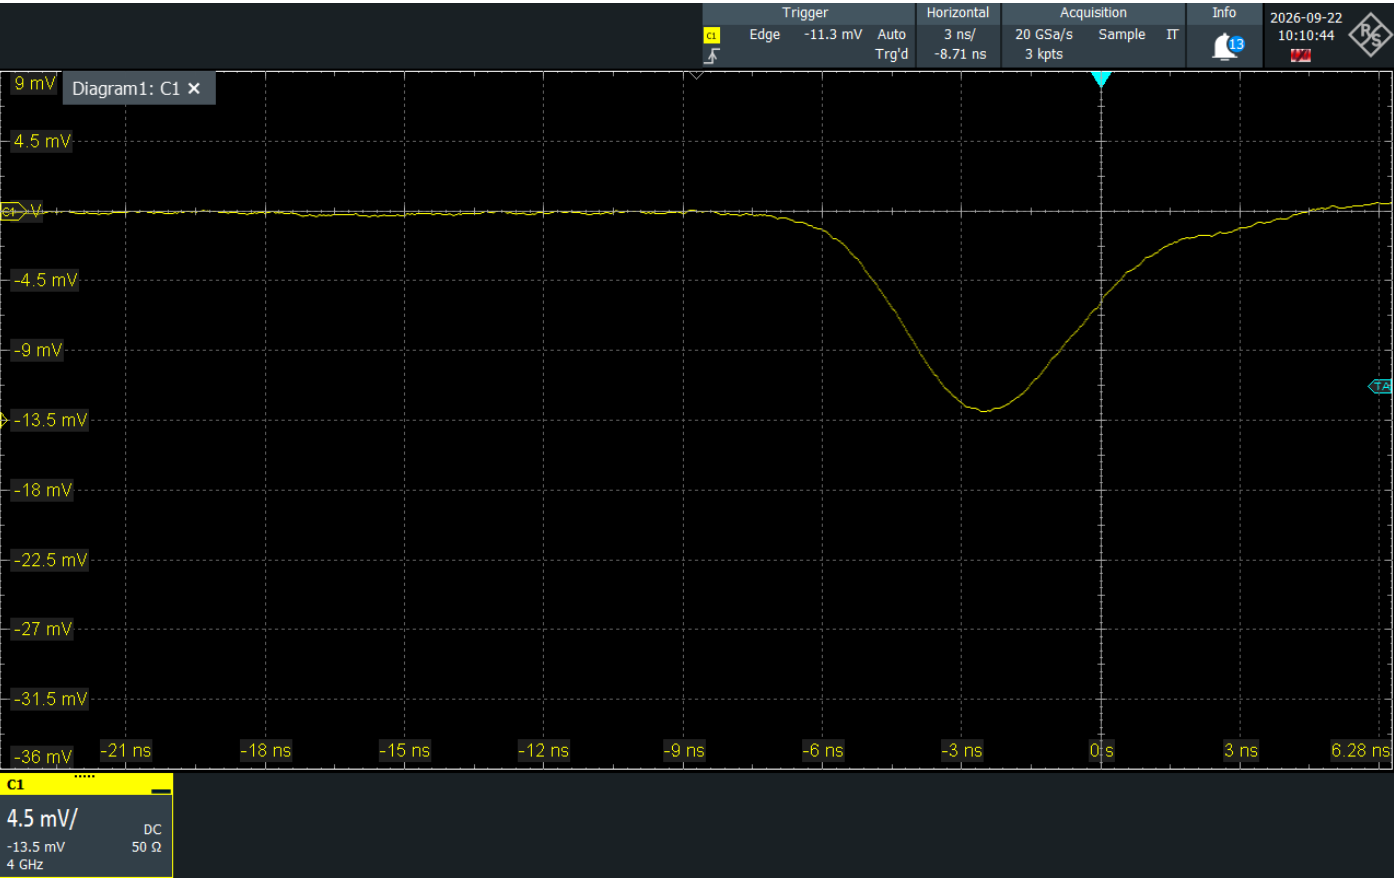

Acquisition

Time scale	3 ns/div	Record length	3 kpts
Resolution	10 ps	Acquisition Mode	Normal
Sample rate	100 GSa/s	Resolution enhancement	Interpolated time
Acquisition time	30 ns	Horizontal position	-8.71 ns

Channels

	Ch1	Ch2	Ch3	Ch4
Color				
Vertical scale	4.5 mV/div			
Position	0 div			
Offset	-13.5 mV			
Skew offset	0 s			
Coupling	50 O (DC)			
Bandwidth	4 GHz			
Probe Name	None			
Probe Serial No				
Probe attenuation	1:1			

Trigger

Type	Edge	Trigger level	-11.3 mV
Slope	Positive	Trigger mode	Auto
Source	Channel 1		