


TITLE: spectrometer


Document Number:

REV:

Date: 11.11.20 11:05

Sheet: 1/1

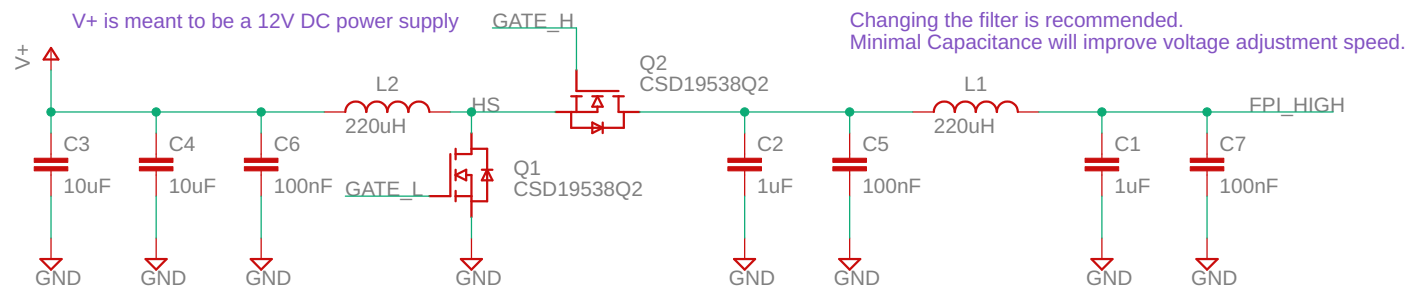

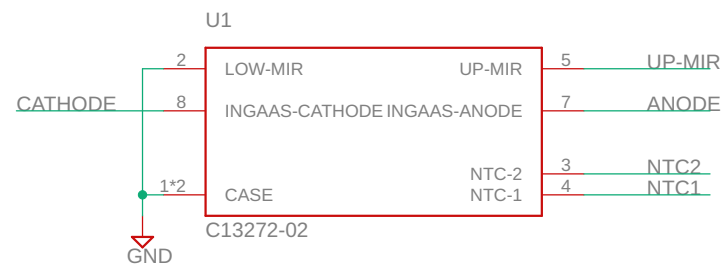

TITLE: spectrometer


Document Number:

REV:


Date: 11.11.20 11:05

Sheet: 1/1

+12V Vin with eFuse (OVP, Reverse Polarity Protection)

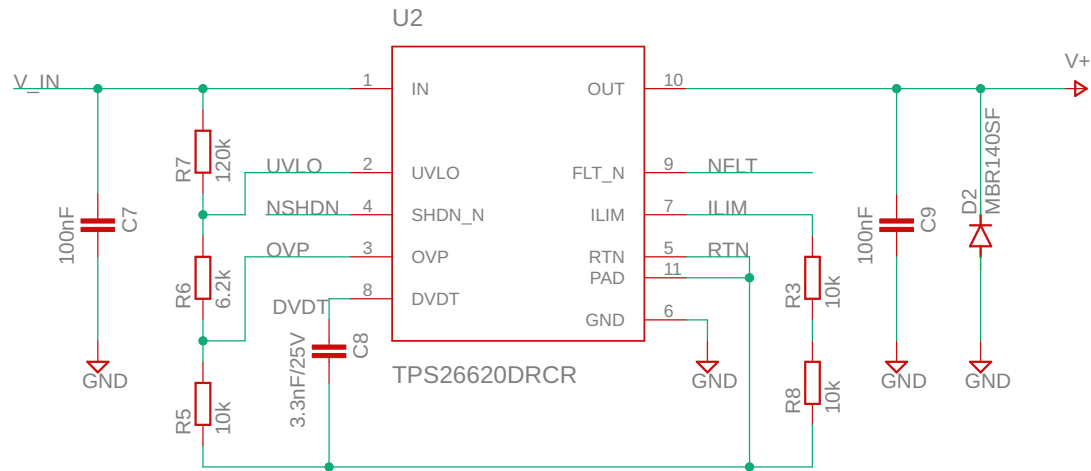

+3V3 has to be set to be +3V5 due to reference voltage regulation.
-> 330k/100k -> +3V44

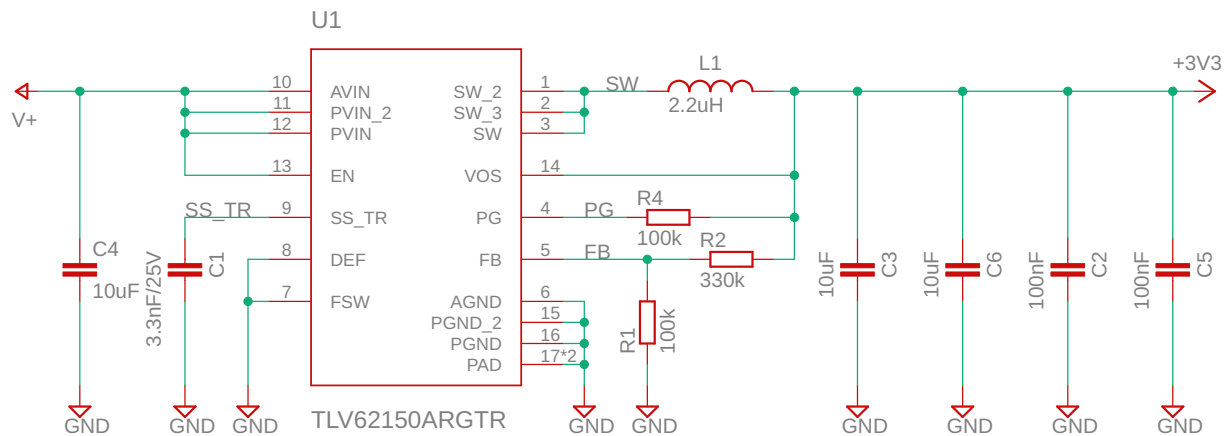



TITLE: spectrometer

Document Number:


REV:

Date: 11.11.20 11:05



Sheet: 1/1

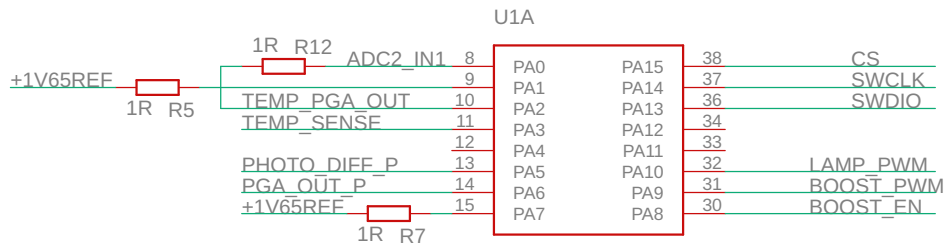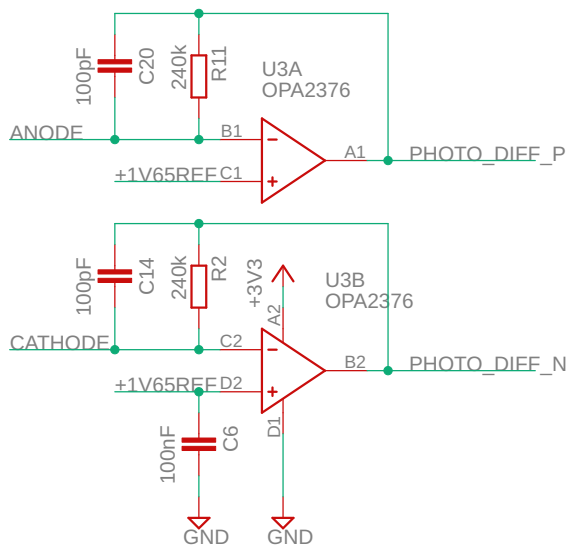






STM32G441xB

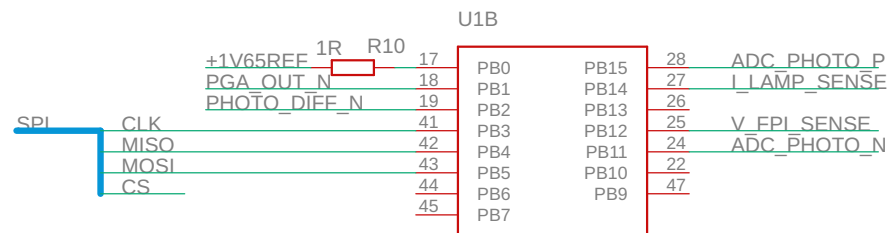

STM32G441xB

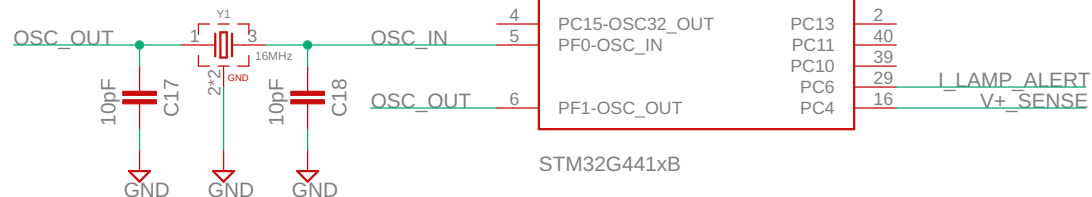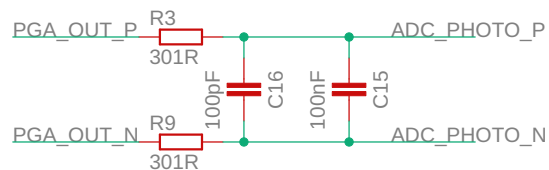

STM32G441xB

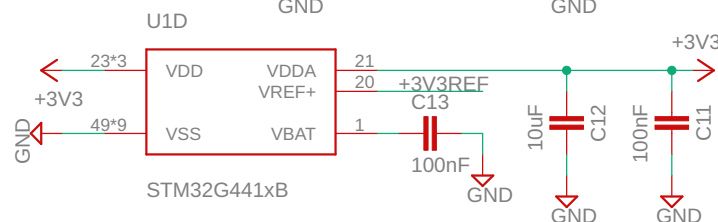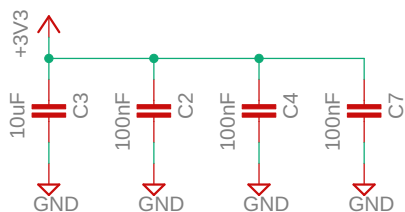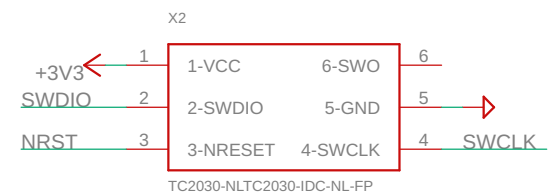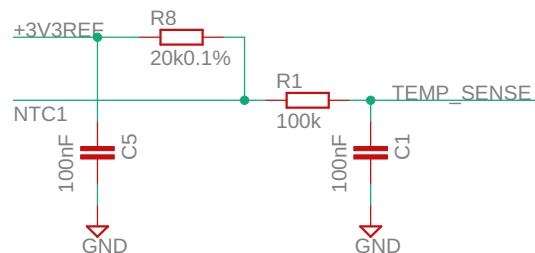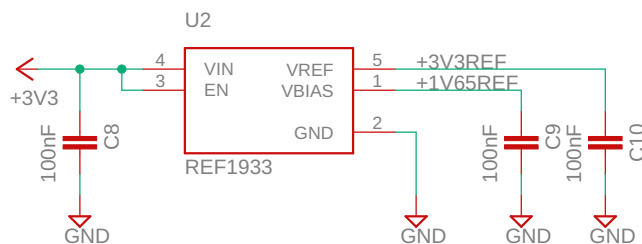

STM32G441xB

TITLE: spectrometer

Document Number:

REV:

Date: 11.11.20 11:05

Sheet: 1/1

