Smart Audio Diagnostics - Analysis Report

24 Oct 2026, 21:32


Group 09 · Digital Signal Processing · ECE, MNNIT Allahabad


File	heart_abnormal_03.wav
Signal type	Medical - heart sound
Auto-detected as	heart (100 % confidence)
Classifier	Random Forest (held-out accuracy 85.7 %)
Trained on	real:C:\dsp\data\physionet2016


RESULT

ABNORMAL

Heart rate
54 bpm

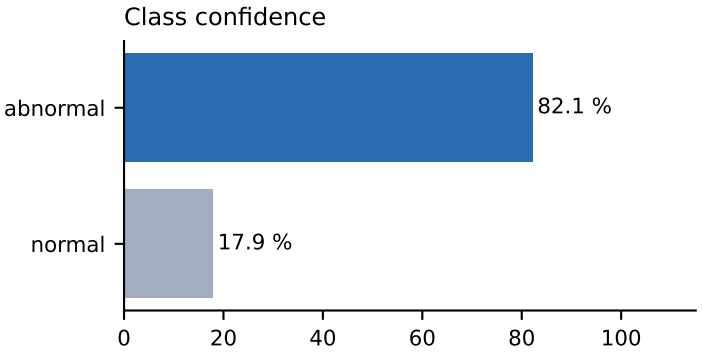

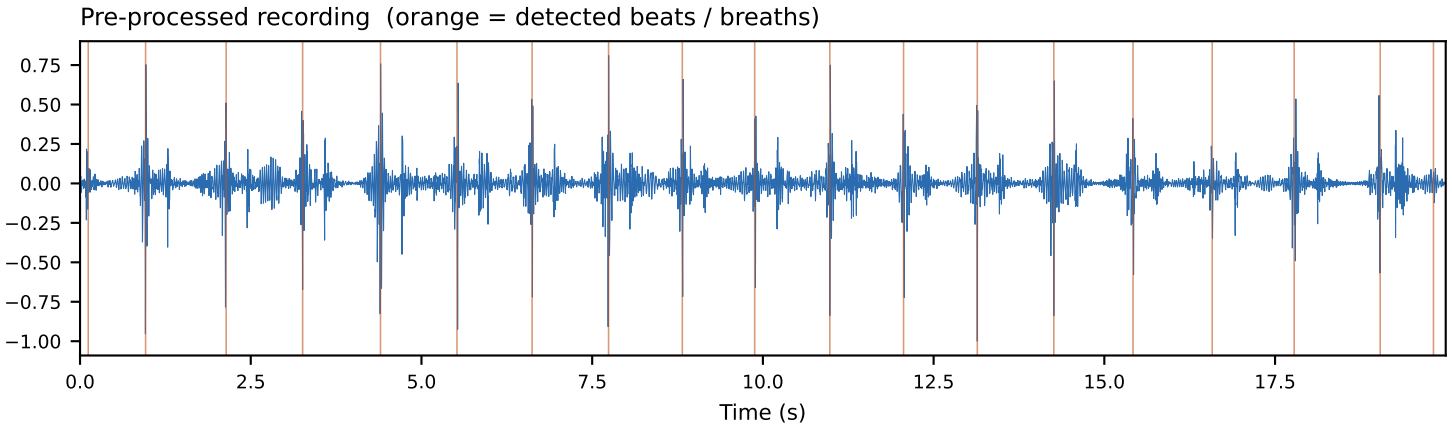

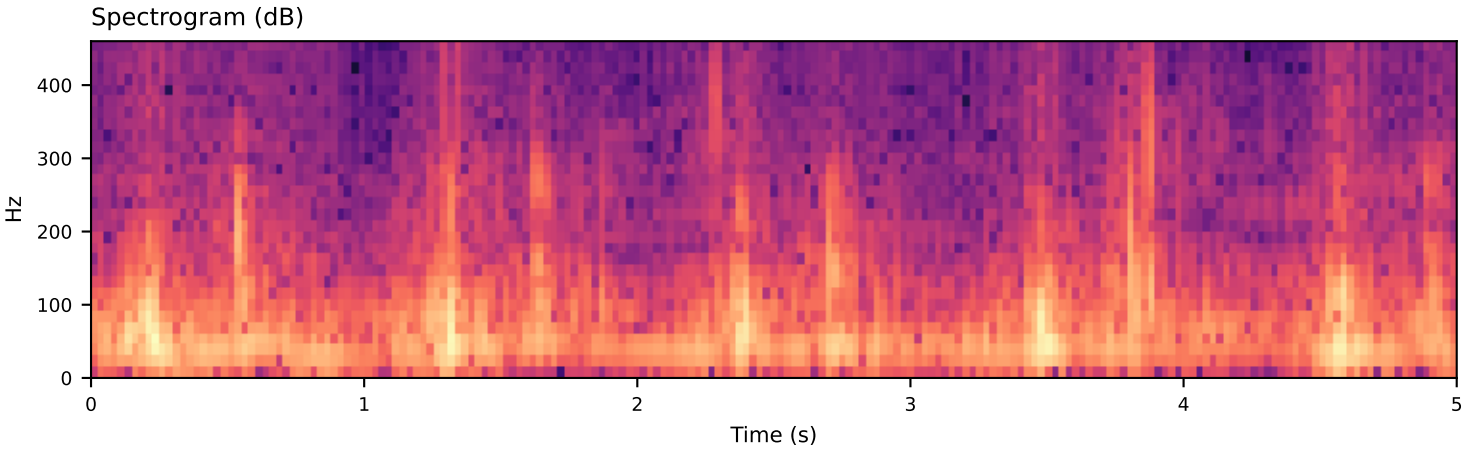

DSP feature	Value	DSP feature	Value
Sampling frequency	2000 Hz	Spectral roll-off 85%	66.8 Hz
Band-pass	25-400 Hz	Spectral flatness	0.0014
Frame / hop	50 / 25 ms	Zero-crossing rate	0.0464
Mel filters	26	Short-time energy	0.00876
Spectral centroid	46.4 Hz	RMS	0.0637
Spectral bandwidth	26.0 Hz	MFCC-1 (mean)	-76.913

Screening / signal-classification output only. This is NOT a clinical diagnosis. Refer to a qualified clinician.