
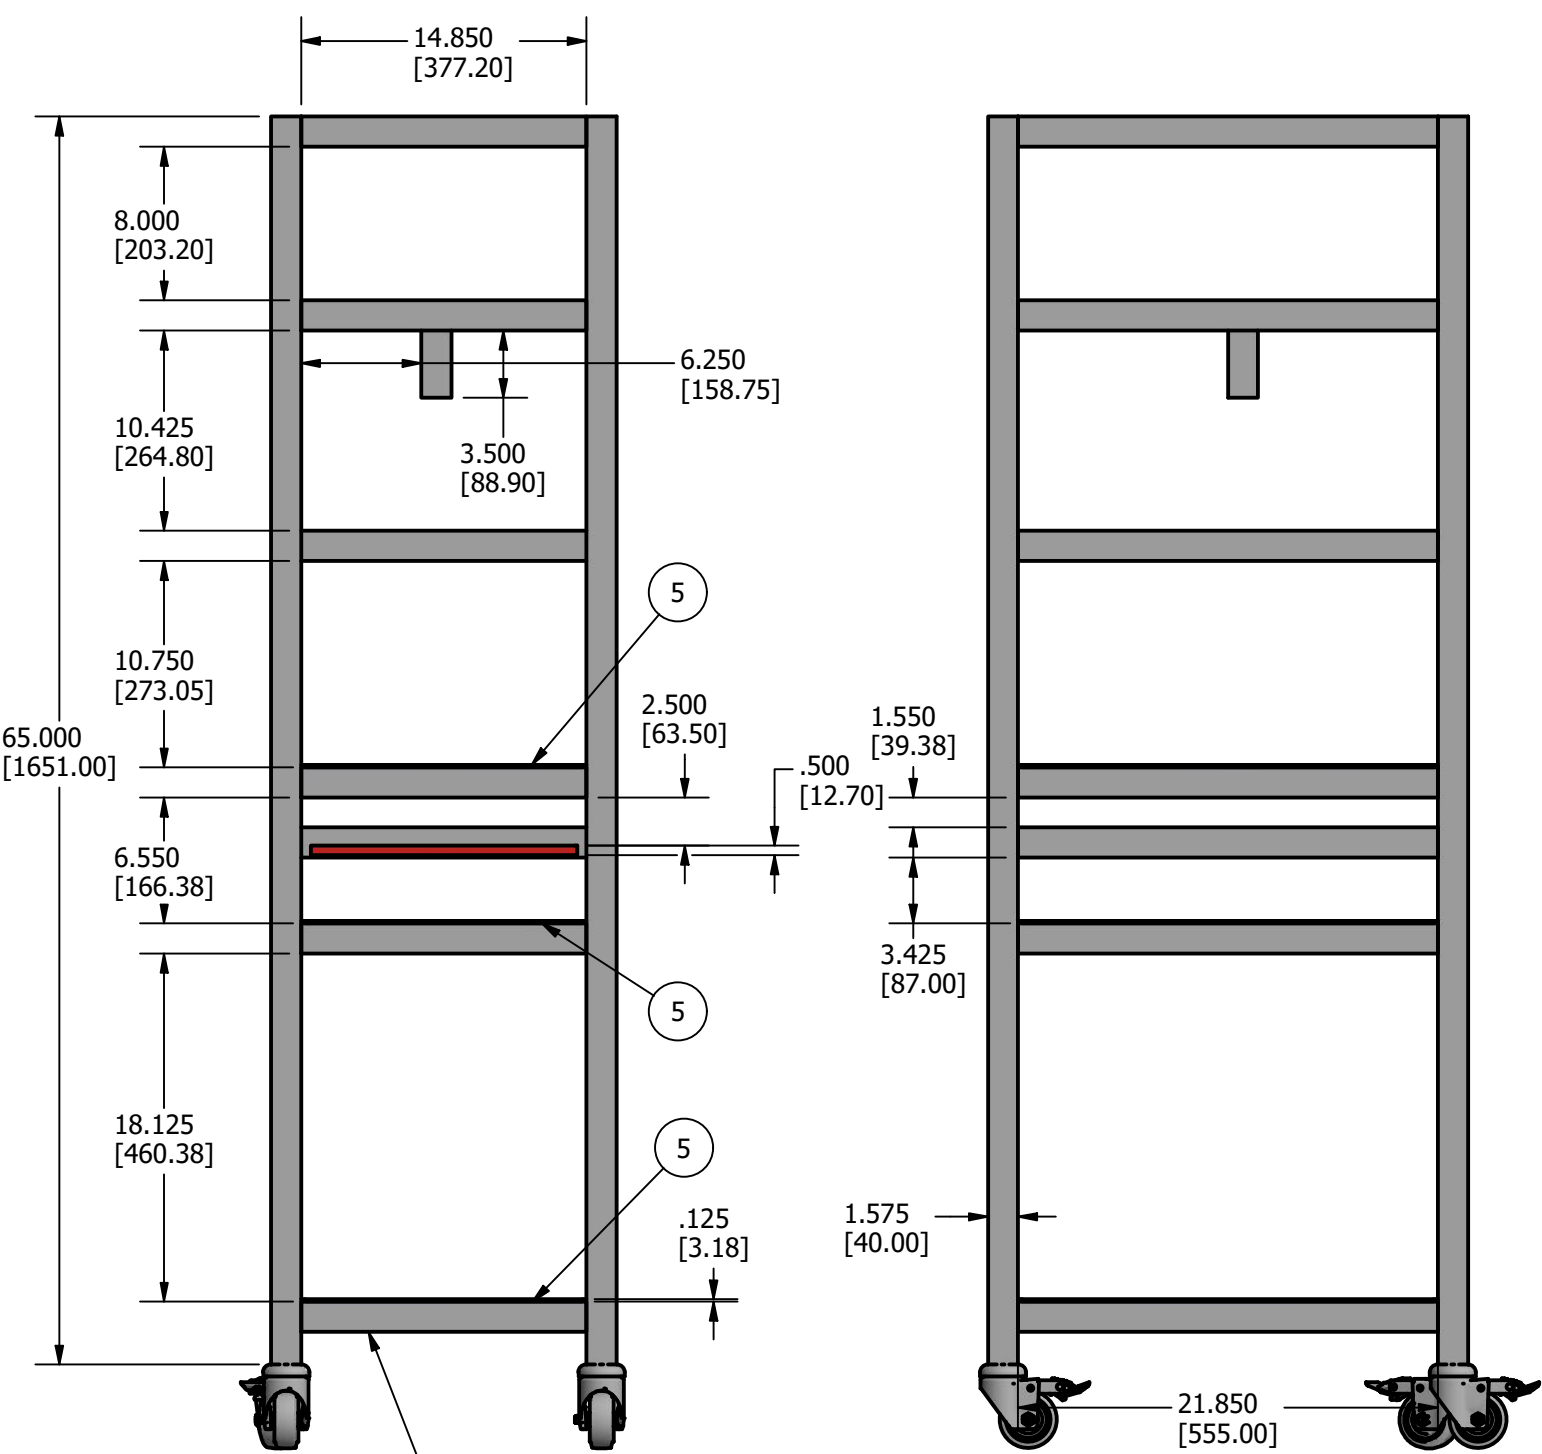
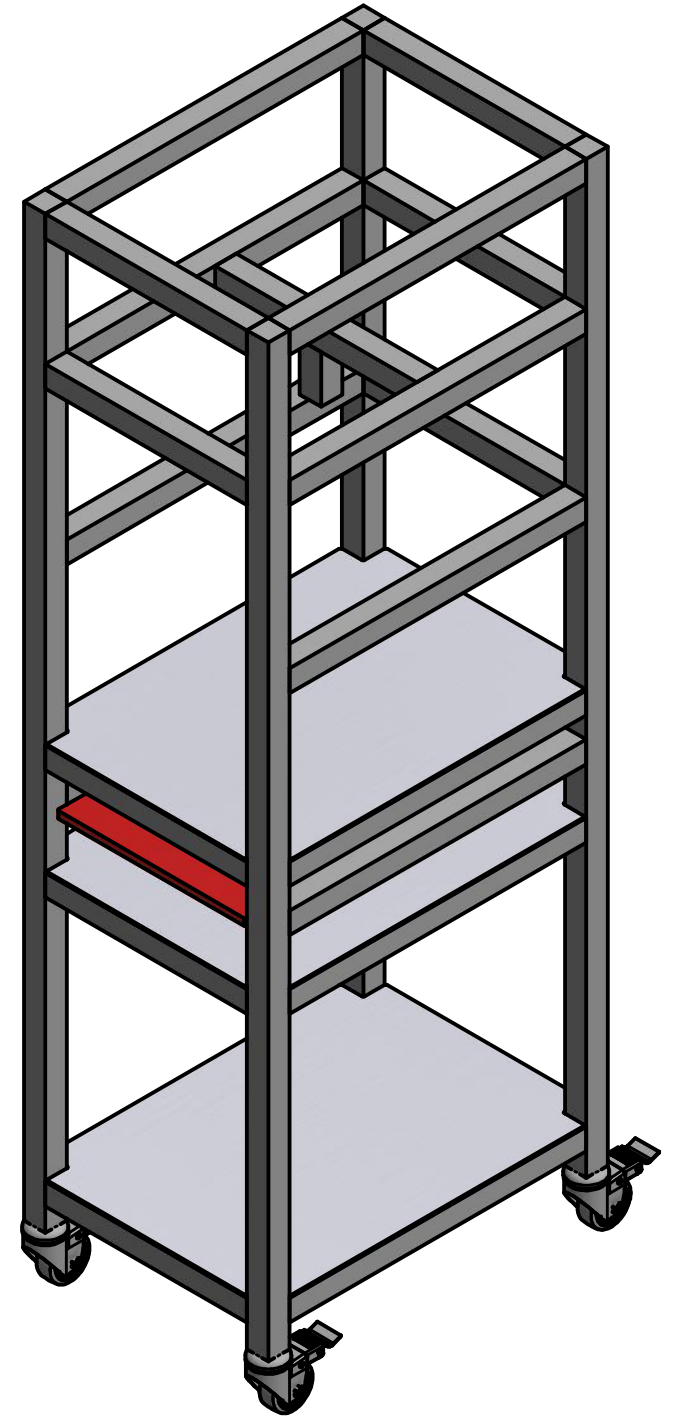


REVISION HISTORY				
ZONE	REV	DESCRIPTION	DATE	APPROVED
	1	QUICK CHANGE	2/1/2022	HHMI\solomone

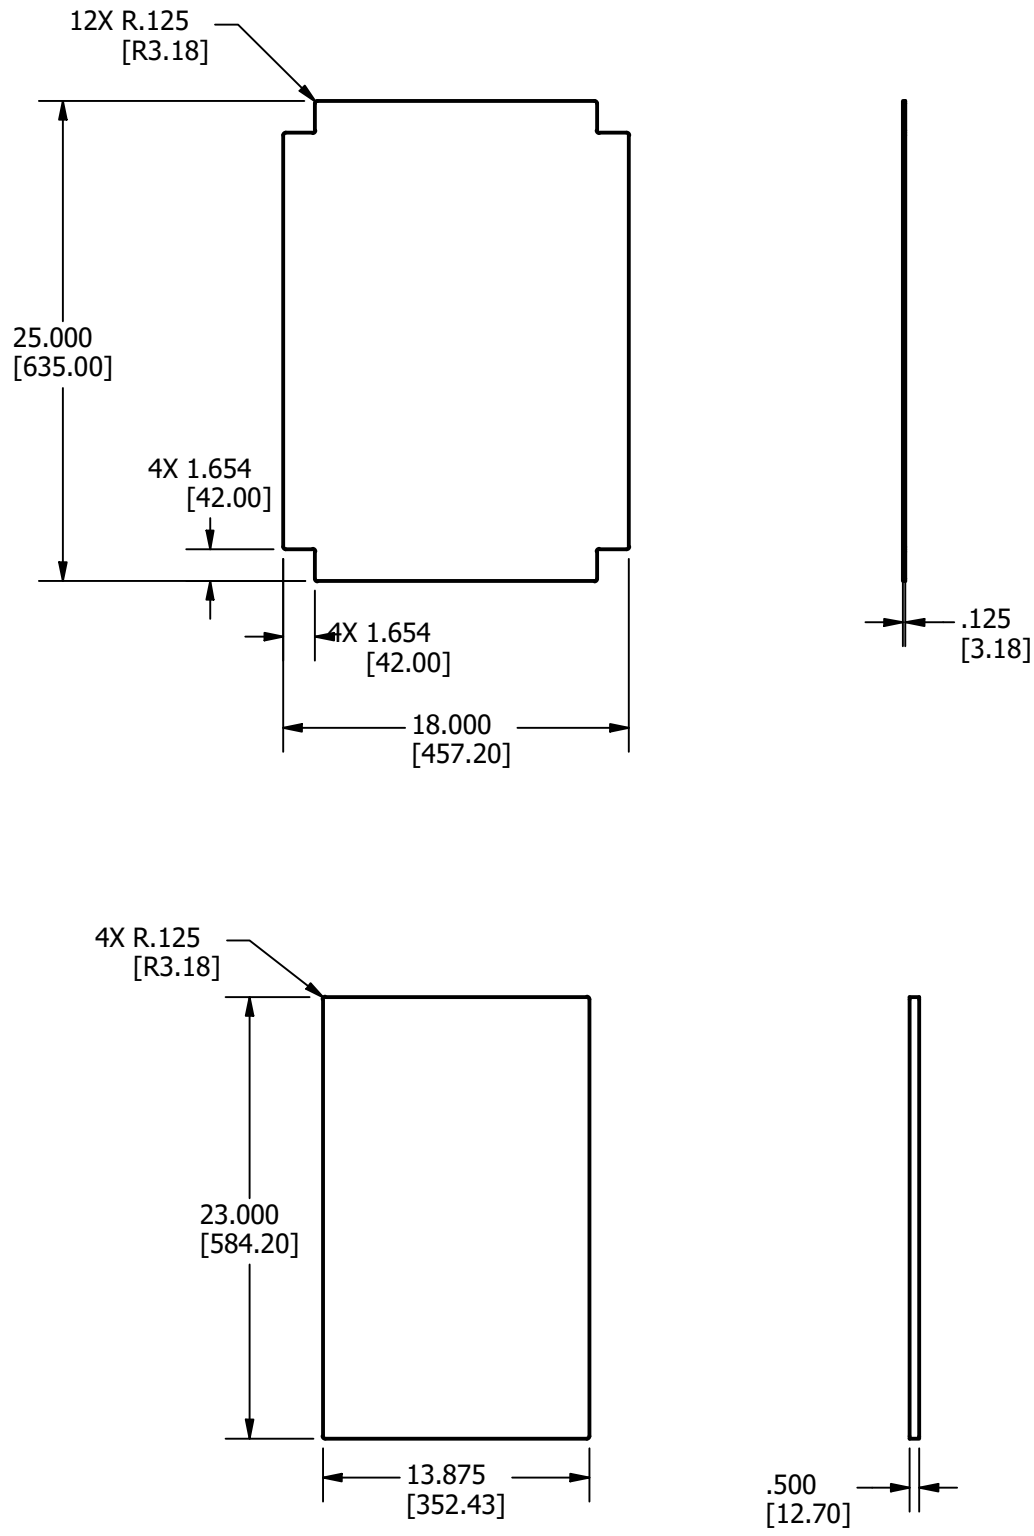

ALL DIMENSIONS BETWEEN FRAME MEMBERS, NOT SHELVES

1	4	65IN RAIL EXTRUSION.ipt	0
2	13	FRONT CROSS BAR.ipt	0
3	14	SIDE CROSS BAR.ipt	0
4	1	CAMERA MOUNT POST.ipt	0
5	3	.125IN SHELF.ipt	0
6	1	DRAWER SHELF.ipt	0
9	4	2384T28_Threaded-Stem Caster with Total Lock.ipt	0
ITEM	QTY	FILE NAME	REV
PARTS LIST			


NOTICE:
INFORMATION CONTAINED IN THIS DOCUMENT OR ANY REPRODUCTION THEREOF, IS PROPRIETARY INFORMATION AND PROPERTY OF HOWARD HUGHES MEDICAL INSTITUTE. IT SHALL NOT BE DISCLOSED, COPIED, DUPLICATED OR USED FOR MANUFACTURE, PRODUCTION OR PROCUREMENT, WITHOUT THE EXPRESS WRITTEN PERMISSION OF HOWARD HUGHES MEDICAL INSTITUTE.


(UNLESS SPECIFIED OTHERWISE)
PRIMARY UNITS: INCHES
[SECONDARY UNITS]: MILLIMETERS

PRIMARY TOLERANCES:
X.X ± 0.020
X.XX ± 0.010
X.XXX ± 0.005
X.XXXX ± 0.0005
ANGULAR ± 0.5 DEG

- DO NOT SCALE DRAWING -

THIRD ANGLE PROJECTION:

 Howard Hughes Medical Institute

 **janelia**
Research Campus

FLY BUBBLE RIG FRAME ASSY.iam

SIZE C	PART NUMBER 1	REV 0	SHEET 1 OF 1
-----------	------------------	----------	-----------------