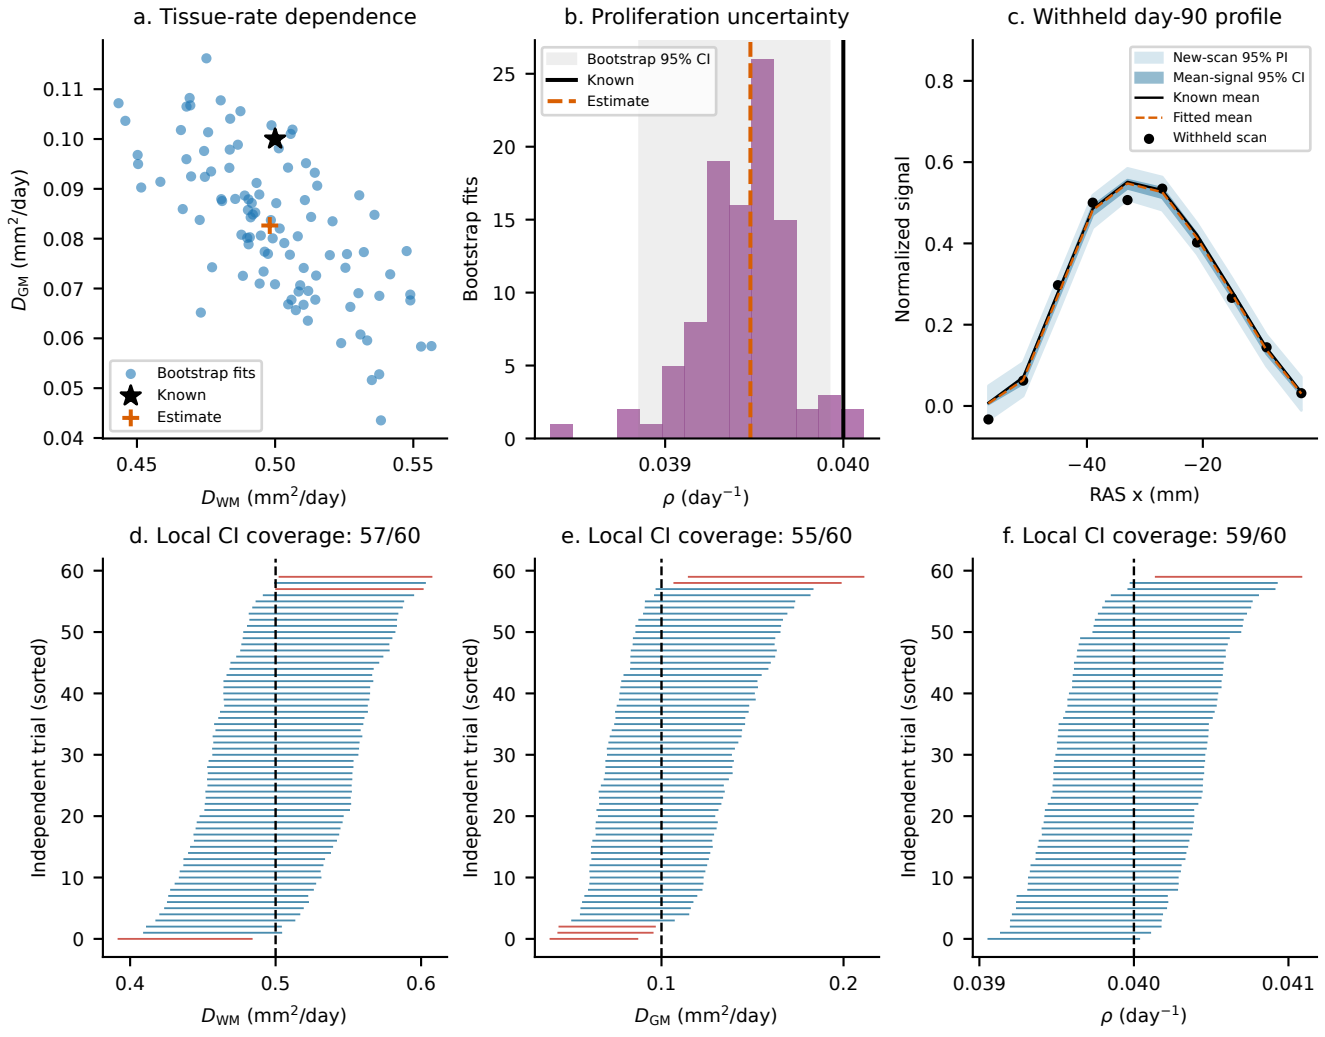
a. Tissue-rate dependence
D_{GM} (mm^2/day)
D_{WM} (mm^2/day)
Bootstrap fits
Known
Estimate
b. Proliferation uncertainty
Bootstrap fits
ρ (day^{-1})
Bootstrap 95% CI
Known
Estimate
c. Withheld day-90 profile
Normalized signal
RAS x (mm)
New-scan 95% PI
Mean-signal 95% CI
Known mean
Fitted mean
Withheld scan
d. Local CI coverage: 57/60
e. Local CI coverage: 55/60
f. Local CI coverage: 59/60
Independent trial (sorted)
D_{WM} (mm^2/day)
D_{GM} (mm^2/day)
ρ (day^{-1})