


(a) Reliability diagram -- raw probabilities
ConvNeXt-Tiny, ThyroidXL test, n=739, 10 bins



(b) Expected calibration error, ConvNeXt-Tiny
ThyroidXL test

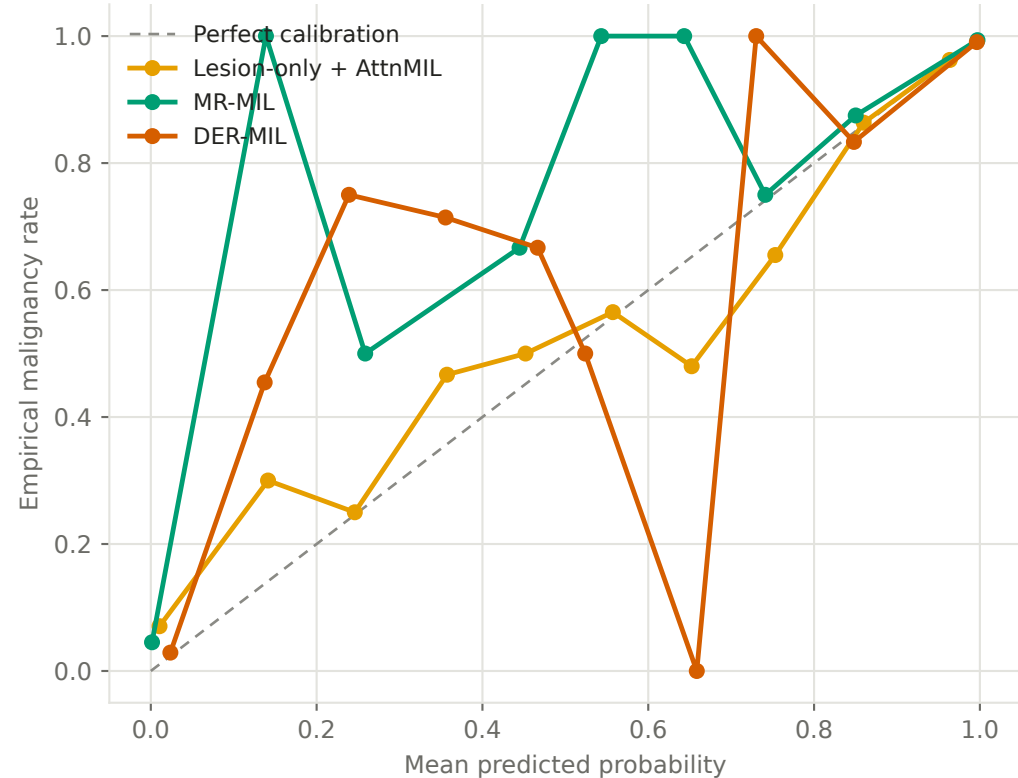