



(a) Outcome counts, threshold 0.5
ConvNeXt-Tiny, ThyroidXL test, n=739

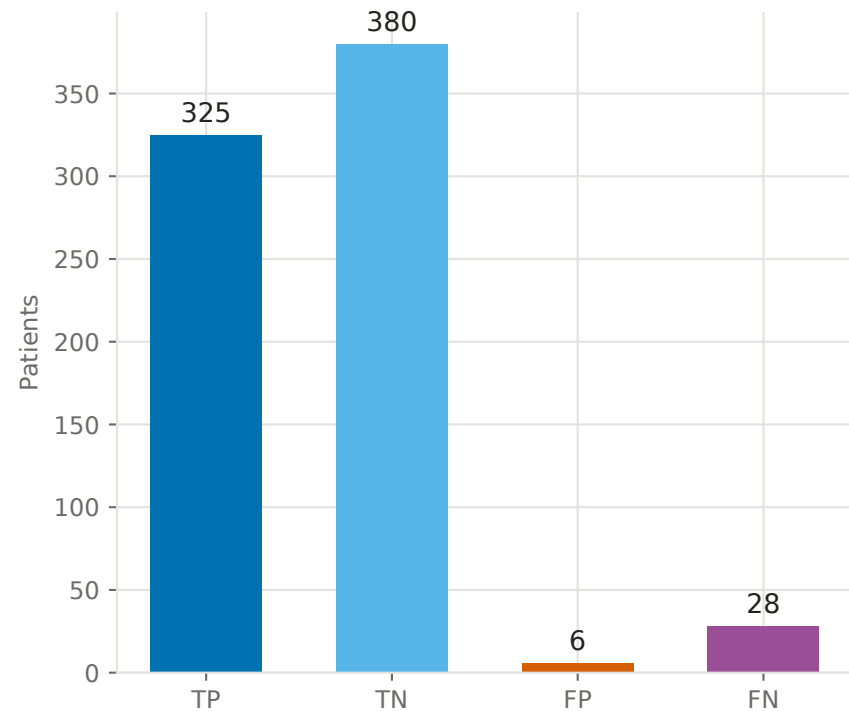

(b) False-negative rate by TI-RADS
(among malignant test patients)

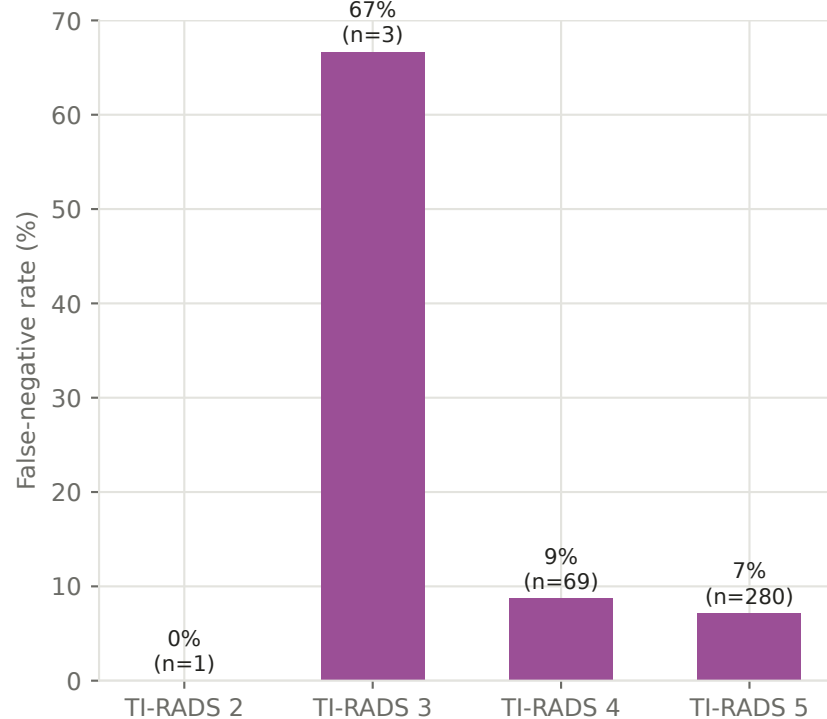

(c) Outcome vs frames available per patient
(jittered for visibility)

