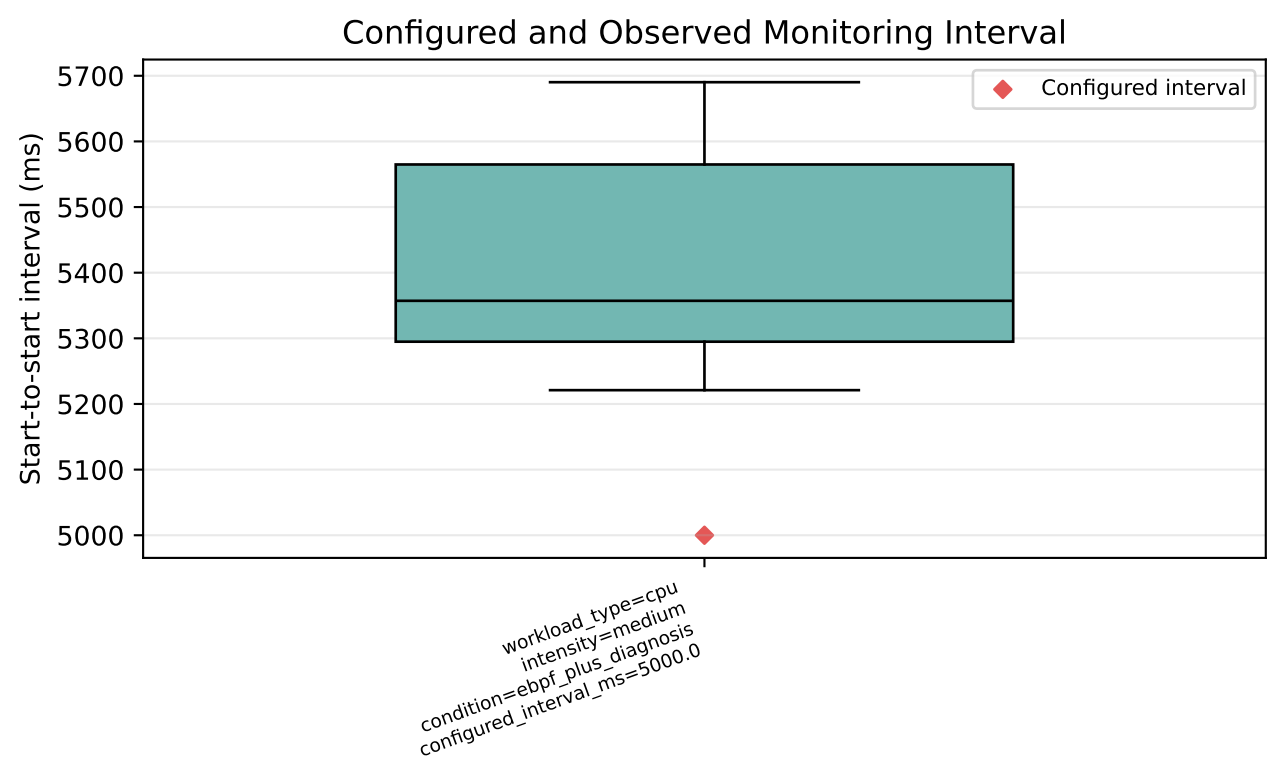
Configured and Observed Monitoring Interval
Start-to-start interval (ms)
5700
5600
5500
5400
5300
5200
5100
5000
Configured interval
workload_type=cpu
intensity=medium
condition=ebpf_plus_diagnosis
configured_interval_ms=5000.0