



Set up the System

To prepare the system, the Support Staff completes the non-sterile preparation:

- Lower the cart completely before moving.

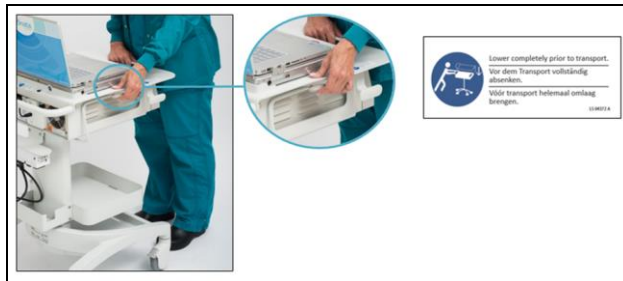

- Connect the power supply.
- Adjust the cart height for viewing by the Physician.
- Once positioned, lock at least two (2) wheels.

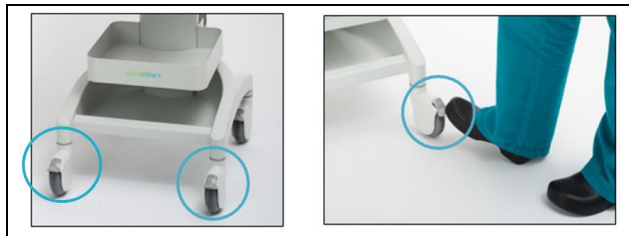

i For more information, refer to the ***Sonata Operator's Manual*** or the Non-Sterile Prep section in the ***Quick Reference Guide***.