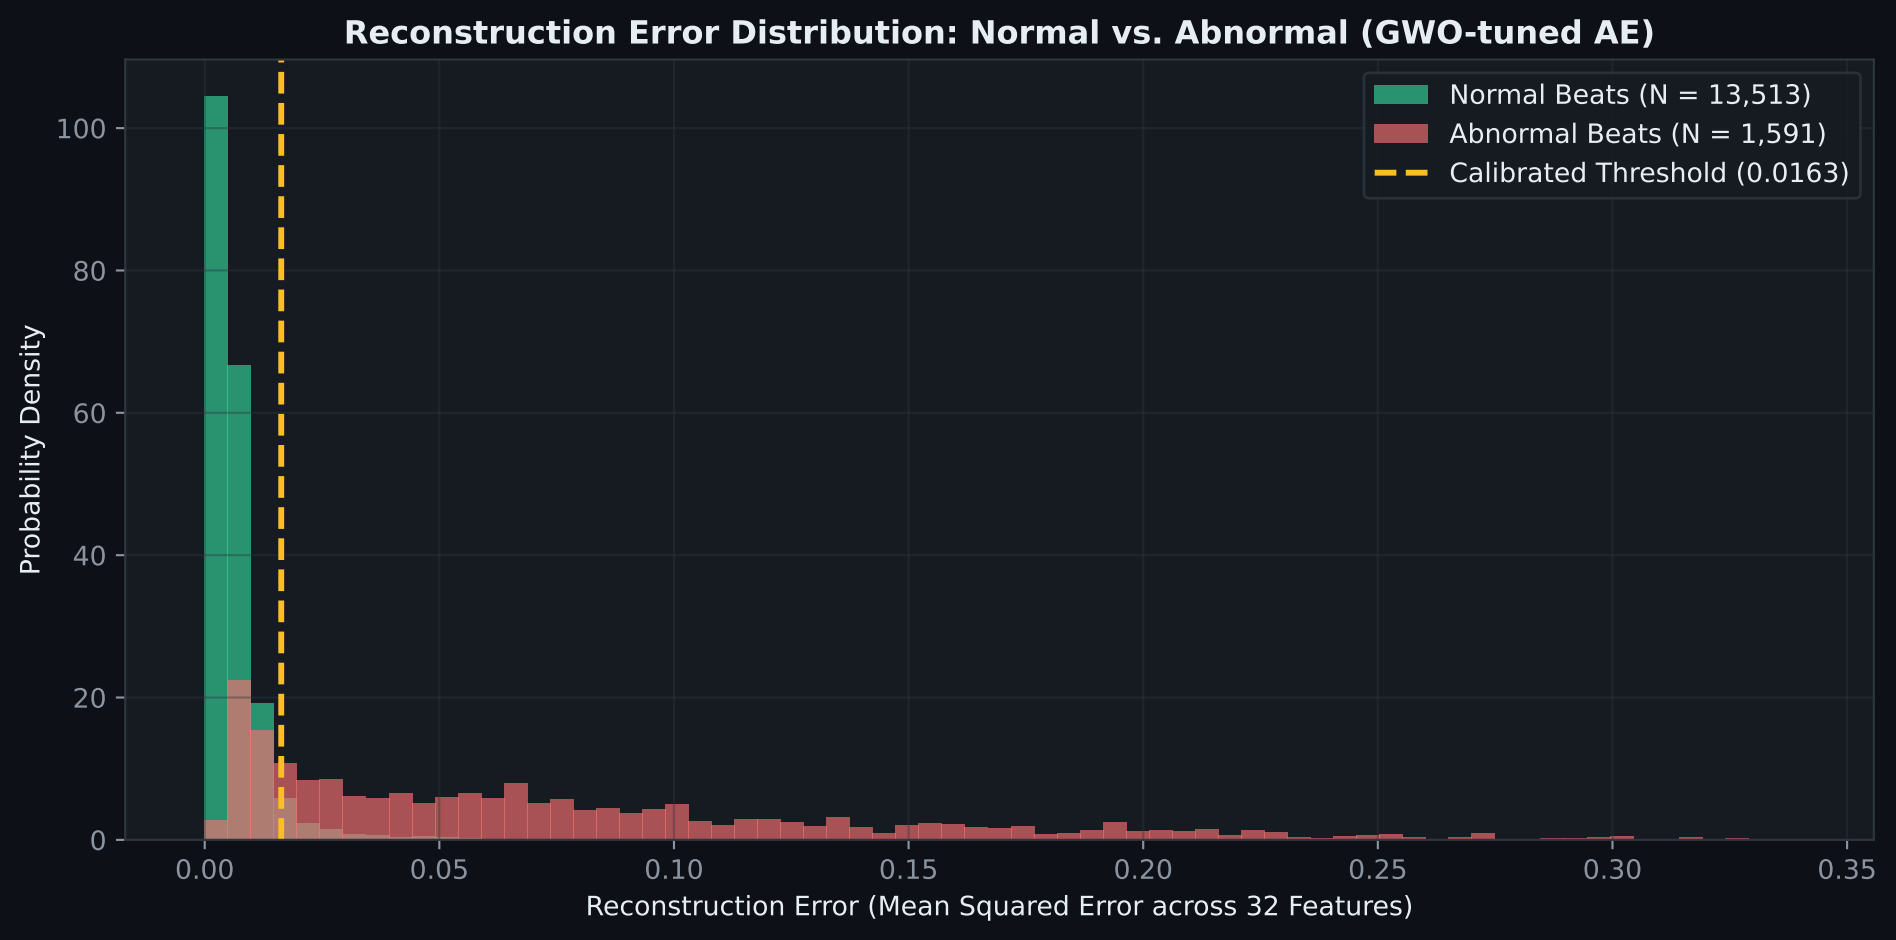
Reconstruction Error Distribution: Normal vs. Abnormal (GWO-tuned AE)
Normal Beats (N = 13,513)
Abnormal Beats (N = 1,591)
Calibrated Threshold (0.0163)
Probability Density
0
20
40
60
80
100
0.00
0.05
0.10
0.15
0.20
0.25
0.30
0.35
Reconstruction Error (Mean Squared Error across 32 Features)