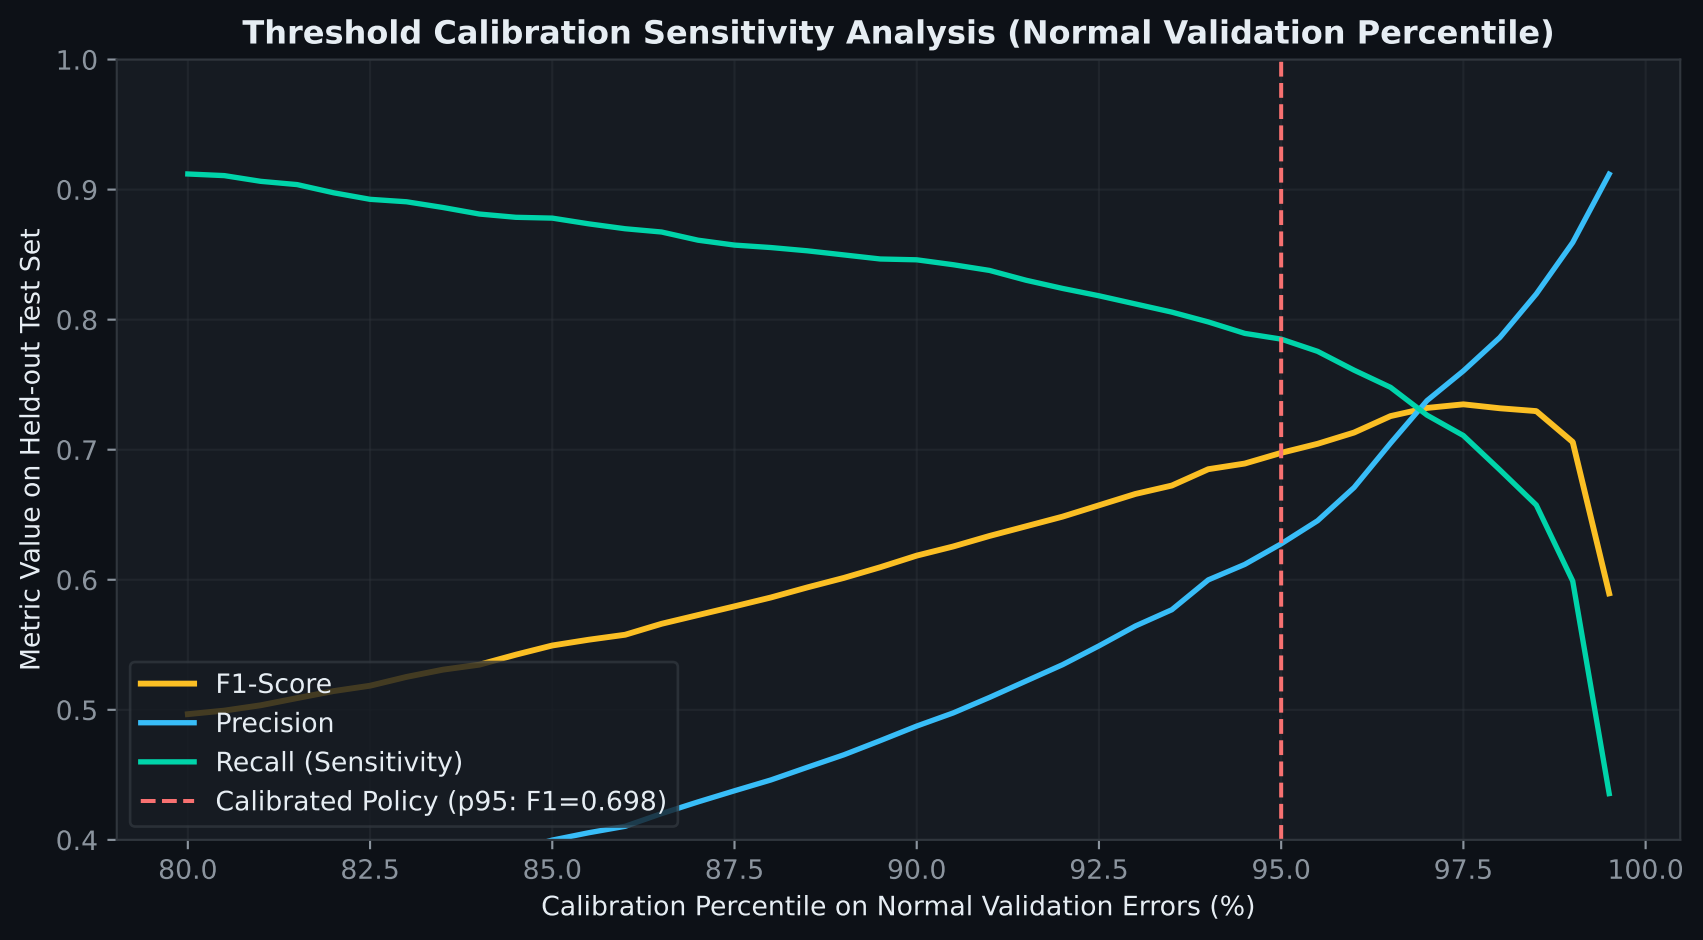
Threshold Calibration Sensitivity Analysis (Normal Validation Percentile)
Metric Value on Held-out Test Set
Calibration Percentile on Normal Validation Errors (%)
1.0
0.9
0.8
0.7
0.6
0.5
0.4
80.0
82.5
85.0
87.5
90.0
92.5
95.0
97.5
100.0
F1-Score
Precision
Recall (Sensitivity)
Calibrated Policy (p95: F1=0.698)