


Distribution of pulse peak values, Sep 2017 batch 703, channel 4, sensor: SiPM-AFP

Number (N)

700
600
500
400
300
200
100
0

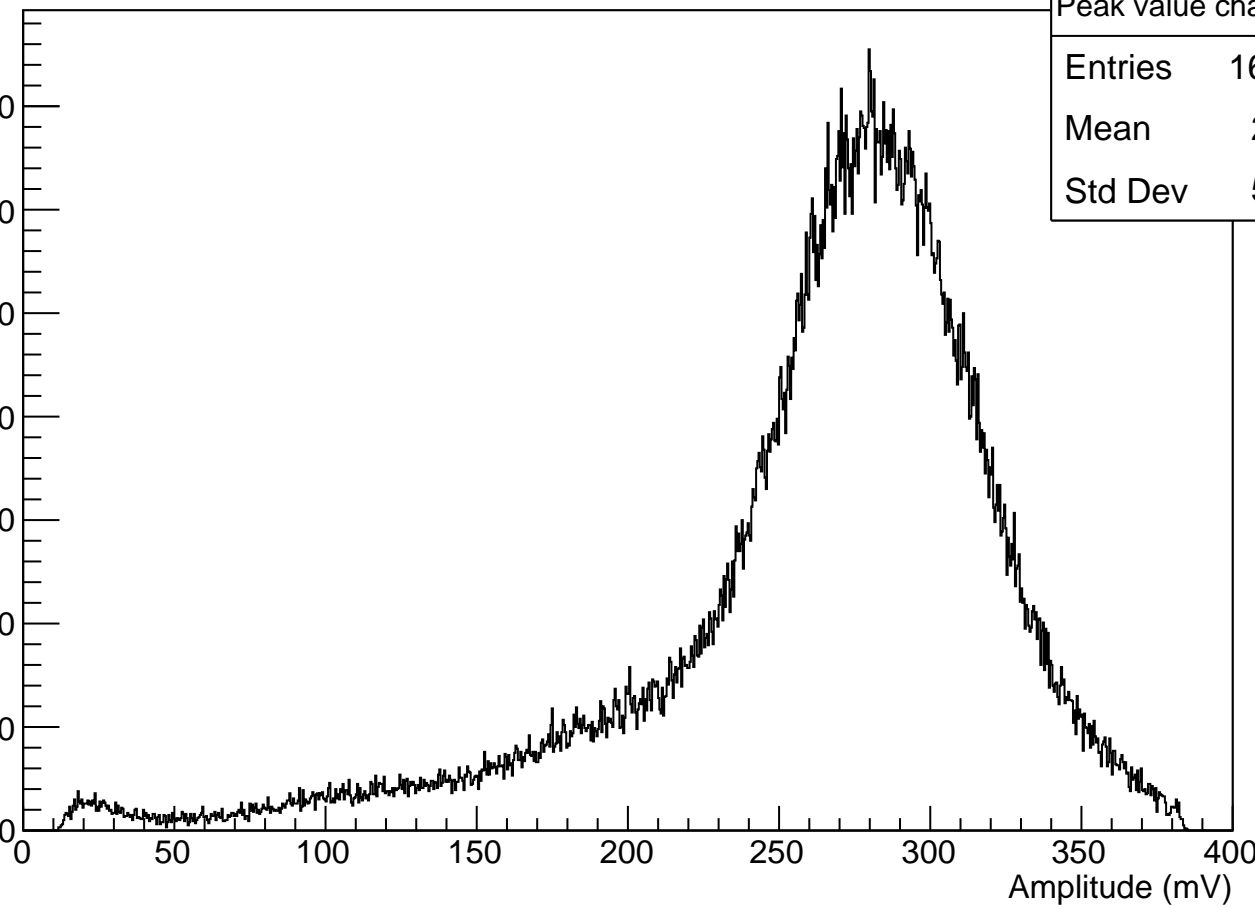

Peak value channel 4	
Entries	165291
Mean	264.5
Std Dev	59.47