


Distribution of pulse peak values, Sep 2017 batch 707, channel 7, sensor: W4-S204_6e14

Number (N)

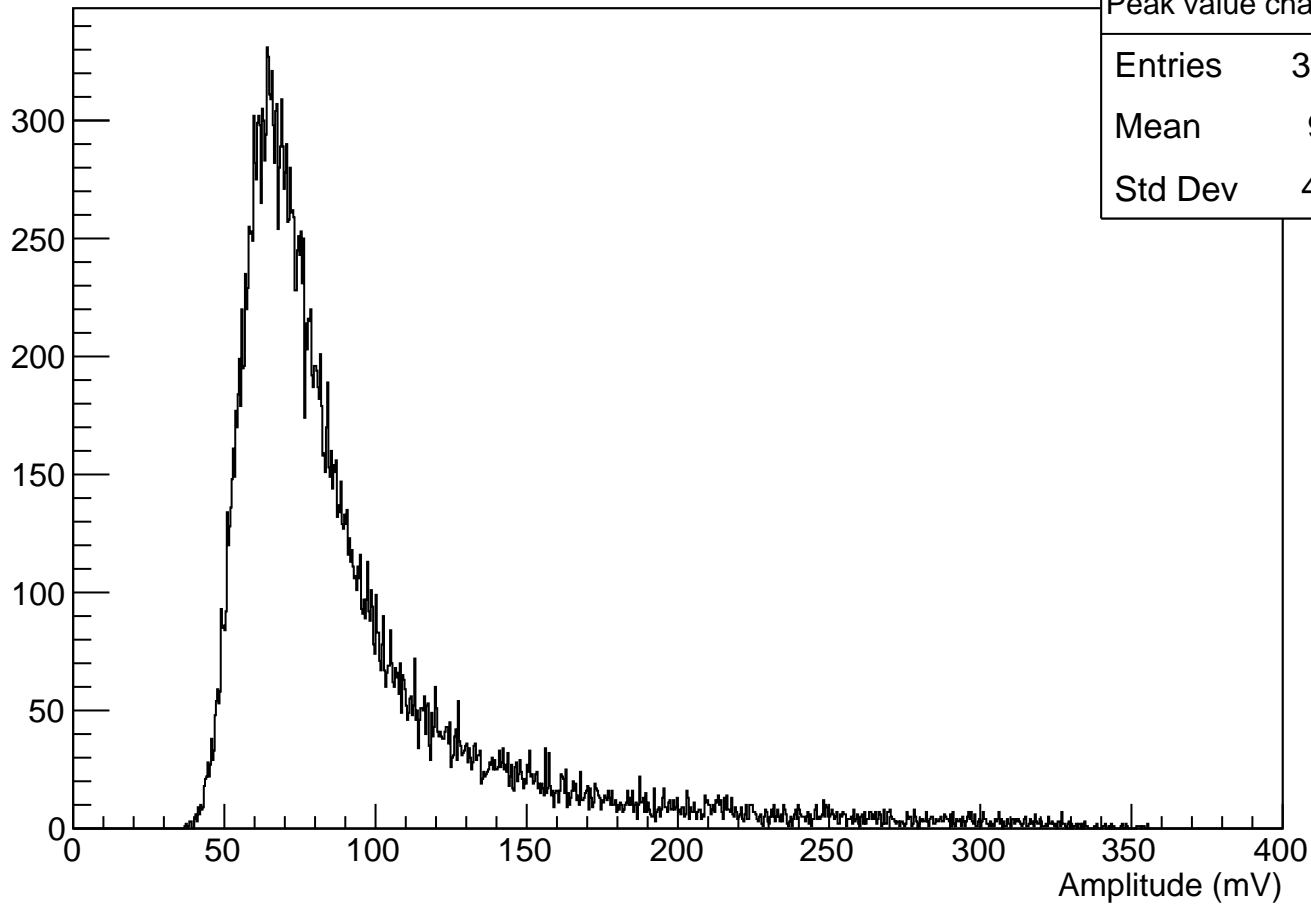

Peak value channel 7

Entries 33847

Mean 92.01

Std Dev 46.85