


Distribution of pulse peak values, Sep 2017 batch 407, channel 0, sensor: W4-S203

Number (N)

400
350
300
250
200
150
100
50
0

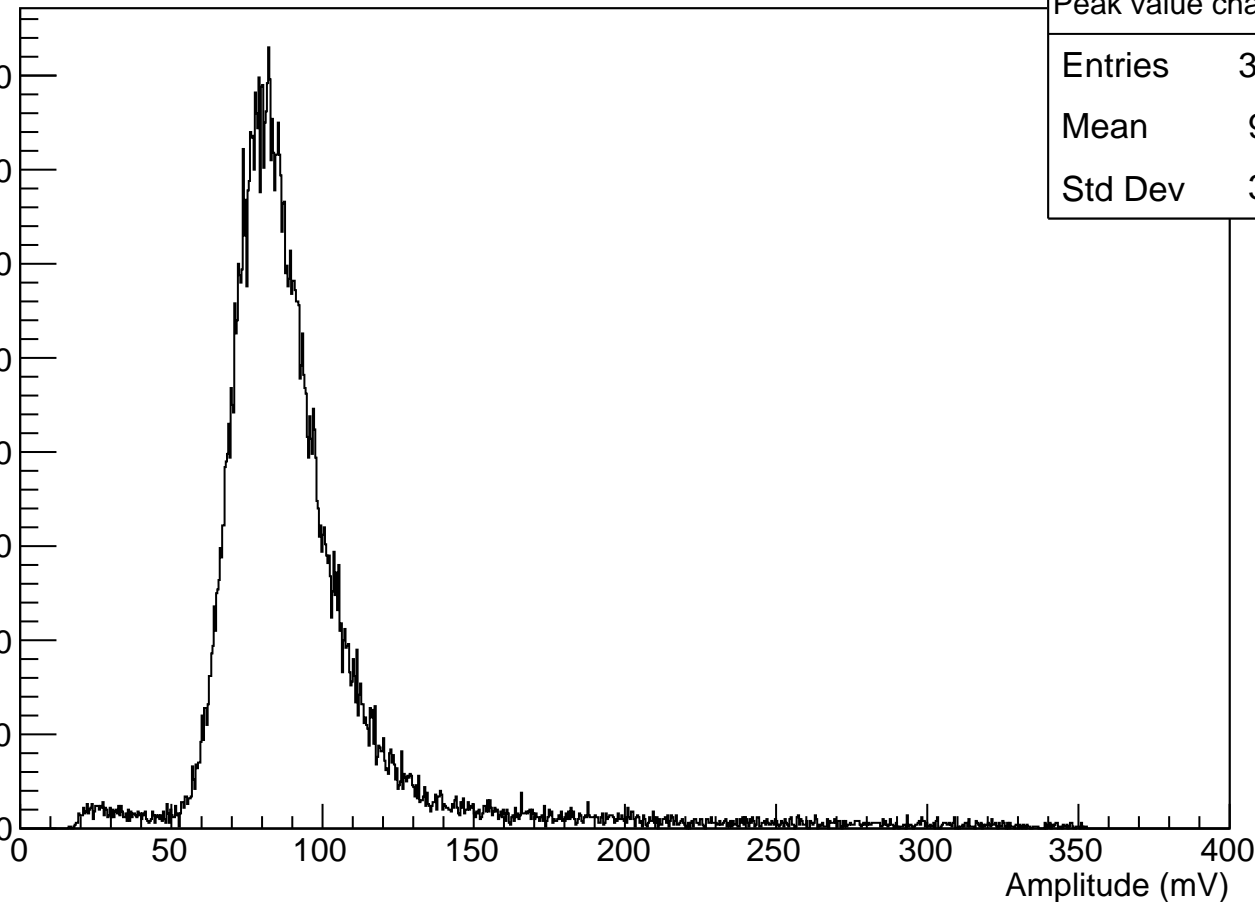

Peak value channel 0

Entries 34423

Mean 93.15

Std Dev 36.55

Amplitude (mV)