


Distribution of pulse peak values, Sep 2017 batch 503, channel 0, sensor: W4-S203

Number (N)

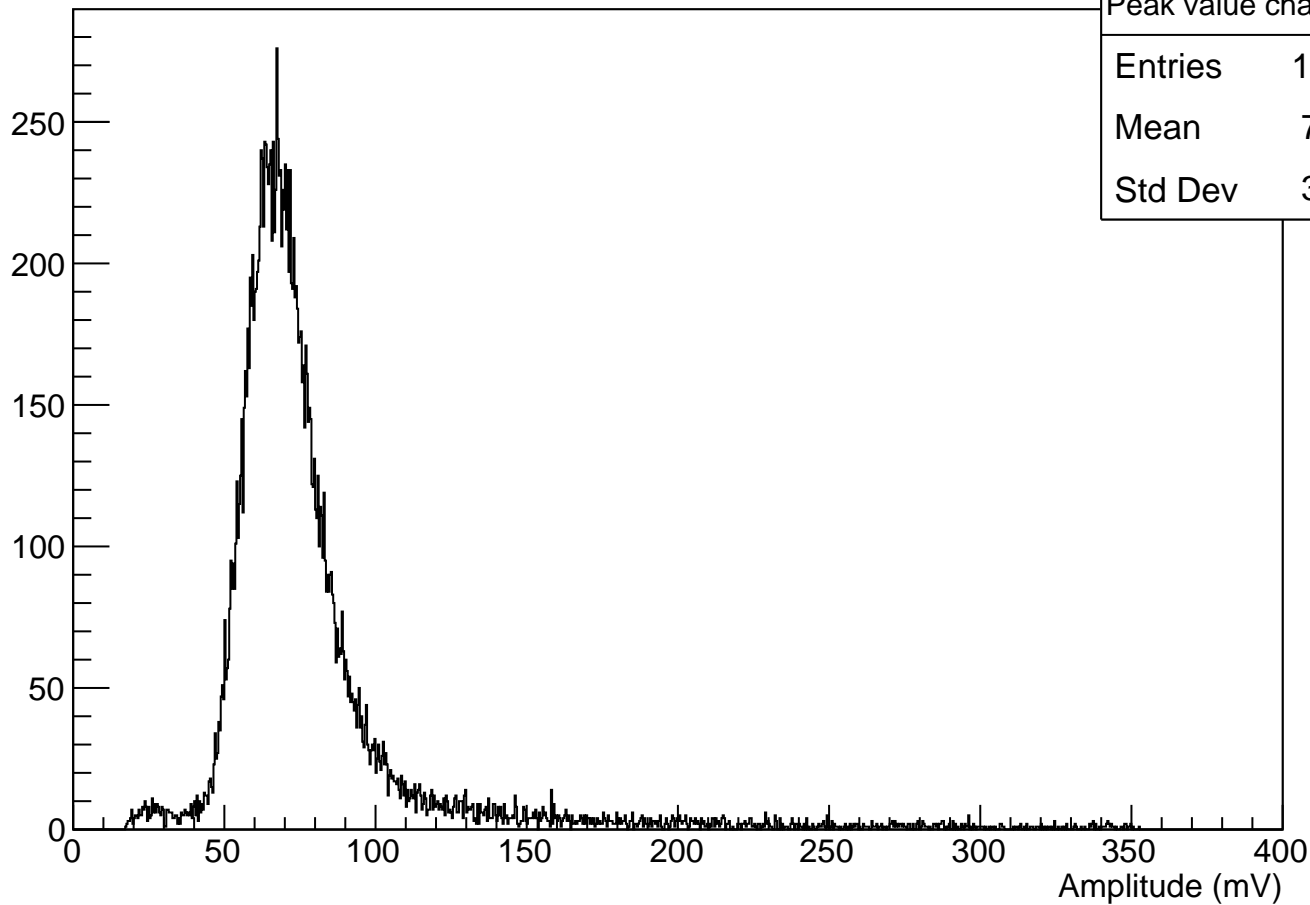

Peak value channel 0

Entries 19167

Mean 78.68

Std Dev 36.65