


Distribution of pulse peak values, Sep 2017 batch 204, channel 1, sensor: 50D-GBGR2

Number (N)

140
120
100
80
60
40
20
0

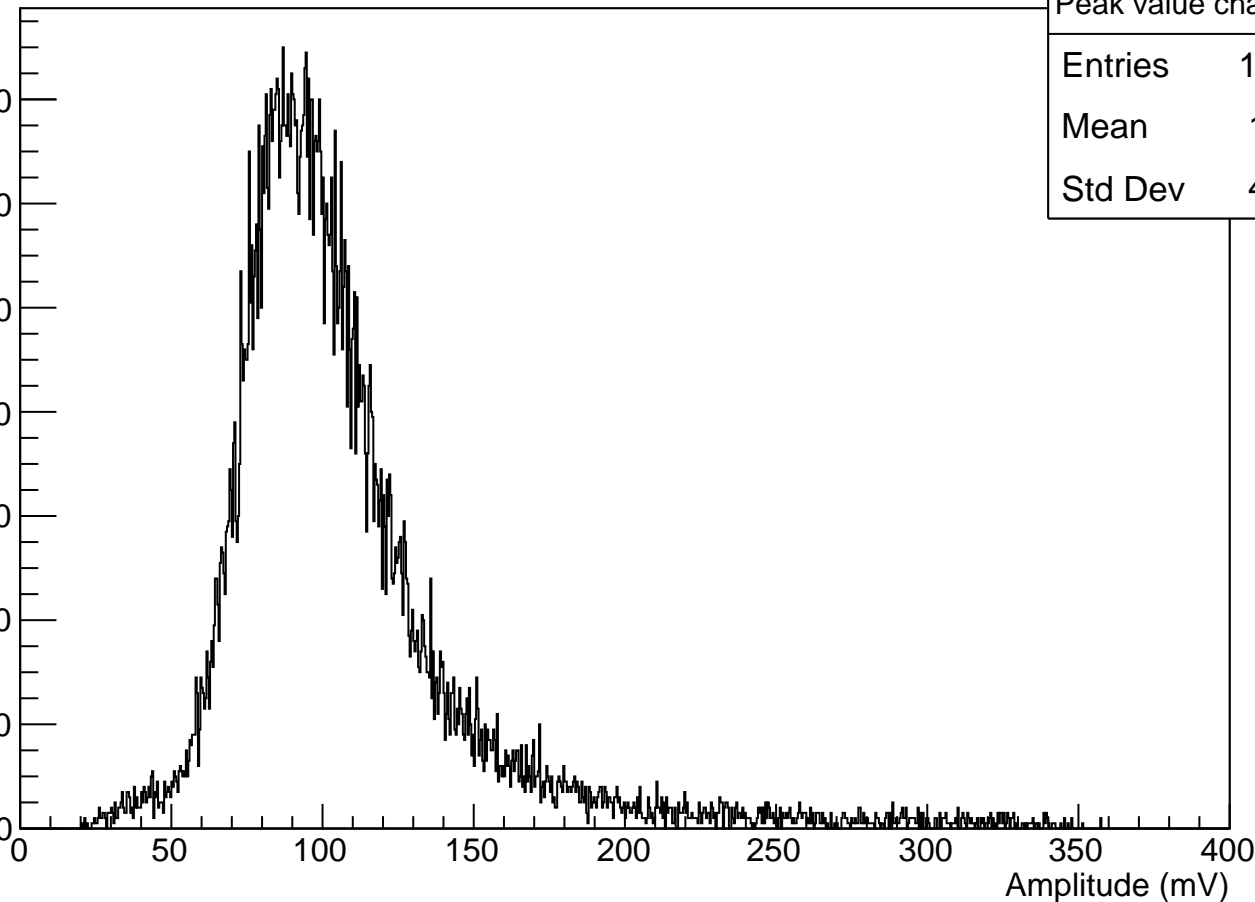

Peak value channel 1

Entries 19890

Mean 106.4

Std Dev 40.58

Amplitude (mV)