


Distribution of pulse peak values, Sep 2017 batch 705, channel 4, sensor: SiPM-AFP

Number (N)

700  
600  
500  
400  
300  
200  
100  
0

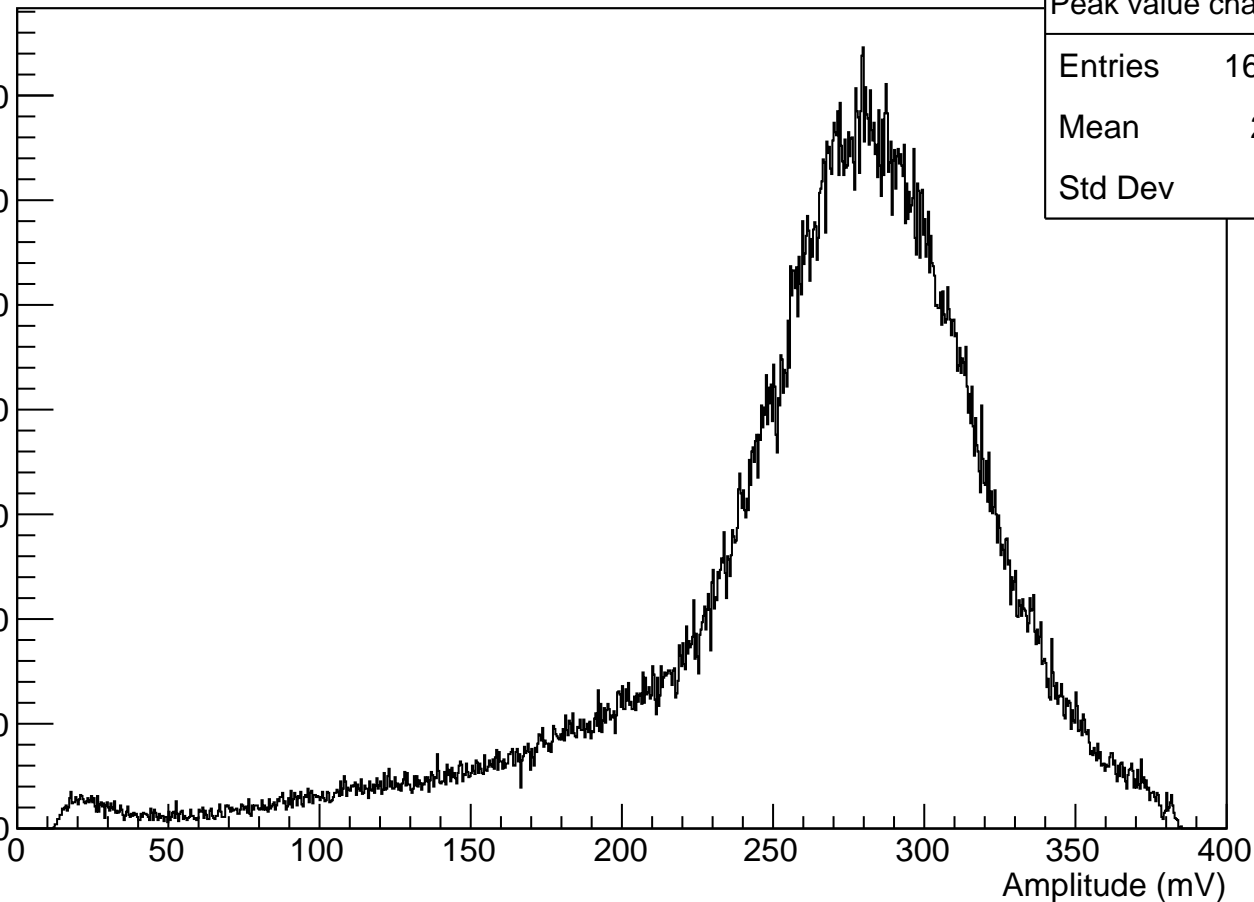

Peak value channel 4

Entries 164549

Mean 264.4

Std Dev 59.41