


Distribution of pulse peak values, Sep 2017 batch 703, channel 3, sensor: W4-S1022

Number (N)

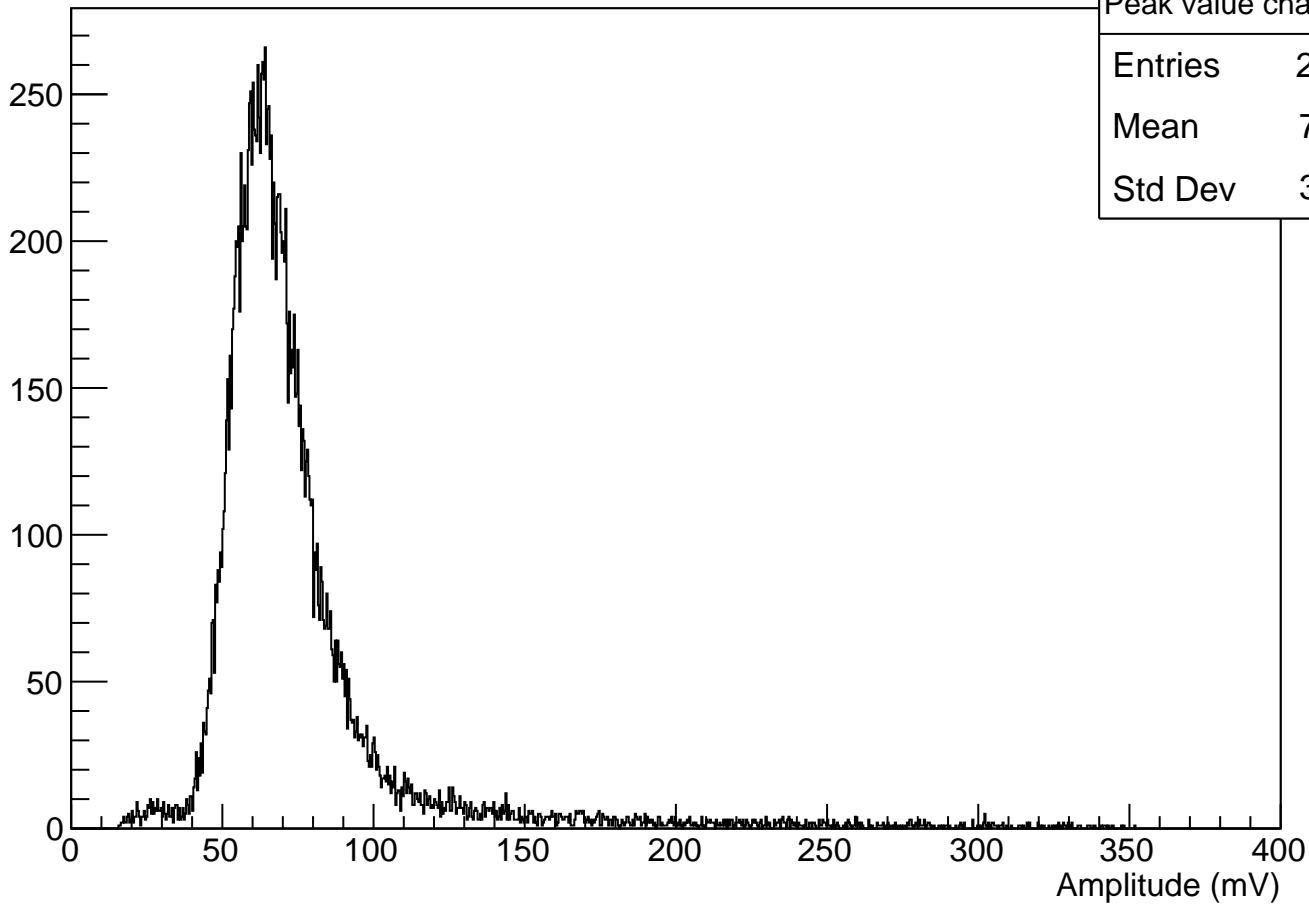

Peak value channel 3

Entries 20071

Mean 74.66

Std Dev 34.56