


Distribution of pulse peak values, Sep 2017 batch 401, channel 6, sensor: W4-S215

Number (N)

700
600
500
400
300
200
100
0

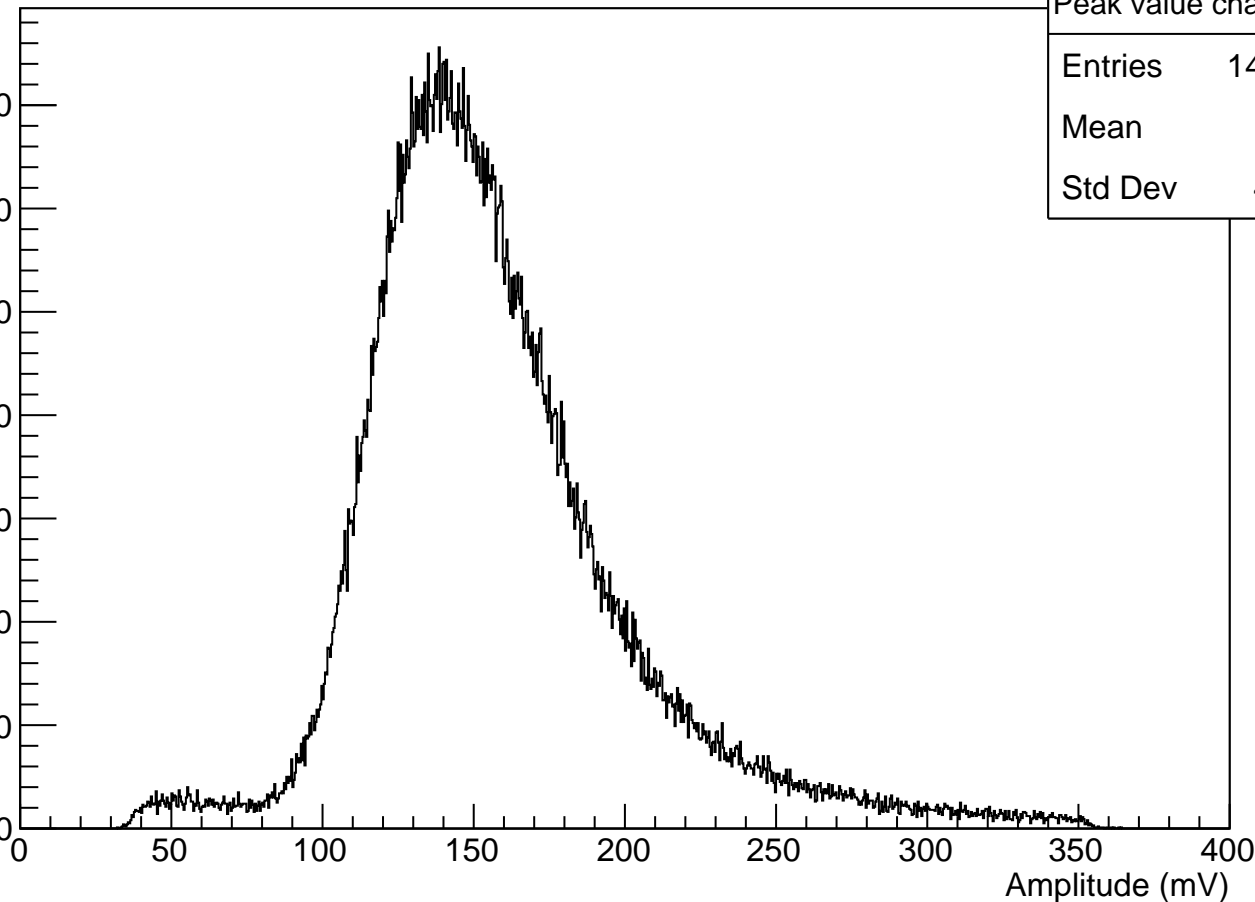

Peak value channel 6

Entries 141750

Mean 156.9

Std Dev 43.63

Amplitude (mV)