


Distribution of pulse peak values, Sep 2017 batch 407, channel 6, sensor: W4-S215

Number (N)

180
160
140
120
100
80
60
40
20
0

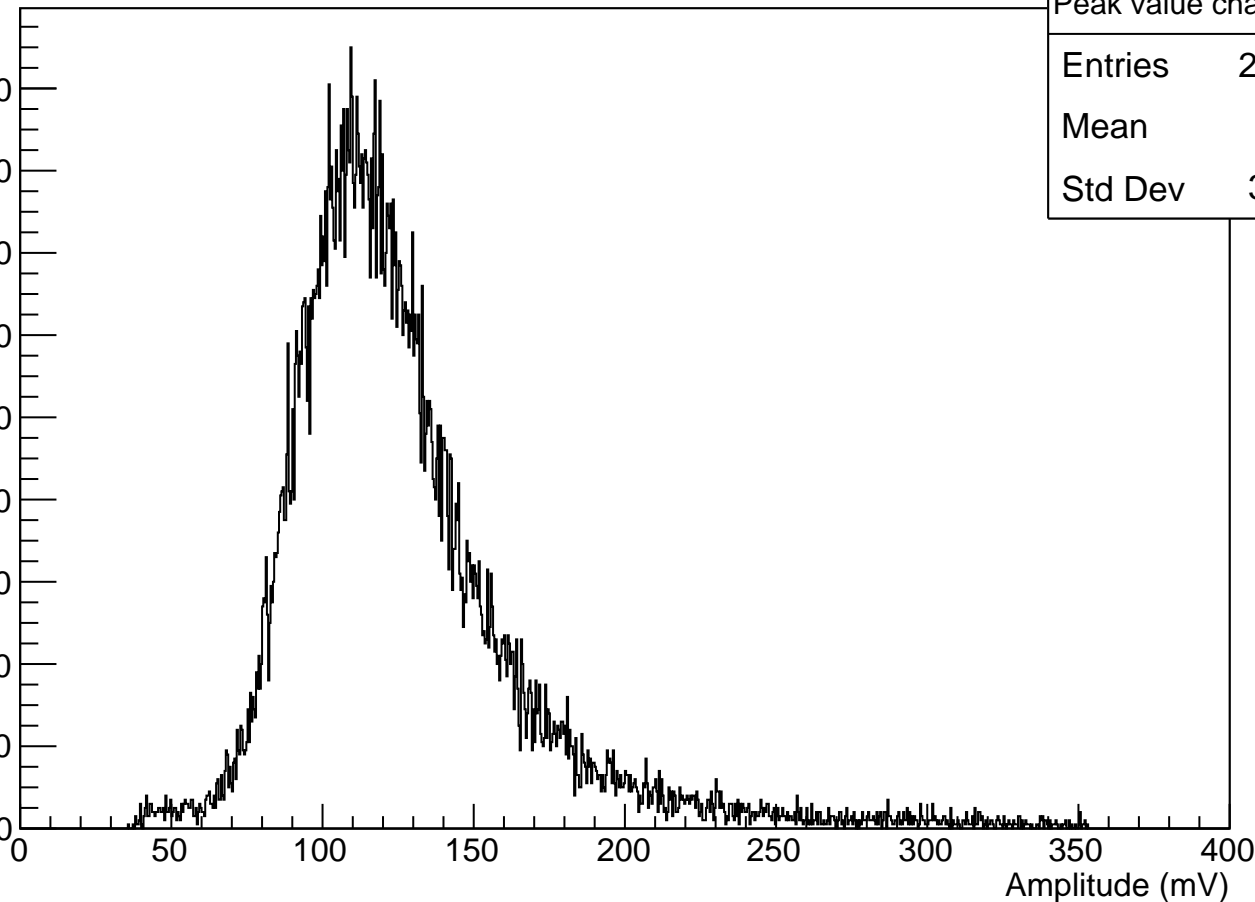

Peak value channel 6

Entries 26144

Mean 126

Std Dev 39.23

Amplitude (mV)