


Distribution of pulse peak values, Sep 2017 batch 702, channel 0, sensor: W4-S203

Number (N)

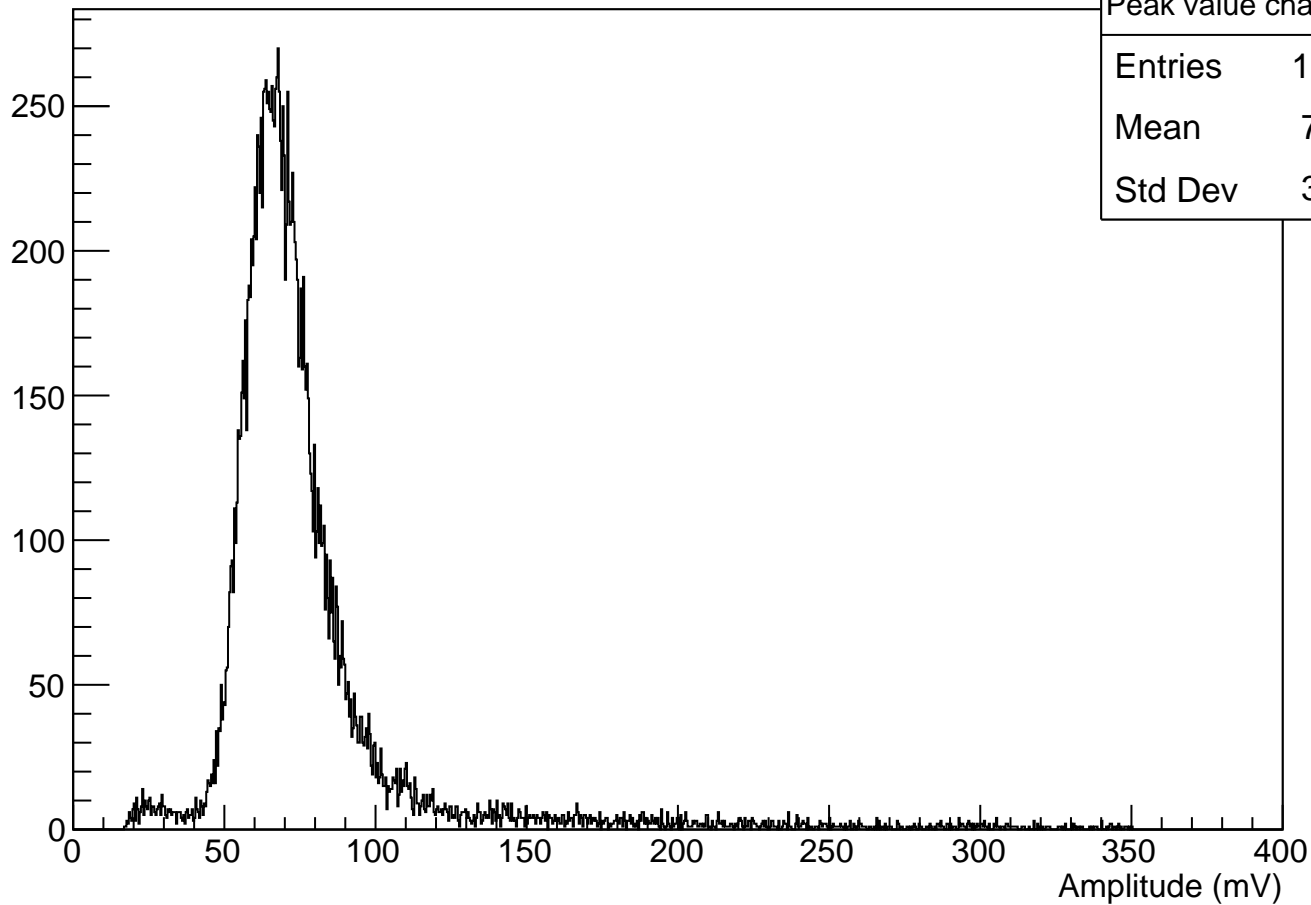

Peak value channel 0

Entries 19362

Mean 77.43

Std Dev 35.84