


Distribution of pulse peak values, Sep 2017 batch 701, channel 0, sensor: W4-S203

Number (N)

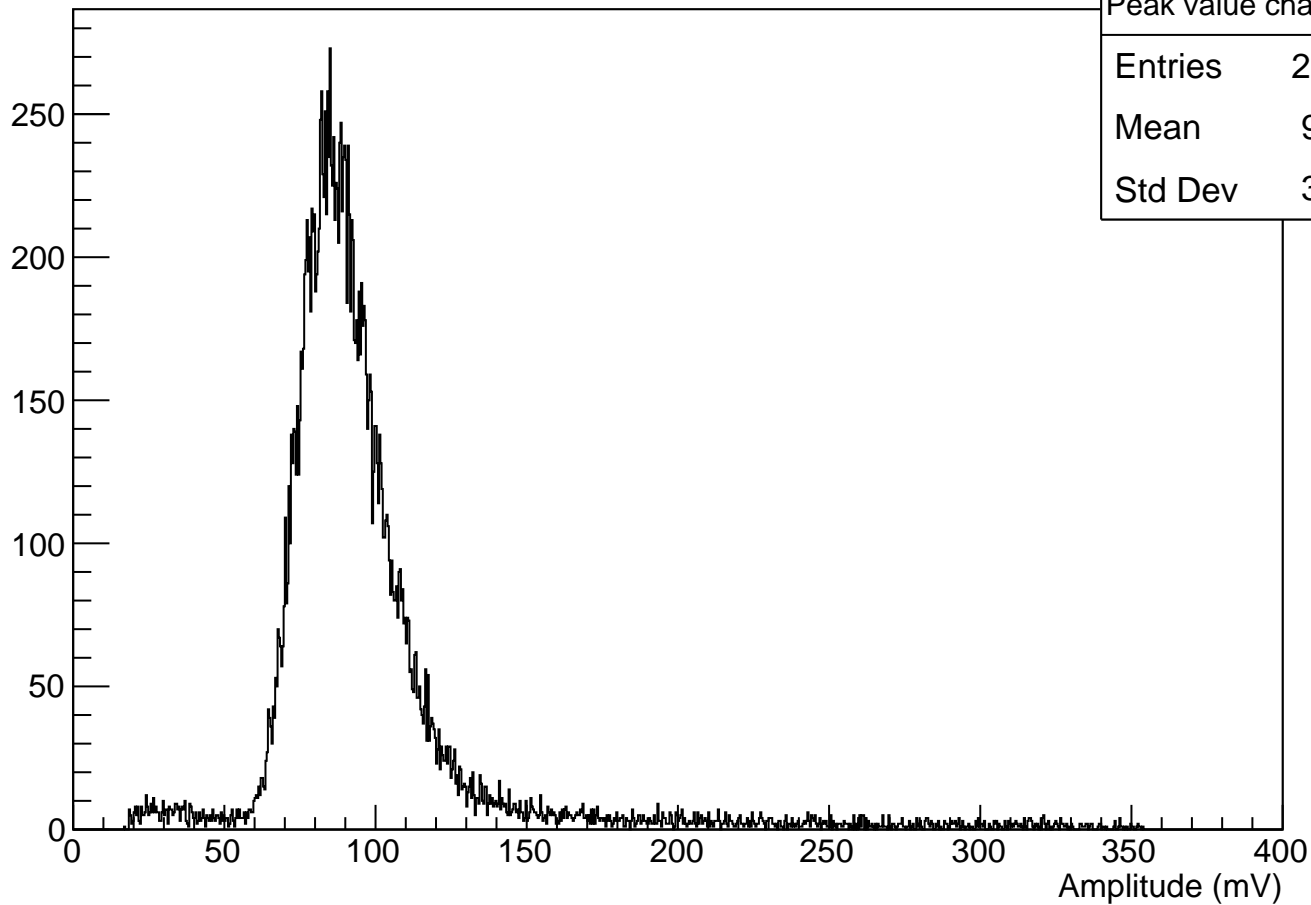

Peak value channel 0

Entries 21389

Mean 97.27

Std Dev 37.78