


Distribution of pulse peak values, Sep 2017 batch 102, channel 5, sensor: W4-S215

Number of entries (N)

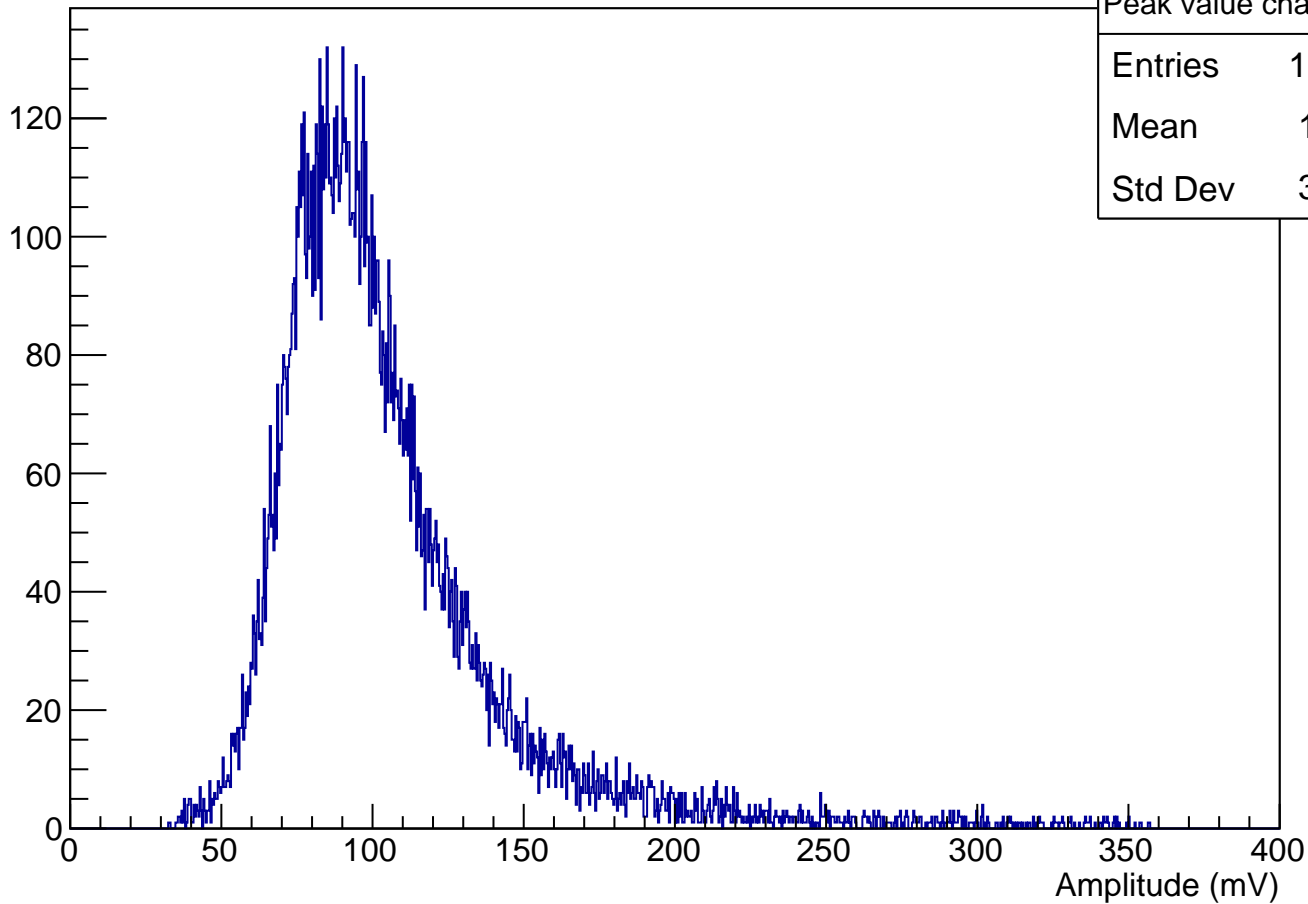

Peak value channel 5

Entries 16635

Mean 104.6

Std Dev 39.47