


Distribution of pulse rise times, Sep 2017 batch 707, channel 1, sensor: W4-S215

Number (N)

500
400
300
200
100
0

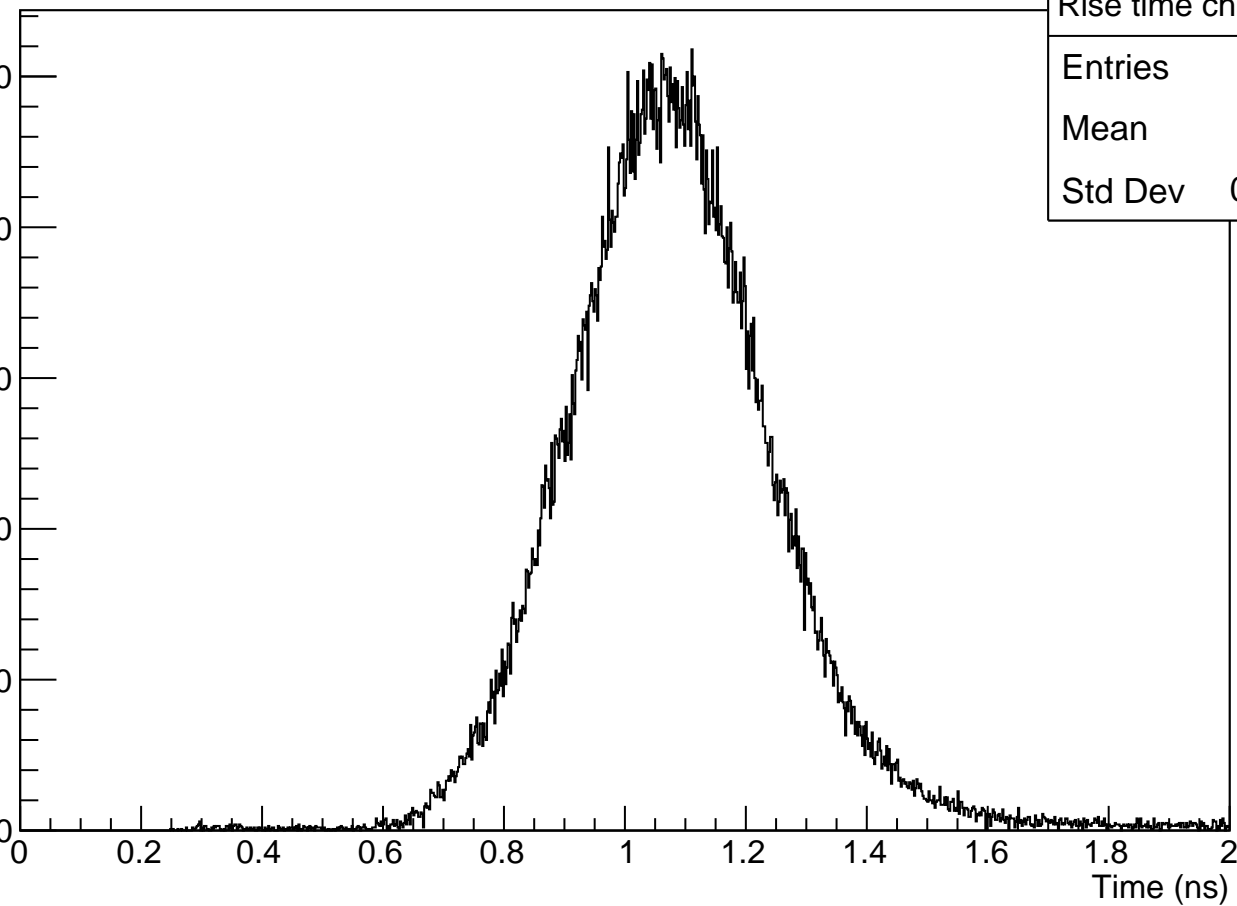

Rise time channel 1

Entries 98012

Mean 1.081

Std Dev 0.1768