


Distribution of pulse peak values, Sep 2017 batch 405, channel 0, sensor: W4-S203

Number (N)

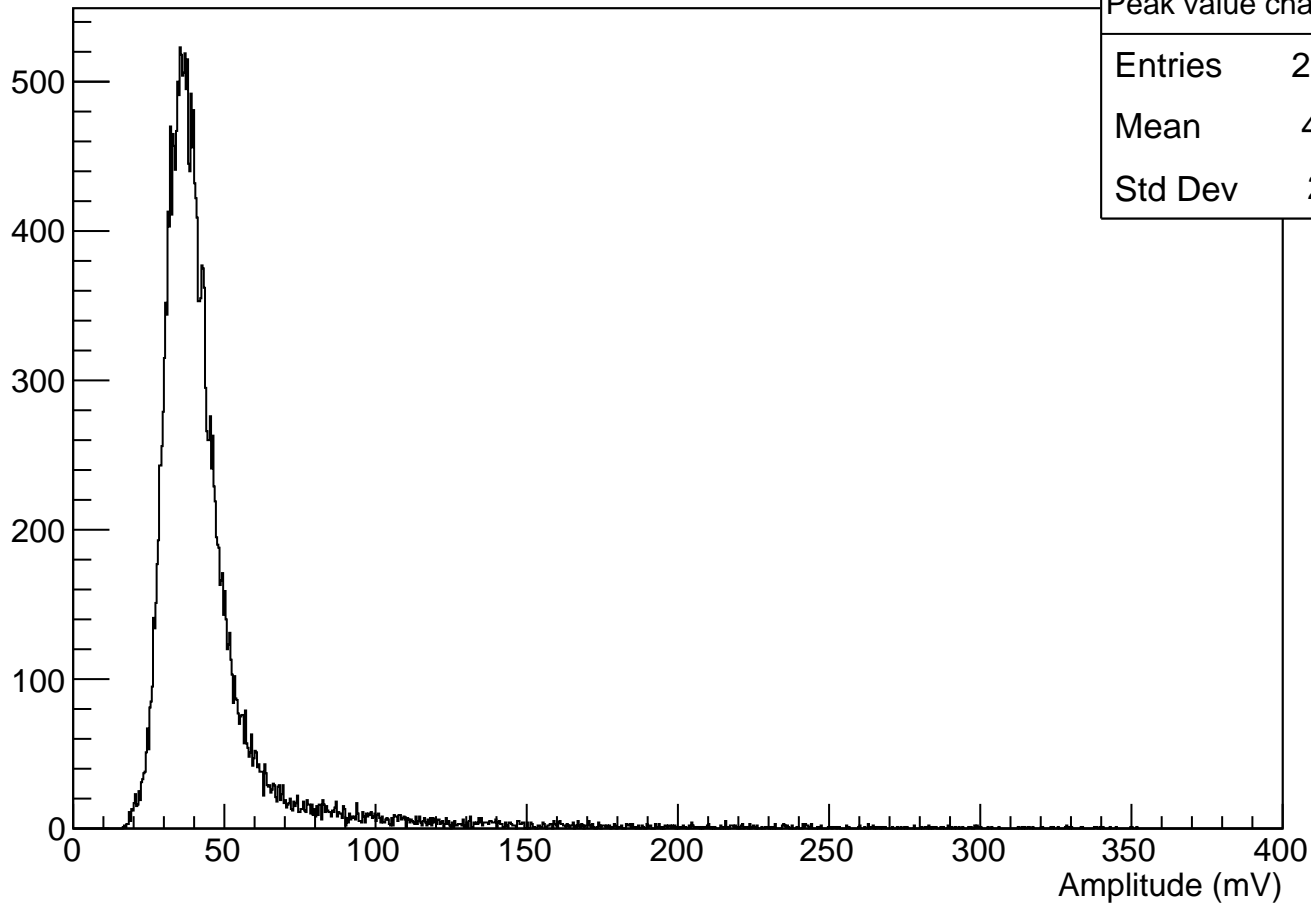

Peak value channel 0

Entries 25648

Mean 45.52

Std Dev 27.81