


Distribution of pulse peak values, Sep 2017 batch 108, channel 6, sensor: W4-S215

Number (N)

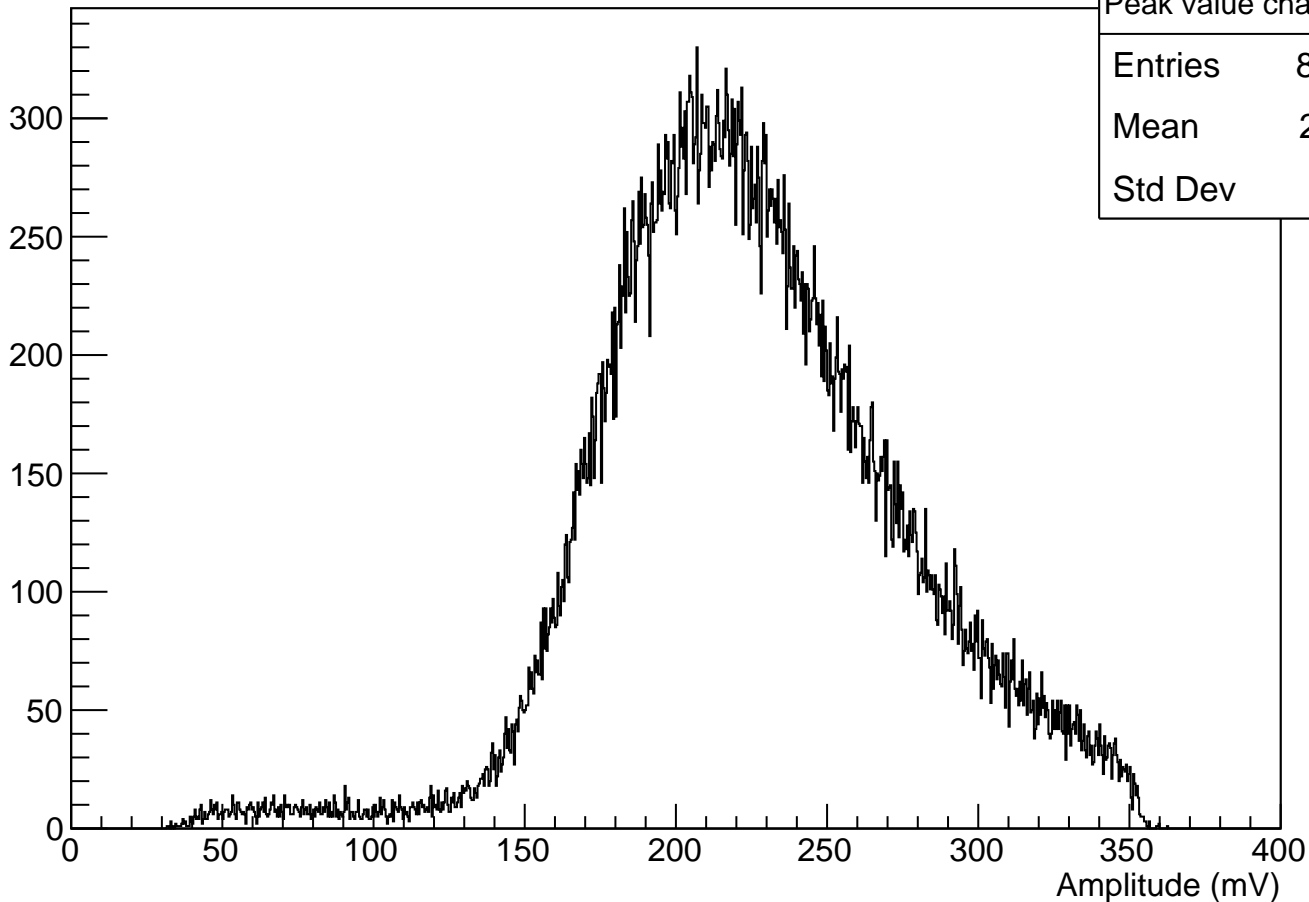

Peak value channel 6

Entries 81291

Mean 224.6

Std Dev 49.2