


Distribution of pulse peak values, Sep 2017 batch 105, channel 1, sensor: 50D-GBGR2

Number (N)

140
120
100
80
60
40
20
0

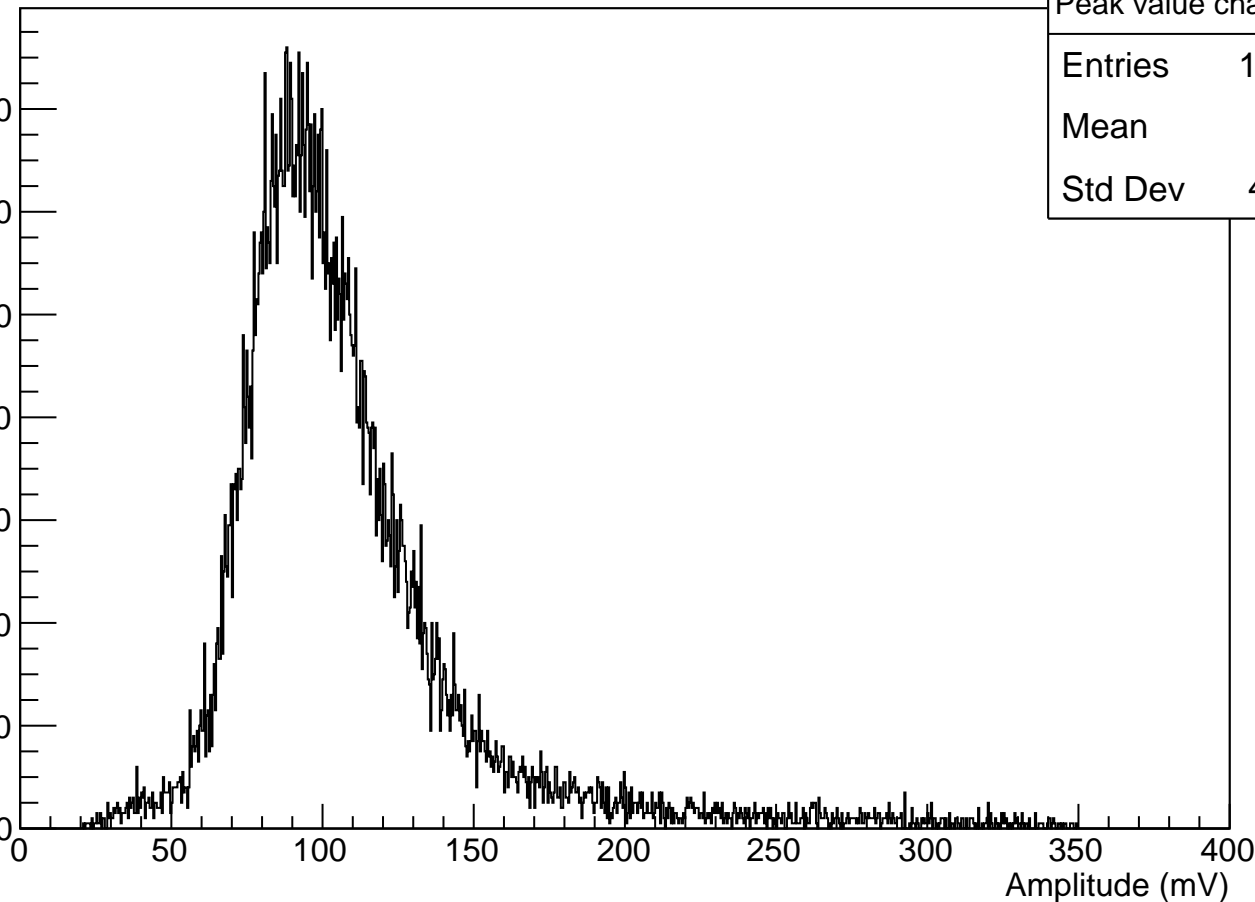

Peak value channel 1

Entries 19353

Mean 108

Std Dev 40.86

Amplitude (mV)