


Distribution of pulse peak values, Sep 2017 batch 701, channel 1, sensor: W4-S215

Number (N)

100
80
60
40
20
0

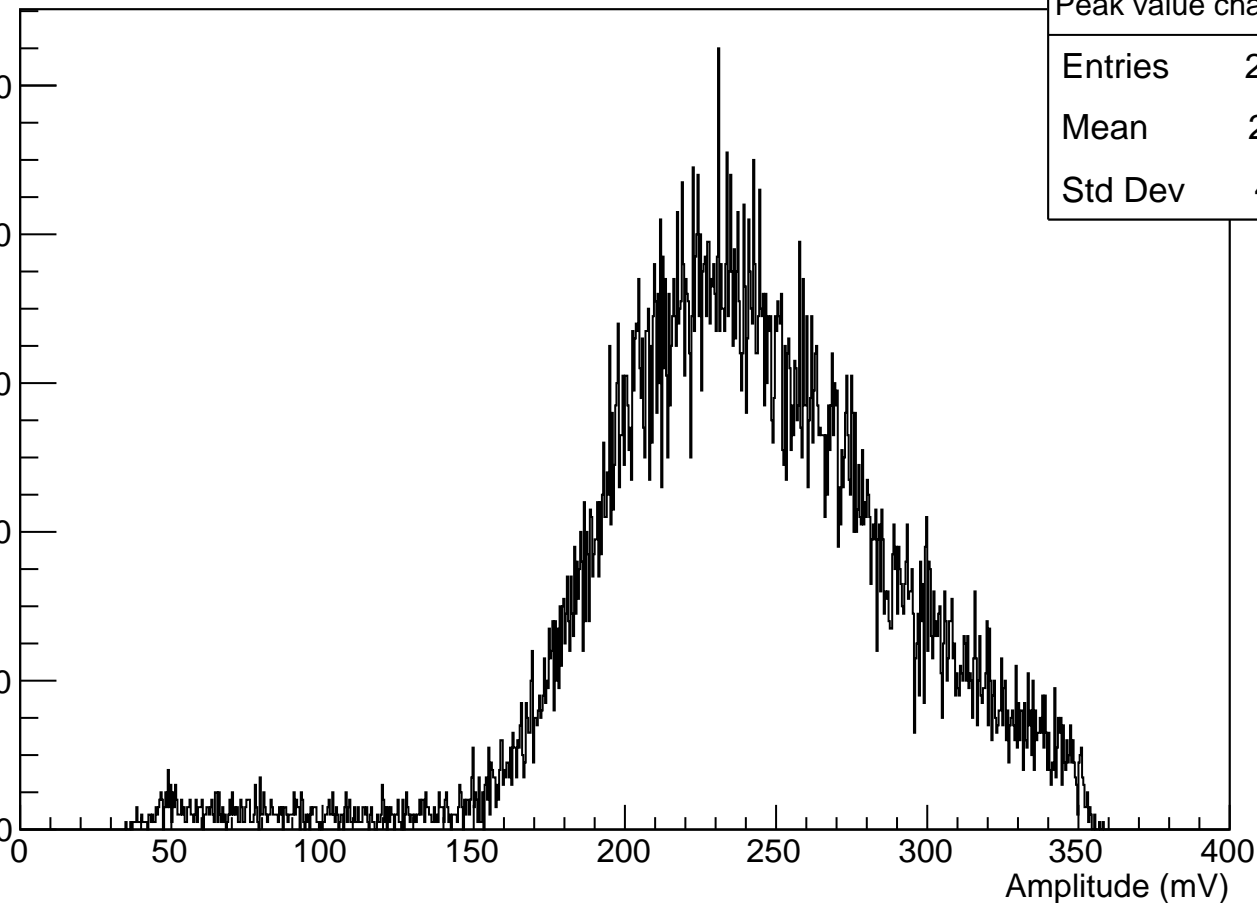

Peak value channel 1

Entries 20321

Mean 238.8

Std Dev 49.71

Amplitude (mV)