














- **ANF Device** is made of a special material that can send, receive and reflect neuro frequencies
- Medical Device, additional tool to implement in the clinic settings
- Goal: normalize weakened or damaged neurological frequencies by sending the correction signal to optimize the neural oscillation

ANF ACADEMY

ANF Device



ANF Neuro-Tech Device

			
Wearable Medical Device	Made of carbonized metal, 22.8% pure metal	Safe, strong & flexible PET material	Skin-friendly antibacterial 3M adhesive tape
			
Registered Medical Class 1/ Non-invasive	No chemical/ organic substances enter the body	Material that can send, receive and reflect the neuro frequencies	Over 300 devices with unique PURE frequencies

ANF ACADEMY

ANF Device Properties



ANF Neuro-Tech Device

- The Device is activated by body infrared heat
- It doesn't require additional source of heat
- Effective for 72 hours
- Compatible with personal hygiene routine
- Babies (durable for five days, preferable until Devices fall off)
- Intermittent use is possible (re-attaching with tape/spray)

Device Categories AP1

Pain & Inflammation Devices



P 200

P-9

Mental Device



MC

Immune System Devices




AGL

ACA


M2

Combine those three categories for the most effective protocols to normalize inflammation

P&I Devices - Frequencies Scale

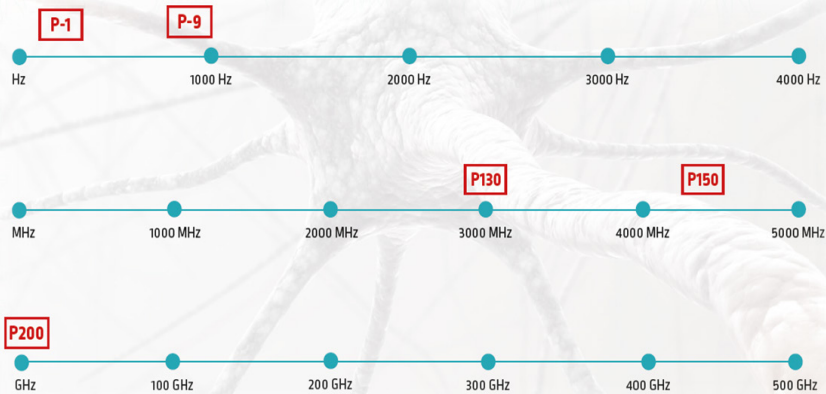

Device Frequencies - Tissue Layers

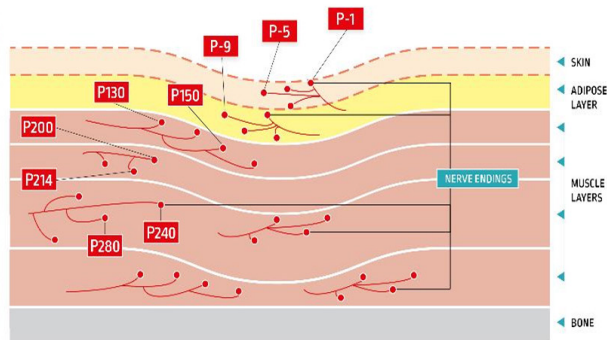

- The depth
- Tissue type
- Type of inflammation
- Treated surface area
- Patient's age and condition
- First or follow-up visit
- Detox symptoms
- Phase of treatment

ANF Device · Use Instructions

- Do not cut or modify the shape of the device
- Do not apply directly to open wounds
- Make sure the skin is clean and dry
- **Please do not rip off** the device; remove them gently from the skin
- In reddening of the skin occurs, place it in the nearest free area



ANF Device · Storage & Incompatibilities

Storage:

- Device must always be kept in antistatic bags
- Do not mix different Device types in one bag
- Keep away from heating sources or electrical equipment

While wearing the Device:

- Avoid using the hair dryer directly on the Device
- Do not use direct heat modalities like infrared, laser, shockwave, or ultrasound on the treated area
- Remove the Device prior to X-ray/MRI



Precautions & Contraindications

Precautions: High frequency (P200) or a high number of Devices on vulnerable population

- below 12 years old (contraindication on babies)
- above 70 years old
- very weak patients
- severe diseases (ex., active cancer, organ failure, autoimmune disorders) due to a lack of resources

Contraindications based on your current level (AP program):

- Pregnancy: No Devices applied around the abdomen
- No treatment with ANF Therapy® on patients' cases above the education level

Key Points to Remember

- Medical device to normalize neural oscillation
- Material that can send, receive and reflect the neuro frequencies
- To approach inflammation, use a combination of P+, P-, and AOs Devices
- Low frequencies for superficial layers, stronger frequencies for deeper ones
- Make sure the skin is dry and clean before application
- Devices are activated by body infrared heat; avoid direct heat on them
- Remove them gently from the skin after 72 hours
- Use the Devices according to instructions and based on your scope of practice

Ready to Get started with
the Medicine of the Future ?



Course Content

1. ANF Device
2. ANF Device Properties
3. The Device Categories AP1
4. P&I Devices - Frequencies Scale
5. Device frequencies – tissue layers
6. ANF Device - Instructions for use
7. ANF Device - Storage & Incompatibilities
8. Precautions & Contraindications
9. Key Points to Remember

* Click on the title to get transferred to the slide



www.anfcourses.com

ANF Academy
Calle de Las Adelfas 5
Marbella, Spain

academy@anfacademy.com

Patented Model
U202032252
ES1259974