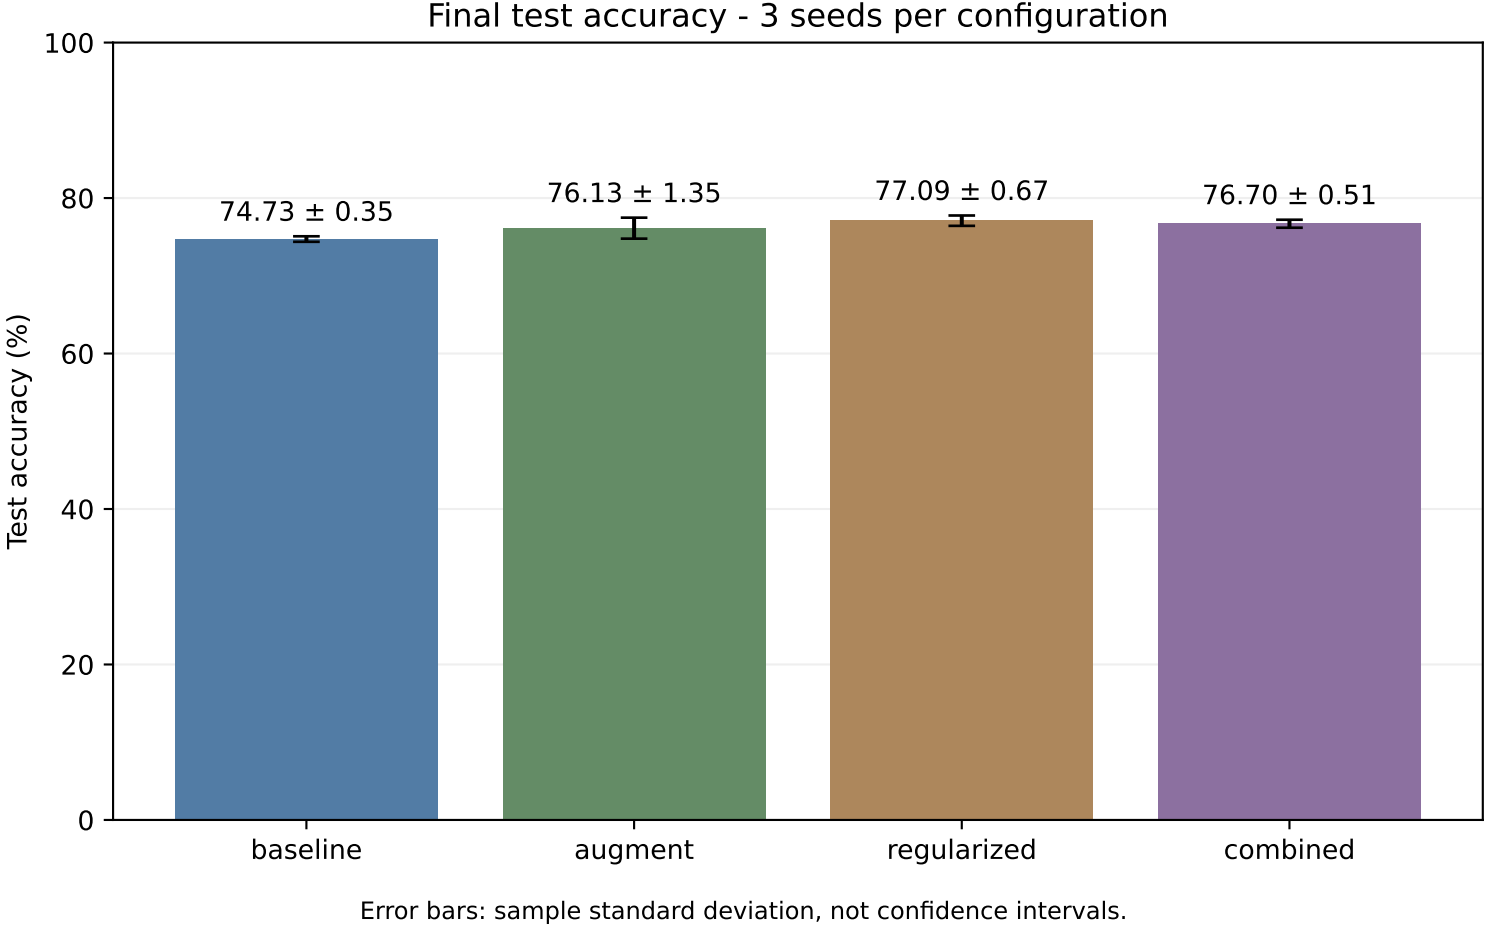
Final test accuracy - 3 seeds per configuration
Test accuracy (%)
100
80
60
40
20
0
74.73 ± 0.35
76.13 ± 1.35
77.09 ± 0.67
76.70 ± 0.51
baseline
augment
regularized
combined
Error bars: sample standard deviation, not confidence intervals.