

An Enhanced IoT-Based Healthcare Monitoring System for Obese Adults

Lahcen Atti^{1*}, Mohamed Saber¹, Nacer Boubkraoui¹,
Mouhamed Dib¹, Hassan Ouahi¹

^{1*}Faculty of Applied Sciences – Ait Melloul, Ibn Zohr University, Ait Melloul, Morocco.

*Corresponding author(s). E-mail(s): atti.lahcen@gmail.com;

Contributing authors: mohamed.saber@edu.uiz.ac.ma;

n.boubkraoui@uiz.ac.ma; m.dib@uiz.ac.ma; h.ouahi@uiz.ac.ma;

Abstract

This paper presents an enhanced Internet-of-Things (IoT) healthcare monitoring prototype for obese adults, inspired by the work of Gupta et al. [1]. The prototype combines a DS18B20 digital ambient-temperature probe, a MAX30102 pulse-oximeter/heart-rate sensor, and a dual-core ESP32 microcontroller behind a patient-authenticated on-device menu, publishing telemetry over MQTT to a ThingsBoard cloud dashboard. Relative to the baseline platform, the system improves ambient-temperature sensing accuracy (± 0.1 °C vs. ± 0.5 °C), replaces an 8-bit microcontroller and unencrypted HTTP transport with a Wi-Fi-capable ESP32 and MQTT, and moves from a proprietary paid cloud subscription to an open-source dashboard. A companion Android application concept for multi-patient dashboards and threshold-based alerting is also described. This paper reports the hardware design, firmware architecture, and cloud integration of the prototype; clinical validation against a reference instrument is identified as future work.

Keywords: IoT, Healthcare monitoring, Obesity, ESP32, MQTT, ThingsBoard

1 Introduction

Obesity affects over 650 million adults worldwide and increases the risk of cardiovascular and metabolic complications [2]. Continuous monitoring of vital signs –

blood-oxygen saturation (SpO_2) and heart rate – together with ambient temperature logging can support early detection of complications, but commercial remote patient monitoring (RPM) devices remain cost-prohibitive for many deployments. This paper presents a low-cost IoT-based monitoring prototype for obese adults that builds on the platform proposed by Gupta et al. [1]. Relative to that baseline, four improvements are targeted:

- higher-accuracy digital temperature sensing ($\pm 0.1^\circ\text{C}$ vs. $\pm 0.5^\circ\text{C}$);
- MQTT-based telemetry in place of unencrypted HTTP polling;
- an open-source ThingsBoard cloud dashboard in place of a proprietary subscription service;
- a rechargeable Li-ion power supply in place of a fixed 12 V DC adapter.

This paper makes the following contributions:

1. A hardware and firmware redesign of the baseline platform using an ESP32 microcontroller, a DS18B20 digital thermometer, and a MAX30102 pulse oximeter, with an on-device patient-login menu (Sect. 3).
2. An MQTT/ThingsBoard cloud-integration layer with a defined topic hierarchy and JSON telemetry schema (Sect. 4).
3. A concept design for a multi-patient Android dashboard application with threshold-based alerting (Sect. 5).

2 Related Work

The baseline platform proposed by Gupta et al. [1] combines an Arduino ATmega328 microcontroller, an LM35 analogue temperature sensor ($\pm 0.5^\circ\text{C}$), a wrist-worn blood-pressure cuff, and unencrypted HTTP transmission to a proprietary cloud service (iotgecko.com). It established feasibility for obesity-focused wearable monitoring, but four limitations motivate the present work: (i) the 8-bit AVR core has no native wireless connectivity and requires an external radio module; (ii) the analogue thermometry chain is limited to $\pm 0.5^\circ\text{C}$ accuracy by ADC quantisation noise; (iii) HTTP transmission carries no transport-layer encryption; and (iv) the cloud subscription incurs recurring licensing cost around a closed dashboard.

3 System Design

3.1 Hardware Architecture

Figure 1 shows the end-to-end data path. The microcontroller is an ESP32-WROOM-32D development board (dual-core Xtensa LX6, integrated Wi-Fi/BLE), replacing the Arduino ATmega328 and its external wireless module. Ambient temperature is sampled by a DS18B20 waterproof digital probe over a 1-Wire bus, removing the ADC quantisation noise of the baseline’s analogue LM35 chain. SpO_2 and heart rate are sampled by a MAX30102 pulse-oximeter module over I²C, accessed through a MAX30100-compatible pulse-oximeter driver library. A four-button matrix keypad and a 20×4 character I²C LCD provide local patient interaction (DS18B20 data line

Table 1 Baseline vs. enhanced platform (component-level comparison).

Feature	Baseline [1]	This work
Microcontroller	Arduino ATmega328	ESP32 (dual-core, Wi-Fi/BLE)
Temperature sensor	LM35 ($\pm 0.5^\circ\text{C}$)	DS18B20 ($\pm 0.1^\circ\text{C}$)
Cloud platform	iotgecko.com (proprietary)	ThingsBoard (open-source)
Transport	HTTP (unencrypted)	MQTT ¹
Power source	12 V DC adapter	Li-ion battery ($\sim 8\text{ h}$)
BP sensing	Wrist cuff	Clinical arm cuff ²

¹The demonstrated prototype uses the MQTT broker’s default unencrypted listener for development; TLS on the broker’s secure port is the intended production configuration (Sect. 4).

²Hardware slot present on the board design; firmware integration is future work (Sect. 7).

on GPIO4; keypad keys 1–4 on GPIO27, GPIO26, GPIO12, and GPIO14; LCD at I²C address 0x27).

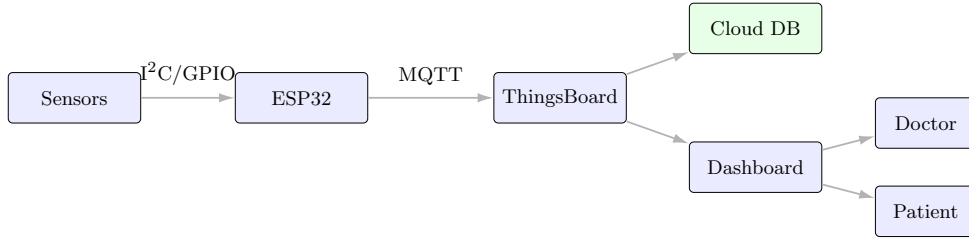


Fig. 1 System architecture: on-board sensors feed the ESP32, which publishes MQTT telemetry to ThingsBoard; the cloud dashboard is consumed by clinicians and patients.

3.2 Firmware Architecture

The firmware implements a menu-driven state machine, shown live on the on-device LCD in Fig. 3. On boot, the patient must enter a 4-digit code on the keypad before any measurement is available; a successful verification unlocks the main menu (Fig. 3a), from which the patient selects SpO₂, heart rate (BPM), temperature, or data transfer. Each measurement runs as a non-blocking 5-second state (Fig. 3b) so that the pulse-oximeter driver (`pox.update()`) and keypad polling continue to execute during the on-screen countdown animation, rather than blocking on a fixed `delay()`, before the result is displayed (Fig. 3c). On “Data Transfer”, the device assembles a JSON payload from the most recent readings and publishes it to the cloud (Sect. 4).

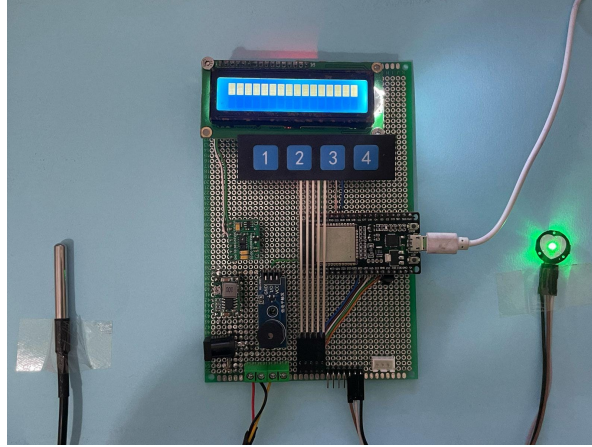


Fig. 2 Assembled prototype: LCD, keypad, ESP32, DS18B20 ambient temperature probe, and MAX30102 pulse-oximeter sensor.

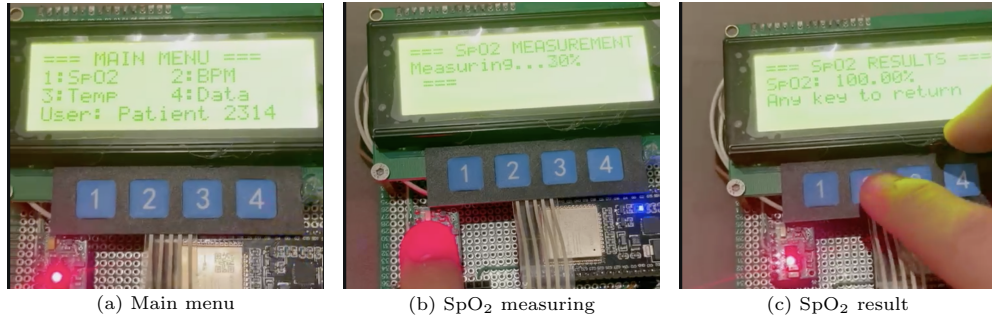


Fig. 3 On-device LCD menu, captured live: (a) main menu after patient login, (b) non-blocking SpO₂ measurement in progress, (c) SpO₂ result screen.

Wi-Fi and MQTT broker credentials are configured at startup (Listing 1); the device token and network credentials shown here are anonymised.

Listing 1 Wi-Fi and MQTT configuration (credentials anonymised).

```
// Wi-Fi credentials
const char* ssid = "ANONYMIZED_SSID";
const char* password = "ANONYMIZED_PASSWORD";

// MQTT broker (ThingsBoard server)
const char* mqtt_server = "demo.thingsboard.io";
const int mqtt_port = 1883;
const char* mqtt_client_id = "ESP32_Client";
const char* mqtt_username = "ANONYMIZED_DEVICE_TOKEN"; // ThingsBoard device token
```

4 Cloud Connectivity and MQTT Implementation

4.1 Telemetry Path

On “Data Transfer”, the firmware builds a JSON object from the patient code and the most recent SpO₂, heart-rate, and temperature readings, and publishes it on ThingsBoard’s fixed device telemetry topic (Listing 2).

Listing 2 JSON payload construction and MQTT publish (device firmware).

```
String payload = "{";
payload += "\"patient_id\": \"" + patientCode + "\",";
payload += "\"SpO2\": " + String(oldSpO2) + ",";
payload += "\"BPM\": " + String(oldBPM) + ",";
payload += "\"Temperature\": " + String(oldTemp);
payload += "}";

client.publish("v1/devices/me/telemetry", payload.c_str());
```

The device authenticates to the broker using its ThingsBoard access token as the MQTT username, following ThingsBoard’s standard device-token authentication scheme [3]. The demonstrated prototype connects to the public demo broker (`demo.thingsboard.io`) on its default unencrypted port 1883 for development; the broker’s TLS listener on port 8883, with the same token-based authentication, is the intended configuration for a production deployment.

4.2 Why ThingsBoard

ThingsBoard was selected over commercial alternatives (e.g. AWS IoT, Azure IoT Hub) for its open-source licensing, drag-and-drop dashboard builder, and built-in device-provisioning tools, avoiding the recurring per-device subscription fee of the baseline platform’s cloud service. Figure 4 shows the resulting dashboard, with live SpO₂, heart-rate, and temperature widgets and a rolling line chart.

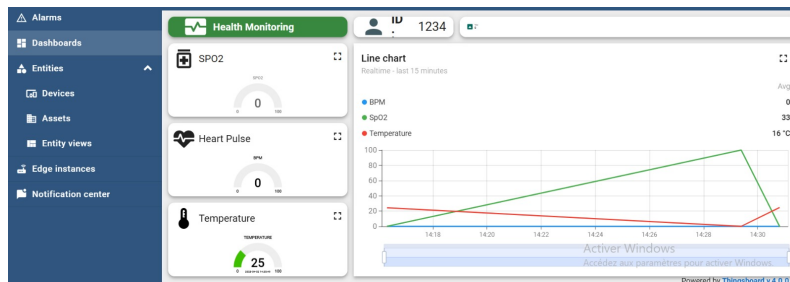


Fig. 4 ThingsBoard patient-monitoring dashboard: live vital-sign widgets and a rolling 15-minute line chart.

4.3 Why MQTT

MQTT’s fixed binary header (as small as 2 bytes) is an order of magnitude smaller than HTTP’s textual headers, and its publish/subscribe model avoids the round-trip overhead of polling-based protocols [7]. Quality-of-Service level 1 (“at least once”)

is used for telemetry publishing, giving guaranteed delivery without the duplicate-suppression overhead of level 2.

4.4 Topic Hierarchy

Two MQTT paths are used in the system: the firmware publishes combined telemetry to ThingsBoard’s fixed ingestion topic (`v1/devices/me/telemetry`, Listing 2); a second, per-vital topic hierarchy on a public HiveMQ broker is used by the companion Android application (Fig. 5, Sect. 5):

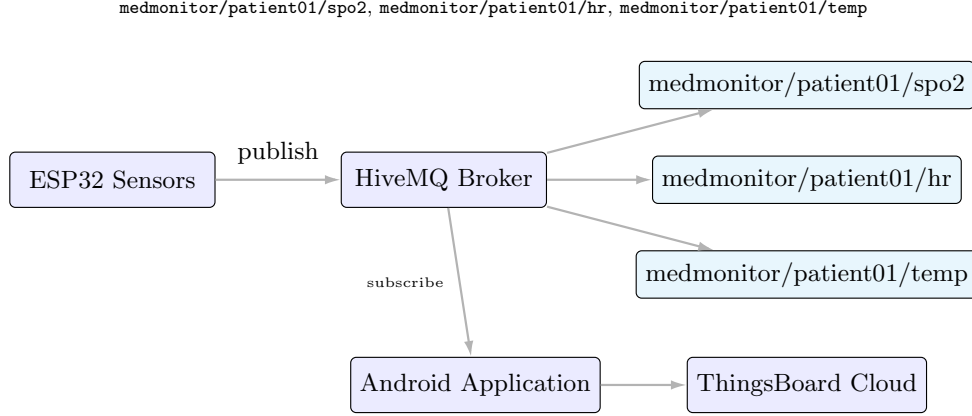


Fig. 5 MQTT topic hierarchy for the Android companion application: per-vital topics on a HiveMQ broker, subscribed to by the mobile app.

5 Mobile Application

An Android companion application is under development as the primary patient/clinician interface (Fig. 6). Planned features are: real-time vital-sign cards, a rolling historical chart, threshold-based colour-coded alerts ($\text{SpO}_2 < 90\%$, heart rate > 100 bpm, ambient temperature $> 38^\circ\text{C}$), and multi-patient profile switching. The application subscribes to the per-vital HiveMQ topics of Fig. 5; during development, the broker’s web console confirmed three active topic subscriptions corresponding to the SpO_2 , heart-rate, and temperature topics.

6 Discussion

Relative to the baseline of Gupta et al. [1] (Table 1), the prototype replaces an 8-bit microcontroller with an integrated-wireless 32-bit dual-core ESP32, replaces analogue LM35 thermometry with a digital DS18B20 probe removing ADC quantisation noise, and replaces unencrypted HTTP polling to a proprietary cloud service with MQTT publishing to an open-source dashboard. The on-device patient-login menu adds a basic access-control step absent from the baseline description.

Limitations. (i) No clinical or statistical validation of measurement accuracy against a reference instrument has been performed; the system has been exercised on a single

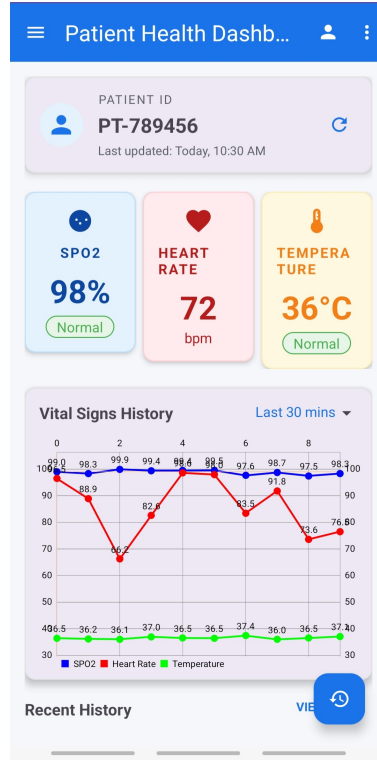


Fig. 6 Android application interface: vital-sign cards and a 30-minute history chart, captured live during a test session.

benchtop prototype. (ii) The demonstrated MQTT link uses the broker’s default unencrypted port for development, not the TLS listener intended for production. (iii) Blood-pressure sensing hardware is present on the board design but not yet integrated into the firmware. (iv) The Android application has been exercised with live sensor data during development but has not undergone formal usability evaluation with patients or clinicians.

7 Future Perspectives

Near-term work includes: (i) clinical validation trials against a reference vital-signs monitor at partner hospitals; (ii) TLS-secured production MQTT deployment (broker port 8883) with the same token-based device authentication; (iii) blood-pressure module integration (HX711 load-cell front end) to complete the sensor set; (iv) portable ECG integration (AD8232 module); (v) non-invasive glucose monitoring; (vi) predictive machine-learning models trained on longitudinal vital-sign data to forecast patient-specific health-risk trajectories, extending the current threshold-based anomaly detection; (vii) additional physiological and environmental sensors (e.g., accelerometer-based activity/fall detection and ambient humidity) to broaden the monitored parameter set; (viii) migration from the current breadboard prototype to

a custom printed-circuit board, reducing per-unit cost and power consumption for a battery-optimised, mass-producible device; and (ix) a voice interface.

8 Conclusion

This paper presented an IoT-based healthcare monitoring prototype for obese adults that improves on the platform of Gupta et al. [1] through: (i) MQTT-based telemetry in place of unencrypted HTTP polling; (ii) high-accuracy digital ambient-temperature sensing (DS18B20, ± 0.1 °C); (iii) a patient-authenticated on-device interface feeding a JSON telemetry pipeline to an open-source cloud dashboard; and (iv) a concept design for a multi-patient mobile dashboard with threshold-based alerting. Clinical validation of measurement accuracy, TLS-secured production deployment, and blood-pressure sensing integration are identified as near-term future work.

Declarations

- Funding: Not applicable.
- Conflict of interest/Competing interests: The authors declare no competing interests.
- Ethics approval and consent to participate: Not applicable; the study did not involve experiments on live vertebrates, higher invertebrates, human participants, or human samples.
- Consent for publication: The individuals appearing in device photographs are members of the author team and have consented to the use of these images.
- Data availability: Not applicable.
- Materials availability: Not applicable.
- Code availability: The ESP32 firmware source is available from the corresponding author upon reasonable request.
- Author contribution: L.A., M.S., N.B., and M.D. carried out the hardware design, firmware development, and cloud integration; H.O. supervised the project and reviewed the manuscript. All authors read and approved the final manuscript.

References

- [1] Gupta, D., Parikh, A., Swarnalatha, R.: Integrated healthcare monitoring device for obese adults using Internet of Things (IoT). *Int. J. Electr. Comput. Eng.* **10**(2), 1239–1247 (2020). <https://doi.org/10.11591/ijece.v10i2.pp1239-1247>
- [2] World Health Organization: Obesity and overweight fact sheet. WHO Press, Geneva (2023). <https://www.who.int/news-room/fact-sheets/detail/obesity-and-overweight>
- [3] ThingsBoard Inc.: ThingsBoard Community Edition Documentation. <https://thingsboard.io/docs/>

- [4] Espressif Systems: ESP32-WROOM-32D Datasheet. Espressif Systems, Shanghai (2023). https://www.espressif.com/sites/default/files/documentation/esp32-wroom-32d_esp32-wroom-32u_datasheet_en.pdf
- [5] Analog Devices (Maxim Integrated): MAX30102 High-Sensitivity Pulse Oximeter and Heart-Rate Sensor Datasheet (Rev. 1, 2018). <https://www.analog.com/media/en/technical-documentation/data-sheets/max30102.pdf>
- [6] Analog Devices (Maxim Integrated): DS18B20 Programmable Resolution 1-Wire Digital Thermometer Datasheet (2019). <https://www.analog.com/media/en/technical-documentation/data-sheets/ds18b20.pdf>
- [7] OASIS: MQTT Version 3.1.1 Specification. OASIS Standard (2014). <https://docs.oasis-open.org/mqtt/mqtt/v3.1.1/>