




a B3LYP: raw spectrum vs HPLC shape (calibration target)
calibrated shift $dE = +0.043 \pm 0.008$ eV

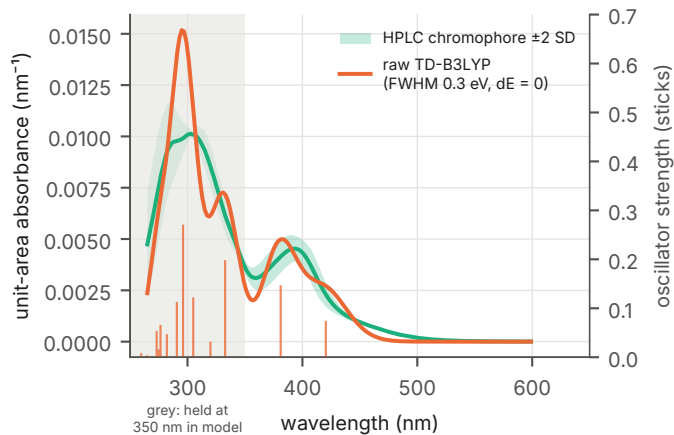

b CAM-B3LYP: raw spectrum vs HPLC shape (calibration target)
calibrated shift $dE = -0.786 \pm 0.019$ eV

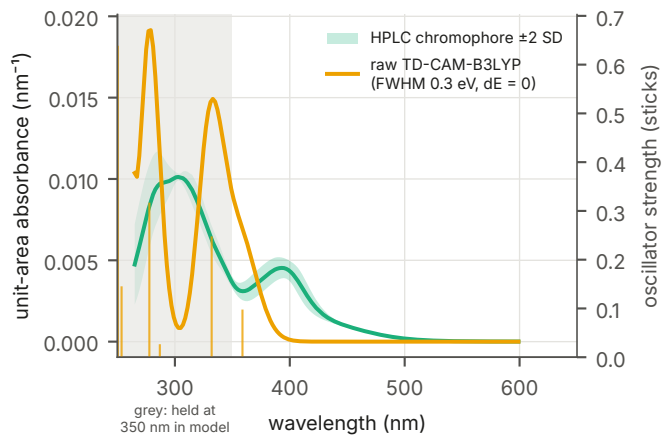

c Calibrated MAC vs extract (both fitted to it; not validation)

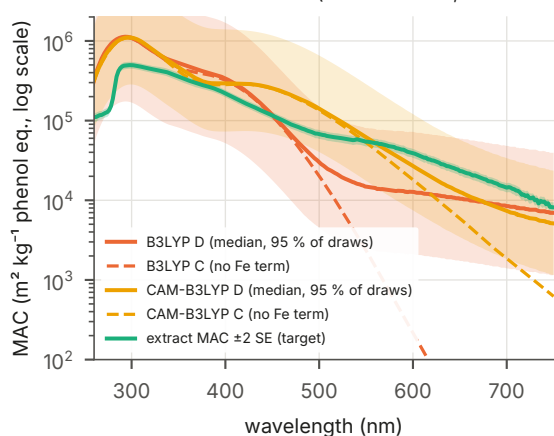

d The calibration absorbs a 0.8 eV functional error

