Healthcare Robot

Ayushi Gupta, Rahul Bansal, Utkarsh Singh
Department of Instrumentation & Control Engineering
JSS Academy Of Technical Education Noida

Abstract-- In this project we describe the design of a Healthcare Robot. Healthcare Robot is used to monitor patients without any physical contact of medical health care staff. Robots have the capability to move at every surface with controllable speed and self-containing light.

Health monitoring system is mounted on a bot which is able to measure oxygen level, beat per minute and temperature and transfer the data on the web.

Bot capable of sending continuous video streaming on the web and through which we can control bot accordingly

I. INTRODUCTION

The main purpose of this paper is to design the prototype of a health care bot used in the medical field. This project presents a healthcare robot that consists of four wheels around the body and a health monitoring system which will help the health care workers to examine a particular patient without having a physical contact. Robots will serve as a platform where we can add different sensor components that can be programmed to perform complex actions like temperature, heartbeat, oxygen level measurement.

Robot consist of a healthcare system mounted on top of a robot which measures beat per minute, oxygen percentage and temperature with sensors and reflect all the data to the web with the help of a microcontroller. A continuous steaming of the location of the robot is displayed on the web with the help of ESP32 cam and this also helps in controlling the robot accordingly.

Main purpose for representing this healthcare robot is to save the life of those who are acting like a god nowadays.

Moving Robots serves different tasks and uses in the health care sectors with in the conventional methods and scope of surgical and surveillance and robots are designed to become one of the most important scientific and technological innovations and advancement of the century. In this project a brief comprehensive overview of most of the readily potential uses and applications of robotics in healthcare amidst this corona virus and pandemic situation.

II. WORKING

In working of healthcare robot, the camera of esp32 records the live streaming and this streaming goes to the microcontroller and microcontroller sends this value to the web through wifi and this controls the bot from web page and sensor senses the value of temperature, beat per minute and oxygen level according deflect on blink app and the value of sensors and monitors the patients can be recorded.
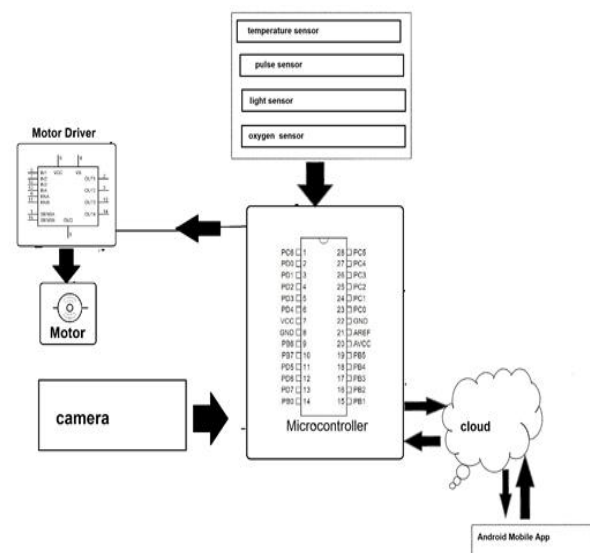

Figure 1. Healthcare Robot Working

the steaming of camera is recorded on web page just below that there are some buttons that control health care robot motion, also there are two sliders to control light and motor speed of the robot. Parallelly the value of the sensor is recorded. There are four gauges (room temperature, BPM, oxygen level and body temperature). It consists of some sensor, motor controller, camera, microcontroller, web for perform this functionality Let's discuss about each component of. Temperature sensor and oximeter fetch the information deflects it's on blink app with the help of microcontroller (ESP8266) and video and control the health robot with the help of ESP32 cam has fetched.
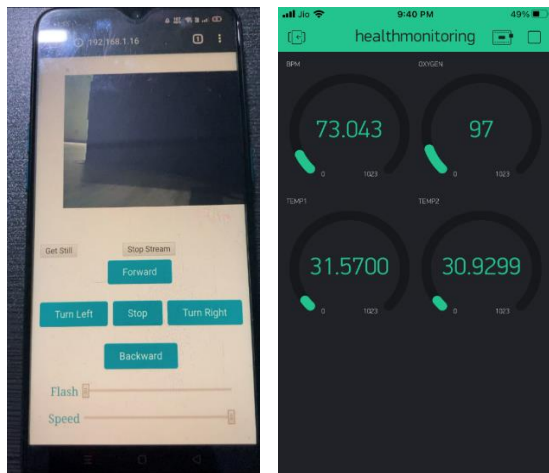
Figure 2. Web Page Of Healthcare Robot

III. FLOW DIAGRAM

A. Robot Controlling

Start give command from smart phone if moving command is received the it will act according to command and stop. If no command received the program stop.

Esp32 cam which give us platform to control healthcare robot. In this project, a web page on which we are getting video steaming and there are some buttons to control the movement of healthcare robot. Command is given with the help of web page through Wi-Fi we get that command and according to that esp32 give command to motor controller.
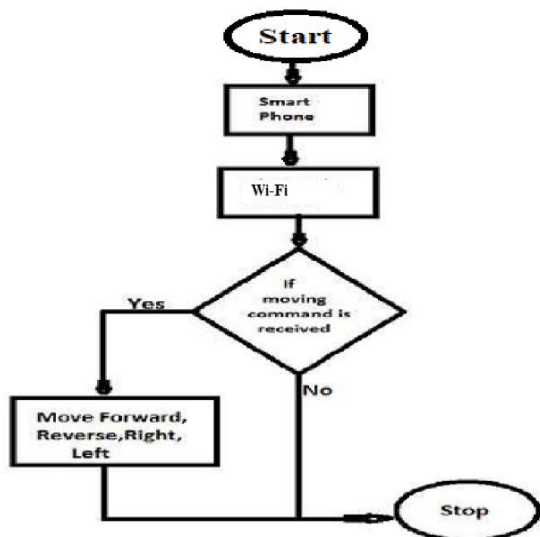

Figure 3. Flow Diagram Of Robot Controlling

B. Health Monitoring System

Start and sensor went into the continuous and read the value. After fetching the information, it will display and went again in continuous loop and exit.

Temperature sensor and oximeter sense the value of temperature, oxygen percent and BPM and the value is fetched by nodemcu8266 and with the help of Wi-Fi the value is send to the blink app.
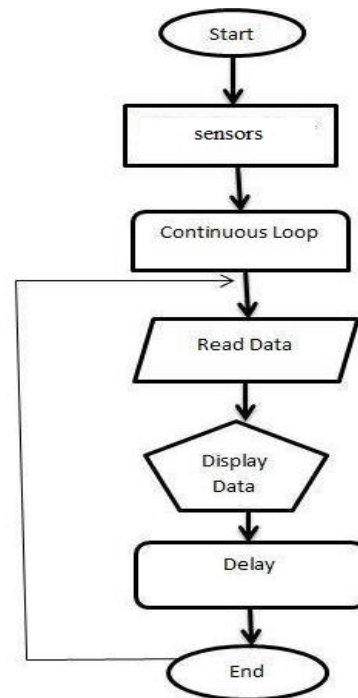

Figure 4. Health Monitoring System Flow Diagram

IV CONCLUSION

This project presents a robot and mount a health monitoring system which will help the health care workers to examine a particular patient without having a physical contact.

Communicable disease can be transmitted to health care workers and also between patients reducing contact help in solving these issues.

V FUTURE ENHANCEMEN

By using new features, health care robots are expected to increase quality, efficiency, accuracy, and safety in the delivery of health services. AI development will provide a new feature in robotics. As expected, the combination of artificial intelligence and robots will make operation faster and more secure. Apart from this, data analytics, development of hardware and software programs will differentiate the range of robots in other healthcare fields. Investment and partnerships between robotic companies and healthcare providers will improve the Healthcare robotics market. However, the cost of robots and the ability to pay for the average person will remain important challenges to deal with.

REFERENCES

[1] H. Nguyen, A. Jain, C. Anderson and C. C. Kemp, "A clickable world: Behavior selection through pointing and context for mobile manipulation", *2008 IEEE/RSJ International Conference on Intelligent Robots and Systems*, pp. 787-793, Sept. 2008.

[2] L. Jackel, E. Krotkov, M. Perschbacher, J. Pippine, no C. Sullivan, "IDARPA LAGR Program: Goals, challenges, performance, and outcomes of phase I, "*Field Robotics Journal vol. 23, no. 11-12, pp. 945-973, 2006.*

[3] H. Admoni, T. Weng and B. Scassellati, "Modeling communicative behaviors for object References in human-robot interaction", 2016 IEEE International Conference on Robotics and Automation (ICRA), pp. 3352-3359, May 2016.

[4] A. D. Dragan, K. C. T. Lee and S. S. Srinivasa, "Legibility and predictability of robot motion", *2013 8th ACM/IEEE International Conference on Human-Robot Interaction (HRI)*, pp. 301-308, Mar. 2013.

[5]Chàvez-Clemente, D. Gait ""Optimization for Multi-legged Walking Robots, with Application to a Lunar Hexapod."" *Ph.D. Thesis, Stanford University, California, CA, USA*, 2011.

[6] Jun, B.H.; Shim, H, Kim, B,Park, J.Y, Baek, H,Yoo, S Lee, P.M.'' Development of seabed walking robot CR200". *In Proceedings of the OCEANS'13 MTS/IEEE of the Conference, San Diego, CA, USA, 23–26 September 2013*; pp. 1–5.

[7] Bares, J., Hebert, M., Kanade, T., Krotkov, E., Mitchell, T., Simmons, R, Whittaker, W. Ambler: "An autonomous rover for planetary exploration*". IEEE Comput. 1989*, 26, 6–18.

[8] G. A. Lynch, L. Rome, and D. E. Koditschek, "Sprawl angle in simplified models of ver- overgrowth: the meaning of robots and roaches, "*at the International Conference on AppliedBionics and Biomechanics, Venice, Italy*, 2010.

[9] J. Hollerbach, I. Hunter, and J. Ballantyne, "Comparative Analysis of actuator technologies-gies for robotics, "*in A Review of Robots 2. MIT Press,* 1992, p. 342.

[10] Concepts of efficiency and economy in global locomotion, pages 97-131

[11] R. Kornbluh, R. Pelrine, J. Eckerle, and J.Joseph,cle actuators, "in Proceedings of the IEEE International Conference on Robotics and Automation

[12] Anwar Islam and Tuhin Biswas, "Health System in Bangladesh: Challenges and Opportunities", *American Journal of Health Research*, vol. 2, no. 6, pp. 366-374, 2014.

[13] M.E. Hoff, "Single-Chip N-Mos Microcomputer Processes Signals in Real Time", *Electronics*, pp. 105-110, March 1979.

[14] S. Ouma and M. E. Herselman, "E-health in rural areas: Case of developing countries", *International Journal of Biological and Life Sciences*, vol. 4, no. 4, pp. 194-200, 2008.

[15] K. Romer, B. Ostermaier, F. Mattern, M. Fahrmair and W. Kellerer, "Real-time search for real-world entities: A survey", *Proc. IEEE*, vol. 98, no. 11, pp. 1887-1902, Nov. 2010.