


Natural class distribution of the 60-second slice
volumetric DoS 87.26%, benign 7.42%, brute force 5.32%

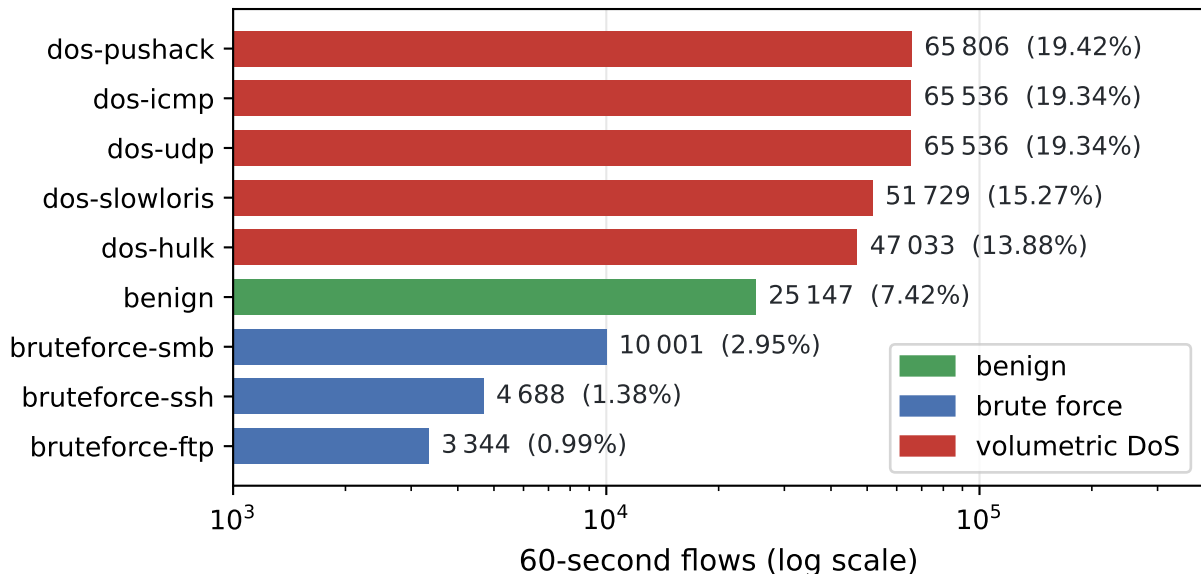

The 20% test partition holds 5 030 benign flows, so a single false positive is 0.0199 percentage points, and every false-positive rate reported in this paper is an integer multiple of that step.