


Detection F_1 of every full-montage electrode operating as its own self-contained detector

Frontal Central Parietal Occipital

Internal

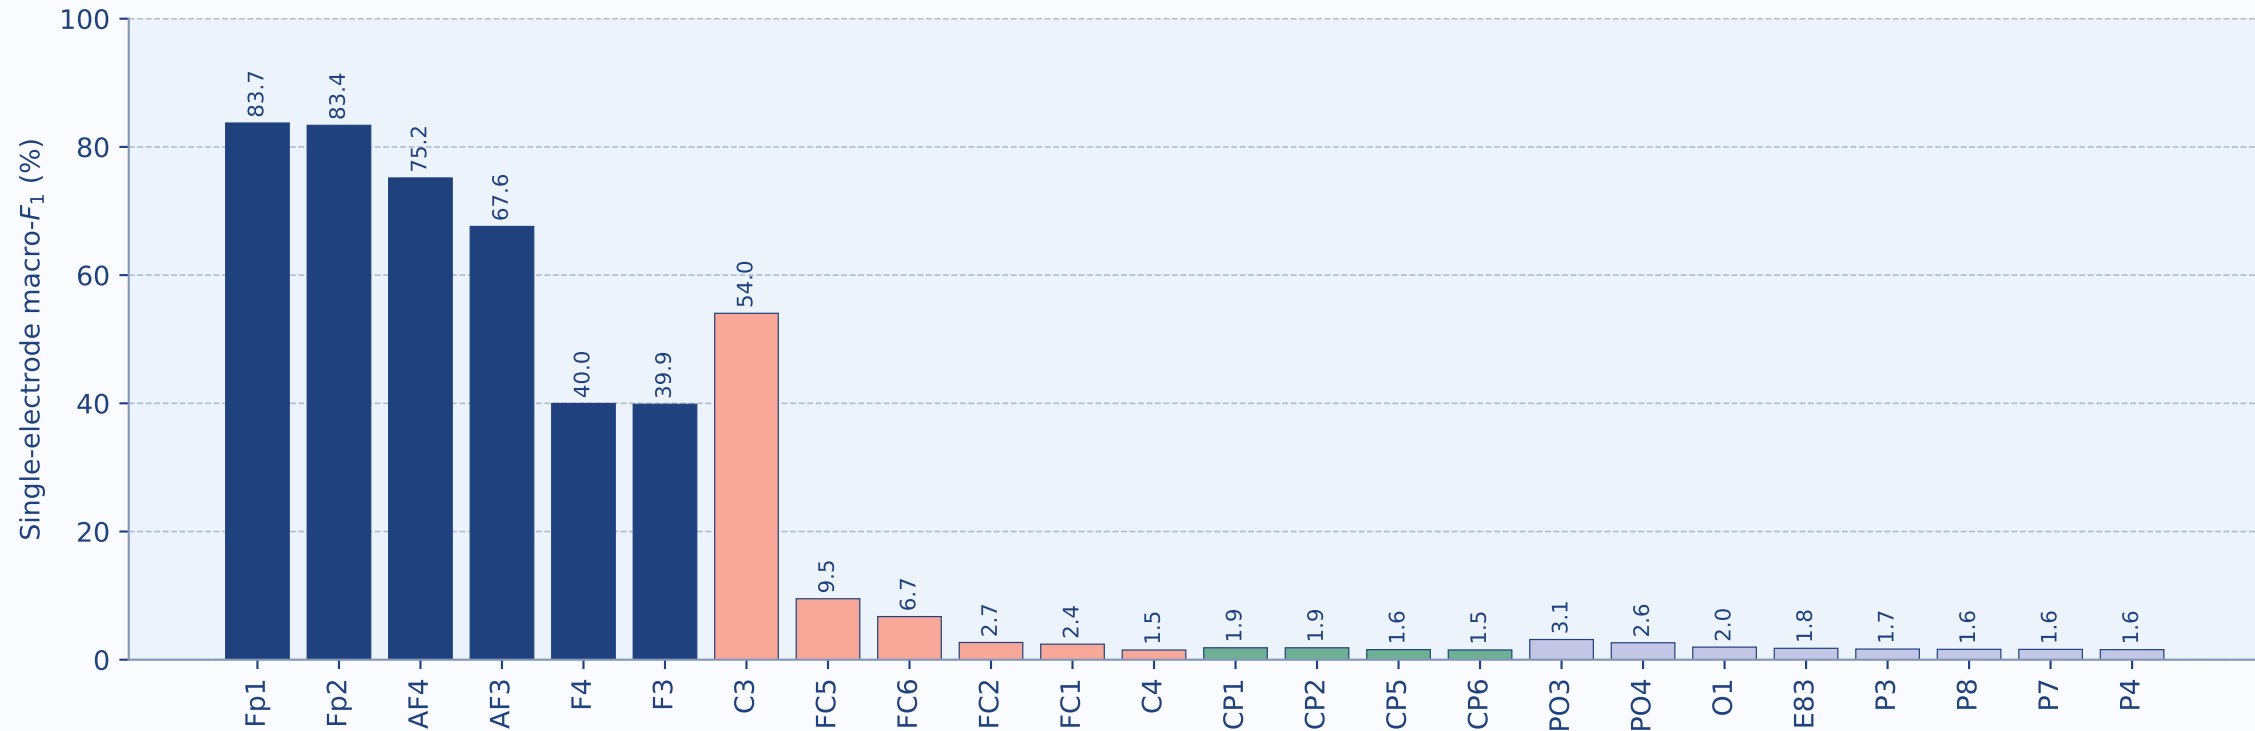

Cao2018

