

¹ A new angle on light-sheet microscopy
² and real-time image processing

³

Bálint Balázs

⁴



⁵

Pázmány Péter Catholic University

⁶

Faculty of Information Technology and Bionics

⁷

Roska Tamás Doctoral School of Sciences and Technology

⁸

Advisor: Balázs Rózsa, *M.D., Ph.D.*

⁹

A thesis submitted for the degree of

¹⁰

Doctor of Philosophy

¹¹

2017

¹ Abstract

² Light-sheet fluorescence microscopy, also called single plane illumination microscopy, has
³ numerously proven its usefulness for long term imaging of embryonic development. This
⁴ thesis tackles two challenges of light-sheet microscopy: high resolution isotropic imaging
⁵ of delicate, light-sensitive samples, and real-time image processing and compression of
⁶ light-sheet microscopy images.

⁷ A symmetric light-sheet microscope is presented, featuring two high numerical aperture
⁸ objectives arranged in 120°. Both objectives are capable of illuminating the sample
⁹ with a tilted light-sheet and detecting the fluorescence signal. This configuration allows
¹⁰ for multi-view, isotropic imaging of delicate samples where rotation is not possible. The
¹¹ optical properties of the microscope are characterized, and its imaging capabilities are
¹² demonstrated on *Drosophila melanogaster* embryos and mouse zygotes.

¹³ To address the big data problem of light-sheet microscopy, a real-time, GPU-based
¹⁴ image processing pipeline is presented. Alongside its capability of performing commonly
¹⁵ required preprocessing tasks, such as image fusion of opposing views immediately during
¹⁶ image acquisition, it also contains a novel, high-speed image compression method. This
¹⁷ algorithm is suitable for both lossless and noise-dependent lossy image compression, the
¹⁸ latter allowing for a significantly increased compression ratio, without affecting the results
¹⁹ of any further analysis. A detailed performance analysis is presented of the different
²⁰ compression modes for various biological samples and imaging modalities.

¹ Contents

² Abstract	ⁱⁱ
³ List of Figures	^{vi}
⁴ List of Tables	^{vii}
⁵ List of Abbreviations	^{viii}
⁶ Introduction	^x
⁷ 1 Live imaging in three dimensions	¹
⁸ 1.1 Wide-field fluorescence microscopy	²
⁹ 1.2 Point scanning methods	⁸
¹⁰ 1.3 Light-sheet microscopy	¹²
¹¹ 1.4 Light-sheet microscopy for mouse imaging	¹⁹
¹² 2 Image compression	²⁶
¹³ 2.1 Basics of information theory	²⁶
¹⁴ 2.2 Entropy coding	²⁷
¹⁵ 2.3 Decorrelation	³¹
¹⁶ 3 Dual Mouse-SPIM	³⁵
¹⁷ 3.1 Microscope design concept	³⁶
¹⁸ 3.2 Optical layout	³⁹
¹⁹ 3.3 Optical alignment	⁴³
²⁰ 3.4 Control unit	⁴⁸
²¹ 3.5 Results	⁵¹
²² 3.6 Methods	⁵⁸
²³ 3.7 Conclusions	⁶⁰

1	4 GPU accelerated image processing and compression	61
2	4.1 Challenges in data handling for light-sheet microscopy	61
3	4.2 Real-time preprocessing pipeline	62
4	4.3 B ³ D image compression	71
5	4.4 Conclusions	83
6	5 Discussion	84
7	5.1 New scientific results	84
8	5.2 Application of the results	86
9	Appendix	88
10	A Bill of materials	88
11	B Supplementary Tables	90
12	C Light collection efficiency of an objective	92
13	D 3D model of Dual Mouse-SPIM	93
14	References	95
15	Acknowledgements	107

¹ List of Figures

2	1.1	Tradeoffs in fluorescence microscopy for live imaging	1
3	1.2	Excitation and emission spectrum of enhanced green fluorescent protein (EGFP)	2
4	1.3	Wide-field fluorescence microscope	4
5	1.4	Axial cross section of the PSF and OTF of a wide-field microscope	6
6	1.5	Airy pattern	7
7	1.6	Resolution of a wide-field microscope	9
8	1.7	Basic optical components of a confocal laser scanning and confocal-theta microscope	10
9	1.8	Axial cross section of the PSF and OTF of a confocal laser scanning mi- croscope	11
10	1.9	Basic concept of single-plane illumination microscopy	12
11	1.10	Different optical arrangements for light-sheet microscopy	14
12	1.11	Basic optical components of a SPIM	15
13	1.12	Light-sheet dimensions	17
14	1.13	DSLM illumination	19
15	1.14	Inverted light-sheet microscope for multiple early mouse embryo imaging.	21
16	1.15	Imaging mouse post-implantation development	23
17	1.16	Imaging adult mouse brain with light-sheet microscopy.	24
18	2.1	Building the binary Huffman tree	30
19	2.2	Context for pixel prediction	33
20	3.1	Dual view concept with high NA objectives	36
21	3.2	Lateral and axial resolution of a multi-view optical system.	38
22	3.3	The core unit of the microscope	40
23	3.4	Illumination branch splitting unit	42
24	3.5	Dual Mouse SPIM optical layout	44
25	3.6	Detection branch switching unit	45
26	3.7	Microscope control hardware and software architecture	49

LIST OF FIGURES

1	3.8	Digital and analog control signals	50
2	3.9	Completed DualMouse-SPIM	52
3	3.10	Stability measurements of view switcher unit	53
4	3.11	Illumination beam profile	54
5	3.12	Simulated and measured PSF of Dual Mouse-SPIM	55
6	3.13	Combined PSF of 2 views	56
7	3.14	Maximum intensity projection of a <i>Drosophila melanogaster</i> embryo recording	57
8	3.15	Multi-view recording of a mouse zygote	58
10	4.1	Experiment sizes and data rate of different imaging modalities	62
11	4.2	Real-time image processing pipeline for multi-view light-sheet microscopy	62
12	4.3	Operating principle of MuVi-SPIM	63
13	4.4	Multi-view fusion methods for light-sheet microscopy	65
14	4.5	Classes of LVCUDA library	66
15	4.6	Applying mask to remove background	68
16	4.7	Comparison of 3D and 2D fusion of beads	68
17	4.8	GPU fused images of a <i>Drosophila melanogaster</i> embryo	69
18	4.9	Image contrast depending on z position for raw and fused stacks	70
19	4.10	B ³ D algorithm schematics	73
20	4.11	Options for noise dependent lossy compression	75
21	4.12	Theoretical and measured increase in image noise for WNL compression	76
22	4.13	Compression performance	77
23	4.14	Image quality of a WNL compressed dataset	77
24	4.15	Compression error compared to image noise	78
25	4.16	Influence of noise dependent lossy compression on 3D nucleus segmentation	79
26	4.17	Influence of noise dependent lossy compression on 3D membrane segmentation	79
28	4.18	Influence of noise dependent lossy compression on single-molecule localization	80
30	4.19	Change in localization error only depends on selected quantization step	80
31	C1	Light collection efficiency of an objective	92
32	D1	3D model of DualMouse-SPIM	94

¹ List of Tables

²	2.1 Examples of a random binary code (#1) and a prefix-free binary code (#2)	28
³	2.2 Letters to be Huffman coded and their probabilities	29
⁴	2.3 Huffman code table	30
⁵	B1 Data sizes in microscopy	90
⁶	B2 Lossless compression performance	90
⁷	B3 Datasets used for benchmarking compression performance	91
⁸		

¹ List of Abbreviations

- ² **2D** two-dimensional.
- ³ **3D** three-dimensional.
- ⁴ **BFP** back focal plane.
- ⁵ **CCD** charge coupled device.
- ⁶ **CLSM** confocal laser scanning microscopy.
- ⁷ **CMOS** complementary metal oxide semiconductor.
- ⁸ **CPU** central processing unit.
- ⁹ **DCT** discrete cosine transform.
- ¹⁰ **DFT** discrete fourier transform.
- ¹¹ **DPCM** differential pulse code modulation.
- ¹² **DSLM** digitally scanned light-sheet microscopy.
- ¹³ **dSTORM** direct stochastic optical reconstruction microscopy.
- ¹⁴ **DWT** discrete wavelet transform.
- ¹⁵ **eCSD** electronic confocal slit detection.
- ¹⁶ **EM-CCD** electron multiplying CCD.
- ¹⁷ **FEP** fluorinated ethylene propylene.
- ¹⁸ **FN** field number.
- ¹⁹ **FOV** field of view.
- ²⁰ **FPGA** field programmable gate array.
- ²¹ **fps** frames per second.
- ²² **FWHM** full width at half maximum.
- ²³ **GFP** green fluorescent protein.
- ²⁴ **GPU** graphics processing unit.
- ²⁵ **HEVC** high efficiency video codec.
- ²⁶ **ICM** inner cell mass.

- ¹ **JPEG** joint photographic experts group.
- ² **LSFM** light-sheet fluorescence microscopy.
- ³ **MIAM** multi-imaging axis microscopy.
- ⁴ **MuVi-SPIM** Multiview SPIM.
- ⁵ **NA** numerical aperture.
- ⁶ **OPFOS** orthogonal plane fluorescent optical sectioning.
- ⁷ **OTF** optical transfer function.
- ⁸ **PEEK** polyether ether ketone.
- ⁹ **PSF** point spread function.
- ¹⁰ **RESOLFT** reversible saturable optical fluorescence transitions.
- ¹¹ **ROI** region of interest.
- ¹² **sCMOS** scientific CMOS.
- ¹³ **SMLM** single molecule localization microscopy.
- ¹⁴ **SNR** signal-to-noise ratio.
- ¹⁵ **SPIM** single plane illumination microscopy.
- ¹⁶ **STED** Stimulated Emission Depletion.
- ¹⁷ **TE** trophoectoderm.
- ¹⁸ **TLSM** thin light-sheet microscopy.
- ¹⁹ **WNL** within noise level.
- ²⁰ **YFP** yellow fluorescent protein.

¹ Introduction

2 Imaging techniques such as microscopy are one of the most extensively used tools in
3 medical and biological research. The reason for this is simple: visualizing something
4 invisible to the naked eye is an extremely powerful way to gain insight into its inner
5 workings. Our brain has evolved to receive and process a multitude of signals from
6 various sensors, and arguably the most powerful of these is vision.

7 As a branch of optics, microscopy (from ancient Greek *mikros*, “small” and *skopein*,
8 “to see”) is based on observing the interactions of light with an object of interest, such
9 as a cell. To be able to see these interactions, the optics of the microscope magnifies the
10 image of the sample, which can be recorded on a suitable device. For the first microscopes
11 in the 17th century, this was just an eye at the end of the ocular, and the recording was
12 a drawing of the observed image [1].

13 Microscopy is a truly multidisciplinary field: even in its simplest form, just using
14 a single lens, the principles of physics are applied to gain a deeper understanding of
15 biology and nature. Today, microscopy encompasses most of natural sciences and builds
16 on various technological advancements. While physics and biology are still in the main
17 focus, chemistry (fluorescent molecules), engineering (automation) and computer science
18 (image analysis) are all integrated in a modern microscopy environment.

19 Light-sheet fluorescence microscopy (LSFM), also called single plane illumination
20 microscopy (SPIM), is a relatively new addition to the arsenal of tools that comprise light
21 microscopy methods, and is especially suitable for live imaging of embryonic samples over
22 extended periods of time [2–5]. It is also easily adapted to the sample, allowing to image
23 a large variety of specimens, from entire organs [6], to the subcellular processes occurring
24 inside cultured cells [7].

25 This work tackles two challenges in light-sheet microscopy: high-resolution live imaging
26 of delicate samples, such as mouse embryos, and real-time image processing and
27 compression of large light-sheet datasets. Before discussing the work in detail, Chapter 1
28 and Chapter 2 will give a short introduction to the concepts this thesis builds on. The
29 basics of fluorescence microscopy, light-sheet microscopy, information theory and image
30 compression will be covered.

31 Chapter 3 is devoted to presenting a new light-sheet microscope, the Dual Mouse-

1 SPIM, designed for isotropic imaging of light-sensitive specimens. This microscope is
2 based on two identical objectives positioned in 120° as opposed to the conventional 90°
3 orientation used in light-sheet microscopy, and it offers dual-view detection through both
4 lenses. We discuss the benefits of this arrangement and the design principles and optical
5 layout of the microscope. After characterizing the optical properties of the microscope,
6 we demonstrate its imaging capabilities on various samples.

7 In Chapter 4 we present a GPU-based real-time image processing pipeline designed
8 to efficiently handle large amounts of microscopy data. As 3D imaging is gaining more
9 and more traction, image data is generated at a faster pace than ever. We present a
10 real-time preprocessing solution for multiview light-sheet microscopy, and a new image
11 compression algorithm to significantly reduce data size by taking image noise into ac-
12 count. The theory behind these methods will be discussed before demonstrating their
13 capabilities and evaluating their performance on multiple biological samples.

14 Finally, Chapter 5 will give a summary of the new results presented in this thesis,
15 and discuss the potential future applications.

¹ Chapter 1

² Live imaging in three dimensions

³ Live imaging is indispensable to understand the processes during embryonic development.
⁴ In an ideal setting, the ultimate microscope would be able to record a continuous, three
⁵ dimensional (3D), multicolor dataset of any biological process of interest with the highest
⁶ possible resolution. Due to several limitations in physics and biology this is not possible.
⁷ Therefore, a compromise is necessary. The diffractive nature of light, the lifetime of
⁸ fluorescent probes and the photosensitivity of biological specimens all require microscopy
⁹ to be able to adapt to answer the question at hand. In order to acquire useful data one
¹⁰ has to choose a tradeoff between spatial and temporal resolution and signal contrast,
¹¹ while making sure the biology is not affected by the imaging process itself (Figure 1.1)
¹² [8].

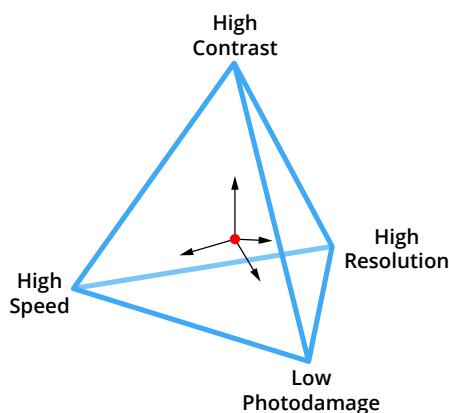


Figure 1.1: Tradeoffs in fluorescence microscopy for live imaging. Also called the “pyramid of frustration”. When optimizing the imaging conditions (red dot), a tradeoff has to be made between resolution, contrast, and imaging speed, while avoiding photodamage. One can only be improved at the expense of the others due to the limited photon budget of the fluorescent molecules. Adapted from [8].

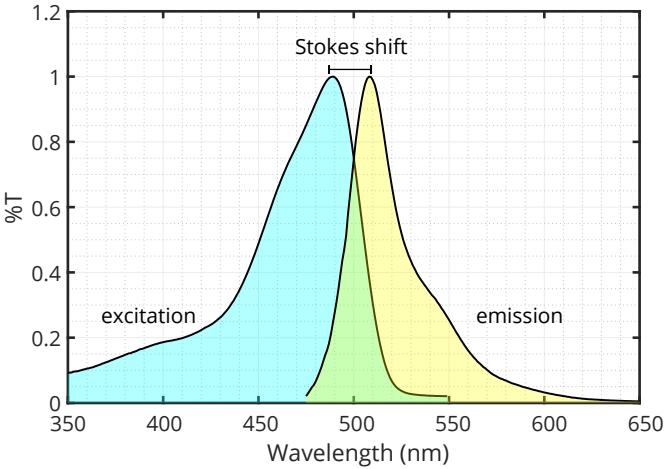


Figure 1.2: Excitation and emission spectrum of enhanced green fluorescent protein (EGFP). Excitation spectrum in blue, emission spectrum in yellow. The separation between the two spectra is due to the Stokes shift, which is 19 nm for EGFP. Emission and excitation light can be separated by a long-pass filter at 500 nm. Data from [12].

¹ 1.1 Wide-field fluorescence microscopy

² Fluorescence microscopy [9, 10], as a subset of light microscopy, is one of the few methods
³ that allow subcellular imaging of live specimens. The first use of the term fluorescence is
⁴ credited to George Gabriel Stokes [11], and it refers to the phenomenon of light emission
⁵ following the absorption of light or other electromagnetic radiation. As the name of
⁶ the technique suggests, this method collects fluorescent light from the specimens. Since
⁷ biological tissues are usually not fluorescent, except for some autofluorescence mostly at
⁸ shorter wavelengths, fluorescent dyes or proteins have to be introduced to the system in
⁹ order to be able to collect the necessary information. The advantage of this is that the
¹⁰ signal of the labeled structures will be of very high ratio compared to the background.

¹¹ A fluorescent molecule is capable of absorbing photons in a given wavelength range
¹² (excitation spectrum) and temporarily store its energy by having an electron in a higher
¹³ energy state, *i.e.*, in an excited state. This excited state, however, is not stable, and
¹⁴ the electron quickly returns to the ground state while emitting a photon with equal en-
¹⁵ ergy to the energy difference between the excited and ground states. The energy of the
¹⁶ absorbed and emitted photons are not the same, as energy loss occurs due to internal
¹⁷ relaxation events, and the emitted photon has lower energy than the absorbed photon.
¹⁸ This phenomenon is called the Stokes shift, or red shift, and can be exploited in mi-
¹⁹ croscopy to drastically increase the signal to noise ratio by filtering out the illumination
²⁰ light (Figure 1.2).

1.1.1 Fluorescent proteins

2 Traditionally, synthetic fluorescent dyes were used to label certain structures in the specimens.
3 Some of these directly bind to their target, and others can be used when conjugated
4 to an antibody specific to the structure of interest. A requirement for these methods is
5 that the fluorescent label has to be added to the sample from an external source, and, in
6 many cases, this also necessitates sample preparation techniques incompatible with live
7 imaging, such as fixation [13].

8 The discovery of fluorescent proteins has revolutionized fluorescence microscopy.
9 Since these molecules are proteins, they can be produced directly by the organism if
10 the proper genetic modifications are performed. Even though this was a hurdle at the
11 time of discovering the green fluorescent protein (GFP) [14], genetic engineering techniques
12 evolved since then [15], and not only has its gene been successfully integrated
13 in the genome of a multitude of organisms [16–18], but many variants have been also
14 engineered by introducing mutations to increase fluorescence intensity, and to change the
15 fluorescence spectrum to allow multicolor imaging [18–21]. The usefulness and impact of
16 these proteins are so profound, that in 2008 the Nobel Prize in chemistry was awarded to
17 Osamu Shimomura, Martin Chalfie, and Roger Tsien “for the discovery and development
18 of the green fluorescent protein, GFP” [22].

1.1.2 Wide-field image formation

20 By imaging fluorescently labelled specimens, a wide-field fluorescence microscope has the
21 capability of discriminating illumination light from emitted fluorescent light due to the
22 Stokes shift described in the previous section. The microscope’s operating principle is
23 depicted in Figure 1.3.

24 Light from a source, typically a mercury lamp is focused on the back focal plane of
25 the objective to create even illumination of the sample. Before entering the objective,
26 the light is filtered, so only the wavelengths that correspond to the excitation properties
27 of the observed fluorophores are transmitted. Since the same objective is used for both
28 illumination and detection, a dichroic mirror is utilized to decouple the illumination
29 and detection paths. The emitted light is filtered again to make sure any reflected and
30 scattered light from the illumination source is blocked to increase signal to noise ratio.
31 Finally, the light is focused by a tube lens to create a magnified image on the camera
32 sensor.

33 This type of imaging is called infinity corrected optics, since the back focal point of
34 the objective is in “infinity”, meaning that the light exiting the back aperture is parallel.
35 This is achieved by placing the sample exactly at the focal point of the objective. Infinity
36 corrected optics has the advantage that it allows placing various additional optical
37 elements in the infinity space (*i.e.* the space between the objective and the tube lens)

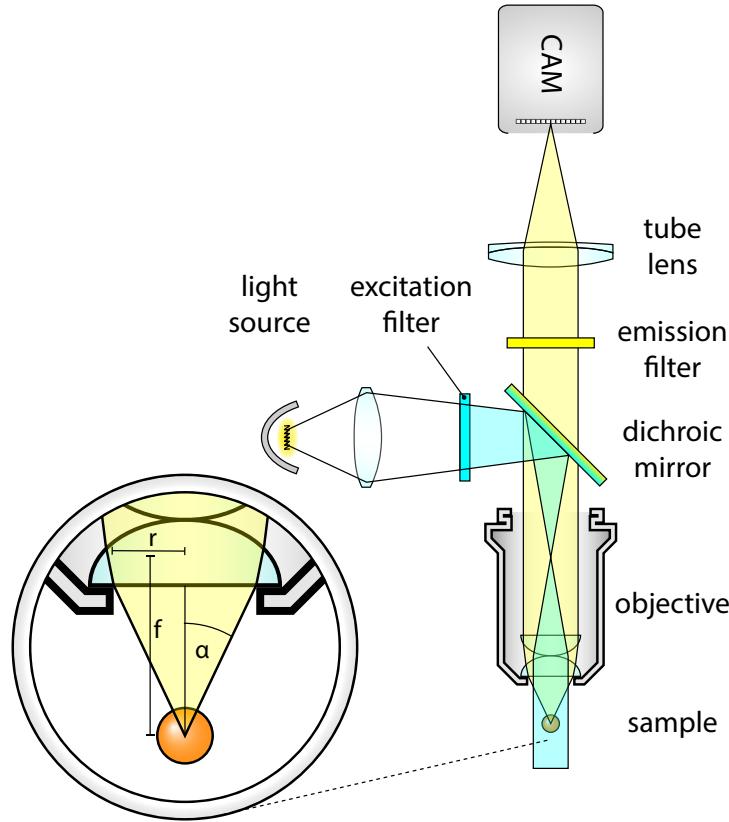


Figure 1.3: Wide-field fluorescence microscope. The light source is focused on the back focal plane of the objective to provide an even illumination to the sample. Emitted photons are collected by the objective, and are separated from the illumination light by a dichroic mirror. Inset: Light collection of an objective lens. α : light collection half-angle; f : focal length; r : radius of lens.

- 1 without affecting the image quality. In this example such elements are the dichroic mirror
- 2 and the emission filter.
- 3 The combination of the objective and tube lens together will determine the magnifi-
- 4 cation of the system, it will be the ratio of the focal lengths of these lenses:

$$M = \frac{f_{TL}}{f_{OBJ}}. \quad (1.1)$$

- 5 The final field of view (FOV) of the microscope will depend on the magnification, and
- 6 also on the size of the imaging sensor (D), and the objective field number (FN):

$$FOV = \frac{\min(D, FN)}{M}. \quad (1.2)$$

- 7 Apart from the magnification, the most important property of the objective is the
- 8 half-angle of the light acceptance cone, α (Figure 1.3, inset). This not only determines
- 9 the amount of collected light, but also the achievable resolution of the system (see Sec-
- 10 tion 1.1.3). This angle depends on the size of the lens relative to its focal length. In other

¹ words it depends on the aperture of the lens, which is why the expression *numerical*
² *aperture* (NA) is more commonly used to express this property of the objective:

$$NA = n \cdot \sin \alpha. \quad (1.3)$$

³ For small α angles, the following approximation holds true: $\sin \alpha \approx \tan \alpha \approx \alpha$. Thus,
⁴ the numerical aperture can also be expressed as a ratio of the radius of the lens and the
⁵ focal length:

$$NA \approx n \frac{r}{f}, \quad \text{when } \alpha \ll 1. \quad (1.4)$$

⁶ 1.1.3 Resolution of a wide-field microscope

⁷ The resolution of an optical systems is defined by the size of the smallest distinguishable
⁸ feature on the image. Practically this means the minimum distance between two point-
⁹ like objects so that the two objects can still be resolved. This mainly depends on two
¹⁰ factors: the NA of the objective, and the pixel size of the imaging sensor.

¹¹ Even if the imaging sensor would have infinitely fine resolution, it is not possible to
¹² reach arbitrarily high resolutions due to the wave nature of light and diffraction effects
¹³ that occur at the aperture of the objective. This means that depending on the wavelength
¹⁴ of the light, any point source will have a finite size on the image, it will be spread out,
¹⁵ limiting the resolution. The shape of this image is called the *point spread function*, or
¹⁶ PSF (Figure 1.4), as this function describes the behavior of the optical system when
¹⁷ imaging a point like source. This property of lenses was already discovered by Abbe in
¹⁸ 1873 [23], when he constructed his famous formula for resolution:

$$\delta = \frac{\lambda}{2 \cdot NA}. \quad (1.5)$$

¹⁹ where δ is the smallest distance between two distinguishable features.

²⁰ Another representation of the optical performance, is the *optical transfer function*,
²¹ or OTF (Figure 1.4), which is the Fourier transform of the PSF:

$$OTF = \mathcal{F}(\text{PSF}). \quad (1.6)$$

²² As this function operates in the frequency space, it describes how the different frequencies
²³ are affected by the system. The resolution can also be defined as the support of the OTF,
²⁴ since this describes the highest frequency that is still transmitted by the optical system.
²⁵ Any pattern with higher frequency will be lost, thus lies beyond the resolution limit. For
²⁶ circularly symmetric PSFs, the OTF will be real valued, however if this is not the case,
²⁷ the Fourier transform also introduces complex components.

²⁸ Abbe's formula can be derived from the scalar theory of diffraction using a paraxial

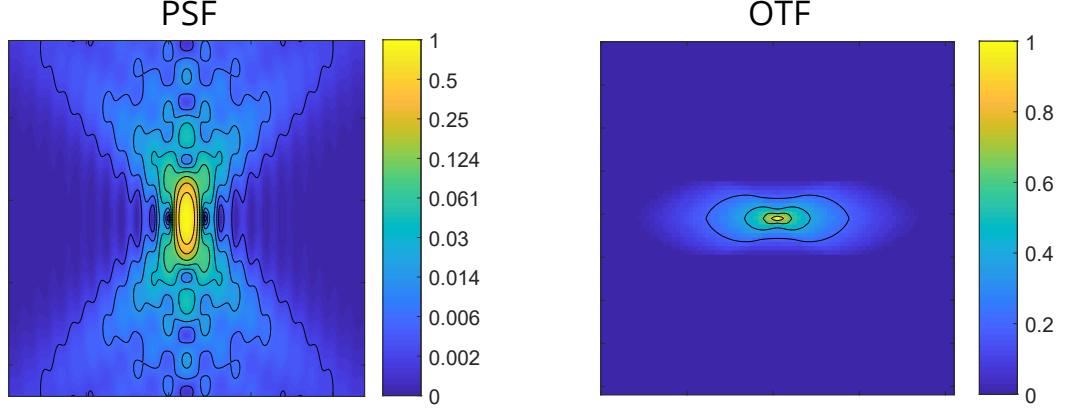


Figure 1.4: Axial cross section of the PSF and OTF of a wide-field microscope. Simulated PSF (left) and OTF (right) for a wide-field microscope with a water immersion objective ($n = 1.33$). $NA = 1.1$, $\lambda = 510 \text{ nm}$

1 approximation (Fraunhofer diffraction, [24]). It describes the intensity of the electric field
 2 in the focus of a lens [25]:

$$H(u, v) = C_0 \left| \int_0^1 J_0(vr) e^{-i\frac{1}{2} \cdot ur^2} r dr \right|^2, \quad (1.7)$$

3 where C_0 is a normalization constant, and J_0 is the zero order Bessel function of the first
 4 kind. Furthermore, instead of the commonly used Cartesian coordinates x , y and z , the
 5 following optical coordinates are defined:

$$v = \frac{2\pi nr}{\lambda_0} \sin \alpha, \quad u = \frac{8\pi nz}{\lambda_0} \sin^2 \frac{\alpha}{2} \quad (1.8)$$

6 where $r = \sqrt{x^2 + y^2}$ is the distance from the optical axis, and α is the light collection
 7 angle as shown on Figure 1.3.

8 To determine the lateral resolution of the system, let's substitute $u = 0$ as the axial
 9 optical coordinate, and evaluate Equation 1.7 which will give the intensity distribution
 10 in the focal plane:

$$H(0, v) = C_0 \left| \int_0^1 J_0(vr) r dr \right|^2 = \left(2 \frac{J_1(v)}{v} \right)^2, \quad (1.9)$$

11
 12 where J_1 is the first order Bessel function of the first kind. This equation describes the
 13 famous Airy pattern (Figure 1.5) which will be the shape of the PSF in the focal plane.
 14 The width of this pattern is the resolution, and although there are multiple definitions
 15 for this, the most commonly accepted is the Rayleigh criterion [24, 26] which defines

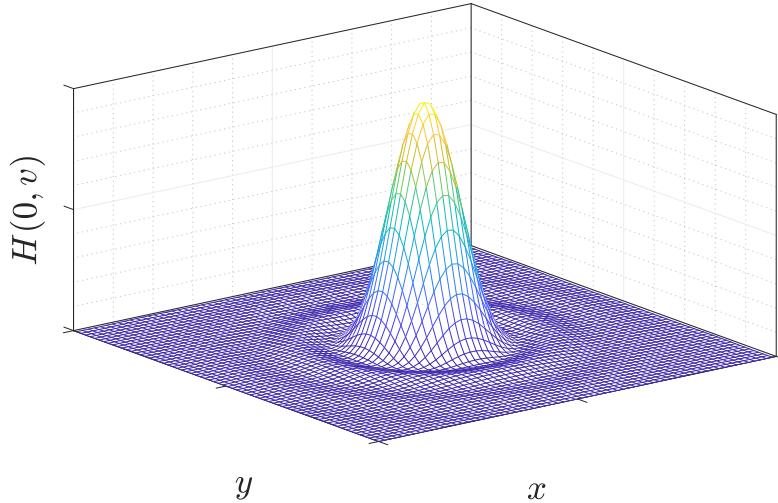


Figure 1.5: Airy pattern. Airy pattern calculated in Matlab based on Equation 1.9

- 1 the resolution as the distance between the central peak and the first local minimum.
- 2 As this lies at $v = 3.38$, the resolution can be expressed by substituting this value to
- 3 Equation 1.8 and solving it for r :

$$\delta_{xy} = r(v = 0.338) = \frac{3.83}{2\pi} \frac{\lambda_0}{n \cdot \sin \alpha} \approx 0.61 \frac{\lambda_0}{NA}, \quad (1.10)$$

- 4 which is equivalent to Abbe's original formula (Equation 1.5). The only difference is the
- 5 scaling factor which is due to the slightly different interpretations of width of the Airy
- 6 disk as mentioned earlier.

7 Similarly, to calculate the intensity distribution along the axial direction, let's sub-
8 stitute $v = 0$ to Equation 1.7:

$$H(u, 0) = C_0 \left(\frac{\sin \frac{u}{4}}{\frac{u}{4}} \right)^2. \quad (1.11)$$

- 9 For this expression the first minimum lies at $u = 4\pi$. Converting back to Cartesian
- 10 coordinates, the axial resolution can be expressed as:

$$\delta_z = \frac{2n\lambda_0}{NA^2}. \quad (1.12)$$

11 So far we only considered a single, point-like emitter. As the intensity function de-
12 scribes how an optical system “spreads out” the image of a point, it is also called the
13 Point Spread Function (PSF, Figure 1.4). In a more realistic scenario, however the emit-
14 ters are neither point-like, nor single. Effectively, however, for every emitter the PSF
15 would be imaged on the sensor, and this creates the final image. In mathematical terms,
16 this can be expressed as a convolution operation between the underlying fluorophore

1 distribution of the object (O) and the PSF (H):

$$I(u, v) = O(u, v) * H(u, v). \quad (1.13)$$

2 The effective result of this kind of diffraction limited image formation is a blurred
3 image with a finite resolution of δ_{xy} in the lateral direction, and δ_z in the axial direction.

4 The PSF is further affected by the illumination pattern as well. Since the number of
5 emitted fluorescent photons are roughly proportional to the illumination intensity, the
6 illumination pattern will have an effect on the overall PSF of the system, which can be
7 expressed as:

$$H_{sys} = H_{ill} \cdot H_{det}, \quad (1.14)$$

8 where H_{ill} is the point spread function of the illumination, and H_{det} is the point spread
9 function of the detection.

10 1.2 Point scanning methods

11 In most cases, a wide-field microscope is used to image a layer of cells, of a sectioned
12 sample, thus axial resolution is not a concern. Imaging live specimens, however is not
13 so straightforward, as these samples are usually much thicker than a typical section. For
14 these samples 3-dimensional (3D) imaging is highly beneficial, which necessitates some
15 kind of optical sectioning technique to be able to discriminate the features at different
16 depths.

17 Due to the design of the wide-field microscope, any photons emitted from outside the
18 focal plane will also be detected by the sensor, however as these are not originating from
19 the focus, only a blur will be visible. This blur potentially degrades image quality and
20 signal-to-noise ratio to such an extent that makes imaging thick samples very difficult if
21 not impossible in a wide-field microscope.

22 Evaluating Equations 1.10 and 1.12 for a range of possible numerical apertures reveals
23 the significant differences in lateral and axial resolution for any objective (Figure 1.6).
24 Especially for low NAs, this can be significant, a factor of ~ 20 difference. For higher
25 (>0.8) NAs the axial resolution increases faster than the lateral, however they will only
26 be equal when $\alpha = 180^\circ$. This means that isotropic resolution with a single lens is only
27 possible if the lens is collecting all light emitting from the sample, which seems hardly
28 possible, and would be highly impractical. For commonly used high NA objectives the
29 lateral to axial ratio will still be around 3–6.

30 Instead of using a single lens to achieve isotropic resolution, it is more practical to
31 image the sample from multiple directions to complement the missing information from
32 different views. When rotating the sample by 90° for example, the lateral direction of

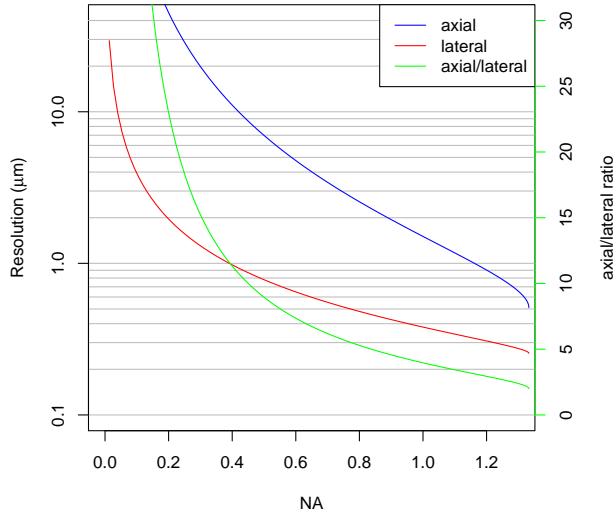


Figure 1.6: Resolution of a wide-field microscope. Axial (blue) and lateral (red) resolutions of a wide-field microscope are shown with respect to the numerical aperture (NA). Resolutions are calculated with $\lambda = 510\text{nm}$, the emission maximum of GFP and $n = 1.33$, the refractive index of water, for water dipping objectives.

the second view will correspond to the axial direction of the first view. If rotation is not possible, using multiple objectives can also achieve similar results, such as in the case of Multi-Imaging Axis Microscopy (MIAM) [27, 28]. This microscope consisted of 4 identical objectives arranged in a tetrahedral fashion to collect as much light as possible from multiple directions, and provide isotropic 3D resolution, albeit at the expense of extremely difficult sample handling, since the sample was surrounded by objectives from all directions.

1.2.1 Confocal laser scanning microscopy

Confocal laser scanning microscopy (CLSM) [29, 30] addresses most of the problems of wide-field microscopy we mentioned in the previous section. It is capable of optical sectioning by rejecting out of focus light, which makes it a true 3D imaging technique. Furthermore, the light rejection also massively reduces out of focus background, and increases contrast.

This is achieved by two significant modifications compared to the wide-field optical path. To be able to reject the out of focus light, an adjustable pinhole is placed at the focus of the tube lens. Light rays originating from the focal point will meet at this position, and are able to pass through the pinhole, however out-of-focus light will converge either before or after the aperture, and thus the aperture blocks these rays. To maximize the fluorescence readout efficiency for the single focal point, a photomultiplier tube is used

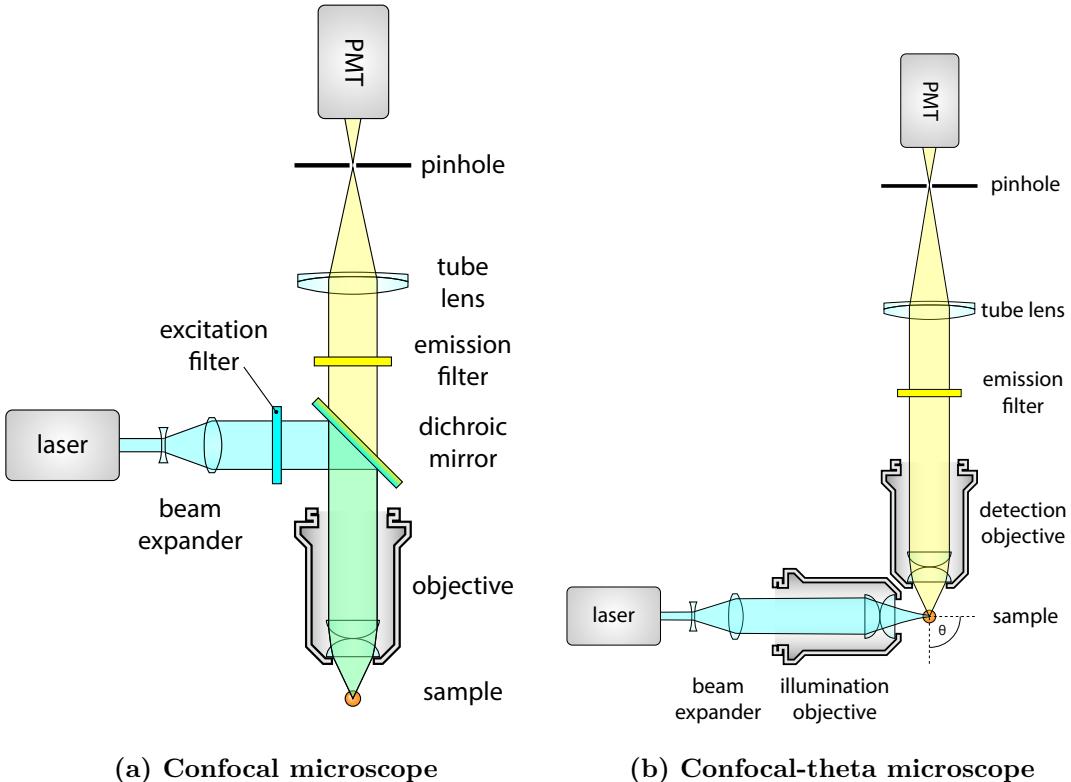


Figure 1.7: Basic optical components of a confocal laser scanning and confocal-theta microscope. Both types of microscopes use confocal image detection, which means that a pinhole is used to exclude light coming from out of focus points. Light intensity is measured by a photomultiplier for every point in the region of interest. The final image is generated on a computer using the positions and recorded intensity values. A regular confocal microscope (a) uses the same objective for illumination and detection, while a confocal-theta microscope (b) uses a second objective that is rotated by θ around the focus. In this case, $\theta = 90^\circ$.

- 1 instead of an area sensor (Figure 1.7a).
- 2 To maximize the signal from the focal point, the illumination light is also focused
- 3 here by coupling an expanded laser beam through the back aperture of the objective.
- 4 This not only increases illumination efficiency (since other, not detected points are not
- 5 illuminated), but has the added benefit of increasing the resolution as well. This is due
- 6 to the combined effect of illumination and detection PSFs as described in Equation 1.14
- 7 (Figure 1.8). For Gaussian-like PSFs, the final resolution (along a single direction) can
- 8 be calculated in the following way:

$$\frac{1}{\delta_{sys}^2} = \frac{1}{\delta_{ill}^2} + \frac{1}{\delta_{det}^2}, \quad (1.15)$$

- 9 where δ_{ill} and δ_{det} are the resolutions for the illumination and detection, respectively.
- 10 Since the same objective is used for both illumination and detection, and the difference

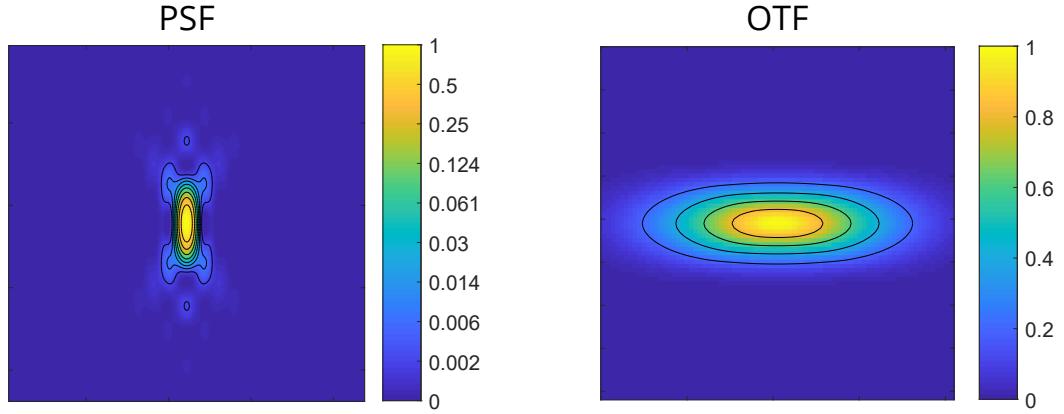


Figure 1.8: Axial cross section of the PSF and OTF of a confocal laser scanning microscope. Simulated PSF and OTF for a laser scanning confocal microscope with a water immersion objective ($n = 1.33$). $NA = 1.1$, $\lambda = 510 \text{ nm}$

1 in wavelength is almost negligible, $\delta_{ill} = \delta_{det} = \delta$, the final system resolution will be:

$$\delta_{sys} = \frac{1}{\sqrt{2}}\delta. \quad (1.16)$$

2 This means that the distinguishable features in a confocal microscope are ~ 0.7 times
3 smaller than in a wide-field microscope using the same objective.

4 Because of the different detection method in a confocal microscope, direct image
5 formation on an area sensor is not possible, since at any given time, only a single point is
6 interrogated in the sample. Instead, it is necessary to move the illumination and detection
7 point in synchrony (or in a simpler, albeit slower solution, to move the sample) to scan
8 the entire field of view. The image can be later computationally reconstructed by a
9 computer program that records the fluorescence intensity of every point of the field of
10 view, and displays these values as a raster image.

11 1.2.2 Confocal-theta microscopy

12 Although confocal microscopy already has 3D capabilities, its axial resolution is still
13 limited compared to the lateral, since it uses only one objective. An alternative realiza-
14 tion of the confocal microscope, the confocal theta microscope [31] introduces a second
15 objective to the system, that is used to illuminate the sample (Figure 1.7b). Since this
16 decouples the illumination and detection, using a dichroic mirror is no longer necessary.
17 The second objective is rotated by θ around the focus, this is where the name of this
18 setup originates from.

19 As in the case of standard confocal microscopy, the system PSF is improved by the
20 illumination pattern. Here, however, the axial direction of the detection coincides with



Figure 1.9: Basic concept of single-plane illumination microscopy. The sample is illuminated from the side by laser light shaped to a light-sheet (blue). This illuminates the focal plane of the detection lens, that collects light in a wide-field mode (yellow). The image is recorded, and the sample is translated through the light-sheet to acquire an entire 3D stack.

the lateral direction of the illumination, which results in a dramatic improvement of axial resolution compared to standard confocal microscopy. Lateral resolution will also be increased, but by a smaller extent, resulting in an almost isotropic PSF, and equal axial and lateral resolutions. Although this is a big improvement to confocal microscopy in terms of resolution, this technique did not reach a widespread adoption as it complicates sample handling, while still suffering from two drawbacks of confocal microscopy techniques that limits its live imaging capabilities.

Imaging live specimens for an extended period of time with confocal microscopy although possible [32, 33], is not ideal. For each voxel imaged, a large portion of the specimen has to be illuminated, which results in a very high dose of radiation on the samples. This can be as much as 30–100 times larger, than the dose used for the actual imaging [34]. Illumination with high power of laser for an extended time frame can result in bleaching the fluorophores, which in turn will lower the signal at later times. Furthermore, any absorbed photon has the possibility to disrupt the chemical bonds inside the specimen, which can lead to phototoxic effects. Moreover, the usage of the pinhole although increases resolution, also decreases the detectable signal intensity, thus has a negative impact on image contrast [35].

1.3 Light-sheet microscopy

A selective-plane illumination microscope (SPIM) uses a light-sheet to illuminate only a thin section of the sample (Figure 1.9). This illumination plane is perpendicular to the imaging axis of the detection objective and coincides with the focal plane. This way, only the section in focus will be illuminated, thus providing much better signal to noise ratio.

1.3 Light-sheet microscopy

1 In case of conventional wide-field fluorescence microscopy, where the whole specimen
2 is illuminated, out of focus light contributes to a significant background noise. With
3 selective-plane illumination, this problem is intrinsically solved, and it also provides a
4 true sectioning capability. This makes SPIM especially suitable for 3D imaging.

5 The main principle behind single plane illumination microscopy, that is illuminating
6 the sample from the side by a thin light-sheet, dates back to the early 20th century, when
7 Siedentopf and Zsigmondy first described the ultramicroscope [36]. This microscope used
8 sunlight as an illumination source, that was guided through a precision slit to generate
9 a thin light-sheet. This allowed Zsigmondy to visualize gold nanoparticles floating in
10 and out of the light-sheet. Since these particles are much smaller than the wavelength
11 of the light, the device was called an ultramicroscope. His studies with colloids, and the
12 development of the ultramicroscope led Zsigmondy to win the Nobel Prize in 1925.

13 After Zsigmondy, this method was forgotten until rediscovered in the 1990s, when
14 Voie *et al.* constructed their Orthogonal-plane Fluorescent Optical Sectioning (OPFOS)
15 microscope [37]. They used it to image a fixed, optically cleared and fluorescently labelled
16 guinea pig cochlea. In order to acquire a 3D dataset, the sample was illuminated from the
17 side with a light-sheet generated by a cylindrical lens, then rotated around the center axis
18 to obtain multiple views. Although they only reached a lateral resolution around 10 µm
19 and axial resolution of 26 µm, this method allowed them to generate a 3D reconstruction
20 of the guinea pig cochlea [38].

21 Later, in 2002, Fuchs *et al.* developed Thin Light-Sheet Microscopy (TLSM) [39]
22 and used this technique to investigate the microbial life in seawater samples without
23 disturbing their natural environment (by e.g. placing them on a coverslip). Their light-
24 sheet was similar to the one utilized in OPFOS, being 23 µm thin, and providing a
25 1 mm × 1 mm field of view.

26 Despite these early efforts, the method did not gain larger momentum. The real
27 breakthrough in light-sheet imaging happened at the European Molecular Biology Labo-
28 ratory (EMBL) in 2004, where Huisken *et al.* [40] combined the advantages of endogenous
29 fluorescent proteins and the optical sectioning capability of light-sheet illumination to
30 image Medaka fish embryos, and the complete embryonic development of a *Drosophila*
31 *melanogaster* embryo. They called this Selective-Plane Illumination Microscopy (SPIM),
32 and it quickly became popular to investigate developmental biological questions.

33 Since then, light-sheet based imaging has gained more and more popularity, as it can
34 be adapted and applied to a wide variety of problems. Although sample mounting can
35 be challenging because of the objective arrangement, this can also be an advantage, since
36 new microscopes can be designed with the sample in mind [3, J3] (Figure 1.10). This
37 made it possible to adapt the technique for numerous other specimens, such as zebrafish
38 larvae [49], *C. elegans* embryos [42], mouse brain [6], and even mouse embryos [J2, 50,

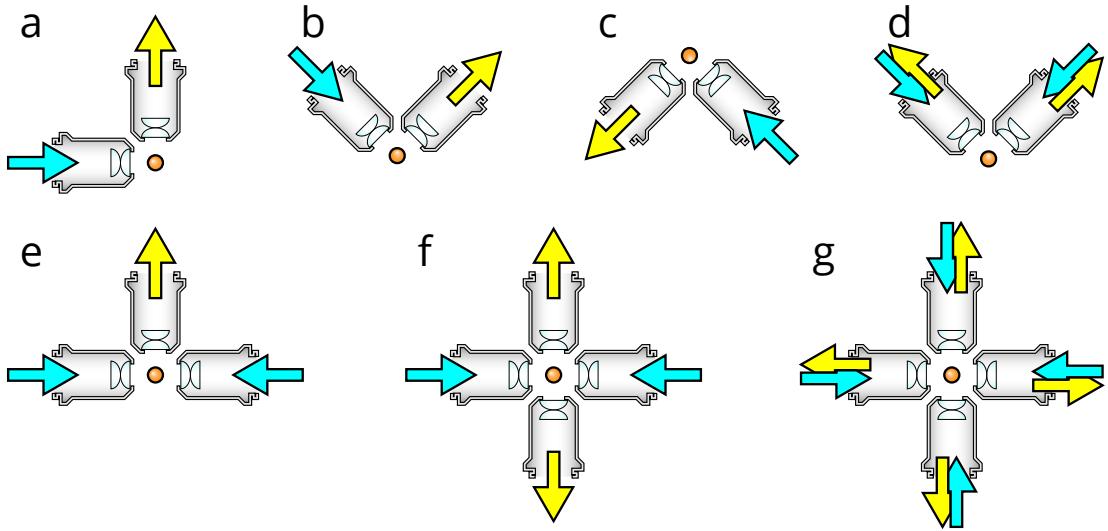


Figure 1.10: Different optical arrangements for light-sheet microscopy. (a) Original SPIM design with a single lens for detection and illumination. [40] (b) Upright SPIM to allow for easier sample mounting such as using a petri dish (iSPIM, [41, 42, J1]). (c) Inverted SPIM, where the objectives are below the sample, which is held by a thin foil [J2]. (d) Dual-view version of the upright configuration, where both objective can be used for illumination and detection (diSPIM, [43]). (e) Multidirectional-SPIM (mSPIM) for even illumination of the sample with two objectives for illumination [44]. (f) Multi-view SPIM with two illumination and detection objectives for *in toto* imaging of whole embryos (MuVi-SPIM [45], SimView [46], Four-lens SPIM [47]). (g) A combination of (d) and (f), using four identical objectives, where both can illuminate and detect in a sequential manner, to achieve isotropic resolution without sample rotation (IsoView [48]).

1 51].

2 As many of these specimens require very different conditions and mounting tech-
3 niques, these microscopes have been adapted to best accommodate them. An upright
4 objective arrangement for example (Figure 1.10b) allows imaging samples on a coverslip,
5 while its inverted version is well suited for mouse embryos, where a foil is separating them
6 from the immersion medium (Figure 1.10c). A modified version of the upright arrange-
7 ment allows for multi-view imaging using both objectives for illumination and detection
8 in a sequential manner (Figure 1.10d) [52].

9 To achieve a more even illumination in larger samples, two objectives can be used from
10 opposing directions to generate two light-sheets (Figure 1.10e) [44]. This arrangement
11 can further be complemented by a second detection objective, to achieve parallelized
12 multi-view imaging (Figure 1.10f) [45–47]. For ultimate speed, 4 identical objectives can
13 be used to achieve almost instantaneous views from 4 different directions by using all
14 objectives for illumination and detection (Figure 1.10g) [48].

15 Furthermore, because of the wide-field detection scheme it is possible to combine
16 SPIM with many superresolution techniques, such as single molecule localization [53],
17 STED [54], RESOLFT [J1], or structured illumination [7, 55, 56].

18 Since illumination and detection for light-sheet microscopy are decoupled, two inde-

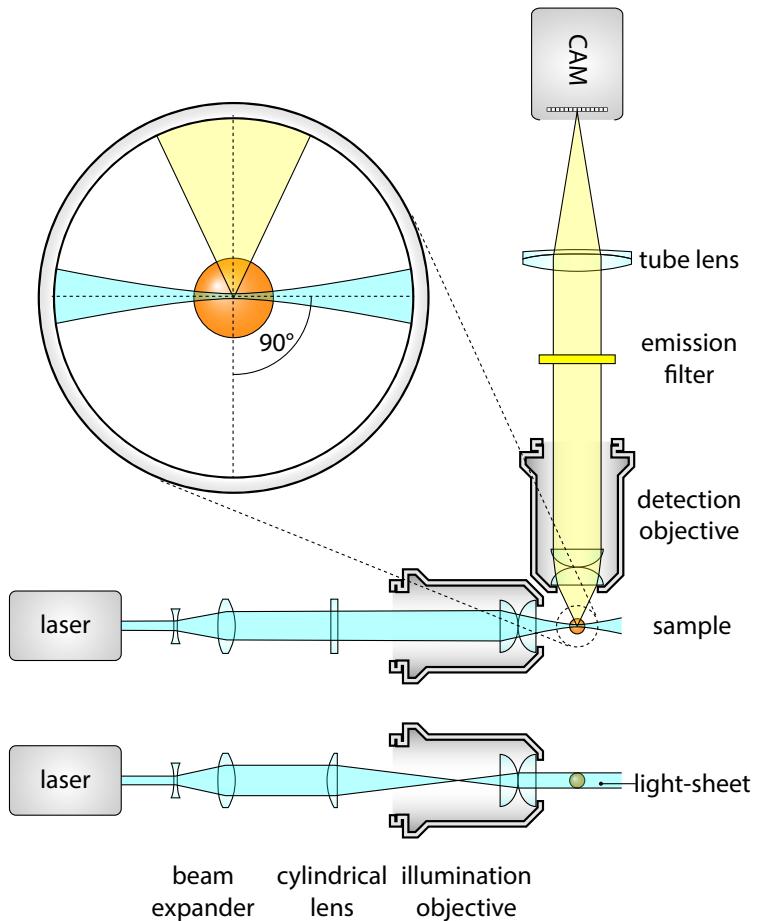


Figure 1.11: Basic optical components of a SPIM. A dedicated illumination objective is used to generate the light-sheet, which is an astigmatic Gaussian beam, focused along one direction. Astigmatism is introduced by placing a cylindrical lens focusing on the back focal plane of the objective. Detection is performed at a right angle, with a second, detection objective. Scattered laser light is filtered out, and a tube lens forms the image on an area sensor, such as an sCMOS camera.

- ¹ pendent optical paths are implemented.
- ² The detection unit of a SPIM is basically equivalent to a detection unit of a wide-field
- ³ microscope, without a dichroic mirror (Figure 1.11). The most important components
- ⁴ are the objective together with the tube lens, filter wheel, and a sensor, typically a CCD
- ⁵ or sCMOS camera.
- ⁶ One of the most important aspects that determines the resolution of the microscope is
- ⁷ the detection objective. Since imaging biological specimens usually requires a water-based
- ⁸ solution, the objectives also need to be directly submerged in the medium to minimize
- ⁹ spherical aberrations. Since the refraction index of water ($n = 1.33$) is greater than the
- ¹⁰ refraction index of air, these objectives tend to have a higher NA, resulting in higher
- ¹¹ resolution. As the illumination is decoupled in this system, the light-sheet thickness also

1 has an influence on the axial resolution. Finally, the resolution also depends on the pixel
2 size of the sensor which determines the spatial sampling rate of the image.

3 Although image quality and resolution greatly depends on the detection optics, the
4 real strength of light-sheet microscopy, the inherent optical sectioning is due to the
5 specially designed illumination pattern, that confines light to the vicinity of the detection
6 focal plane.

7 There are two most commonly used options to generate a light-sheet: either by using
8 a cylindrical lens, to illuminate the whole field of view with a static light-sheet, as in the
9 original SPIM concept [40]; or by quickly scanning a thin laser beam through the focal
10 plane, thus resulting in a virtual light-sheet. This method is called Digitally Scanned
11 Light-sheet Microscopy (DSLM) [49].

12 1.3.1 Static light-sheet illumination

13 For a static light-sheet, the normally circular Gaussian laser beam needs to be shaped
14 in an astigmatic manner, i.e. either expanded or squeezed along one direction, to shape
15 it into a sheet instead of a beam. This effect can be achieved by using a cylindrical lens,
16 which as the name suggests has a curvature in one direction, but is flat in the other, thus
17 focusing a circular beam to a sheet (Figure 1.11).

18 However, to achieve light-sheets that are sufficiently thin for optical sectioning, one
19 would need to use cylindrical lens with a very short focal length, and these are hardly
20 accessible in well corrected formats. For this reason, it is more common to use a longer
21 focal length cylindrical lens in conjunction with a microscope objective, which is well
22 corrected for chromatic and spherical aberrations [57]. This way, the light-sheet length,
23 thickness and width can be adjusted for the specific imaging tasks.

24 Light-sheet dimensions

25 The shape of the illumination light determines the optical sectioning capability and the
26 field of view of the microscope, so it is important to be able to quantify these measures.
27 The most commonly used illumination source is a laser beam coupled to a single mode
28 fiber, thus its properties can be described by Gaussian beam optics.

29 For paraxial waves, i.e. waves with nearly parallel wave front normals, a general wave
30 equation can be approximated with the paraxial Helmholtz equation [58]

$$\nabla_T^2 U + i2k \frac{\partial U}{\partial z} = 0 \quad (1.17)$$

31 where $\nabla_T^2 = \frac{\partial^2}{\partial x^2} + \frac{\partial^2}{\partial y^2}$, $U(\vec{r})$ is the wave function, $k = \frac{2\pi}{\lambda}$ is the wavenumber and z is in
32 the direction of the light propagation.

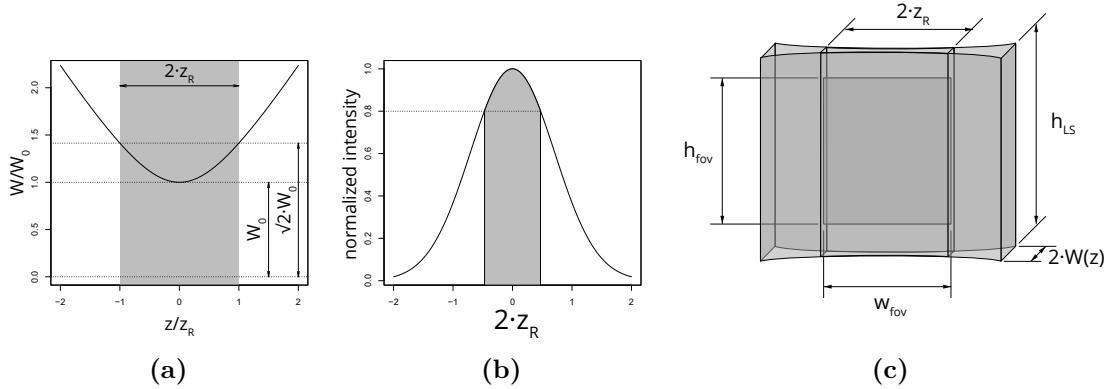


Figure 1.12: Light-sheet dimensions. (a) The width and thickness of the field of view depends on the Rayleigh length of the beam ($z_{R,y}$) and the beam waist (W_0). (b) The height of the field of view is determined by the Gaussian profile of the astigmatic beam. (c) shows a light sheet, with the field of view indicated. Since the light-sheet intensity is uneven, the field of view has to be confined to a smaller region.

1 A simple solution to this differential equation is the Gaussian beam:

$$U(r, z) = A_0 \cdot \frac{W_0}{W(z)} \cdot e^{-\frac{r^2}{W^2(z)}} \cdot e^{-i \cdot \phi(r, z)} \quad (1.18)$$

2 where A_0 is the amplitude of the wave, W_0 is the radius of the beam waist (the thinnest
 3 location on the beam), $r = \sqrt{x^2 + y^2}$ is the distance from the center of the beam, $W(z)$
 4 is the radius of the beam z distance from the waist, and $\phi(r, z)$ is the combined phase
 5 part of the wave-function (Figure 1.12a). Furthermore:

$$W(z) = W_0 \sqrt{1 + \left(\frac{z}{z_R}\right)^2} \quad (1.19)$$

6 where the parameter z_R is called the Rayleigh-range, and is defined the following way:

$$z_R = \frac{\pi W_0^2}{\lambda}. \quad (1.20)$$

7 Apart from the circular Gaussian beam, the elliptical Gaussian beam is also an eigen-
 8 function of Helmholtz equation (Equation 1.17) which describes the beam shape after a
 9 cylindrical lens:

$$U(x, y, z) = A_0 \cdot \sqrt{\frac{W_{0,x}}{W_x(z - z_{0,x})}} \sqrt{\frac{W_{0,y}}{W_y(z - z_{0,y})}} \cdot e^{-\frac{x^2}{W_x^2(z - z_{0,x})}} \cdot e^{-\frac{y^2}{W_y^2(z - z_{0,y})}} \cdot e^{-i \cdot \phi(x, y, z)} \quad (1.21)$$

This beam still has a Gaussian profile along the x and y axes, but the radii ($W_{0,x}$ and $W_{0,y}$), and the beam waist positions ($z_{0,x}$ and $z_{0,y}$) are uncoupled, which results in an elliptical and astigmatic beam. The beam width can now be described by two independent

equations for the two orthogonal directions:

$$W_x(z) = W_{0,x} \sqrt{1 + \left(\frac{z}{z_{R,x}}\right)^2} \quad \text{and} \quad W_y(z) = W_{0,y} \sqrt{1 + \left(\frac{z}{z_{R,y}}\right)^2}. \quad (1.22)$$

Since the beam waist is different along the two axes, the Rayleigh range is also different:

$$z_{R,x} = \frac{\pi W_{x,0}^2}{\lambda}, \quad z_{R,y} = \frac{\pi W_{y,0}^2}{\lambda}. \quad (1.23)$$

Based on these equations, the light-sheet dimensions and usable field of view can be specified (Figure 1.12c). The light-sheet thickness will depend on the beam waist, $W_{0,y}$ (if we assume the cylindrical lens is focusing along y), and the length of the light-sheet can be defined as twice the Rayleigh range, $2 \cdot z_{R,y}$. As these are coupled (see Equation 1.23), having a thin light-sheet for better sectioning also means the length of it will be relatively short. Fortunately, because of the quadratic relation, to increase the field of view by a factor of two, the light-sheet thickness only needs to increase by a factor of $\sqrt{2}$.

Light-sheet height is determined by the intensity profile of the beam along the vertical axis (Figure 1.12b). Since this is a Gaussian function (see Equation 1.18), only a small part in the middle can be used for imaging, because towards the sides the intensity dramatically drops. To allow a maximum 20% drop-off in intensity at the edges, the light-sheet height becomes $h_{fov} = 2 \cdot 0.472 \cdot W_{x,0} = 0.944 \cdot W_{x,0}$.

1.3.2 Digitally scanned light-sheet illumination

Although generating a static light-sheet is relatively straightforward, with the simple addition of a cylindrical lens to the light path, it has some drawbacks. As already mentioned in the previous section, the light intensity distribution along the field of view is not constant, as the light-sheet is shaped from a Gaussian beam. Furthermore, along the lateral direction of the light-sheet the illumination NA is extremely low, resulting in effectively collimated light. Because of this, shadowing artifacts can deteriorate the image quality [44].

A more flexible way of creating a light-sheet is by scanning a focused beam in the focal plane to generate a virtual light-sheet (digital scanned light-sheet microscopy, DSLM [49]). Although this method might require higher peak intensities, it solves both drawbacks of the cylindrical lens illumination. By scanning the beam, the light-sheet height can be freely chosen, and a homogenous illumination will be provided. Focusing the beam in all directions evenly introduces more angles in the lateral direction as well, which shortens the length of the shadows.

The basic optical layout of a DSLM is shown on Figure 1.13. A galvanometer controlled mirror is used to alter the beam path that can quickly turn around its axis which

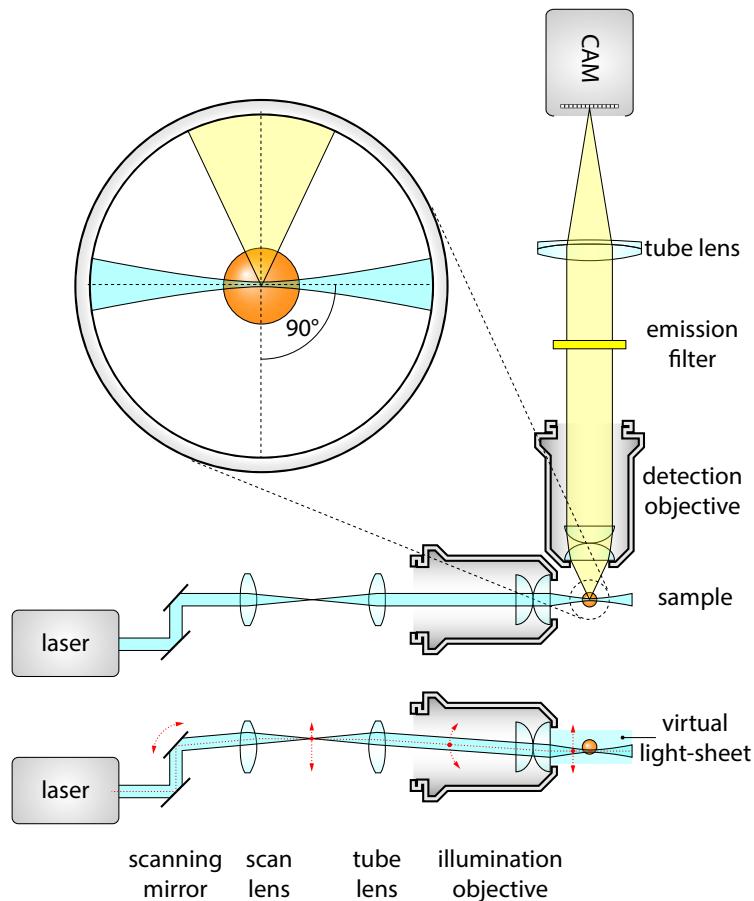


Figure 1.13: DLSM illumination. DLSM illuminates a specimen by a circularly-symmetric beam that is scanned over the field of view. This creates a virtual light-sheet, which illuminates a section of a specimen just like the SPIM. The light-sheet in DLSM is uniform over the whole field of view and its height can be dynamically altered by changing the beam scan range.

1 will result in an angular sweep of the laser beam. To change the angular movement to
 2 translation, a scan lens is used to generate an intermediate scanning plane. This plane is
 3 then imaged to the specimen by the tube lens and the illumination objective, resulting
 4 in a scanned focused beam at the detection focal plane. The detection unit is identical
 5 to the wide-field detection scheme, similarly to the static light-sheet illumination. By
 6 scanning the beam at a high frequency, a virtual light-sheet is generated, and the flu-
 7 orescence signal is captured by a single exposure on the camera, resulting in an evenly
 8 illuminated field of view.

9 1.4 Light-sheet microscopy for mouse imaging

10 Because of its optical sectioning capabilities, combined with the high specificity of flu-
 11 orescent labels, confocal microscopy had an immense influence on biological research,

1 and has been the go-to technique for decades for many discoveries [59–61]. Live imaging
2 capabilities of confocal microscopy are, however, limited. This is mostly due to the illu-
3 mination scheme: to collect information from a single point, almost the whole embryo
4 has to be illuminated. This unwanted illumination can easily lead to bleaching of the
5 fluorophores, and also to phototoxic effects that can prevent further embryonic develop-
6 ment. The point scanning nature of image acquisition also implies an inherent constraint
7 to the maximum imaging speed, as it can be only increased at the expense of reducing
8 signal intensity (Figure 1.1).

9 One improvement to address both of these drawbacks is the use of a spinning disk with
10 a specific pattern (also called Nipkow disk) of holes to generate multiple confocal spots
11 at the same time [60]. If these spots are far enough from each other, confocal rejection
12 of out-of-focus light can still occur. As the disk is spinning, the hole pattern will sweep
13 the entire field of view, eventually covering all points [62]. The image is recorded by an
14 area detector, such as a CCD or EM-CCD, which speeds up image acquisition [63].

15 Although out-of-focus illumination is still an issue, spinning disk confocal microscopy
16 was successfully used to investigate the mechanisms of symmetry breaking in early mouse
17 embryonic development [64], and the mechanisms leading to the first cell fate specification
18 that will differentiate extraembryonic tissue from the embryo proper [33, 65, 66]. Even
19 though these studies were carried out with live embryos, only a few hours of time-lapse
20 imaging is possible before the accumulation of phototoxic effects arrests development
21 [67]. Compared to this, just the pre-implantation phase of mouse embryonic development
22 spans 3 days, and the full development is 18 days [68].

23 1.4.1 Imaging pre-implantation development

24 Pre-implantation is the first phase of mouse embryonic development, that starts right
25 after fertilization. The embryo in this phase is still in the oviduct, travelling towards
26 the uterus, where it will implant into the uterine wall. The developmental stage between
27 fertilization and the implantation is called the pre-implantation stage. Here the embryo
28 divides, and already the first cell fate specifications start when forming the trophoecto-
29 derm (TE) and the inner cell mass (ICM) at the blastocyst stage. ICM cells will form
30 the embryo proper, while TE cell will contribute to the formation of the extraembryonic
31 tissues.

32 During this process the embryo is still self-sufficient, which makes it possible to image
33 this stage in an *ex vivo* embryo culture by providing the proper conditions [69]. Long
34 term imaging, however, is extremely challenging due to the very high light sensitivity of
35 the specimens. Imaging these embryos in a confocal microscope will lead to incomplete
36 development, even if the imaging frequency is minimized to every 15 mins [J2].

37 Imaging for just a few hours is already enough to investigate important processes, such

1.4 Light-sheet microscopy for mouse imaging

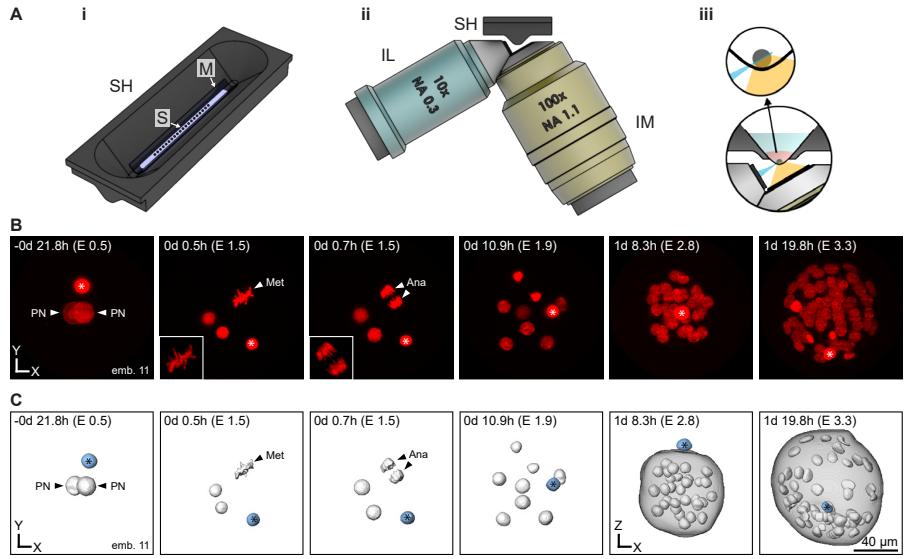


Figure 1.14: Inverted light-sheet microscope for multiple early mouse embryo imaging.. (i) A sample holder (SH), containing a transparent FEP membrane (M) allows multiple embryo samples (S) to be placed in line for multisample imaging. (ii) Inverted objective orientation with side view of the sample holder. One possible configuration is to use a 10 \times 0.3 NA illumination objective (IL) and another 100 \times 1.1 NA detection objective placed at a right angle to the illumination. (iii) Close up on side view of sample on FEP membrane with both objectives. Since the FEP membrane is transparent on water, it provides no hindrance to the illumination beam in penetrating the sample or for the emitted fluorescence on reaching the detection objective. (B) Still images of one particular timelapse experiment, and (C) corresponding segmented nuclei. The star depicts the polar body. Adapted from Strnad *et al.* [J2]

1 as cell fate patterning [70]. Other approaches aim to lower the phototoxicity by either
 2 using 2-photon illumination which operates at longer wavelengths [71–73], or by lowering
 3 imaging frequency as a compromise [74]. These approaches, however either require highly
 4 specialized equipment, such as an ultra-short pulsed laser, or is compromising on the time
 5 resolution.

6 Light-sheet microscopy, on the other hand, drastically lowers phototoxic effect by
 7 using a much more efficient illumination scheme (see Section 1.3), and thus makes a
 8 better use of the photon budget. Using this technique, it is possible to image the full pre-
 9 implantation development at high spatial and temporal resolution without any negative
 10 impact on the developmental process. Such a microscope was developed by Strnad *et al.*
 11 at EMBL [J2], who used it to understand when exactly the first cell fate specification is
 12 decided in the embryonic cells.

13 As a mouse embryo culture is not compatible with the standard agarose-based sample
 14 mounting techniques, a completely new approach was taken, which resulted in a micro-
 15 scope designed around the sample. The sample holder forming a V-shape was built with
 16 a bottom window, and it is lined with a thin FEP (fluorinated ethylene propylene) foil
 17 that supports the embryos (Figure 1.14A, i). This arrangement allows the utilization of
 18 the standard microdrop embryo culture, while providing proper viewing access for the
 19 objectives. As the embryos are relatively small (100 μ m) and transparent, a single illu-

mination and single detection objective arrangement is enough for high quality imaging.
A low resolution ($NA=0.3$) objective is used to generate the scanned light-sheet, and
a high resolution ($NA=1.1$) objective is detecting the fluorescence at $50\times$ magnification
(Figure 1.14A, ii). As the foil is curved, it allows unrestricted access to the embryo, while
separating the imaging medium from the immersion liquid (Figure 1.14A, iii). Furthermore,
its refractive index is matching the refractive index of water, so optical aberrations
are minimized.

Using this setup, Strnad *et al.* were able to pinpoint the exact timing of the first cell
fate decision that leads either to ICM or TE cells. More than 100 embryos expressing
nuclear (H2B-mCherry) and membrane (mG) markers were imaged for the entire 3 days
of pre-implantation development (Figure 1.14B). The image quality was sufficient to
segment all nuclei in the embryos (Figure 1.14C), and track them from 1 to 64 cell stage,
building the complete lineage tree. Based on the lineage trees, and the final cell fate
assignments, it was determined that at the 16 cell stage the final specification is already
decided, while earlier than this it is still random.

1.4.2 Imaging post-implantation development

After the initial 3 days of pre-implantation, the embryo undergoes the implantation
process, during which it is inaccessible to microscopical investigations. Although a new
method was recently developed that allows *in vitro* culturing of the embryos embedded
in a 3D gel [76], this has not reached wider adoption yet. Because of this, developmental
processes during implantation have only been investigated in fixed embryos.

Following the implantation process, at the post-implantation phase, *ex vivo* embryo
culturing becomes possible again [77, 78], and these embryos can be kept alive for several
days in an artificial environment. During this process especially interesting stages are the
late blastocyst ($\sim E4.5$), gastrulation ($\sim E6.5$), and somite formation ($\sim E8.5$). Before live
imaging techniques became available, these stages were mostly investigated using *in situ*
visualization techniques to shed light on several developmental processes [79]. Many
pathways playing important roles have been identified this way, however live imaging is
still necessary to validate these results, and ensure continuity in the same specimen [80].

Light-sheet microscopy is a good choice for imaging these stages, just like in the case
of pre-implantation embryos. These embryos, however, present new challenges for sample
handling and culturing. Owing to their extreme sensitivity, dissection can be difficult,
especially for earlier stages (E4.5). Furthermore, since the embryo is also growing during
development, gel embedding is not an option, as this might constrain proper development.
Thus, special handling and mounting techniques had to be developed in order to allow
live 3D imaging of these specimens.

Ichikawa *et al.* [50] designed a custom mounting apparatus manufactured from acrylic

1.4 Light-sheet microscopy for mouse imaging

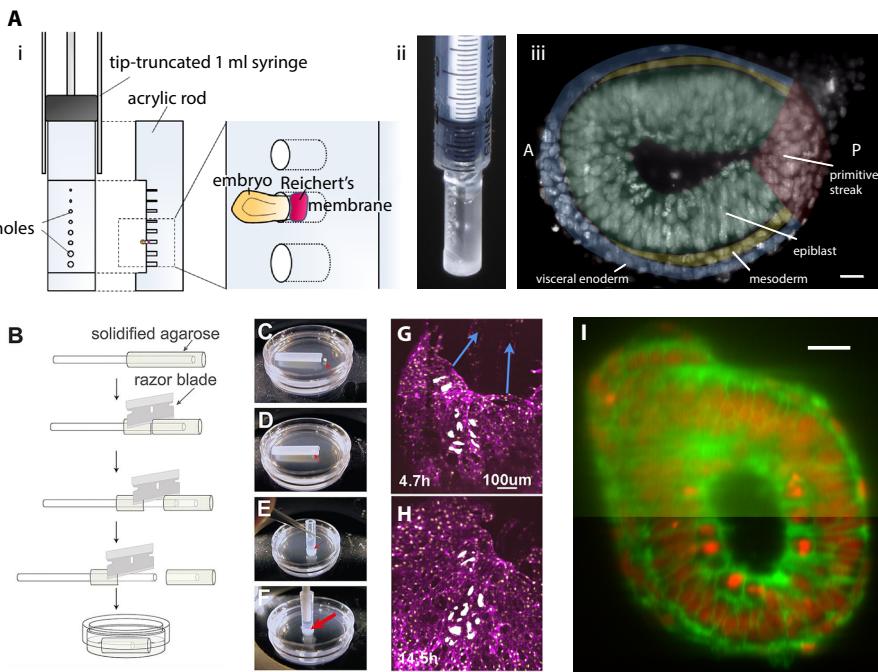


Figure 1.15: Imaging mouse post-implantation development. (A) (i, ii) Mounting technique for E5.5 to E6.5 embryos. A tip-truncated 1 mL syringe holds an acrylic rod, cut and drilled with holes of different size in order to best fit the mouse embryo by its Reichert's membrane, leaving the embryo free inside the medium. (iii) Maximum intensity projection of a 13 µm thick slice at 78 µm from distal end of an E6.5 mouse embryo. The different tissues corresponding to the rudimentary body plan are annotated. Scale bar: 20 µm. (B) For stages ranging between E6.5 and E8.5, mounting using a hollow agarose cylinder has also successfully been proposed. Optimal sizes for the corresponding embryonic stage to be imaged can be produced, so that the embryo can grow with least hindrance. (C–F) Steps for mounting the mouse embryo inside the agarose cylinder. The inner volume of the cylinder can be filled with optimal medium, allowing the much larger chamber volume to have less expensive medium. (G–H) Example images of a 9.8 h timelapse with the mounting shown in (B) where the expansion of the yolk sac can be observed in direction of the blue arrows. (I) In order to aid multiview light-sheet setups in overcoming the higher scattering properties of embryos at this stage, and to allow faster and easier data recording, electronic confocal slit detection allows better quality images to be taken at shorter acquisition times. Scale bar: 20 µm. Adapted from Ichikawa *et al.* [50], Udan *et al.* [51] and de Medeiros and Norlin *et al.* [75].

in the shape of a rod that fits in a standard 1 mL syringe with its tip truncated (Figure 1.15A, i). In the rod several holes were drilled with different sizes that can accommodate different sized embryos, which are held by an extraembryonic tissue, the Reichert's membrane (Figure 1.15A, ii). Mounting this way doesn't disturb the embryo itself, and it can freely develop in the culturing medium, while it is also stationary for the purpose of imaging. Using this technique, Ichikawa *et al.* were able to image through several stages of development, including interkinetic nuclear migration at stages E5.5–6.5 (Figure 1.15A, iii).

A second method of sample mounting for light-sheet imaging was developed by Udan *et al.* who were able to record a full 24 h time-lapse of living embryos focusing on the gastrulation and yolk sac formation processes (Figure 1.15G–I). Their mounting technique comprised of producing a hollow agarose container shaped like a cylinder that could support the embryo from below without constraining its growth (Figure 1.15B–F).

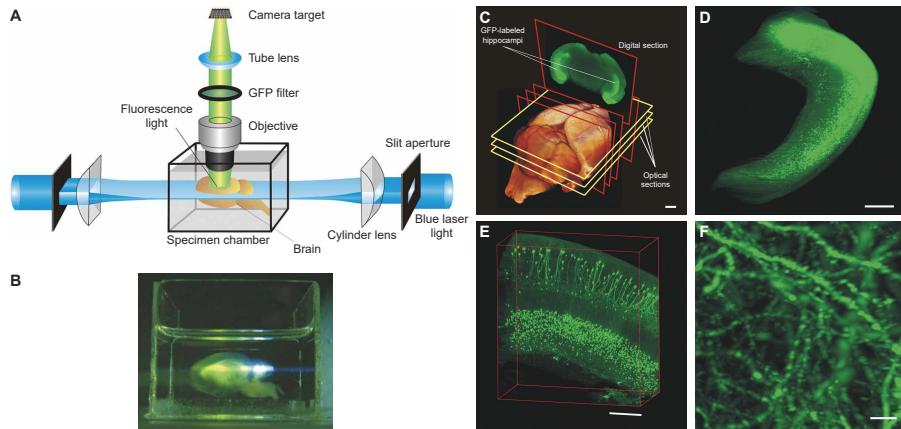


Figure 1.16: Imaging adult mouse brain with light-sheet microscopy.. (A) Schematics of the ultramicroscope for brain imaging. The specimen is embedded in clearing medium to ensure necessary imaging depth. Illumination is applied from two sides to achieve even illumination for the whole field of view. Light-sheet is generated by a slit aperture followed by a cylindrical lens. The specimen is imaged from the top using wide-field detection method. (B) Photograph of the imaging chamber with a mounted cleared specimen and light-sheet illumination. (C) Surface rendering of a whole mouse brain, reconstructed from 550 optical sections. GFP and autofluorescence signal was recorded. Hippocampal pyramidal and granule cell layers are visible in the digital section. Scale bar: 1 mm. Objective: Planapochromat 0.5×. (D) Reconstruction of an excised hippocampus from 410 sections. Note that single cell bodies are visible. Scale bar: 500 µm. Objective: Fluar 2.5×. (E) 3D reconstruction of a smaller region of an excised hippocampus from 132 sections. Scale bar: 200 µm. Objective: Fluar 5×. (F) 3D reconstruction of CA1 pyramidal cells imaged with a higher resolution objective (LD-Plan Neofluar 20× NA 0.4) in a whole hippocampus (430 sections). Dendritic spines are also visible, even though usually a higher NA objective (>1.2) is required to visualize these. Scale bar: 5 µm. Adapted from Dodt *et al.* [6].

1 Another consideration to keep in mind, is the growing size of the embryo. As it
 2 gets bigger, illumination is less efficient, and scattering can dominate at larger depths.
 3 As mentioned in earlier (Figure 1.3) this can be alleviated by multi-view imaging: illu-
 4 minating and detecting from multiple directions. Electronic confocal slit detection can
 5 further improve the signal to noise ratio by rejecting unwanted scattered light, which
 6 allows deeper imaging in large specimens, even up to E7.5 (Figure 1.15I) [75].

7 1.4.3 Imaging adult mice

8 Imaging adult mice is especially interesting for answering neurobiological questions. Since
 9 development is over at this stage, the use of an environmental chamber is no longer neces-
 10 sary. The biggest challenge for imaging these samples is their size, as they are centimeters
 11 in size instead of less than a millimeter as in the embryonic stage. Furthermore, the tis-
 12 sues of adult mice are much more opaque which severely limits imaging depth. Light-sheet
 13 microscopy can already deal with large specimens, however to achieve (sub)cellular res-
 14 olution for an entire brain for example, multiple recordings have to be stitched together
 15 after acquisition [81].

16 Light scattering and absorption depends on the tissue composition, and also imaging
 17 depth. Especially the brain with a high concentration of lipids in the myelinated fibers
 18 pose a real challenge for imaging. Live imaging is usually performed with 2-photon mi-

1.4 Light-sheet microscopy for mouse imaging

1 croscopy which can penetrate the tissue up to 800 µm deep [82]. Using fixed samples,
2 however, the scattering problem can be eliminated by the use of tissue clearing methods.

3 Tissue clearing is a process that removes and/or substitutes scattering and absorbing
4 molecules by a chemical process while keeping the tissue structure intact and preserving
5 fluorescence. The most dominant contributors to these effects are the proteins and lipids.
6 Proteins in the cells locally change the refractive index of the tissue which leads to
7 scattering, while lipids predominantly absorb the light. Clearing methods tackle these
8 problems by chemically removing and substituting lipids by certain types of gel, and
9 immersing the whole sample in a medium with higher refractive index to match the
10 optical properties of proteins. Numerous methods have been developed for tissue clearing,
11 such as ScaleA2 [83], 3DISCO [84, 85], SeeDB [86], CLARITY [87], CUBIC [88] and
12 iDISCO [89].

13 The first combination of optical clearing and light-sheet microscopy for whole brain
14 imaging was performed by Dodt *et al.* using a custom ultramicroscope consisting of
15 two opposing illumination arms and a single detection with an objective from above
16 (Figure 1.16A). The light-sheets were positioned horizontally, and the cleared samples
17 could be placed in a transparent imaging chamber filled with the clearing medium (Figure
18 1.16B). Imaging was performed from both top and bottom after rotating the sample
19 180°. By changing the detection lens, it is possible to adapt the system to different sam-
20 ples: low magnification is capable of imaging the whole brain (Figure 1.16C), while for
21 smaller, dissected parts, such as the hippocampus, higher magnification with higher res-
22 olution is more appropriate (Figure 1.16D). With this configuration individual cell-cell
23 contacts can be recognized (Figure 1.16E), and even dendritic spines can be visualized
24 (Figure 1.16F).

25 Although light-sheet microscopy is highly suitable for imaging cleared specimens, even
26 entire mice [90], brain imaging in live animals is more challenging due to the standard
27 two-objective setup of a conventional SPIM microscope. Two light-sheet based methods,
28 however offer a solution for this, axial plane optical microscopy (APOM) [91] and swept
29 confocally-aligned planar excitation (SCAPE) [92] both use only a single objective to
30 generate a light-sheet and detect the fluorescence as well. This is done by rotating the
31 detection plane at an intermediate image (APOM), or by rotating both the light-sheet
32 and detection plane simultaneously (SCAPE).

¹ Chapter 2

² Image compression

³ As we will see later (Section 4.1), light-sheet microscopy is capable of generating an
⁴ immense amount of data in a short amount of time. For this reason not only fast data
⁵ processing, but data compression also plays an important role when evaluating, sharing
⁶ and storing the images. In this chapter we will briefly introduce the core concepts of
⁷ image compression and show some examples as a background for Chapter 4. For a more
⁸ comprehensive review on data compression fundamentals, the interested reader is referred
⁹ to the works of Sayood [93], and Salomon and Motta [94].

¹⁰ There are two distinct ways of data compression: lossless and lossy. This is an impor-
¹¹ tant difference, and the choice between the two greatly depends on the application itself.
¹² For some types of data no loss is acceptable, for example computer programs or text.
¹³ Here, even a small change could drastically influence the meaning of the original data.
¹⁴ For other applications, such as audio and video compression, some loss can be tolerated
¹⁵ as long as there is no perceived change or distortion. For scientific applications mostly
¹⁶ lossless compression is used. Even for image data, where lossy compression can signifi-
¹⁷ cantly increase the compression ratio (original size / compressed size), lossy compression
¹⁸ is usually not recommended, as it can alter the measurement results in unpredictable
¹⁹ ways [95].

²⁰ 2.1 Basics of information theory

²¹ As compression is the art of reducing the size of a message while keeping the same
²² amount of information, it is necessary to briefly discuss the theory behind information,
²³ and how to quantify it. These concepts were first introduced by Shannon, in his highly
²⁴ influential papers [96–98]. As a rigorous mathematical explanation is outside the scope
²⁵ of this work, we refer the interested reader to the aforementioned works.

²⁶ Informally, information can be quantified as the amount of surprise. Any statement,
²⁷ if it has a high probability carries a low amount of information, while if it has a small

1 probability, there is more information. Consider the following example: “It is July”. If it is
 2 indeed July, this statement doesn’t provide too much information. Continuing with “It is
 3 snowing outside”, carries more information, as it is unexpected under the circumstances
 4 (provided the conversation takes place on the Northern Hemisphere).

5 The self-information of event A can be defined the following way:

$$I(A) = \log_b \frac{1}{P(A)} = -\log_b P(A), \quad (2.1)$$

6 where $P(A)$ is the probability of event A occurring. The base of the logarithm can
 7 be chosen freely, but usually the preferred base is $b = 2$. With this choice, the unit
 8 of information is 1 bit, and $I(A)$ represents how many bits are required to store the
 9 information contained in A .

10 The average self-information, also called the entropy, for a random variable X can
 11 be calculated based on the self-information of the outcomes A_i :

$$H(X) = \sum_i P(A_i)I(A_i) = -\sum_i P(A_i) \log_b P(A_i) \quad (2.2)$$

12 If we consider a data stream S , where each symbol records the outcome of independent,
 13 identical random experiments X , then the average information in each symbol will be
 14 $H(X)$. As a consequence, as stated by Shannon’s source coding theorem [96], the shortest
 15 representation of S will require at least $N \cdot H(X)$ bits, where N is the number of symbols
 16 in the stream. This defines the theoretical lower bound that any naïve compression
 17 algorithm, also called entropy coding, can achieve without losing any information.

18 The requirement, however, is that the symbols are independent of each other, which
 19 is usually not true for most of the data types we (humans) are interested in. In order to
 20 achieve ideal compression, the data needs to be modeled, or transformed, to represent it
 21 as a sequence of independent variables. This pattern of modeling and coding [99] is the
 22 core of all modern compression algorithms. The following sections will briefly introduce
 23 these concepts by two examples: Huffman coding, and pixel prediction.

24 2.2 Entropy coding

25 Entropy coding algorithms aim to reduce data size and reach the limit of entropy for
 26 any kind of input, provided the probability distribution of the possible symbols. All of
 27 these algorithms work in a similar way, as their aim is to represent the symbols of the
 28 input data by codewords in a way to minimize the overall length of the data. Variable
 29 length codes for example replace the more common symbols with short codewords, while
 30 for less frequent symbols they use longer codewords. The ideal length of a codeword for
 31 symbol A is actually equal to $I(A)$, as this was the definition of self-information.

Table 2.1: Examples of a random binary code (#1) and a prefix-free binary code (#2). Code #2 is uniquely decodable, while for code #1 it's necessary to introduce boundaries between codewords to be able to distinguish them.

Letter	Code #1	Code #2
a_1	0	10
a_2	11	11
a_3	00	00
a_4	10	010
a_5	111	011

1 **Prefix-free codes**

2 Fix length codes have the convenience that there is no need to indicate the boundaries
3 between them, as they are all the same length (*e.g.* 8 bits for ASCII codes). For variable
4 length codes, as the name implies this is not possible, which necessitated the development
5 of various strategies to demarcate these codewords.

6 One way to indicate the end of a codeword is by using a specific delimiting se-
7 quence which is not part of any of the codewords. While this is an obvious solution, it is
8 also wasteful, as these sequences will not contain any information regarding the original
9 source. Prefix-free codes were developed to be able to omit these sequences, while still
10 allowing unique decodability, making them very popular. This is achieved by making
11 sure that once a codeword was assigned, no other codeword would start with that se-
12 quence. In other words, no codeword is a prefix of another codeword, hence the name
13 of the technique. During decoding the bits are read until a valid codeword is matched.
14 Since it is guaranteed that no other codeword will start with the same sequence, the
15 decoder can record the symbol corresponding for that codeword, and continue reading
16 the compressed stream.

17 Let's take the example in Table 2.1. Five letters are coded in binary code by Code
18 #1 and by Code #2. Code #1 is not a prefix code, and because of this when reading the
19 encoded sequence we can not be sure when we reach the end of a codeword. Decoding
20 the sequence 0000 for example could be interpreted as 4 letters of a_1 or 2 letters of a_3 .
21 For Code #2 it is clear that the sequence decodes to 2 letters of a_3 .

22 **Huffman coding**

23 Huffman coding is a prefix-free, optimal code that is widely used in data compression.
24 It was developed by David A. Huffman as a course assignment on the first ever course
25 on information theory at MIT, and was published shortly afterwards [100]. It is able to
26 achieve optimal compression in a sense that no other prefix-free codes will produce a
27 shorter output. Due to its simplicity combined with a good compression ratio it is still

Table 2.2: Letters to be Huffman coded and their probabilities.

Letter	Probability	Codeword
a_2	0.4	$c(a_2)$
a_1	0.2	$c(a_2)$
a_3	0.2	$c(a_2)$
a_4	0.1	$c(a_2)$
a_5	0.1	$c(a_2)$

¹ widely used in many compression algorithms, such as in JPEG, bzip2, or DEFLATE
² (zip) [94].

³ The Huffman coding procedure is based on two observations regarding optimal and
⁴ prefix-free codes:

- ⁵ 1. For a letter with higher frequency the code should produce shorter codewords, and
⁶ for letters with lower frequency it should produce longer codewords.
- ⁷ 2. In an optimum code, the two least frequent codewords should have the same
⁸ lengths.

⁹ From these statements it is trivial to see that the first is correct. If the more frequent
¹⁰ letters would have longer codewords than the less frequent letters, the average codeword
¹¹ length (weighted by the probabilities) would be larger than in the opposite case. Thus,
¹² more frequent letters must not have longer codewords than less frequent letter.

¹³ The second statement at first glance might not be so intuitive, so let's consider the
¹⁴ following situation. Let's assume that the two least frequent codewords do not have
¹⁵ the same lengths, and least frequent is longer. However, because this is a prefix code,
¹⁶ the second longest codeword is not a prefix of the longest codeword. This means, if
¹⁷ we truncate the longest codeword to the same length as the second longest, they will
¹⁸ still be distinct codes and uniquely decodable. This way we have a new coding scheme
¹⁹ which requires less space on average to code the same sequence as the original code, from
²⁰ which we can conclude the original code was not optimal. Therefore, for an optimal code,
²¹ statement 2 must be true.

To construct such a code, the following iterative procedure can be used. Let's consider an alphabet with five letters $A = [a_1, a_2, a_3, a_4, a_5]$ with $P(a_1) = P(a_3) = 0.2$, $P(a_2) = 0.4$ and $P(a_4) = P(a_5) = 0.1$ (Table 2.2). This distribution represents a source with 2.122 bits/symbol. Let's order the letters by probability, and consider the two least frequent. Since the codewords assigned to these should have the same lengths, they can be assigned as

$$c(a_4) = \alpha_1 * 0 \\ c(a_5) = \alpha_1 * 1$$

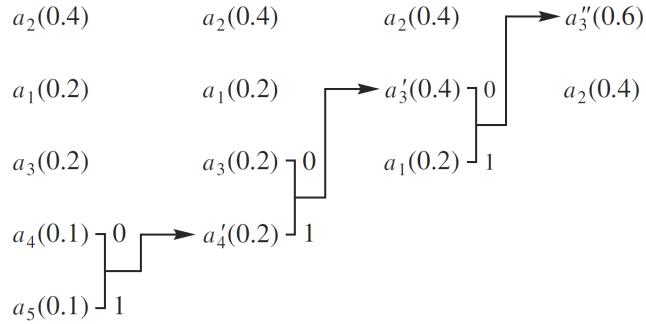


Figure 2.1: Building the binary Huffman tree. The letters are ordered by probability, these will be the final leaves of the tree. To create the branches, at every iteration we join the two nodes with the smallest probability, and create a new common node with the sum of the probabilities. This process is continued until all nodes are joined in a root node with probability of 1. Now, if we traverse down the tree to each leaf, the codeword will be defined by their position.

Table 2.3: Huffman code table.

Letter	Probability	Codeword
a_2	0.4	1
a_1	0.2	01
a_3	0.2	000
a_4	0.1	0010
a_5	0.1	0011

where $c(a_i)$ is the assigned codeword for letter a_i and $*$ denotes concatenation. Now we define a new alphabet A' with only four letters a_1, a_2, a_3, a'_4 , where a'_4 is a merged letter for a_4 and a_5 with the probability $P(a'_4) = P(a_4) + P(a_5) = 0.2$. We can continue this process of merging the letters until all of them are merged and we have only one letter left. Since this contains all of the original letters, its probability is 1. We can represent the end result in a binary tree (see Figure 2.1), where the leaves are the letter of the alphabet, nodes are the merged letters, and the codewords are represented by the path from the root node to each leaf (compare with Table 2.3). The average length of this code is

$$l = 0.4 \times 1 + 0.2 \times 2 + 0.2 \times 3 + 0.1 \times 4 + 0.1 \times 4 = 2.2 \text{ bits/symbol} \quad (2.3)$$

10 The efficiency of a code can be measured by comparing the average code size to the
11 entropy of the source. For this example, the difference is 0.078 bits/symbols. As the
12 Huffman code operates in base 2, it will produce a code with zero redundancy when the
13 probabilities are negative powers of 2.

1 Limitations of Huffman coding

2 Although the Huffman code is optimal among variable length codes, for certain types of
3 data it can have poor compression ratio. This limit lies in the fact that the length of the
4 shortest code assignable is one. For certain types of data with very low entropy this will
5 result in a relatively high redundancy. Arithmetic coding offers an alternative here, as
6 contrary to Huffman coding it does not rely on substituting symbols with codewords, and
7 thus can compress very low entropy data with minimal redundancy. This coding method
8 maps the whole message to a single number with arbitrary precision in the interval of 0
9 to 1. A more detailed description of arithmetic coding in given in [93].

10 Another alternative for compressing very low entropy data is run-length encoding.
11 This coding method assumes that the same character appears in the message many times
12 consecutively, and instead of storing each of these individually it counts the number of
13 identical symbols in a single run, and encodes the run-length together with the symbol.
14 As this strategy is only efficient for very low entropy data, it is a common practice to
15 combine run-length encoding with Huffman coding to construct a low redundancy coder
16 for a wide range of input data.

17 2.3 Decorrelation

18 Since entropy coding doesn't assume anything about the data structure, it is not capable
19 of recognizing and compressing any regular patterns or correlations between the consec-
20 utive data points. To maximize the efficiency of compression, any correlations should be
21 removed from the data before it is fed to the entropy coder. Here we will briefly discuss
22 some decorrelation strategies for image compression that aim to improve the performance
23 of a successive entropy coder.

24 Transform coding

25 Very popular methods for decorrelation are the transformations that represent the data
26 as a decomposition of orthonormal functions. One of the most common of these trans-
27 formations is the Fourier transform, that represents a periodic signal as a sum of sine and
28 cosine functions. As most natural images are of continuous tone, the idea behind this is
29 that most of the information will be captured by just a few Fourier coefficients. Because
30 of this, compressing the coefficients with an entropy coder should result in a smaller
31 output than encoding the original data.

32 For practical purposes, instead of the discrete Fourier transform (DFT), the discrete
33 cosine transform (DCT) [101] is usually used in image compression applications. This is
34 very similar to DFT, the difference being the periodic extension of the signal. In the DCT
35 transform, the image is mirrored on the sides instead of just repeating, to avoid large

1 jumps at the boundaries that may introduce unwanted high frequency components in the
 2 Fourier transform. If the image is extended in a symmetric way, the Fourier transform will
 3 be able to represent the data with only using cosine functions, hence the name discrete
 4 cosine transformations.

5 One drawback of frequency-based transformations, is that can't capture the spatial
 6 To overcome this limitation, the DCT is usually performed on small chunks of the image,
 7 such as on 8×8 blocks in the JPEG compression. The other option is to use non-periodic
 8 base functions to represent the signal. One good example for this is the use of wavelets,
 9 and based on this, the discrete wavelet transform (DWT) [102, 103].

10 As both DCT and DWT operate with floating point coefficients (although DWT has
 11 integer-based variants), the inverse transformation is not guaranteed to exactly recon-
 12 struct the original data. This is due to the finite machine precision of floating point
 13 numbers. Due to this fact these transformations are generally used in lossy compression
 14 algorithms and the coefficients are quantized based on the required image quality.

15 **Predictive decorrelation**

16 Another family of decorrelation methods is based on predicting the values of each data
 17 point (or pixel) depending on the context of the neighboring values. These techniques are
 18 based on differential pulse code modulation (DPCM), a decorrelation method originally
 19 used for audio compression. Here, before the data stream is entropy coded, a prediction
 20 is made for each value, which is equal to the preceding value. The difference to the
 21 prediction, called the prediction error, or prediction residual (ε) is passed to the entropy
 22 coder.

23 To see how why such an algorithm can increase compression ratio, let's consider the
 24 following sequence:

25	37	38	39	38	36	37	39	38	40	42	44	46	48
----	----	----	----	----	----	----	----	----	----	----	----	----	----

26 Although there is no obvious pattern in this sequence, there are no sharp jumps between
 27 the consecutive values, and this can be exploited by using a prediction scheme. Let's
 28 define the prediction $\text{Pred}(\cdot)$ for each element X_k to be equal to the preceding element.
 29 The prediction error would be $\varepsilon_k = X_k - \text{Pred}(X_k) = X_k - X_{k-1}$:

30	37	1	1	-1	-2	1	2	-1	2	2	2	2	2
----	----	---	---	----	----	---	---	----	---	---	---	---	---

31 As apparent from this new sequence, the number of distinct values are reduced, which
 32 means that fewer bits can represent this sequence than the original. When running these
 33 two sequences through an entropy coder, the error sequence will be much more com-
 34 pressed due to this property.

35 Using a predictive scheme to remove correlations from neighboring elements is a very
 36 good strategy for various applications, where this signal is only slowly changing. It has




Figure 2.2: Context for pixel prediction. X is the current pixel to be encoded and the previously encoded pixels are indicated with gray background. To allow for decoding, only the already encoded pixels are used for the prediction, typically the nearest neighbors (A, B, C, D).

1 been successfully implemented in audio and image compression algorithms as well, such
 2 as lossless-JPEG [104], JPEG-LS [105], CALIC [106], SFALIC [107] and FLIC [108], just
 3 to name a few.

4 For image compression, as the data is inherently multi-dimensional, the prediction
 5 rules can also be multi-dimensional, which can better capture the structure of the data,
 6 and achieve better decorrelation. For a typical encoding scenario, where the pixels are
 7 encoded one by one, the prediction can be based on the already encoded values (gray
 8 in Figure 2.2). This causality constraint is necessary in order to be able to decode the
 9 image.

10 Usually the nearest neighbors are used for the prediction, but this is not necessity;
 11 CALIC for example uses the second neighbors [106], and the third dimension can also
 12 be utilized if the data structure allows this, for example when encoding hyperspectral
 13 recordings [109].

The lossless part of the JPEG standard specifies 7 possible rules for the prediction step [104]:

$$\text{Pred}_1(X) = A$$

$$\text{Pred}_2(X) = B$$

$$\text{Pred}_3(X) = C$$

$$\text{Pred}_4(X) = A + B - C$$

$$\text{Pred}_5(X) = A + (B - C)/2$$

$$\text{Pred}_6(X) = B + (A - C)/2$$

$$\text{Pred}_7(X) = (A + B)/2$$

14 Depending on the patterns of the input image, some predictors can perform better than
 15 others. For general use, predictor 4 or 7 are recommended, as these are not direction
 16 dependent, and usually perform best. Predictor 7 is just the mean of the top and left
 17 neighbors, while predictor 4 assumes that the values for pixels A, B, C and X are on the

1 same plane, and calculates the prediction based on this.

2 Other algorithms try to improve the prediction by adapting it depending on the local
3 texture. The LOCO-I algorithm (part of JPEG-LS), for example uses the median edge
4 detector [105]:

$$\text{Pred}(X) = \begin{cases} \min(A, B) & \text{if } \geq \max(A, B) \\ \max(A, B) & \text{if } \leq \min(A, B) \\ A + B - C & \text{otherwise} \end{cases} \quad (2.4)$$

5 This function tries to estimate if there is an edge close to X. If it detects a vertical edge
6 to the left of X, it picks B for the prediction, while if it detects a horizontal edge above
7 X it tends to pick A. If no edge is detected, the prediction is the same as predictor 4 of
8 the lossless JPEG standard.

9 A useful property of the prediction based methods is, that there is no base change as in
10 the transform coding methods, and it is possible to construct bounded lossy compression
11 algorithms. JPEG-LS, for example defines a near-lossless mode of operation, where the
12 user can select the maximum absolute reconstruction error per pixel. This is achieved by
13 quantizing the prediction residual ε with a quantization step depending on the allowable
14 error. Since the decoding algorithm simply calculates $\hat{X} = \text{Pred}(X) + \varepsilon$, any quantization
15 error of ε is directly reflected in the reconstructed pixel value. Since the quantization
16 error is known, and bounded by the quantization step size, the maximum reconstruction
17 error for each pixel is also bounded. This mode is sometimes used for medical imaging
18 applications, where the preservation of diagnostic quality is required by law, but higher
19 compression ratios are desired than what is possible by lossless compression.

¹ Chapter 3

² Dual Mouse-SPIM

³ Unraveling the secrets of mammalian development has been a long standing challenge
⁴ for developmental biologists and medical professionals alike. This phase of early life is
⁵ an incredibly complex and dynamic process spanning through large scales in space and
⁶ time. Subcellular processes at the nanoscale are happening in the range of milliseconds
⁷ or faster, while whole embryo reorganizations and tissue migration events take place over
⁸ the course of hours [110]. Resolving these processes presents a true challenge, since to
⁹ understand the underlying mechanisms, molecular specificity is just as crucial as high
¹⁰ spatial and temporal resolution. As we have seen in Chapter 1, live imaging of mouse
¹¹ embryonic development is an especially challenging task, but light-sheet microscopy can
¹² offer a good solution owing to its gentle optical sectioning and fast image acquisition.
¹³ The Mouse-SPIM [J2] introduced in the previous chapter also solves the issue of live
¹⁴ imaging with its inverted design: the embryos are held by a foil that not only allows easy
¹⁵ sample handling, but also acts as a barrier and isolates the embryos from the immersion
¹⁶ medium.

¹⁷ As all microscopes, the Mouse-SPIM also had to make a compromise: although its
¹⁸ design allows long term live imaging, it only has a single detection view, as rotation is
¹⁹ not possible with the sample mounting trays. Due to this configuration, its resolution is
²⁰ inherently anisotropic, having an axial to lateral resolution ratio of around 3. Although
²¹ this is sufficient for many applications, such as cell tracking, for detecting subcellular
²² features it might be limiting. One such example is chromosome tracking, which could shed
²³ light on chromosome missegregation mechanisms in the early embryonic development,
²⁴ which is the cause of many congenital diseases also affecting humans.

²⁵ In this chapter, we present a novel light-sheet microscope developed to address the
²⁶ above challenges by using high NA objectives for subcellular isotropic resolution and low-
²⁷ light imaging, and offering multi-view detection without having to rotate the samples.
²⁸ The microscope is designed to be live imaging compatible, offering new perspectives
²⁹ in the research of mouse embryonic development. This chapter will describe the design

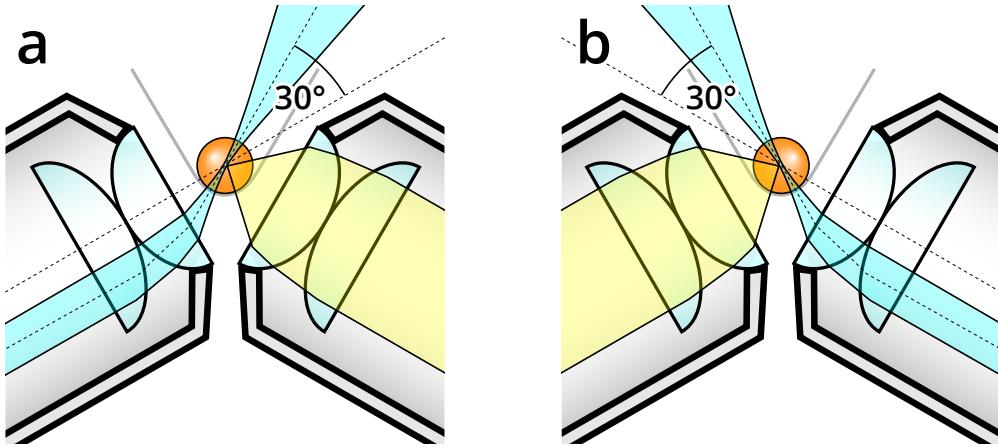


Figure 3.1: Dual view concept with high NA objectives. To achieve multi-view detection while maximizing resolution and light collection efficiency, two high NA objectives are placed in 120° arrangement. The sample (orange) is held from below by a thin FEP foil. To be able to overlap the light-sheet with the focal plane, the light-sheet is tilted 30°. The objectives are used in an alternating sequence for illumination and detection.

- 1 concepts for the microscope, the optical layout, alignment strategies, and the result of
- 2 various performance measurements, and its multi-view imaging capabilities.

3.1 Microscope design concept

4 As the limiting factor for subcellular imaging with the original Mouse-SPIM is the poor
 5 axial resolution relative to the lateral, our first aim was to increase the axial resolution
 6 to ideally reach the lateral resolution. A common way to reach isotropic resolution is
 7 to image a specimen from multiple directions, and combine the resulting images by
 8 multi-view deconvolution [28, 111, 112]. This has the benefit that the high resolution
 9 information from one view can complement the low axial resolution of the other view,
 10 thus providing better resolution in all three directions.

11 As described in the previous chapter, many SPIM implementations allow for recording
 12 multiple views either by rotating the sample, or by surrounding the sample with multiple
 13 objectives that are used for detection (Figure 1.10). For our setup, following the sample
 14 mounting technique of the original Mouse-SPIM, we wanted to keep the open-top sample
 15 mounting possibility, as this was proven to be highly compatible with mouse embryo
 16 imaging. To be able to achieve multi-view detection in this configuration, we designed a
 17 setup where both objectives can be used for illumination and detection in a sequential
 18 manner, inspired by previous symmetrical SPIM designs [43, 113].

19 To achieve the highest possible resolution from two views, the core of our design is
 20 based on the symmetric arrangement of two Nikon CFI75 Apo LWD 25x water dipping
 21 objectives, with a numerical aperture of 1.1. Due to the large light collection angle of
 22 these objectives, we arrange them in 120° instead of the conventional 90° used for light-

3.1 Microscope design concept

sheet imaging. As the light-sheet still needs to coincide with the imaging focal plane of the objectives, we tilt the light-sheets by 30° (Figure 3.1). Due to the low NA of the light-sheet, this is possible without affecting illumination quality.

This 120° arrangement has several benefits when compared to the traditional 90° configuration. When placing the objectives in 90°, the largest possible light collection half-angle for an objective can be $\alpha_{max,90} = 45^\circ$, and the corresponding NA is $NA_{max,90} = n \cdot \sin \alpha_{max,90} = 0.94$, where $n = 1.33$ the refractive index of water. Considering that this is an idealized case, the practically available highest NA is only 0.8. For a 120° arrangement, the theoretical maximum is $NA_{max,120} = n \cdot \sin(120^\circ/2) = 1.15$, with a practical maximum NA of 1.1.

Although the resolution won't be completely isotropic when combining the images from two 120° views (Figure 3.2), as it is for 90° views, due to the higher maximum NA possible, the resolution can be higher in the 120° case. When simulating the combined multi-view PSFs (Figure 3.2), for 0.8 NA objectives in 90° the axial and lateral resolutions are both 317 nm; while for two 1.1 NA objectives in 120° the axial resolution will be identical, 317 nm, and the lateral will be better, 193 nm.

Although this difference in resolution may seem marginal, the 120° configuration has another advantage in light collection efficiency. Collecting as much of the fluorescence signal as possible is crucial in live imaging applications, due to the limited available photon budget (see Figure 1.1 and [8]). Collecting more light from the sample allows to image faster with the same contrast, or to reduce the illumination power and maintain the imaging speed. As light collection efficiency depends on the solid angle subtended by the detection lens, (see Appendix Section C), a 1.1 NA objective can collect twice as many photons as a 0.8 NA objective, which gives the 120° setup a clear edge in low-light imaging.

3.1.1 Light-sheet design

To allow for flexibility in the field of view height, even illumination, reduced stripes, and potential for confocal line detection, we opted to use the beam scanning technique to generate a virtual light-sheet. The effective focal length of the Nikon 25x objective, given the 200 mm focal length tube lens is

$$f_o = \frac{f_{tl}}{M} = \frac{200 \text{ mm}}{25} = 8 \text{ mm}, \quad (3.1)$$

and the back aperture diameter is 17.6 mm.

To generate the tilted light-sheet as shown on Figure 3.1, the illumination beam will need to be displaced by

$$\delta = f_o \cdot \tan 30^\circ = 4.62 \text{ mm} \quad (3.2)$$

3.1 Microscope design concept

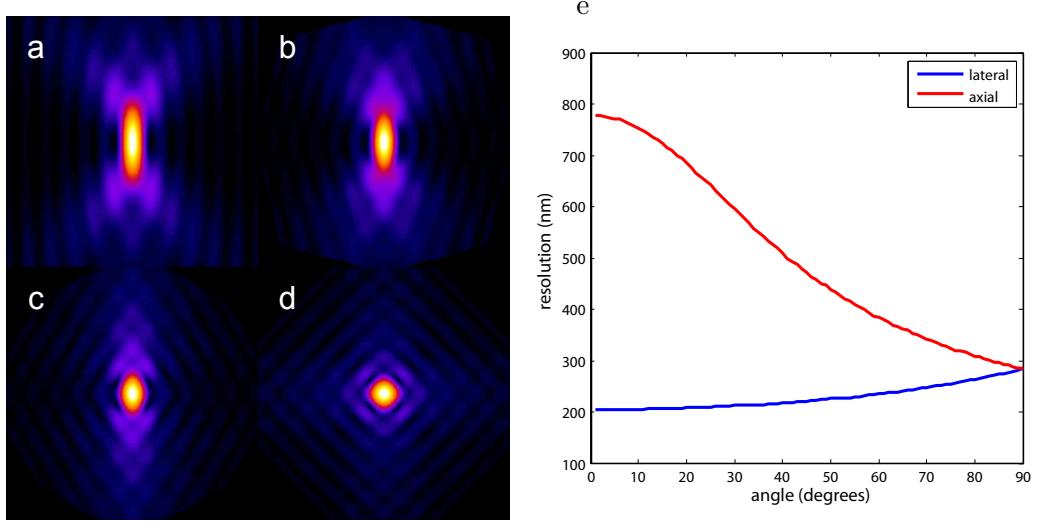


Figure 3.2: Lateral and axial resolution of a multi-view optical system. a) Simulated PSF for a single view. b)–d) Simulated compound PSF of two views aligned in b) 30, c) 60 and d) 90 degrees to each other. e) Axial and lateral resolution of a dual-view setup depending on the rotation angle of the two objectives. Parameters used for calculations: NA=1.1, $\lambda_{ex} = 488\text{nm}$, $\lambda_{det} = 510\text{nm}$, $n = 1.333$ for water immersion.

Since the Gaussian beam is not uniform, only a smaller portion of it can be used to maintain even illumination (Figure 1.12c). Because the size of an early mouse embryo is around $80\text{ }\mu\text{m}$, we require the length and the height of the light-sheet to be at least $100\text{ }\mu\text{m}$.

The length and thickness of the light-sheet

As we saw in Section 1.3.1, the length of the light-sheet is determined by the Rayleigh-range of the beam in the zy plane. Since $l_{fov} = 2 \cdot z_R = 100\text{ }\mu\text{m}$

$$z_R = 50\text{ }\mu\text{m} \quad (3.3)$$

Since the Rayleigh range and the diameter of the beam waist are coupled, the light-sheet thickness can be calculated after rearranging Equation 1.20

$$2 \cdot W_0 = 2 \cdot \sqrt{\frac{z_R \cdot \lambda}{\pi}} = 5.57\text{ }\mu\text{m} \quad (3.4)$$

when $\lambda = 488\text{ nm}$ for GFP excitation. As the beam width for these calculations is defined as $1/e^2$ of the peak intensity, we also calculate the more commonly used full width at half maximum (FWHM):

$$\text{FWHM} = W_0 \cdot \sqrt{2 \ln 2} = 3.28\text{ }\mu\text{m.} \quad (3.5)$$

¹ From this, the divergence angle of the beam is

$$\theta_0 = \frac{\lambda}{\pi W_0, y} = 55.74 \text{ mrad} = 3.196^\circ \quad (3.6)$$

² This means, the numerical aperture needed to produce this light-sheet is:

$$\text{NA}_{ls} = n \cdot \sin(\theta_0) = 0.0743 \quad (3.7)$$

³ Since $\text{NA} = 1.1$, and the diameter of the back aperture is $d = 17.6 \text{ mm}$ and the divergence
⁴ angle $\theta_0 \ll 1$, using paraxial approximation, the necessary beam width at the back focal
⁵ plane in the y direction is

$$b_y = d \cdot \frac{\text{NA}_{ls}}{\text{NA}} = 1.19 \text{ mm} \quad (3.8)$$

⁶ Thus, to generate a light-sheet with appropriate length to cover a whole mouse pre-
⁷ implantation embryo, the laser beam diameter should be $b = 1.19 \text{ mm}$. Larger than this
⁸ will result in a more focused beam and a shorter light-sheet, while a smaller diameter
⁹ beam will have worse optical sectioning capabilities.

¹⁰ **The height of the light-sheet**

¹¹ The height of the light-sheet can be adjusted by changing the beam scanning am-
¹² plitude with the galvo mirror. To scan the entire field of view of $h_{FOV} = 270 \mu\text{m}$,
¹³ the scanning angle range at the back focal plane of the objective will need to be
¹⁴ $\theta = \tan^{-1}(h_{FOV}/2/f_o) = \pm 0.967^\circ$.

¹⁵ **3.2 Optical layout**

¹⁶ Based on the requirements and other considerations shown in the previous section, the
¹⁷ microscope was designed in three main parts: 1) the core unit, 2) illumination and 3)
¹⁸ detection branches. The aim when integrating these units together was to allow for high
¹⁹ level of flexibility with robust operation, while also keeping efficiency in mind. After
²⁰ finalizing the concept, the optical layout of the microscope was designed in SolidWorks.

²¹ **3.2.1 Core unit**

²² As the most important part of the microscope is actually the sample, the design is based
²³ around a core consisting of the imaging chamber and the objectives (Figure 3.3). Also
²⁴ part of the core are two mirror blocks placed at the back of the objectives, and three
²⁵ custom designed rings to hold the objectives in place. The objectives are pointing slightly
²⁶ upwards, closing a 60° angle with the horizontal plane, and 120° angle with each other.

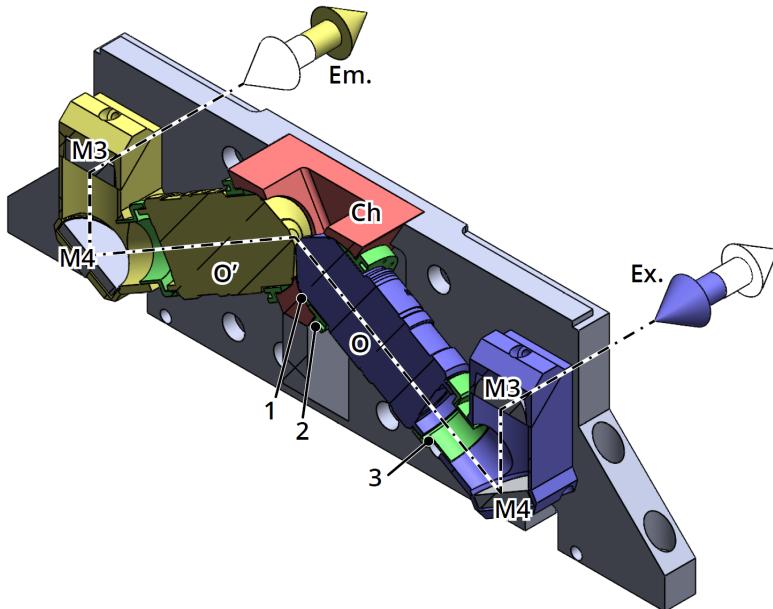


Figure 3.3: The core unit of the microscope. The two objectives (O and O') are mounted on a solid 15 mm thick aluminium plate. Fitting on the objectives, a custom chamber (Ch) is holding the immersion medium for imaging. The mirror block with mirrors $M3$ and $M4$ directs the light to 65 mm optical rails. Excitation (Ex.) and emission (Em.) light paths are indicated by the dash-dot line. Due to the symmetric arrangement, the excitation and illumination paths can be switched around. Objectives are secured with rings 1–3 (green, see main text for details).

¹ Chamber

The chamber serves two purposes: it holds the immersion liquid necessary for imaging, and it also keeps the objectives in the 120° position. The objectives are held by their necks as opposed to the standard mounting method from the back by the threads. The advantage of this is that any axial movements due to thermal expansion are greatly reduced, thus the focal plane position is more stable even when changing the imaging conditions.

The chamber is machined from a high performance plastic, polyether ether ketone (PEEK). This material has many beneficial properties: it is food safe, and chemically extremely inert, resisting to most solvents used in a biology laboratory. Due to these properties, PEEK is live imaging compatible, even for sensitive samples, as it can also be autoclaved. Compared to other plastics its mechanical properties are also superior. It has high tensile and compressive strength, comparable to aluminium, low thermal expansion and low thermal conductivity. This can be beneficial when implementing temperature control, as thermal loss is reduced.

The objectives are kept in place by two custom designed rings (Figure 3.3 1, 2). The first ring has a cross sectional shape of a wedge, and sits tightly against both the objective and the wall of the chamber. The second ring can freely slide on the objective, and has threads matching the chamber. When turned in, the threaded ring pushes the

1 wedge ring further in, which in turn presses against the objective and the chamber wall
2 uniformly, thus preventing the objective from moving, and sealing the chamber at the
3 same time. As the wedge ring is made from a soft plastic (delrin), it will press evenly
4 against the objective preventing any damage. Given the conical shape of the ring, it will
5 also automatically center the objective, ensuring correct positioning.

6 To relieve any rotational stresses from the objective, the back of the objective is also
7 supported by the mirror block, this is not fixed, however. A third ring, made of PEEK
8 is threaded on the objective, and slides in the opening of the mirror block. This reduces
9 the torque on the objectives, while still allowing for some movements that might occur
10 due to thermal expansion.

11 **Mirror blocks**

12 Apart from supporting the objectives from the back, the mirror blocks are housing two
13 broadband dielectric mirrors (Thorlabs, BBE1-E03 and OptoSigma, TFMS-30C05-4/11)
14 to direct the light to and from the objectives on a standard 65 mm height, compatible
15 with the Owis SYS65 rail system. The combination of two mirrors have two benefits
16 compared to using just one. With a single mirror directly reflecting the light to the back,
17 the entire assembly would need to be much higher to reach the desired 65 mm height.
18 This could result in stability problems. Furthermore, due to the 60° rotation angle of the
19 objective, the image of the objective would also be rotated if using only a single mirror.
20 With two mirrors the reflection planes can be kept orthogonal to the optical table, which
21 will result in a straight image after the mirror block. This is not only beneficial when
22 recording the images, but also when aligning the illumination arm. With the use of two
23 mirrors, a convenient vertical scanning is required to produce the light-sheet; with a
24 single mirror, the scanning direction would need to be rotated by 60°.

25 **3.2.2 Illumination**

26 The illumination arm of the microscope directs and shapes the laser beam to generate
27 the proper light-sheet dimension at the sample. As was calculated in Section 3.1.1, a
28 beam diameter of 1.2 mm is ideal for this setup.

29 The illumination arm has three main roles:

- 30 1. expands the laser beam to the calculated 1.2 mm size.
- 31 2. images the galvo scanner to the back focal plane of the objective
- 32 3. switches the laser light between the two objectives during imaging

33 To achieve the desired beam diameter, a 1:2 beam expander (Sill Optics, 112751) is
34 used in the reversed direction. As the output of the laser fiber produces a 3 mm diameter

3.2 Optical layout

beam, this will reduce it to 1.5 mm. As this is already the required beam diameter, the lenses further in the illumination path will not introduce any magnification.

Switching between the two illumination arms is performed by a custom designed beam splitter unit (Figure 3.4). Instead of utilizing a 50/50 beam splitter cube and mechanical shutters, we exploit the fact that a galvo scanner is needed to generate the light-sheet. As this galvo scanner (Cambridge Technology, 6210B) has a relatively large movement range ($\pm 20^\circ$) it is also suitable for diverting the beam from one illumination arm to the other.

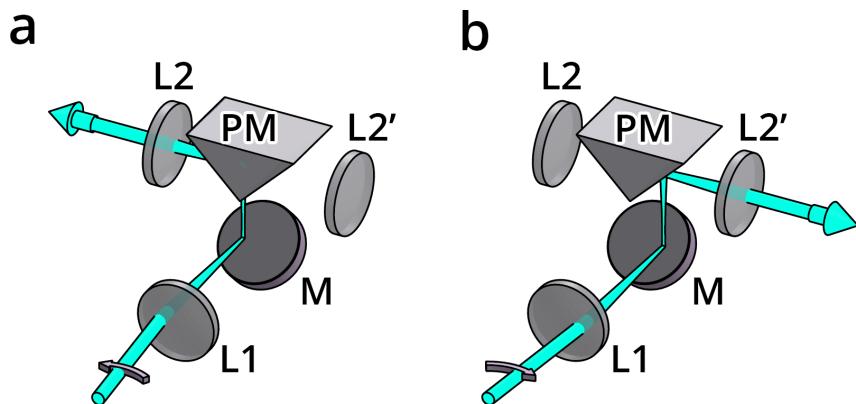


Figure 3.4: Illumination branch splitting unit. To divert the beam to either side, a right angle prism mirror is used in conjunction with a galvanometric scanning mirror. L1 acts as a scan lens, thus the beam is translated on mirror M. Depending on the galvo angle, the beam will be reflected either to the left (a) or to the right (b). L2 and L2' act as relay lenses, and will image the galvo movement to intermediate planes.

Switching illumination side is done the following way. As the galvo is positioned at the focus of the first lens (L1, $f_1 = 75$ mm, Edmunds Optics, #47-639), the rotational movement will result in a linear scanning movement on mirror M and the prism mirror PM (Figure 3.4). Depending on the lateral position of the beam, it will hit either the left or the right leg of the prism (Thorlabs, MRAK25-E02), and will be reflected to either direction. As the galvo mirror can be precisely controlled through our custom software, we can set and save the position when the beam is centered on the left lens L2 ($f_2 = 75$ mm, Edmunds Optics, #47-639) (Figure 3.4a) and the position when the beam is centered on the right lens L2' (Figure 3.4b). Lenses L1 and L2(L2') form a 4f system, and are imaging the galvo scanner on mirror M1(M1') (Figure 3.5). This way we can use the same galvo to generate the light-sheet for both directions, depending on the initial offset position. This not only has the advantage of being able to electronically switch the illumination arms, but only requires a single galvo scanner instead of one for each arm.

Due to the arrangement of the bottom mirror and the prism mirror, the scanning direction will be rotated by 90° . This will result in a vertical scanning plane, which is exactly what we need to generate the light-sheet on the sample (see Section 3.2.1).

1 Further following the illumination path, two achromatic lenses L3 and L4 ($f_3 = f_4 =$
2 200 mm), in a 4f configuration relay the scanning axis to the back focal plane (BFP) of
3 the objective. To couple in the laser with the imaging path, a quad-band dichroic mirror
4 (DM, Semrock, Di03-R405/488/561/635-t3-25x36) is used, matching the wavelengths of
5 the laser combiner.

6 3.2.3 Detection

7 As the emitted light exits the objective and the mirror block, it is decoupled from the
8 illumination path by the dichroic mirror. The light is then focused by a 400 mm achro-
9 matic lens (L5, Edmunds Optics, #49-281) onto the camera sensor (Andor Zyla 4.2
10 sCMOS). Just before the camera, a motorized filter wheel (F, LEP 96A361) is placed to
11 discriminate any unwanted wavelengths from the emission light. Although this is not in
12 the infinity space, due to the very small angles after the 400 mm tube lens, the maximum
13 axial focal shift is ~ 50 nm only, which is negligible compared to the axial resolution of
14 ~ 1.1 μm .

15 Similarly to the common galvo in the illumination path, the two detection arms
16 share the same camera. Although two cameras could also be used, due to the operating
17 principle of the microscope, the two objective are not used for imaging at the same time.
18 This means a single camera is capable of acquiring all the images, however, the two
19 distinct detection arms need to be merged to be able to use a single detector.

20 Our solution to this problem is a custom designed view switching unit comprised of
21 two broadband dielectric elliptical mirrors (Thorlabs,BBE1-E03) facing opposite direc-
22 tions, mounted on a high precision linear rail (OptoSigma, IPWS-F3090). Depending on
23 the rail position, either the left (Figure 3.6a) or the right (Figure 3.6b) detection path
24 will be reflected upwards, to the camera.

25 Moving the switcher unit is performed by a small, 10 mm diameter pneumatic cylinder
26 (Airtac, HM-10-040) that is actuated by an electronically switchable 5/2 way solenoid
27 valve (Airtac, M-20-510-HN). This solution offers a very fast switching between views,
28 up to 5 Hz, depending on the pressure, and it is extremely simple to control, as only a
29 digital signal is necessary to switch the valve.

30 3.3 Optical alignment

31 Precise alignment of the illumination and detection paths are crucial for high quality
32 imaging, and has a pronounced importance for high magnification and high resolution
33 optical systems. Due to the symmetrical setup of the microscope, we will only describe
34 the alignment of one side, as the same procedure is also applicable to the other side.
35 References to optical components will be as defined on Figure 3.5.

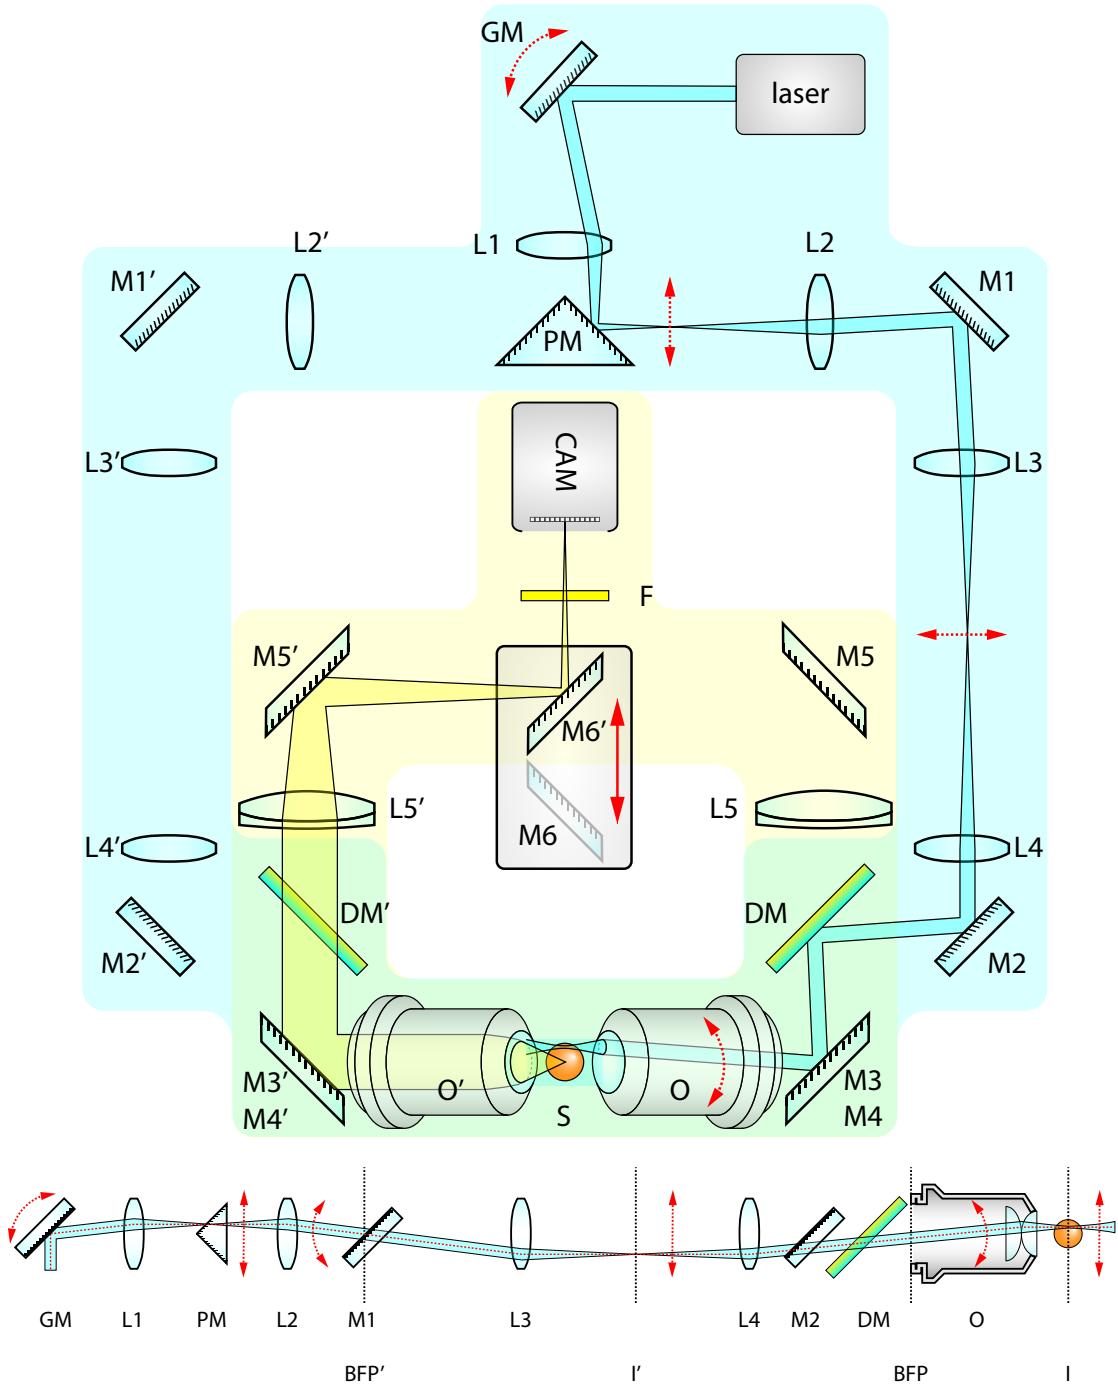


Figure 3.5: Dual Mouse SPIM optical layout. The microscope consists of two main parts, the illumination branches (blue) and detection branches (yellow). For both illumination and detection there are two identical paths implemented. Illumination direction can be changed by applying a different offset to the galvo mirror, which in turn will direct the beam to the opposite face of the prism mirror. L1 and L2 will then image the galvo on M1. Using L3 as a scan lens, and L4 as a tube lens, the scanned beam is coupled to the objective path by quad band dichroic mirror (DM) CAM – camera, DM – dichroic mirror, F – filter wheel, L – lens, M – mirror, O – objective, PM – prism mirror, S – sample

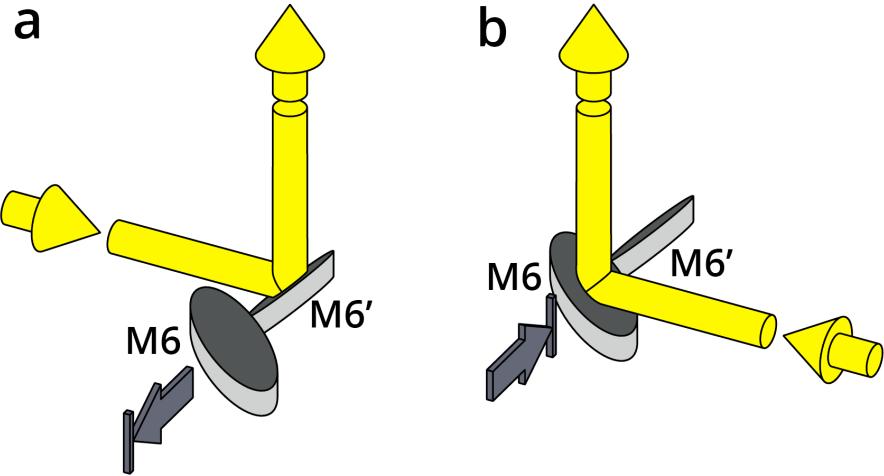


Figure 3.6: Detection branch switching unit. To be able to image both views on the same camera, a moveable mirror unit is introduced. Depending on the imaging direction, the mirror block is either moved backward (a) or forward (b) to reflect the light up to the camera. Since the movement is parallel to the mirrors' surface, the image position on the sensor is not dependent on the exact position of the mirrors.

1 3.3.1 Alignment of illumination branches

2 The two illumination branches start with a common light source, a single mode fiber
 3 coupled to laser combiner, and they also share a galvanometric mirror that performs the
 4 beam scanning to generate the virtual light-sheet. Likewise shared is a scan lens focusing
 5 on the galvo mirror (GM), and the illumination splitter unit (PM, see item 3.2.2).

6 Alignment for the illumination arms are done in three steps. First the laser beam
 7 is aligned on the first rail that holds the galvo, lens L1, and the splitter unit PM. This
 8 is performed by two kinematic mirrors placed between the fiber output and the galvo
 9 mirror (not shown on figure). Using these two mirrors it is possible to freely align the
 10 beam along all four degrees of freedom: translation in two orthogonal directions and
 11 rotation around two orthogonal axes. Beam alignment on the rail is tested by two irises
 12 at the two ends of the rail, if the beam passes through both of them we consider it
 13 centered and straight on the optical axis.

14 After the beam is aligned on the first rail, lens L1 and the splitter unit PM are placed
 15 in the measured positions to image the galvo mirror on mirror M1 using lenses L1 and
 16 L2. Correct positioning of the splitter unit along the rail is crucial, since this will affect
 17 the lateral position and tilt of the beam exiting the unit. To some extent, this can also
 18 be compensated by adjusting the two mirrors before the galvo mirror, but is avoided if
 19 possible as this will also displace the beam from the center of the galvo mirror.

20 After rough alignment of the illumination arms, when the laser is already coupled
 21 in the objective, the fine adjustments are performed based on the image of the beam
 22 through the other objective. The beam is visualized by filling the chamber with a 0.1%
 23 methylene blue solution. As this solution is fluorescent, and can be excited in a very large

1 range, it is well suited to visualize the beam during adjustment.

2 **Adjusting beam position** Beam position can be adjusted by either translating the
3 beam in a conjugated image plane (I'), or by rotating the beam in a conjugated back focal
4 plane (BFP'). The setup was designed in a way, that BFP' coincides with mirror M1.
5 This mirror is mounted in a gimbal mirror mount, allowing to rotate the mirror exactly
6 around its center, which avoids unwanted translational movements, and results in pure
7 rotation of the beam. Lens L3 is positioned exactly 1 focal length from the mirror, thus
8 acting as a scan lens, and transforming the rotational movements to translation. This
9 translation is further imaged and demagnified by the tube lens L4 and the objective O
10 onto the sample.

11 **Adjusting beam tilt** Beam tilt can be adjusted by either rotating the beam in an in-
12 termediate image plane (I'), or translating it at the back focal plane (BFP). As mirror M2
13 is relatively far from the back focal plane, adjusting this will mostly result in translation
14 that will rotate the beam. This movement, however, will also introduce translations, and
15 has to be compensated by adjusting mirror M1. As the light-sheet needs to be tilted by
16 30° to coincide with the focal plane of the other objective, this level of adjustment is not
17 possible with M2. In order to allow for a pure rotation of the light-sheet, we mounted the
18 dichroic mirrors on linear stages (OptoSigma, TSDH-251C). By translating the dichroic
19 mirror, the illumination laser beam gets translated at the back focal plane, which will
20 result in a pure rotational movement at the sample. Rough alignment of the light-sheet
21 is performed by adjusting the dichroic position while inspecting the light-sheet through
22 a glass window in the chamber. Precise alignment is afterwards done based on the image
23 of the beam visualized in a fluorescent medium.

24 **Adjusting scanning plane angle** After the beam is properly aligned, i.e. it is in focus
25 and in the center of field of view, it is still necessary to check if the scanning direction
26 is parallel to the imaging plane. It is possible that the beam is in focus in the center
27 position, but when moved up or down it drifts out of focus due to a tilted scanning
28 angle. This tilt can be compensated by mirror M1, that is placed at the conjugated back
29 focal plane BFP' . Between lenses L3 and L4 a magnified version of the light-sheet will
30 be visible, and the tilt can be checked by placing an alignment target in the optical path
31 while scanning the beam. By tilting mirror M1 up or down, the scanning pattern not only
32 moves up or down, but is also rotated if the mirror surface is not exactly vertical. Since
33 M1 and GM are in conjugated planes, the tilt and offset can be performed independently.
34 The tilt is first fixed by M1 while inspecting the target, and the beam is re-centered by
35 changing the offset on the galvo mirror. Moving the galvo mirror will not introduce tilt,
36 since in this case rotation axis is perpendicular to the reflection plane.

1 3.3.2 Alignment of detection branches

2 Since the detection path is equivalent to a wide-field detection scheme, its alignment is
3 much simpler than that of the illumination branches. The only difference is the detection
4 branch merging unit (see Section 3.2.3.) that features two moving mirrors. This, however,
5 doesn't affect the alignment procedure, since the movement direction is parallel to both
6 mirrors' surfaces, meaning that the exact position of the mirrors will not affect the
7 image quality, as long as the mirrors are not clipping the image itself. A stability test
8 was performed to confirm the consistent switching performance of the mirror unit before
9 the final alignment took place (see Section 3.5.1).

10 **Positioning the tube lens** The position of the tube lens determines the focal plane
11 that is being imaged on the camera sensor. Ideally, the tube lens' distance from the
12 camera sensor is exactly the tube lens' focal length, which will ensure the best imaging
13 performance. If the tube lens' distance is not correct, the focal plane will be slightly
14 shifted in the axial direction. Although small shifts will not necessarily have detrimen-
15 tal effect on the image quality, because the light sheet can also be shifted accordingly.
16 Because of the shifted focal and image planes, however, the magnification of the system
17 will be affected, and will change depending on the amount of defocus. For this reason we
18 aim for positioning the tube lens as close to the theoretical position as possible.

19 Our tube lens is a compound, achromatic lens with a center thickness of 12.5 mm, and
20 edge thickness of 11.3 mm. Its effective focal length is 400 mm which will produce a 50x
21 magnified image. Back focal length is 394.33 mm which we measured from the camera
22 chip, and the lens was positioned at this theoretically optimal position.

23 **Adjusting correction collar** The Nikon 25x objectives used for this setup have a
24 built in correction ring that can be used to correct spherical aberrations resulting from
25 refractive index differences when imaging samples behind a coverslip. This can be also
26 effectively used to correct for any spherical aberrations occurring from imaging through
27 the FEP foil. Although these aberrations are expected to be extremely low, due to the
28 relatively thin, 50 μm foil thickness, and the close matching of refractive index ($n_{FEP} =$
29 1.344, $n_{H_2O} = 1.333$), for optimal, aberration free image quality it can't be neglected.

30 The correction collars are adjusted by inspecting a gel suspended fluorescent bead
31 specimen with the microscope, where the beads can act as a reporter of the point spread
32 function of the microscope. The alignment can be performed "live" by inspecting the
33 bead image quality for any aberrations. By gradually changing the correction collar, the
34 ring artifacts are minimized on out-of-focus beads, and the peak intensity is maximized
35 for in-focus beads. By moving the correction ring, the focal plane is also slightly shifted,
36 which has to be compensated by shifting the light-sheet correspondingly to coincide with

1 the correct imaging plane.

2 **Adjusting field of view** To allow for proper sampling of the image, we use $50\times$ magnification, which combined with the $6.5\text{ }\mu\text{m}$ pixel pitch of our sCMOS camera, will result
3 in a $0.13\text{ }\mu\text{m}$ pixel size. The full field of view recorded by the camera is $2048 \times 0.13\text{ }\mu\text{m} =$
4 $266.24\text{ }\mu\text{m}$. To ensure the best image quality, we align the center of the objective field of
5 view on the camera sensor, since this region has the best optical properties in terms of
6 numerical aperture, aberration correction and field flatness.
7

8 Field of view alignment can be performed using mirror M4 just before the detection
9 merging unit. To identify the center region of the field of view, diffuse white light is
10 used to illuminate the entire sample chamber and is imaged on the camera. Then, mirror
11 M4 is adjusted until the top edge of the field of view becomes visible, *i.e.* where the
12 illumination from the chamber is clipped. This will have a circular shape. Afterwards,
13 adjusting the mirror in the orthogonal direction, the left-right position of the field of
14 view can be adjusted, by centering the visible arc on the camera sensor.

15 After the horizontal direction is centered, vertical centering is performed. This, how-
16 ever can't be centered the same way as the horizontal direction, since for that we would
17 have to misalign the already aligned horizontal position. To determine the center, we
18 move the field of view from the topmost position to the bottom. During this process
19 the number of turns of the adjustment screw is counted (this can be done accurately by
20 using a hex key). After reaching the far end of the field of view, the mirror movement is
21 reversed, and the screw is turned halfway to reach the middle.

22 3.4 Control unit

23 The microscope's control and automation is performed by an in-house designed modular
24 microscope control system developed in LabVIEW [113]. The core of the system is a
25 National Instruments cRIO-9068 embedded system that features an ARM Cortex A9
26 processor, and a Xilinx Zynq 7020 FPGA. Having both chips in the same device is a
27 great advantage, since the main processor can be used to run most of the microscope
28 control software, while the FPGA can be used to generate the necessary output signals
29 in real time and with high precision.

30 The embedded system is complemented by a high performance workstation that is
31 used to display the user interface of the microscope, and to record the images of the
32 high-speed scientific complementary metal–oxide–semiconductor (sCMOS) camera.

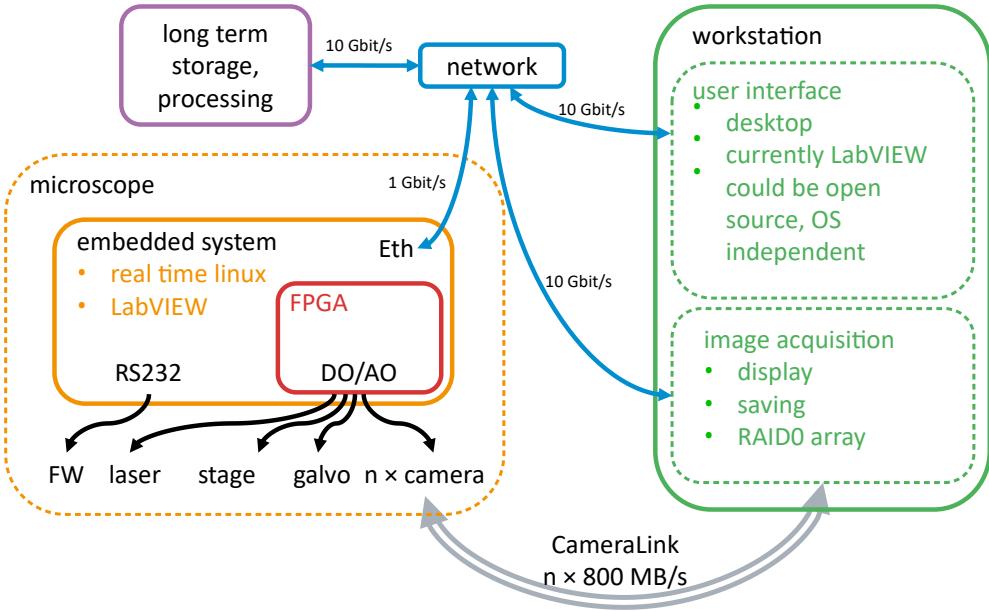


Figure 3.7: Microscope control hardware and software architecture. The embedded system responsible for the hardware control and the workstation are communicating through the network using the WebSocket protocol. The electronic devices of the microscope are either controlled through digital/analog signals, or through serial communication. The camera is also connected to the workstation with a CameraLink connection, which transmits the recorded images.

1 3.4.1 Hardware

2 Various components need to be synchronized with high precision to operate the mi-
 3 croscope: a laser combiner to illuminate the sample; a galvo scanner to generate the
 4 light-sheet; stages to move the samples; filter wheel to select the imaging wavelengths;
 5 and a camera to detect the fluorescence signal. For high speed image acquisition, all of
 6 these devices have to be precisely synchronized in the millisecond range, and some even
 7 in the microsecond range. Although they require different signals to control them, we
 8 can split them into three main categories:

digital input	analog input	serial communication
camera exposure	galvo position	filter wheel
laser on/off ($\times 3$)	laser intensity ($\times 3$)	stages ($\times 2$)

10 All devices are connected to the NI cRIO 9068 embedded system, either to the built
 11 in RS232 serial port, or to the digital and analog outputs implemented by C-series
 12 expansion modules (NI 9401, NI 9263, NI 9264). The workstation with the user interface
 13 is communicating with the embedded system through the network. The only device with
 14 a connection to both systems is the camera: the embedded system triggers the image
 15 acquisition, while the images are piped to the workstation through a dual CameraLink
 16 interface, capable of a sustained 800 MB/s data transfer rate (Figure 3.7).

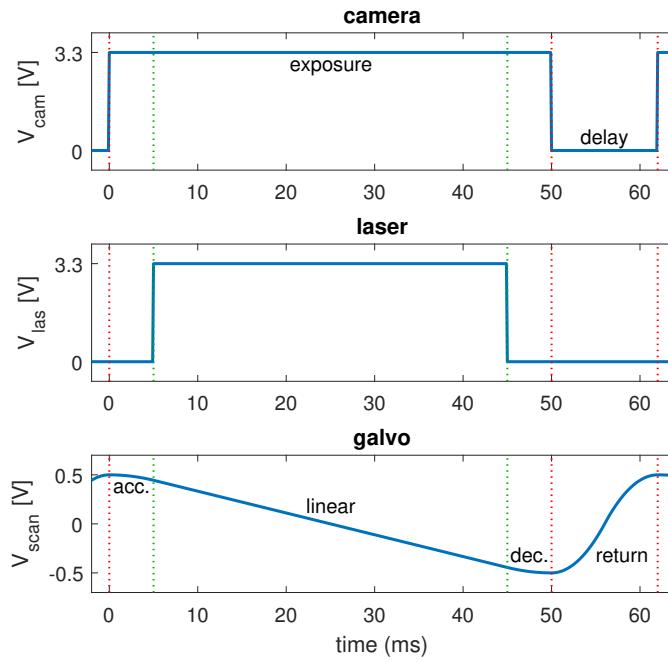


Figure 3.8: Digital and analog control signals. Example traces for recording a single plane with 50 ms exposure time and 12 ms delay. During the exposure of the camera the galvo has 3 sections: acceleration (acc.), linear, and deceleration (dec.). The laser line is synchronized with the galvo linear section to ensure even illumination.

1 3.4.2 Software

2 Being able to precisely control all of the instruments not only relies on the selected hardware,
 3 but just as much on the software. Our custom software is developed in LabVIEW,
 4 using an object oriented approach with the Actor Framework. The embedded system is
 5 responsible for the low level hardware control, for keeping track of the state of all devices,
 6 saving the user configurations, and automating and scheduling the experiments. It also
 7 offers a Javascript Object Notation (JSON) based application programming interface
 8 (API) through WebSocket communication. This is mainly used to communicate with the
 9 user interface, however it also offers the possibility of automated control by an external
 10 software.

11 **FPGA software**

12 The on-board FPGA is responsible for generating the digital and analog output signals
 13 based on the microscope settings (Figure 3.8). To avoid having to calculate all the traces
 14 for a whole stack, the main software only calculates a few key parameters of the traces
 15 that are necessary to completely describe them. The FPGA then calculates the signals
 16 in real time, and outputs them with microsecond precision.

17 To describe the traces, we define them as a concatenation of *sections*. Each section has
 18 3 or 5 parameters, depending on if their type is digital or analog. Both types have three

1 common properties: `value`, `length`, and `type`. The analog sections additionally contain a
2 `dValue` and a `ddValue` element describing the velocity and the acceleration of the signal.
3 This allows us to generate piecewise functions made of second order polynomials.

4 The `type` element contains information on which value should be updated for the
5 current section. Setting the lowest bit high will update the `value`, setting the second bit
6 high will update the `dValue`, and setting the third bit high will update the `ddValue`.
7 This feature allows to define smooth transitions between the sections, and also to define
8 more complex signals, as long as they are periodic in the second derivative.

9 3.5 Results

10 Following the design phase, all custom parts were manufactured by the EMBL mechanical
11 workshop, and microscope was assembled on a MellesGriot optical table (Figure 3.9 and
12 Figure D1). The microscope was equipped with an Andor Zyla 4.2 sCMOS camera, that
13 offers a large field of view of 2048×2048 pixels with a pixel pitch of $6.5 \mu\text{m}$. It offers
14 a high dynamic range of 1:30,000, and high frame rate at 100 frames per second (fps),
15 while readout noise is minimal (0.9 e^-).

16 To evaluate the performance of the microscope, we conducted various measurements,
17 concerning the stability and the resolution of the system. The methods and results of
18 these measurements will be presented in this section.

19 3.5.1 Stability of view switcher unit

20 As the view switcher unit is a custom designed solution for this microscope, it is necessary
21 to evaluate the effect of the switching on the field of view. Given that this is a moving
22 unit, many mechanical imprecisions can introduce a drift in the final image.

23 To assess the reproducibility in the movement of the detection branch switching unit,
24 a long term stability test was conducted. To exclude all other factors (such as sample
25 drift), we imaged the opening of two closed irises that were mounted on the detection
26 optical rail. Image formation was done by two achromatic lenses ($f = 75 \text{ mm}$) positioned
27 directly after mirrors M5 and M5'.

28 The apertures were imaged from both views every 10 seconds, for 4 h, for a total
29 of 1440 images per view, and 2880 switches. The center of the aperture was segmented
30 on all images using Matlab, and tracked to assess any drift occurring during the 4 h
31 time lapse (Figure 3.10). To visualize the uncertainty of the aperture's position, we
32 performed principal component analysis (PCA) on the positions and visualized the results
33 by plotting the 95% confidence ellipse on the images. Although the right view had a
34 significant spread with a standard deviation of 4.37 px and 2.26 px along the long and
35 short axes respectively, the left view was extremely stable, and the standard deviation

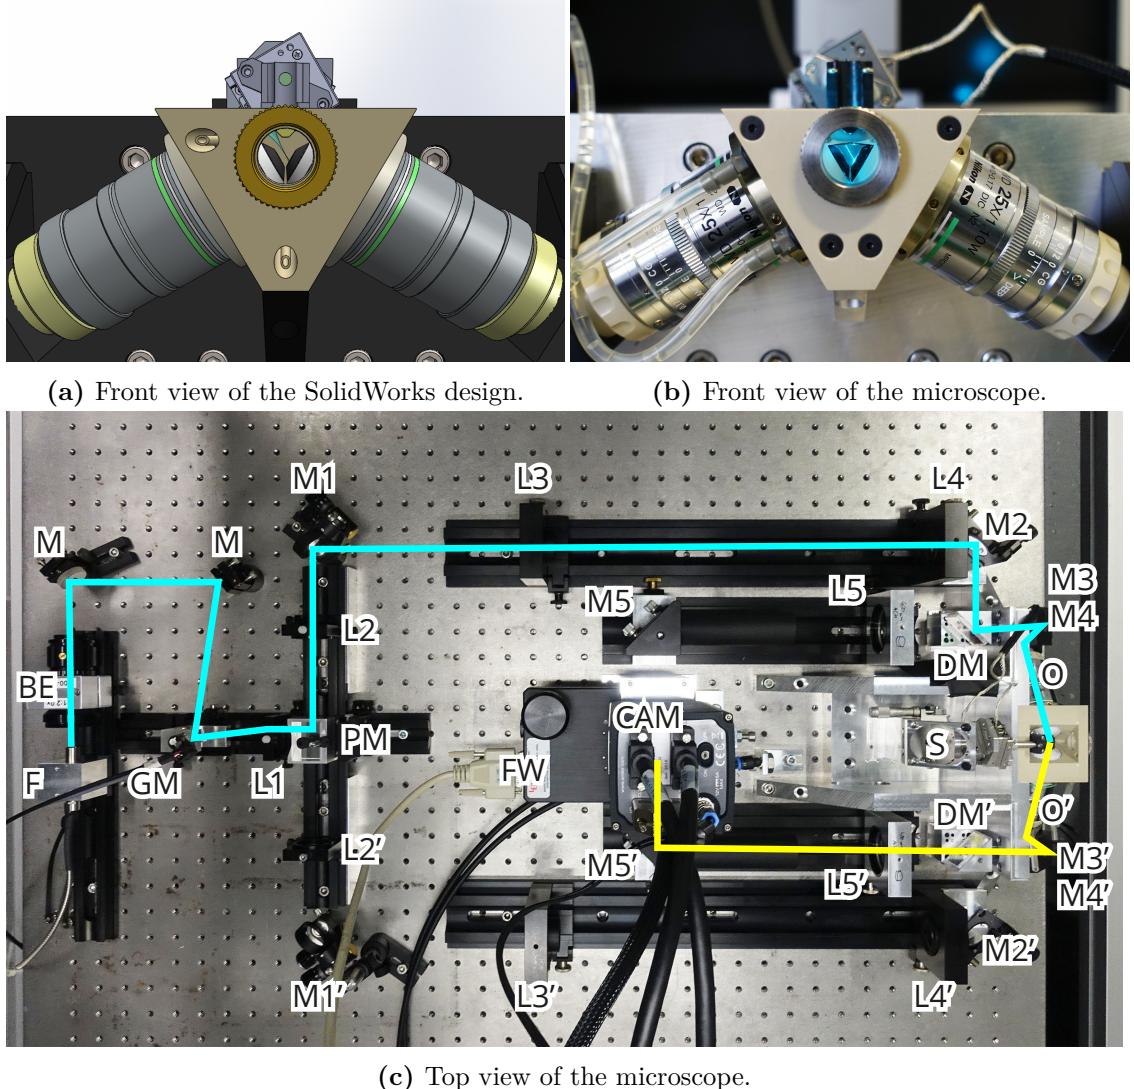


Figure 3.9: Completed DualMouse-SPIM. The excitation and emission light paths are depicted with blue and yellow lines respectively. Component numbering corresponds to Figure 3.5. Detection branch merging unit, and mirrors M6 and M6' are underneath the camera and filter wheel. BE – beam expander, CAM – camera, DM – dichroic mirror, F – fiber, FW – filter wheel, L – lens, M – mirror, O – objective, PM – prism mirror, S – stage

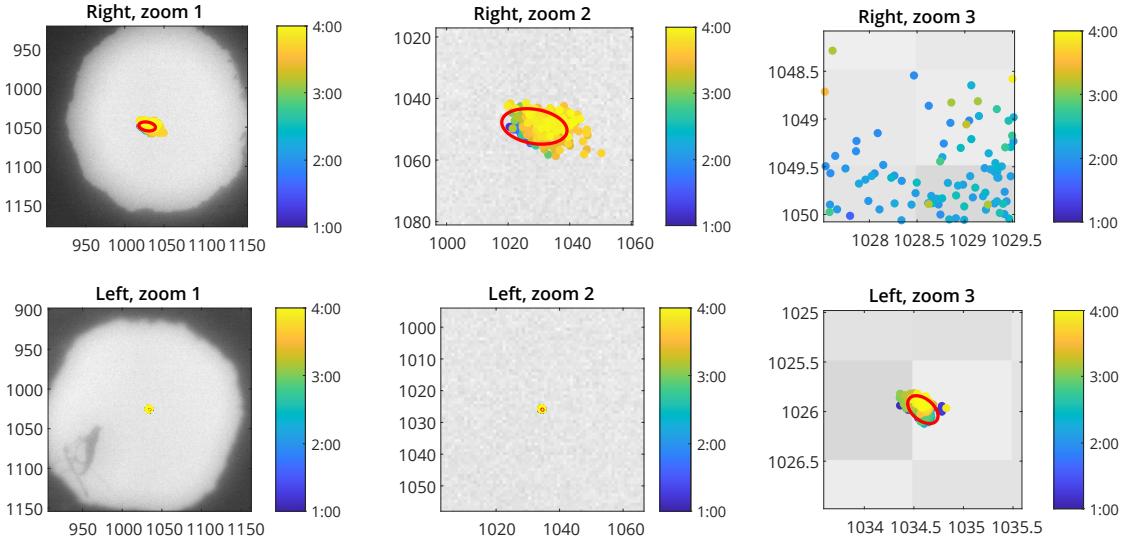


Figure 3.10: Stability measurements of view switcher unit. A closed aperture was imaged on the camera from both views, every 10s, for 4h. The dots represent the center of each frame, color coded with the time. The red ellipse represents the 95% confidence interval of the measured positions based on principal component analysis. Standard deviations for right view: $\sigma_1 = 4.37 \text{ px}$, $\sigma_2 = 2.26 \text{ px}$; for left view: $\sigma_1 = 0.07 \text{ px}$, $\sigma_2 = 0.04 \text{ px}$.

- 1 was only 0.07 px and 0.04 px for the long and short axes respectively. This result implies
- 2 that there is no conceptual limitation in reaching sub-pixel reproducibility with the view
- 3 switching unit, although some optimization is still needed for the right view to reach the
- 4 same stability as the left view.

5 3.5.2 Characterizing the illumination profile

- 6 Since a Gaussian beam is used for illumination, its intensity profile is dependent of
- 7 the axial position (Equation 1.18). Although the total intensity at any cross section of
- 8 the beam is constant, because of the divergent properties, the peak intensity varies. To
- 9 assess any non-uniformities in the illumination pattern, we measured the illumination
- 10 beam intensity for each view.

11 To visualize the beam, the chamber was filled with a fluorescent solution (0.1 %
 12 methylene blue in distilled water). In order to increase the signal to noise ratio of these
 13 images, a long exposure time of 200 ms was used, and 500 images of each beam was
 14 averaged. Dark images were acquired by repeating the image acquisition with the laser
 15 turned off. The average of the dark images were subtracted from the averaged beam
 16 images, resulting in the beam intensity profile (Figure 3.11).

17 To determine the beam waist position, we measured the beam thickness (FWHM)
 18 for each column of the averaged images, and located the position of the minimal width.
 19 The beam width at the waist position for the left view was $3.70 \mu\text{m}$, and for the right
 20 view it was $3.58 \mu\text{m}$ (Figure 3.11). We also measured the usable length of the beams

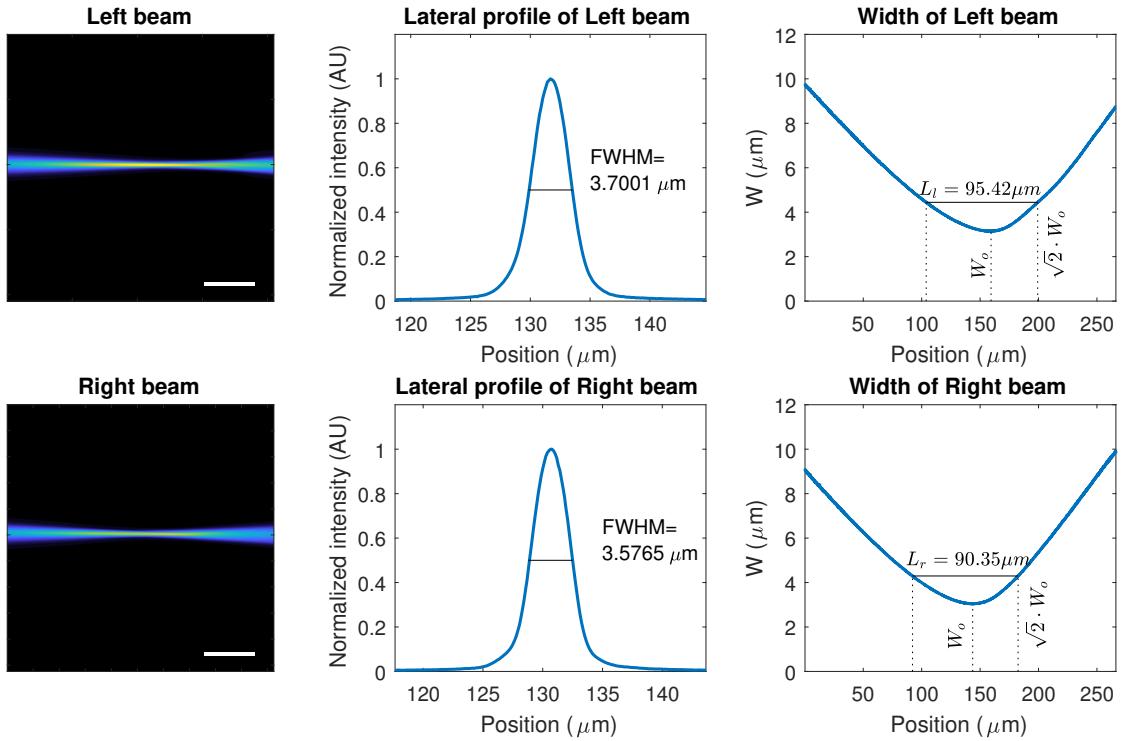


Figure 3.11: Illumination beam profile. Average of 500 stationary beam images for both left (top left) and right objectives (bottom left). Beam intensity profile along the waist of each beam is plotted in the center column. The right column shows the beam width profile of each beam ($1/e^2$).

1 (Section 1.3.1). The distance between the points where the beam has expanded by a
 2 factor of $\sqrt{2}$ relative to the waist is $95.42 \mu\text{m}$ for the left view, and $90.35 \mu\text{m}$ for the
 3 right view. This corresponds well to the original requirement of a minimal field of view
 4 of $100 \mu\text{m}$. Depending on the sample and the required level of optical sectioning, the
 5 practical field of view can be larger than this, as the camera sensor allows for a field of
 6 view of $266 \mu\text{m}$.

7 3.5.3 Resolution and point spread function measurement

8 In order to establish an ideal, reference PSF, we simulated the theoretical PSF of the
 9 microscope with the Gibson-Lanni model [114], using the MicroscPSF Matlab implemen-
 10 tation [115]. The advantage of this model is that it accounts for any differences between
 11 the experimental conditions and the design parameters of the objective, and thus it can
 12 simulate any possible aberrations that may arise. The adjustable parameters are the
 13 thicknesses (t) and refractive indices (n) of the immersion medium (i), coverslip (g),
 14 and sample (s). To simulate the reference PSF, we accounted for the slight mismatch in
 15 refractive index between the FEP foil ($n_g = 1.344$) and water ($n_i = 1.33$). The working
 16 distance of the objective is 2 mm, while the thickness of the foil is 50 μm .

17 It is apparent from the simulations that even though the FEP refractive index is

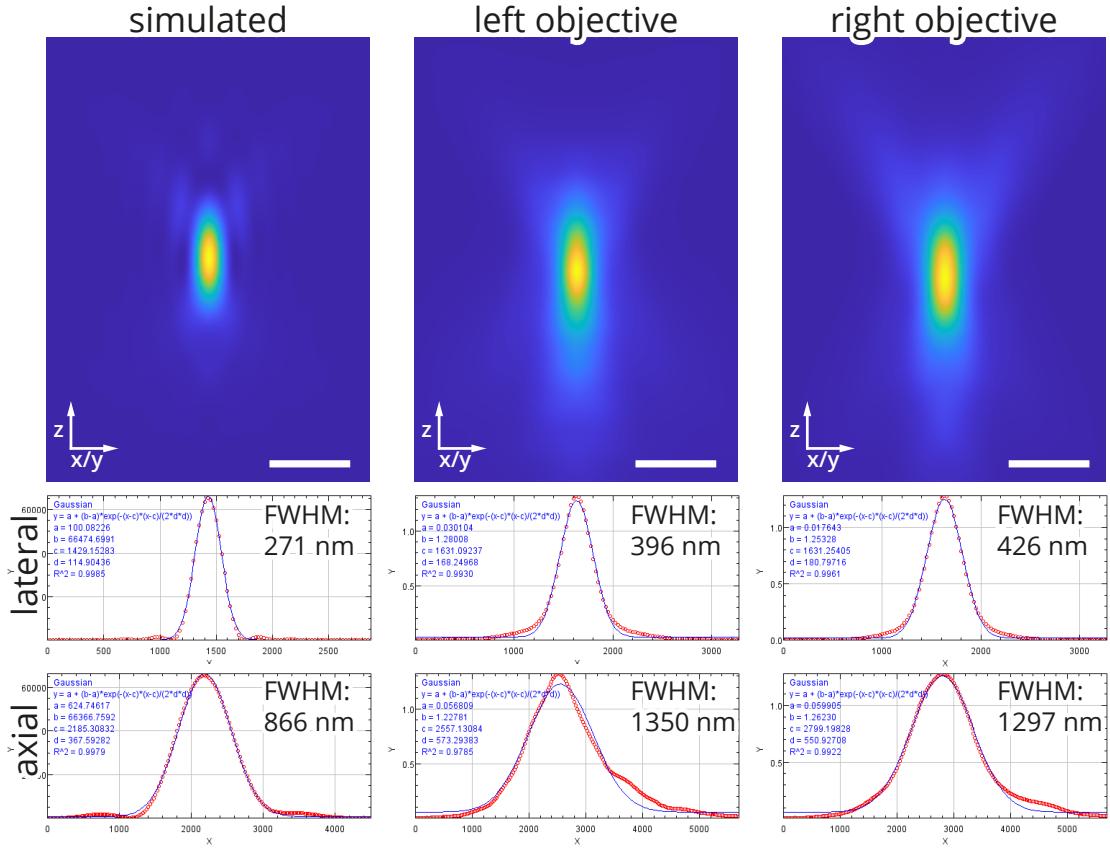


Figure 3.12: Simulated and measured PSF of Dual Mouse-SPIM. Top row: axial sections of simulated and measured point spread functions. Middle row: lateral intensity profile and Gaussian fit. Bottom row: Axial intensity profile and Gaussian fit. Simulations were performed based on the Gibson-Lanni model. Immersion medium and sample refractive index: 1.330, coverslip (FEP foil) refractive index: 1.344, coverslip distance: 1900 μm , coverslip thickness: 50 μm . Excitation wavelength: $\lambda_{ex} = 561 \text{ nm}$. Emission wavelength: $\lambda_{em} = 600 \text{ nm}$. Scale bar: 1 μm .

1 almost identical to the refractive index of water, a slight spherical aberration is still
 2 present even for the ideal case (Figure 3.12, left). The resolution measured as the FWHM
 3 of the intensity profile through the lateral and axial cross sections is 271 nm and 866 nm
 4 respectively. FWHM was measured in Fiji by fitting a Gaussian curve, and multiplying
 5 the standard deviation of the resulting fit by $2\sqrt{2 \ln 2}$.

6 To experimentally determine the resolution of the microscope and characterize its
 7 optical performance, we measured the point spread function using fluorescently labeled
 8 beads suspended in 0.8% GelRite (Section 3.6). The gel was loaded in glass capillaries
 9 and allowed to cool. After the gel solidified, a $\sim 1 \text{ mm}$ piece was cut off and placed in
 10 the microscope sample holder. The beads were imaged from both views using the 561 nm
 11 laser line with the 561 long-pass filter (Semrock, BLP02-561R-25).

12 From both views 12 beads were averaged using Fiji [116] and the 3D PSF estimator
 13 of the MOSAIC suite [117]. In order to acquire a more accurate PSF, the averaged
 14 bead images were deconvolved with the ideal image of the bead (uniform sphere with a

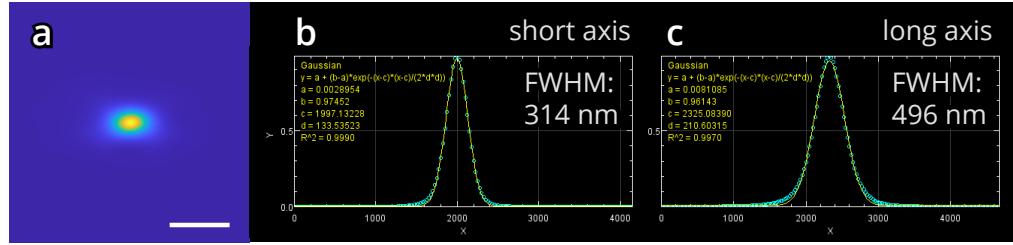


Figure 3.13: Combined PSF of 2 views. (a) The measured PSFs (Figure 3.12) were rotated to their corresponding orientations and multiplied. (b) Gaussian fit along the short axis of the combined PSF; FWHM=314 nm. (c) Gaussian fit along the long axis of the combined PSF; FWHM=496 nm. Scale bar, 1 μm

1 diameter of 500 nm) using the DeconvolutionLab2 Fiji plugin [118]. The results of the
2 deconvolution are shown on Figure 3.12. Similarly to the simulation, we measured the
3 axial and lateral resolutions on the experimental PSFs. For the left view, the measured
4 resolutions were 386 nm in the lateral direction, and 1350 nm in the axial direction. For
5 the right view the lateral resolution was 326 nm, and the axial was 1297 nm.

6 To estimate the achievable multi-view resolution of the system, we combined the two
7 measured PSFs. First, the PSFs were rotated by $\pm 60^\circ$ to correspond to the objective
8 orientations. The PSF images were then normalized by scaling the maximum to 1, and
9 the two rotated and normalized PSFs were multiplied (Figure 3.13). Resolution of the
10 combined PSF is much improved in all directions: along its shortest axis the FWHM
11 is 314 nm, and along the longest axis the FWHM is 496 nm (Figure 3.13). Both are
12 better than the corresponding resolutions for a single view, especially along the long
13 axis, where the FWHM is 2.67 times smaller. This is almost perfectly matching the
14 theoretically expected increase in the axial direction (compare with Section 3.1).

15 3.5.4 Resolution inside a *Drosophila melanogaster* embryo

16 Apart from measuring the point spread function and resolution in an ideal bead sample,
17 we also wanted to know the resolution inside a biological sample, as the tissues usually
18 introduce some aberrations to the light path. Although these aberrations highly depend
19 on the sample, as a worst case scenario, we measured the point spread function inside
20 a *Drosophila melanogaster* embryo. As this specimen is highly opaque and scattering, it
21 gives a good estimate for the upper bound of the resolution.

22 Instead of the fluorescent beads, we imaged a *Drosophila* embryo expressing H2A-
23 mCherry marking the nuclei, and ASL-YFP marking the centrosomes (Figure 3.14a, and
24 Section 3.6). As the centrosomal protein ASL is diffraction limited in size [119], its image
25 gives a good estimate for the point spread function inside the specimen.

26 Similarly to the bead recordings, 15 centriole images were averaged with the 3D PSF
27 tool of the MOSAIC plugin in Fiji (Figure 3.14c). On the averaged image we measured

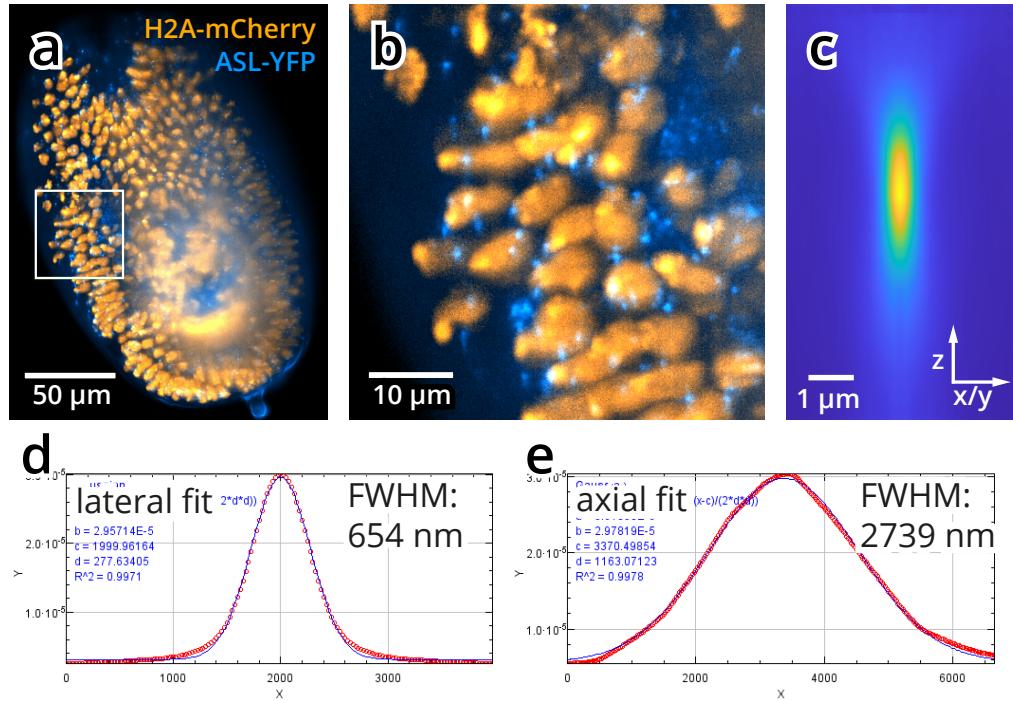


Figure 3.14: Maximum intensity projection of a *Drosophila melanogaster* embryo recording. Maximum intensity projection of a 30 μm thick substack. Orange: nuclei (H2A-mCherry), blue: centrioles (ASL-YFP). 50x magnification. (a) Overview of the embryo. (b) Zoomed in view to the region marked in (a). (c) Average image of 15 centrioles distributed evenly in the embryo. (d) Gaussian fit on the lateral intensity profile of the averaged centrioles; FWHM=654 nm. (e) Gaussian fit on the axial intensity profile of the averaged centrioles; FWHM=2739 nm.

1 the resolution by fitting a Gaussian function on the lateral and axial intensity profiles
 2 (Figure 3.14d,e), and calculating the FWHM of the fitted Gaussian. The size of the
 3 averaged centrioles was 654 nm in the lateral, and 2739 nm in the axial direction.

4 3.5.5 Multi-view imaging of a mouse zygote

5 To demonstrate the multi-view capabilities and improved image quality of the micro-
 6 scope, we performed dual-view imaging of a fixed mouse zygote and combined the images
 7 using the Multiview Reconstruction [112] plugin of Fiji (Figure 3.15). The microtubules
 8 were stained with Alexa Fluor 488 coupled secondary antibodies, and the zygote was
 9 imaged from both views with 0.5 μm inter-plane distance.

10 Anisotropy in the resolution becomes apparent in the single-view recordings, when
 11 the stacks are resliced from a different direction than the imaging plane. Even though the
 12 native view of each objective (Figure 3.15a,d) shows good contrast, and easy to recognize
 13 features, when rotated and sliced corresponding to the view of the other objective, the
 14 contrast is almost completely gone, and resolution is decreased (Figure 3.15b,e). The
 15 fused stack, after the multi-view deconvolution contains the high resolution informa-
 16 tion from both views, and thus both directions show good quality and high contrast

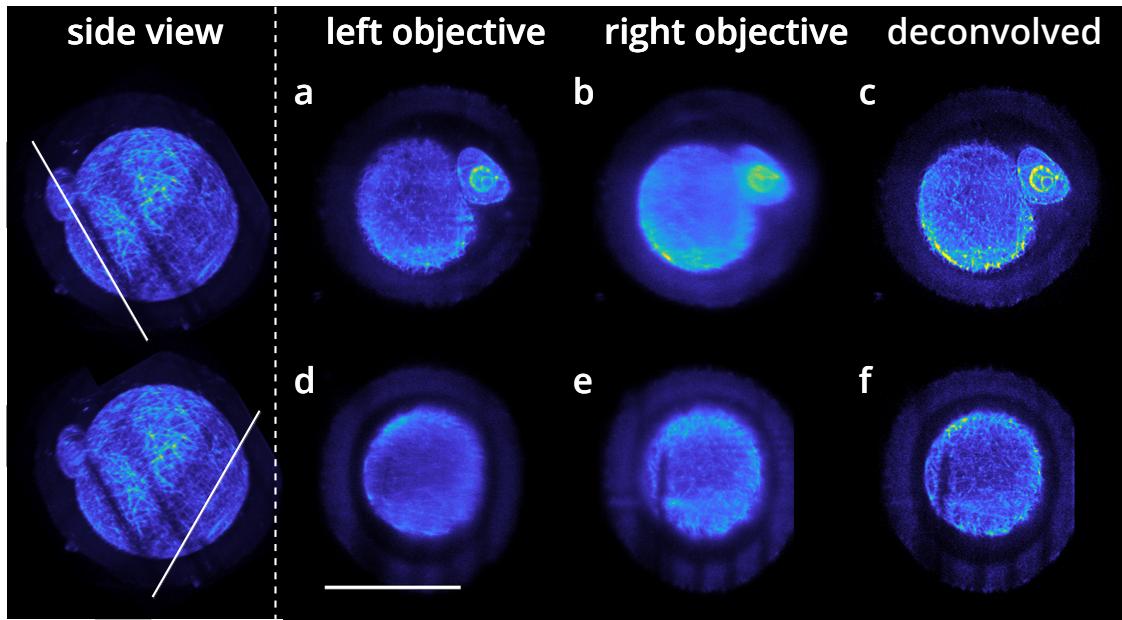


Figure 3.15: Multi-view recording of a mouse zygote. Dual-view imaging was performed on a fixed mouse zygote. Microtubules were stained with Alexa Fluor 488 coupled secondary antibodies. Top row: view of Left objective. Bottom row: view of Right objective. (a) Raw image from left objective. (b) Rotated view of Right objective. (c) Multi-view deconvolution of stacks (a) and (b). (d) Rotated slice from left objective. (e) Raw image from right objective. (f) Multi-view deconvolution of stacks (d) and (e). Scale bar: 50 µm. The darker banding artifacts visible on the side view are due to bleaching.

¹ (Figure 3.15c,f).

² 3.6 Methods

³ 3.6.1 Preparation of fluorescent bead samples

⁴ For registration and resolution measurements we used TetraSpeck 0.5 µm diameter fluo-
⁵ rescently labeled beads (ThermoFisher, T7281). The stock bead solution was thoroughly
⁶ vortexed and sonicated for 5 min before diluting it 1:100 in distilled water. The diluted
⁷ bead solution saw stored at 4 °C until use. GelRite (Sigma-Aldrich, G1910) gel was pre-
⁸ pared in distilled water at 0.8% concentration with 0.1% MgSO₄ · 7H₂O and kept at
⁹ 70 °C until use. 50 µl of the diluted bead solution was added with a heated pipette tip to
¹⁰ 450 µl of gel solution at 70° to prevent polymerization. The gel was thoroughly vortexed,
¹¹ and loaded to glass micropipettes (Brand 100 µl). The gel was allowed to cool to room
¹² temperature and stored in a petri dish under dH₂O at 4° until use. For imaging, a small
¹³ piece of gel was extruded from the capillary, cut off, and placed in the sample holder.
¹⁴ After positioning the gel to the bottom of the sample holder, the holder was filled with
¹⁵ 200 µl dH₂O.

1 3.6.2 Preparing the sample holder

2 The sample holder was lined with 12.5 μm (PSF measurements) or 50 μm (mouse zygote
3 and *Drosophila* embryo imaging) thin FEP foil (Lohmann, RD-FEP050A-610). The FEP
4 foils were cut to size, washed with 70% ethanol followed by a second wash with dH₂O.
5 After washing, both surfaces of the foils were chemically activated by a 20 s plasma
6 treatment (PlasmaPrep2, Gala Instrumente). The foils were then stored in a petri dish
7 until further use separated by lens cleaning tissues (Whatman, 2105-841). Before imaging,
8 the sample holder was cleaned with dish soap, rinsed with tap water, rinsed with 70%
9 ethanol, and rinsed with dH₂O. The prepared foils were glued to the inside of the cleaned
10 sample holder with medical grade silicon glue (twinsil speed, picodent). During the 5 min
11 curing process the foil was pressed against the sample holder by a custom made press
12 fitting the shape of the sample holder. Final dilution of the stock bead solution in the
13 gel is 1:1000.

14 3.6.3 Drosophila embryo imaging

15 *Drosophila melanogaster* embryos (fly stock AH1) expressing fluorescent nuclear (H2A-
16 mCherry) and centriole (ASL-YFP) markers were collected on an agar juice plates and
17 dechorionated in 50% bleach solution for 1 min. After rinsing the bleach with deionized
18 water, the embryos were placed in the sample holder under PBS solution. A small piece of
19 gel containing fluorescent beads were also placed next to the samples to aid in multi-view
20 registration.

21 3.6.4 Mouse zygote imaging

22 Fixed mouse zygotes labeled with Alexa Fluor 488 (microtubules) and Alexa Fluor 647
23 (kinetochores) coupled secondary antibodies were kindly provided by Judith Reichmann.
24 Zygotes were transferred to the sample holder, and imaged in PBS. To allow for multi-
25 view reconstruction, a small piece of gel containing fluorescent beads was placed next to
26 the zygote in the sample holder. After imaging the zygote from both views, the beads
27 were also recorded using the same stack definitions. After data acquisition, the multi-view
28 datasets were registered and deconvolved in Fiji [116] using the Multiview Reconstruction
29 Plugin [112, 120]. The deconvolution was based on a simulated PSF generated in Fiji
30 with the PSF Generator plugin [121] using the Born-Wolf PSF model [24]. NA_{ex} = 0.1,
31 NA_{em} = 1.1, n=1.33, λ_{ex} = 488 nm, λ_{em} = 510 nm.

3.7 Conclusions

2 In this chapter we have presented a novel light-sheet microscope designed for subcellular
3 imaging of mouse embryos. The microscope has two identical, high NA (1.1) objectives,
4 positioned in a 120° angle, and operates with a 30° tilted light-sheet. Due to the symmet-
5 rical design both objectives can be used for detection and illumination as well, providing
6 multi-view capabilities without sample rotation.

7 We have characterized the optical properties of the microscope by measuring the light-
8 sheet dimensions (average length: 93 µm, average thickness: 3.6 µm), and by measuring
9 the point spread function. When combining the two views, the resolution is much closer
10 to an ideal isotropic shape, being 496 nm along the long axis and 314 nm along the short
11 axis as opposed to 1323 nm and 411 nm measured for a single view. This 2.67 times
12 increase in axial resolution can potentially make the difference in being able to track all
13 chromosomes in a developing mouse embryo.

14 To be able to surpass the proof-of-concept state, the microscope still needs some
15 improvements. The detection view switching unit needs to be improved to minimize
16 field of view drift of both views. Data processing for long term experiments would be
17 extremely challenging otherwise. Another necessity for long term experiments is the
18 implementation of an environmental chamber to provide the appropriate conditions for
19 live embryo imaging.

20 The use of high NA objectives also keep the door open for future upgrades, such
21 as adding structured illumination [55, 56], or coupling in a high power pulsed laser for
22 photomanipulation capabilities [122]. Another natural extension to the system would
23 be an addition of a third objective, that would allow for truly isotropic imaging and
24 two-sided sample illumination.

25 Single-view solutions for isotropic imaging only allow a very limited field of view. For
26 diffraction-limited optical sectioning a Gaussian beam is diverging too fast [123], while
27 the use of other, non-diffractive beams rely on self-interference [7], which breaks down
28 after a few tens of micrometers inside the sample. Our dual-view high NA solution allows
29 for isotropic resolution even for large field of views, such as for entire mouse zygotes or
30 embryos (120 µm×120 µm×120 µm)

¹ Chapter 4

² GPU accelerated image
³ processing and compression

⁴ 4.1 Challenges in data handling for light-sheet microscopy

⁵ When using any kind of microscopy in research, image processing is a crucial part of
⁶ the workflow. This is especially true for light-sheet microscopy, since it is capable of
⁷ imaging the same specimen for multiple days, producing immense amounts of data. A
⁸ single overnight experiment of *Drosophila* development (which is a very typical use-case
⁹ for light-sheet microscopy) can produce multiple terabytes of data.

¹⁰ Apart from light-sheet microscopy, many other microscopy modalities are also suf-
¹¹ fering from this problem. Methods, such as high content screening [124–126], where tens
¹² of thousands of different genotypes are imaged generating millions of images; and sin-
¹³ gle molecule localization microscopy (SMLM) [127–129], where just a single plane of a
¹⁴ sample is imaged hundreds of thousands of times to acquire super-resolved images.

¹⁵ Not only these methods are capable of generating data extremely fast, but with
¹⁶ the sustained high data rate a single experiment can easily reach multiples of terabytes
¹⁷ (Figure 4.1). Handling this amount of data can quickly become the bottleneck for many
¹⁸ discoveries, which is a more and more common issue in biological research [130–132].

¹⁹ This chapter will focus on addressing these challenges by presenting a real-time,
²⁰ GPU-based image preprocessing pipeline developed in CUDA [133] consisting of two
²¹ parts (Figure 4.2). The first part is a fast image fusion method for our workhorse light-
²² sheet microscope, the MuVi-SPIM [45], that enables live fusion of the images arriving
²³ from two opposing cameras. The second part of the pipeline, which can also be used in
²⁴ a standalone way, is a real-time image compression library that allows lossless and noise
²⁵ dependent lossy compression of the data directly during acquisition even for high-speed
²⁶ sCMOS cameras.

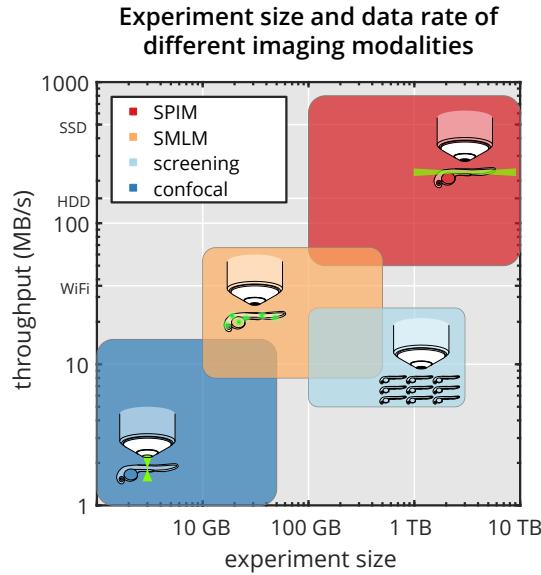


Figure 4.1: Experiment sizes and data rate of different imaging modalities. Comparison of single-plane illumination microscopy (SPIM, red), high-content screening (light blue), single molecule localization microscopy (SMLM, orange) and confocal microscopy (blue) by typical experiment size and data production rate (see also Table B1 in Appendix B).

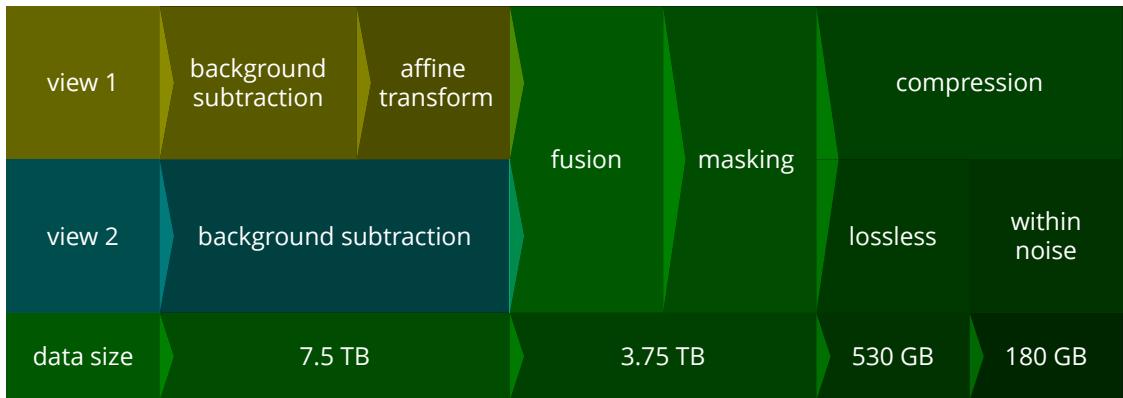


Figure 4.2: Real-time image processing pipeline for multi-view light-sheet microscopy.

4.2 Real-time preprocessing pipeline

Similarly to the DualMouse-SPIM, our currently used production microscope, the Multiview-SPIM (MuVi-SPIM) [45] also uses multiple imaging directions to improve the image quality. In this case, however, the aim is completeness rather than increasing the resolution. As the MuVi-SPIM is capable of imaging much larger specimens, such as entire *Drosophila* embryos, the sample size itself can present some challenges, especially for opaque specimens. As light scattering and absorption impact both the illumination and detection optics, the negative effects for SPIM are more pronounced compared to single-lens systems [134].

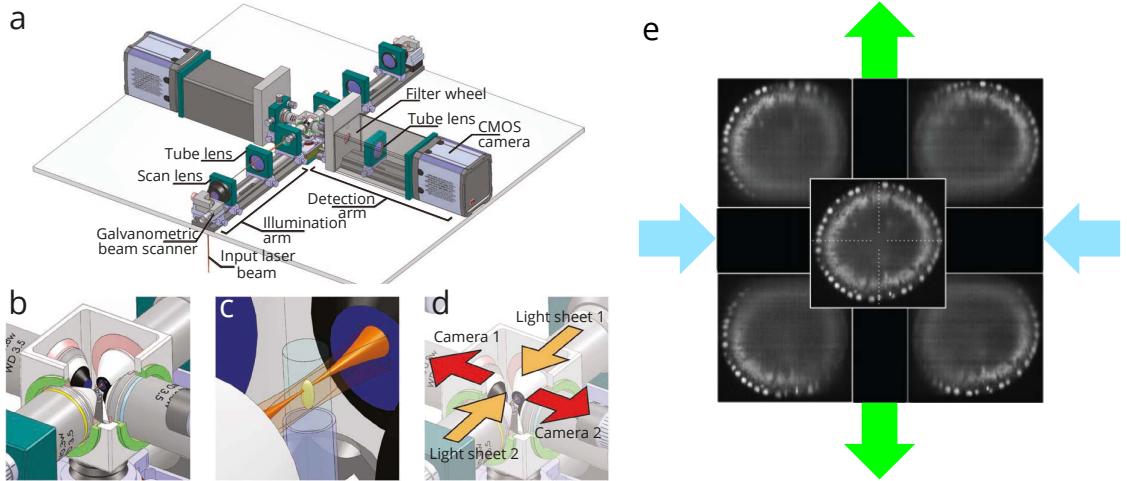


Figure 4.3: Operating principle of MuVi-SPIM. (a) The microscope consists of two illumination and two detection arms for simultaneous multi-view illumination and detection. (b) The 4 arms meet in the imaging chamber that is filled with water, and contains the sample. (c) The sample is held by a glass capillary, in a GelRite cylinder. Optical sectioning is achieved by a virtual light-sheet. (d) The light-sheets can be generated from two sides (Light sheet 1 and 2), and detection is also double sided (Camera 1 and 2). Adapted from [45].

1 4.2.1 Multiview SPIM for *in toto* imaging

2 MuVi-SPIM provides an elegant solution for multi-view imaging. A standard SPIM setup
 3 with a single detection and a single illumination lens would rotate the sample to acquire
 4 images from multiple directions. MuVi-SPIM, on the other hand, utilizes two opposing
 5 objectives for illumination and two opposing objectives for detection (Figure 4.3a). As
 6 the sample is held by an aqueous gel inside the imaging chamber, all objectives have
 7 unobstructed view of it from multiple directions (Figure 4.3b,c).

8 Data acquisition is done in two steps: the sample is illuminated by Light sheet 1, and
 9 fluorescence is collected by both detection objectives at the same time, after which Light
 10 sheet 2 is activated, and both cameras record the fluorescence again (Figure 4.3d). This
 11 process will result in 4 datasets, all with partial information due to scattering effects.
 12 The 4 views are later fused to a single, high quality dataset (Figure 4.3e). This fusion
 13 process is necessary before any further analysis steps can be performed, however, due to
 14 the sheer size of the data, it takes a considerable amount of time after the acquisition.

15 By combining scanned light-sheet [49] with confocal slit detection on the camera chip
 16 [135], it is possible to exclude out of focus, scattered illumination light. This way it is
 17 possible to illuminate simultaneously with both light-sheets, which leaves us with only
 18 two views, the views of the two opposing cameras [75].

¹ **4.2.2 Image registration**

² To perform image fusion of multiple views, first image registration is necessary: the
³ coordinate systems of the views have to be properly overlapped. Ideally a single mirroring
⁴ transformation would be enough to superpose the two camera images, however in practice
⁵ the microscope can never be aligned with such precision. Other types of transformations
⁶ are also necessary: translation to account for offsets in the field of view; scaling in case of
⁷ slightly different magnifications; and also shearing if the detection plane is not perfectly
⁸ perpendicular to the sample movement direction [136]. To combine all of these effects,
⁹ a full, 3D affine transformation is necessary to properly align the two camera images
¹⁰ (Figure 4.4 a). This transformation can be represented by a matrix multiplication with
¹¹ 12 different parameters:

$$\begin{pmatrix} x, \\ y, \\ z, \\ 1 \end{pmatrix} = \begin{pmatrix} a & b & c & d \\ e & f & g & h \\ i & j & k & l \\ 0 & 0 & 0 & 1 \end{pmatrix} \times \begin{pmatrix} x \\ y \\ z \\ 1 \end{pmatrix} = \begin{pmatrix} ax + by + cz + d \\ ex + fy + gz + h \\ ix + jy + kz + l \\ 1 \end{pmatrix}$$

¹² where x, y, z are the coordinates in the original 3D image, x', y', z' are coordinates in the
¹³ transformed image, and a, b, \dots, l are the affine transformation parameters.

¹⁴ These parameters are traditionally acquired by a bead based registration algorithm
¹⁵ after imaging fluorescent beads from each view of the microscope [120, 137]. The beads
¹⁶ are segmented by using a difference of Gaussian filter, and the registration param-
¹⁷ eters are acquired by matching the segmented bead coordinates in each view. Identifying
¹⁸ the corresponding beads is done by a translation and rotation invariant local geomet-
¹⁹ ric descriptor. This matches the beads based on their relative position to their nearest
²⁰ neighbors. After the matching beads are identified, the affine transformation parameters
²¹ are calculated by minimizing the global displacement for each pair of beads.

²² For the two opposing views of MuVi-SPIM, these parameters are only dependent
²³ on the optical setup itself, and not on the sample or on the experiment. Because of
²⁴ this, it is sufficient to determine the transformation parameters only after modifying the
²⁵ microscope (*e.g.* after realignment).

²⁶ In our currently used fusion pipeline, after the parameters are acquired, the 3D stacks
²⁷ are fused by transforming one of the views to the coordinate system of the other (using
²⁸ the affine transformation parameters from the bead based registration), and fusing the
²⁹ two stack by applying a sigmoidal weighted average (4.4a). The weights are determined
³⁰ in a way to exclude the parts of the stacks that have worse image quality and comple-
³¹ ment these from the other view's high quality regions. When using the electronic confocal slit
³² detection (eCSD) weighting is not necessary, as the scattered light is already rejected in
³³ these recordings, and a simple sum of the two stacks gives the best results regardless of

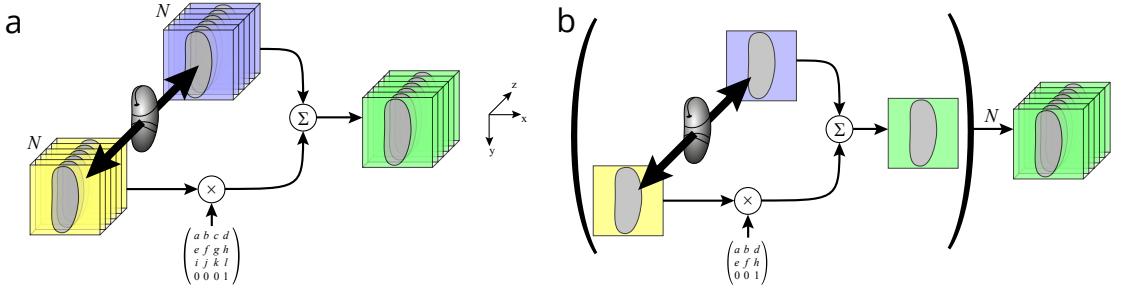


Figure 4.4: Multi-view fusion methods for light-sheet microscopy. a) Full 3D stacks are acquired from the opposing views (yellow and blue), which are then registered in 3D space using previously acquired affine transformation parameters. Registered stacks are then weighted averaged to create the final fused stack (green). b) Images from opposing views are directly fused plane by plane. Registration takes place in 2D space thus reducing computational effort and memory requirements. The registered planes are then weighted averaged to create the final fused image.

1 the sample [75].
 2 The fusion process itself can be very resource intensive and take a considerable
 3 amount of time. This is simply due to the size of the 3D stacks: a single stack is usually
 4 between 2 and 4 GB in size. Thus, the necessary memory requirement to fuse 2 of these
 5 stacks is $3 \cdot 4 \text{ GB} = 12 \text{ GB}$, as the result will also take up the same space. Just reading
 6 and writing this amount of information to the hard disk takes a considerable amount of
 7 time. When using an SSD drive for example, with a 500 MB/s read and write speed, just
 8 the read/write operations will take around $\frac{12 \text{ GB}}{500 \text{ MB/s}} = 24 \text{ s}$.

9 4.2.3 2D fusion of opposing views

10 To speed up the image processing, we take a new approach to fusing the images. As the
 11 two objectives of MuVi-SPIM ideally image the same z plane, it should be possible to
 12 reduce the alignment problem to a 2D affine transformation:

$$\begin{pmatrix} x' \\ y' \\ 1 \end{pmatrix} = \begin{pmatrix} a & b & d \\ e & f & h \\ 0 & 0 & 1 \end{pmatrix} \times \begin{pmatrix} x \\ y \\ 1 \end{pmatrix} = \begin{pmatrix} ax + by + d \\ ex + fy + h \\ 1 \end{pmatrix}$$

13 The advantage of a simplified transformation is not only the reduced computational
 14 complexity, but also the massively reduced memory requirement, as in this case it is
 15 sufficient to store 3 planes in memory instead of 3 entire stacks (Figure 4.4 b). Performing
 16 the 2D direct fusion on the GPU immediately after acquisition has two benefits: first,
 17 only the fused images are stored to the hard drive, which directly results in 50% savings
 18 in storage space. Second, since the fusion is faster than the camera acquisition speed, the
 19 fused image can be displayed for the users instead of the 2 raw images. This would greatly
 20 improve user experience and speed up the initial, set-up phase of each experiment.

In order to allow for the direct, 2D fusion, the microscope needs to be very well

4.2 Real-time preprocessing pipeline

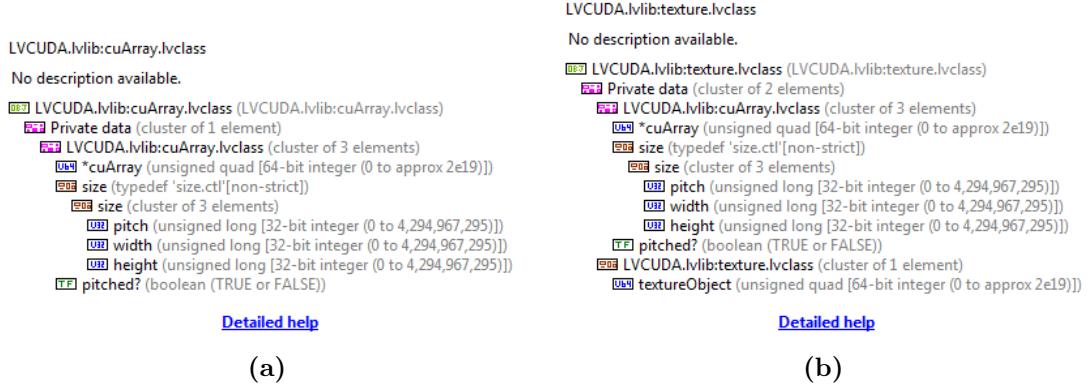


Figure 4.5: Classes of LVCUDA library. (a) **CuArray** class, wrapping a 1D or 2D pitched device memory for use in LabVIEW. (b) **Texture** class, wrapping a CUDA texture object for use in LabVIEW.

aligned to minimize any adverse effects arising from discarding some of the transformation parameters. The requirements for this are the following:

$$|cz| < \sigma_{xy} \quad \forall z \quad (4.1)$$

$$|gz| < \sigma_{xy} \quad \forall z \quad (4.2)$$

$$|ix + jy + (k - 1)z + l| < \sigma_z \quad \forall x, y, z \quad (4.3)$$

1 where σ_{xy} is the lateral resolution, and σ_z is the axial resolution of the microscope, which
 2 are 277 nm and 1099 nm respectively.

3 If these conditions are fulfilled (*i.e.* the microscope is properly aligned), direct plane
 4 by plane fusion will not result in any loss of information compared to the full 3D image
 5 fusion.

6 4.2.4 CUDA implementation of direct fusion

7 Our custom microscope control software (Section 3.4.2) is developed in LabVIEW and
 8 we implemented the pipeline as a combination of a CUDA and a LabVIEW library. The
 9 CUDA library implements all the necessary low level functions and exposes these in a
 10 dynamically linked library (dll). The LabVIEW library, **LVCUDA.lvlib** implements two
 11 high level classes: **cuArray**, and **Texture** (Figure 4.5). These classes interface with the
 12 CUDA dll, and allow to easily build a flexible CUDA-based image processing pipeline in
 13 LabVIEW.

14 As the pipeline operates on 2D images, both classes support 1D or 2D arrays in a
 15 pitched configuration. **CuArray**, as the parent class, stores the pointer to the array, as
 16 well as the pitch, width and height. LabVIEW natively doesn't support pointer opera-
 17 tions, therefore the pointer is simply cast to a 64 bit unsigned integer internally. As this
 18 is a private member of the class there is no danger of accidental modification. Being a

1 descendent of `cuArray` class, the `Texture` class adds a further member to store the refer-
2 ence to a CUDA texture object. This class is used to implement the affine transformation,
3 as it supports floating point indexing and automatic linear interpolation.

4 Since the processing is actually bottlenecked by the data transfer rate between the
5 main memory and GPU memory, we implemented multiple commonly used image prepro-
6 cessing operations for our pipeline to maximize the utility of the GPU. These functions
7 include background subtraction, background masking and image compression. We will
8 discuss these features in the following sections of the chapter.

9 **4.2.5 Bakcground subtraction and masking**

10 As an additional step of the preprocessing pipeline, background subtraction and back-
11 ground masking was also implemented. Background subtraction can improve image qual-
12 ity as it removes any system-specific signal, while background masking is beneficial for
13 the consecutive compression step.

14 To perform the background subtraction, dark images are recorder without the laser
15 turned on. Typically 500–2000 images are taken which are averaged, to capture the pixel
16 non-uniformities of the camera sensors. As this is camera specific, the step is repeated
17 for all cameras. If necessary, the recordings can be repeated under different conditions,
18 such as different exposure times, or different sensor modes (such as global shutter and
19 rolling shutter). The averaged background images are saved in a custom file format in an
20 HDF5 container [138] together with the camera serial number. The microscope software
21 can read these files and applies the background subtraction to the appropriate cameras
22 during imaging.

23 Background masking is a useful step to increase the efficiency of image compression.
24 For light-sheet microscopy, where typically an entire embryo is imaged, the boundary
25 of the specimen, and thus the area of interest is well defined. Anything outside the
26 embryo is just noise which does not contribute to any useful information. For image
27 compression, however, these regions are extremely difficult to compress, as due to the
28 random nature of noise, almost no reduction is achievable (see 2.1). To circumvent this
29 issue, the background pixels outside the specimen can be set to 0, which will greatly
30 increase the compression ratio without compromising any data of interest [139].

31 The masking is performed in the following way. As the sample has much higher signal
32 compared to the background, a thresholding operation is sufficient. In order to have a
33 smooth mask, the images are first blurred by a Gaussian kernel, and the thresholding
34 is done on the blurred image. This will define a binary mask with smooth boundaries
35 which is applied to the original image (Figure 4.6). The threshold can be calculated
36 automatically by the Triangle method [140], or can also be user specified.

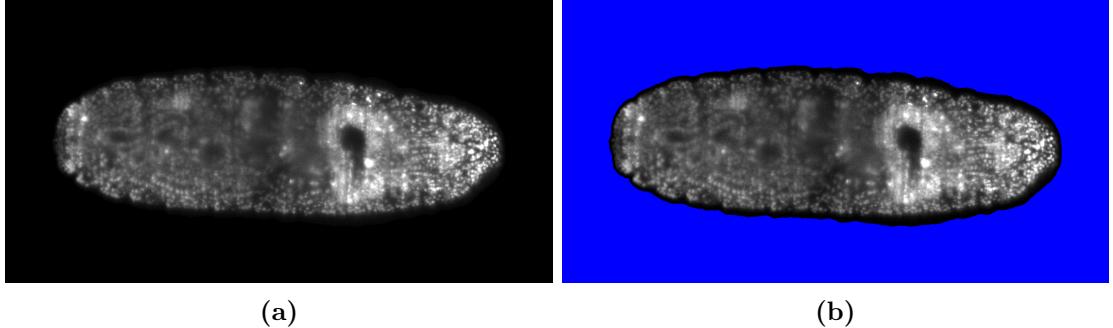


Figure 4.6: Applying mask to remove background. (a) Original image of a *Drosophila* embryo. (b) Background selected by thresholding the blurred image.

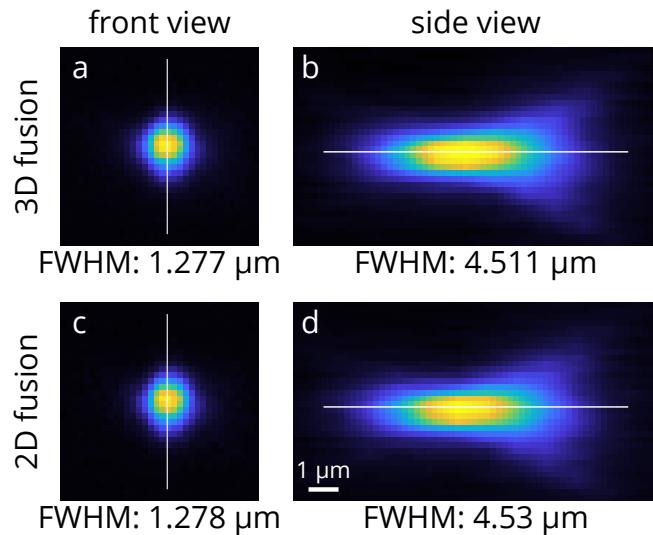


Figure 4.7: Comparison of 3D and 2D fusion of beads. Front and side views of a representative bead after 3D full affine fusion (a, b) and after 2D planewise fusion (c,d). FWHM was measured along the indicated lines, through the center of the bead image. Scale bar: 1 μm .

4.2.6 Results

The image preprocessing pipeline was tested on our MuVi-SPIM microscope [45]. For the background subtraction we recorded 1500 dark images with each camera and averaged them, in order to obtain the camera specific background images. Prior to image acquisition these were uploaded to the GPU memory, and were readily available for the pipeline. The implemented CUDA pipeline with background subtraction, 2D fusion and masking reached a throughput of 135.8 frames per second (fps), while a single-threaded CPU implementation could only process 7.4 images per second on average.

Following careful alignment of the microscope to meet the previously discussed requirements (Eqs. 4.1 – 4.3), we imaged fluorescent beads in a gel suspension to obtain the affine transformation parameters. The measured 3D transformation parameters were the following:

$$\begin{pmatrix} 1.013 & 2.494 \times 10^{-3} & \mathbf{7.182 \times 10^{-3}} & -21.67 \\ -1.697 \times 10^{-3} & 1.014 & \mathbf{-3.192 \times 10^{-5}} & -4.161 \\ \mathbf{-9.694 \times 10^{-5}} & \mathbf{1.937 \times 10^{-7}} & \mathbf{1.003} & \mathbf{-0.433} \\ 0 & 0 & 0 & 1 \end{pmatrix}$$

Substituting these values to Eqs. 4.1 – 4.3 and evaluating for the full range of x, y, z , the maximum contribution of the discarded coefficients for each coordinate will be:

$$\begin{aligned} \max |cz| &= 0.070 \mu\text{m} \\ \max |gz| &= 3.11 \times 10^{-4} \mu\text{m} \\ \max |ix + jy + (k - 1)z + l| &= 0.7789 \mu\text{m} \end{aligned}$$

1 As these are below the resolution of the microscope, discarding the coefficients and
 2 reducing the 3D transformation to a 2D transformation will not have any negative effects
 3 on the image quality.

4 To validate our hypotheses, we fused bead stacks that were acquired for the calibra-
 5 tion using both the 3D and the 2D transformations. The 2D, planewise fused beads do
 6 not exhibit any pathological morphologies compared to the 3D fused beads (Figure 4.7).
 7 When measuring the size of the bead images (FWHM) along the lateral and axial di-
 8 rections, the difference is less than 0.5% compared to the 3D fused dataset. This is well
 9 below any resolvable features.

10 We applied the direct fusion method to various biological specimens, such as
 11 *Drosophila melanogaster* embryos, zebrafish larvae, *Phallusia mammillata* embryos and

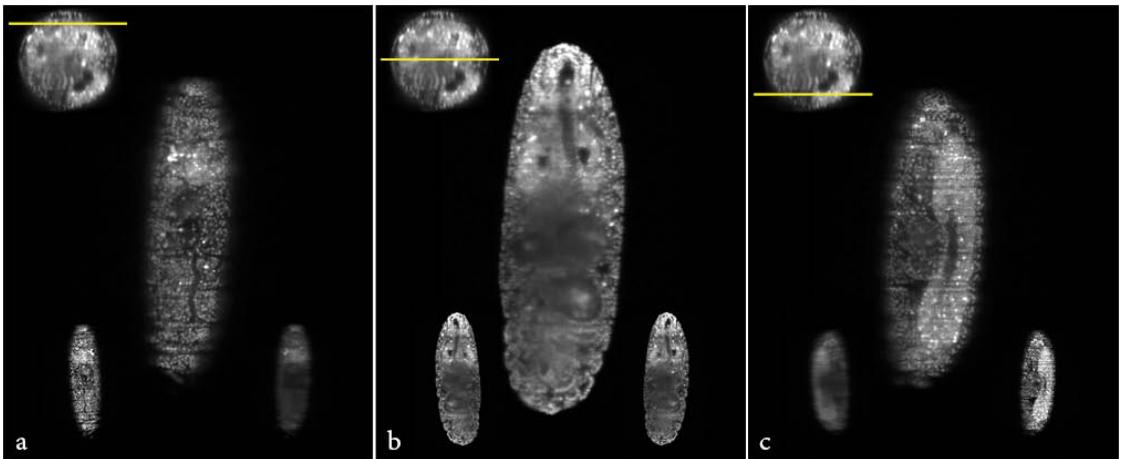


Figure 4.8: GPU fused images of a *Drosophila melanogaster* embryo. Two stacks were taken in quick succession first without fusion, then with fusion enabled. Fused images are shown in the middle of each subfigure, while the individual camera images are in the bottom insets. The top-left inset depicts the z-position of the shown images. (a) Image from closer to the left camera. (b) Image from the center of the embryo. (c) Image from closer to the right camera.

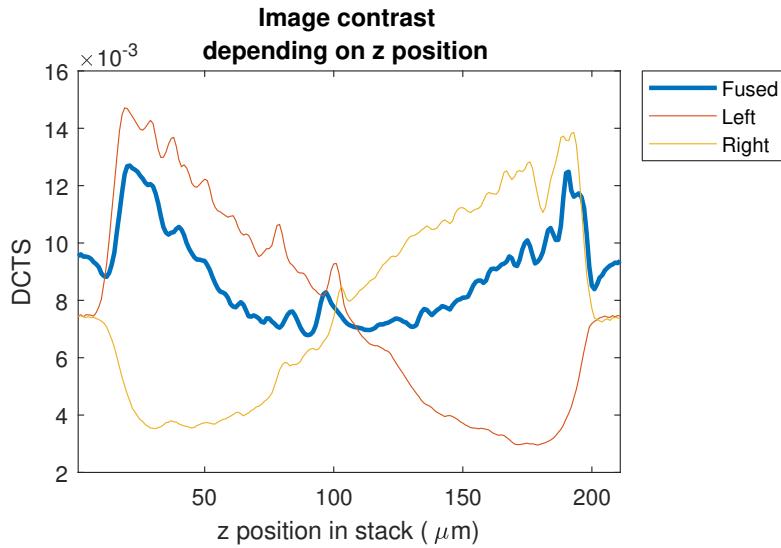


Figure 4.9: Image contrast depending on z position for raw and fused stacks. Image contrast was measured as the Shannon entropy of the normalized Discrete Cosine Transform of the sections [141]. Contrast measurements were performed on the images shown on Figure 4.8.

1 *Volvox* algae. As a demonstration, here we show the results of imaging *Drosophila* embryos expressing H2Av-mCherry histone marker. The embryos were imaged first without
 2 direct fusion enabled, and immediately afterwards with direct fusion enabled (Figure 4.8).
 3 Image quality dependency on the depth of the imaging plane is especially apparent in
 4 single-view stacks. Planes closer to the objective give a sharp, high contrast image, while
 5 planes deeper inside the embryo are severely degraded due to scattering (Figure 4.9).

6 Stacks obtained with the live fusion enabled show a consistently high image quality
 7 throughout the entire stack, independent of the depth (Figure 4.9). This allows us to
 8 keep only the already fused data, thus effectively reducing the storage requirement by
 9 half, and facilitating further data processing steps.

11 4.2.7 Methods

12 Speed measurements

13 Processing speed of the CPU and GPU implementation of the processing pipeline was
 14 measured with the profiling tool of LabVIEW, and are an average of . The benchmarking
 15 computer had 2 Intel Xeon E5620 processors with 8 processing cores running at 2.4 GHz,
 16 24 GB RAM and an Nvidia GeForce GTX 750 graphics card. Test images were 2048×2048
 17 pixels at 16 bit depth.

4.3 B³D image compression

The second part of our GPU-based image preprocessing pipeline is a new image compression algorithm that allows for extremely fast image compression to efficiently reduce data sizes already during acquisition. Although this would not reduce the requirements for image processing power and time, it still has a big impact on the necessary background infrastructure. By reducing the data size, not only the cost for storage can be reduced, but the time it takes to transfer the data during the various steps of data processing. A fast compression method would also greatly improve 3D data browsing possibilities, as more data could be piped to the rendering software.

Despite the advantages, real-time compression for high-speed microscopy has not been available, and this is mostly due to the lack of appropriate compression methods suitable for scientific imaging that also offers the high throughput demanded by these applications. Typically used lossless compression methods, such as JPEG2000 [142] although offer good compression ratios, are very slow in processing speed, at least compared to the data rate of a modern microscope ($\sim 1 \text{ GB/s}$, Figure 4.1). High speed compression methods that could deal with this data rate have been developed for ultra high definition 4K and 8K digital cameras, such as the high efficiency video codec (HEVC) [143]. These methods, however, have been optimized for lossy image compression which is generally not acceptable for scientific data [95], and rarely support compression of high bit rate originals, which is typically the case for modern sCMOS sensors. Although the HEVC recommendation does specify bit rates up to 16 bits, and lossless compression, the open source version, x265 only supports bit rates up to 12 bit [144].

To address these issues, we developed B³D, a GPU based image compression library that is capable of high speed compression of microscopy images during the image acquisition process. By utilizing the massively parallel processing architecture of a GPU, we were not only able to reach a compression and decompression speed of 1 GB/s, but our algorithm also keeps the load off the CPU, making it available for other computing tasks related to operating the microscope itself.

A second feature of our compression library is a novel algorithm for noise dependent lossy compression of scientific images. Although most lossy compression methods are not suitable for scientific data, our method allows for a deterministic way to control the exact amount of loss. The algorithm was designed in a way that any modification of a single pixel is proportional to the inherent image noise accounting for shot noise and camera read noise. Since this noise already introduces some uncertainty to the raw data, if any changes made are smaller than this, the extractable information by further data analysis steps should not be affected, while the compression ratio is massively increased.

¹ **4.3.1 Compression algorithm**

² **Lossless compression**

³ The algorithm design initially had three main requirements to ensure suitability for a
⁴ high-speed microscopy environment: 1) low complexity for fast execution, 2) no data
⁵ dependencies to enable parallel execution, and 3) full reversibility to ensure lossless com-
⁶ pression. Since existing image compression standards such as JPEG2000 [142] or JPEG-
⁷ LS [105] were designed to maximize compression ratio even at the expense of compression
⁸ speed, these were not suitable for our needs. Furthermore, most steps inherently require
⁹ sequential execution, thus preventing efficient parallelization. Promising efforts have been
¹⁰ made to enable parallel compression by simplifying JPEG-LS, by removing the limiting
¹¹ steps from the algorithm (such as Golomb parameter adaptation or context modeling)
¹² [107, 108]. Although some of these methods could reach a significant speedup with min-
¹³ imal expense in compression ratio, their performance was still not enough for real-time
¹⁴ compression of high-speed microscopy data.

¹⁵ As in the case of other image compression methods, our algorithm has two main
¹⁶ components: decorrelation and entropy coding (Figure 4.10a). In this work we focused
¹⁷ on implementing a parallel encoder and decoder for the decorrelation part that would
¹⁸ also be compatible with the noise dependent lossy compression, as efficient CUDA-based
¹⁹ entropy coders are already available [145]. To decorrelate the data, similarly to JPEG-
²⁰ LS and lossless-JPEG [104], a prediction is performed for each pixel by calculating the
²¹ average of the top and left neighbors (Figure 4.10b). The prediction is subtracted from
²² the real pixel value, resulting in the prediction error term:

$$\varepsilon = X - \text{Pred}(X). \quad (4.4)$$

²³ Since the neighboring pixels have a high chance of correlation, these error terms will
²⁴ typically be very small compared to the raw intensity values. This step is similar to
²⁵ predictor 7 of lossless JPEG (see 2.3).

²⁶ The pixel prediction method is especially well suited for parallel compression, as
²⁷ the it can be performed independently for all pixels. For decompression, the top and
²⁸ left neighbor of a pixel need so be first reconstructed, thus parallelization need some
²⁹ adjustments. An obvious choice is to perform the reverse prediction in tiles, where the
³⁰ number of threads will equal the number of tiles. Parallel execution can be further scaled
³¹ up if the decoding is done in diagonals, starting from the top left corner (Figure 4.10c).
³² With this method the average number of parallel threads will be

$$N_t h = N_t * a_t / 2, \quad (4.5)$$

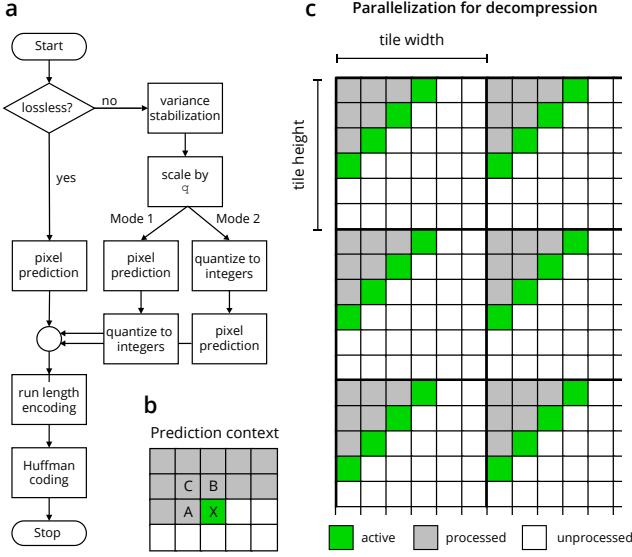


Figure 4.10: B³D algorithm schematics.

(a) Complete algorithm flowchart depicting the main stages of the compression. (b) Prediction context for pixel X, the next sample to be encoded. Three neighboring pixels are considered: left (A), top (B) and top left (C) neighbors. (c) Parallelization scheme for decompression and lossy compression. Already processed pixels are in gray, unprocessed pixels are in white, active pixels are in green.

1 where N_{th} is the number of threads, N_t is the number of tiles, a_t is the tile width and
 2 height for a square tile. Although the threads can be maximized by making smaller tiles,
 3 the compression ratio will be affected, since the corner pixel can't be predicted, and for
 4 the edges only one neighbor can be used instead of 2. We find square tile between 16 and
 5 64 pixels a good choice between decompression speed and compression ratio.

6 The prediction error terms are subsequently run-length encoded and entropy coded
 7 by a fast, CUDA enabled Huffman coder [145, 146] to effectively reduce data size. The
 8 library is making extensive use of parallel prefix sum, which can be used for the effective
 9 parallel execution for both run-length encoding and Huffman coding. For decompression,
 10 the Huffman coding and run-length encoding are first reversed, then each pixel value is
 11 reconstructed from the neighboring values and the prediction errors. Although this im-
 12 plementation sacrifices a little in compression ratio compared to size-optimized methods,
 13 it can surpass a compression speed of 1 GB/s (see Section 4.3.2), which is sufficient even
 14 for the dual camera confocal MuVi-SPIM setup [75].

15 Within noise level compression

16 Noise dependent lossy compression relies on the fact that microscopy images naturally
 17 contain photon shot noise. To increase compression ratio, this method of compression
 18 allows some differences in the pixel values, as long as they are within a predefined pro-
 19 portion of the inherent noise. A special case for this mode is when all compression errors

1 are smaller than the standard deviation of the noise (σ), which we call within noise level
2 (WNL) compression.

3 Our algorithm is inspired by both the near-lossless mode of JPEG-LS [105], where
4 the maximum compression error can be set to a predefined value, and the square root
5 compression scheme [147, 148], that quantizes its input relative to its square. We combine
6 the two methods to achieve noise dependent lossy compression while still retaining good
7 image quality and avoiding banding artifacts.

8 Before the prediction errors are sent to the entropy coder, a quantization can take
9 place that reduces the number of symbols that need to be encoded in order to increase
10 compression ratio. By changing the quantization step, the maximum absolute reconstruc-
11 tion error can be defined, such as when using JPEG-LS. For noise dependent compression,
12 however, the quantization step should be proportional to the image noise, which can be
13 achieved by the following transformation introduced by Bernstein *et al.* [148]:

$$T = 2\sqrt{e + \sigma_{RN}^2}, \quad (4.6)$$

14 where e is the intensity scaled to photoelectrons, and σ_{RN} is the camera read noise. To
15 perform the scaling of digital numbers (DN) to photoelectrons, it's necessary to know
16 the camera offset and conversion parameters: $e = (I - \text{offset}) \cdot g$, where g is the gain
17 in photoelectrons/DN, in I is the original pixel intensity. This transformation assumes
18 a Poisson-Gaussian noise, incorporating the photon shot noise and the camera readout
19 noise, which is a good model for most scientific imaging sensors, such as (EM)CCD or
20 sCMOS.

21 To accommodate for all imaging needs, two options are available in the noise depen-
22 dent lossy mode. In Mode 1, after the stabilizing transform (Equation 4.6), the prediction
23 is performed first, followed by quantization of the prediction errors. This mode reaches
24 a better compression ratio and higher peak signal to noise ratio (PSNR) for the same
25 quantization step compared to Mode 2 (Figure 4.11 a, b), and is recommended for most
26 use cases. For larger quantization steps ($q \geq 3\sigma$), however, Mode 1 might introduce some
27 spatial correlations, because the prediction errors that are being quantized depend on
28 multiple adjacent pixels (Figure 4.11 c, d). Mode 2 excludes this possibility by swapping
29 the quantization and prediction (Figure 4.11 c, d) at the expense of compression ratio.
30 Since no correlations are introduced, Mode 2 is suitable for highly sensitive image anal-
31 ysis tasks, such as single-molecule localization. In this chapter, we use Mode 2 for all
32 single-molecule localization data, and Mode 1 for all other datasets.

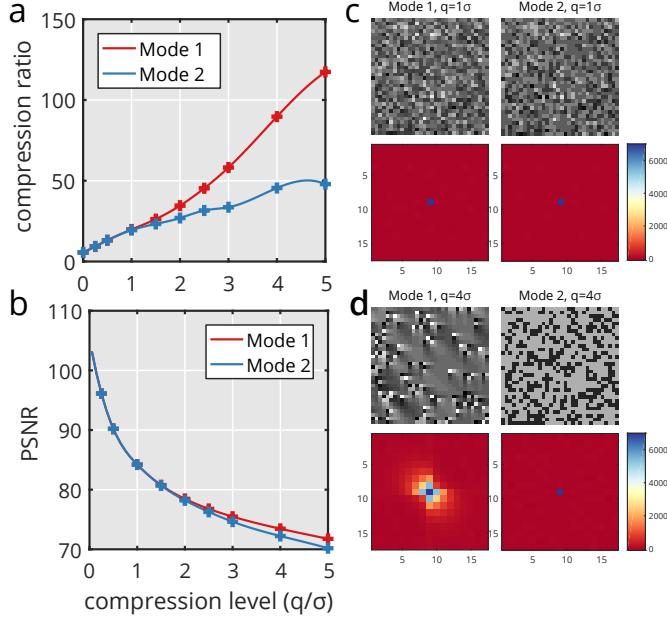


Figure 4.11: Options for noise dependent lossy compression. Comparing Mode 1 (prediction then quantization) and Mode 2 (quantization then prediction) of noise dependent lossy compression in terms of compression ratio, peak signal to noise ratio (PSNR) and spatial correlations introduced to random noise. (a) Compression ratio as a function of the quantization step for Mode 1 and Mode 2. (b) PSNR as a function of the quantization step for Mode 1 and Mode 2. (c, d) Random noise was compressed at various quantization steps both for Mode 1 and Mode 2. Autocorrelation was calculated for the compressed images to see whether the compression introduces any spatial correlation between the pixels. For $q=1\sigma$ both modes are free of correlation (c, top: compressed images, bottom: autocorrelation), however, for $q=2\sigma$ Mode 1 exhibits a correlation pattern (d, top left: compressed image, bottom left: autocorrelation) that is not present in Mode 2 (d, top right compressed image, bottom right: autocorrelation). For more discussion, see Section 4.3.1.

1 Additional noise introduced by compression

- 2 When applying quantization to any kind of data, the quantization error can be modeled as
- 3 an additional uniform noise with standard deviation of $\frac{\delta}{\sqrt{12}}$, where δ is the quantization
- 4 step size [149]. During compression the quantization is proportional to the standard
- 5 deviation of the original image noise, thus the noise on the uncompressed image will be:

$$\sigma_{out} = \sigma_{in} \cdot \sqrt{1 + \frac{q^2}{12}} \quad (4.7)$$

- 6 For the WNL case, when $q = 1\sigma$ this means an increase of 4%, which also coincides with
- 7 the measured increase of localization error for single molecule localization (Figure 4.18a).
- 8 However, this is not the only source of additional noise we have to consider, because at the
- 9 decompression step there is a possibility of getting floating point results after applying
- 10 the inverse of the compression steps, and for most applications these have to be coerced
- 11 to integer numbers. This effectively adds a second quantization, but now at a constant

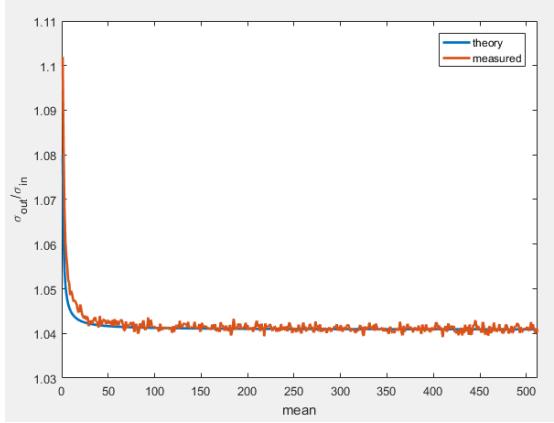


Figure 4.12: Theoretical and measured increase in image noise for WNL compression. Validating Equation 4.8, we plot the relative increase in image noise as a function of the mean. Blue line: plot of Equation 4.8 Red line: plot of measured data. To obtain the measurement, we compressed a stack of 512 images consisting of Poisson noise, each with a different mean. After WNL compression the data was read in Matlab, and the standard deviation was calculated for each frame. The ratio σ_{in}/σ_{out} is plotted as a function of the mean.

1 quantization step of 1. This results in an additional uniform noise with variance of $\frac{1}{12}$:

$$\sigma_{out} = \sigma_{in} \cdot \sqrt{1 + \frac{q^2}{12}} + \frac{1}{12} \quad (4.8)$$

2 We verified this by compressing 512 images (1024×1024 pixels) of random Poisson noise
3 with different means (1..512), and calculated the standard deviation for each frame after
4 the decompression step. Finally, we plotted the ratio σ_{out}/σ_{in} as a function of the mean
5 m (Figure 4.12), and we found that it is in very good agreement with the theory outlined
6 above.

7 4.3.2 Evaluation of the compression algorithm

8 We compared our algorithm's performance with some of the most commonly used image
9 formats in the scientific field: TIFF (LZW) and JPEG2000. Furthermore, we also in-
10 cluded the state of the art KLB compression [139], which was especially designed for fast
11 compression of large light-sheet datasets. We measured compression speed, decompres-
12 sion speed and resulting file size for all algorithms (Figure 4.13a). Only B³D is capable
13 of handling the sustained high data rate of modern sCMOS cameras typically used in
14 light-sheet microscopy, while still maintaining compression ratios comparable to more
15 complex, but much slower algorithms (Table B2 in Appendix B).

16 Using the noise dependent lossy mode with $q = 1\sigma$ (WNL), the compression ra-
17 tio massively increases for all imaging modalities compared to the lossless mode (Fig-
18 ure 4.13b) without any apparent loss in image quality (Figure 4.14). Furthermore, the av-
19 erage compression error is considerably smaller than the image noise itself (Figure 4.15).

4.3 B³D image compression

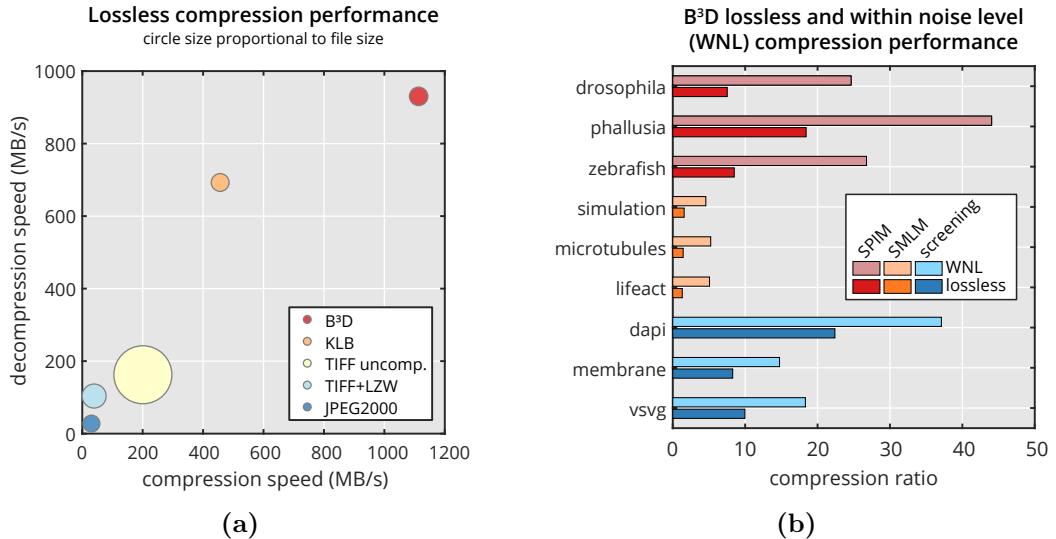


Figure 4.13: Compression performance. (a) Performance comparison of our B³D compression algorithm (red circle) vs. KLB (orange), uncompressed TIFF (light yellow), LZW compressed TIFF (light blue) and JPEG2000 (blue) regarding write speed (horizontal axis), read speed (vertical axis) and file size (circle size). (see also Table B2). (b) WNL compression performance compared with lossless performance for 9 different dataset representing 3 imaging modalities (SPIM, SMLM, screening). Compression ratio = original size / compressed size. For description of datasets see Table B3 in Appendix B.

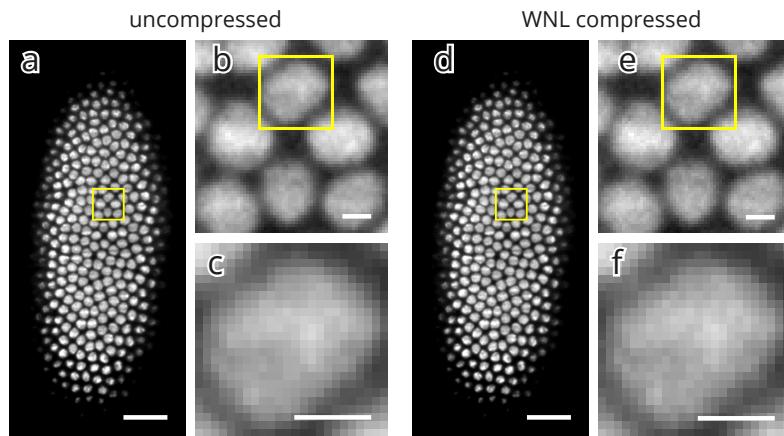


Figure 4.14: Image quality of a WNL compressed dataset. WNL compression of a *Drosophila* recording taken in the MuVi-SPIM setup. Compression ratio: 19.83. (a–c) Uncompressed image of the whole field of view (a), and zoomed in smaller regions (b, c). (d–f) WNL compressed image of the whole field of view (d), and zoomed in smaller regions (e, f). Scale bars: 25 µm (a, e); 2.5 µm (b, c, e, f).

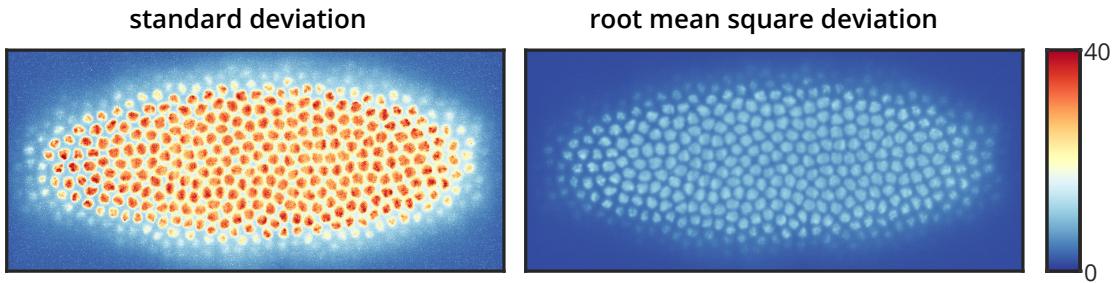


Figure 4.15: Compression error compared to image noise. To compare the difference arising from WNL compression to image noise, we imaged a single plane 100 times in a *Drosophila melanogaster* embryo expressing H2Av-mCherry nuclear marker at 38 ms intervals. The whole acquisition took 3.8 s, for which the sample can be considered stationary. To visualize image noise, the standard deviation was calculated for the uncompressed images (left). All images were then WNL compressed, and the root mean square deviation was calculated compared to the uncompressed images (right). The root mean square deviation on average is 3.18 times smaller than the standard deviation of the uncompressed images.

1 To see how the noise-dependent compression affects common imaging pipelines, we
 2 tested the effect of different levels of compression on 3D nucleus and membrane segmen-
 3 tation in light-sheet microscopy, and on single-molecule localization accuracy in super-
 4 resolution microscopy. First, we imaged a *Drosophila melanogaster* embryo expressing
 5 an H2Av-mCherry nuclear marker in the MuVi-SPIM and segmented the nuclei with
 6 Ilastik [150] (Figure 4.16a and Section 4.3.4). Then we performed noise dependent com-
 7 pression at various quality levels and calculated the segmentation overlap compared to
 8 the uncompressed stack (Section 4.3.4). At WNL compression ($q = 1\sigma$) the segmenta-
 9 tion overlap is almost perfect (Figure 4.16b) with an overlap score of 0.996. Even when
 10 increasing the quantization step to 4σ (Figure 4.16c) the overlap score stays at 0.98 and
 11 only drops below 0.97 when the compression ratio is already above 120 (quantization
 12 step of 5σ , Figure 4.16d). We got similar results for a membrane segmentation pipeline
 13 that is used with *Phallusia mammillata* embryos (Figure 4.17 and Section 4.3.4).

14 Next, we evaluated our compression algorithm in the context of single molecule lo-
 15 calization, and measured how the localization precision is affected by an increasing com-
 16 pression ratio. We compressed a single-molecule localization microscopy (SMLM) dataset
 17 of immuno-detected microtubules (Figure 4.18a) with increasing compression levels. For
 18 WNL compression ($q = 1\sigma$) no deterioration of the image was visible (Figure 4.18b),
 19 and even for the case of $q = 4\sigma$ the compression induced errors were much smaller than
 20 the resolvable features (Figure 4.18c). To quantify the impact of compression on the
 21 localization error, we used a simulated dataset (Section 4.3.4) and compared the local-
 22 ization output of different compression levels to the ground truth (Figure 4.18d). Lossless
 23 compression resulted in a compression ratio of 2.7, whereas WNL compression reached
 24 a compression ratio of 5.0, while increasing the localization error by only 4%. This also
 25 coincides with the theoretical increase of image noise (Section 4.3.1). Furthermore, the
 26 increase in localization error was not dependent on the signal to background noise ratio

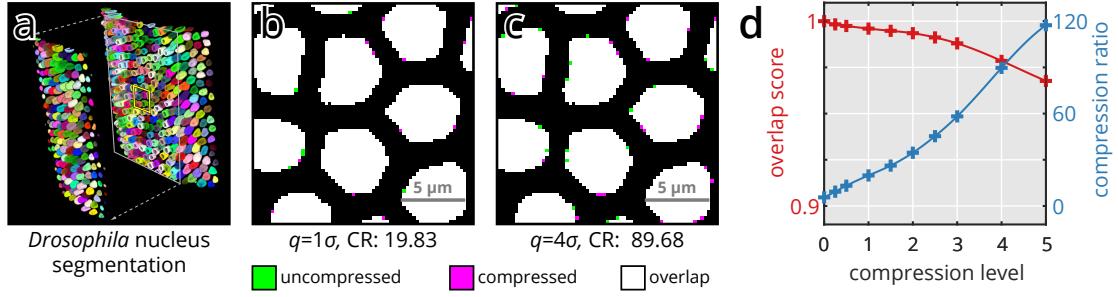


Figure 4.16: Influence of noise dependent lossy compression on 3D nucleus segmentation. A *Drosophila melanogaster* embryo expressing H2Av-mCherry nuclear marker was imaged in MuVi-SPIM [45], and 3D nucleus segmentation was performed (Section 4.3.4) (a). The raw data was subsequently compressed at increasingly higher compression levels, and segmented based on the training of the uncompressed data. To visualize segmentation mismatch, the results of the uncompressed (green) and compressed (magenta) datasets are overlaid in a single image (b, c; overlap in white). Representative compression levels were chosen at two different multiples of the photon shot noise, at $q=1\sigma$ (b) and $q=4\sigma$ (c). For all compression levels the segmentation overlap score (Section 4.3.4) was calculated and is plotted in (d) along with the achieved compression ratios.

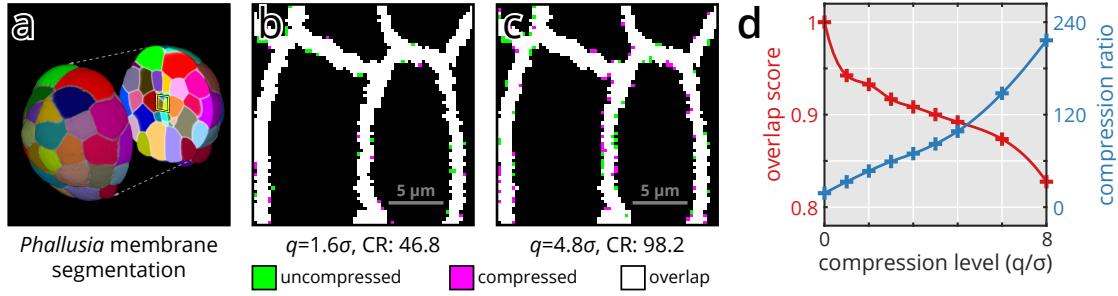


Figure 4.17: Influence of noise dependent lossy compression on 3D membrane segmentation. A *Phallusia mammillata* embryo expressing PH-citrine membrane marker was imaged in MuVi-SPIM [45], and 3D membrane segmentation was performed (Section 4.3.4) (a). The raw data was subsequently compressed at increasingly higher compression levels, and segmented using the same settings as the uncompressed data. To visualize segmentation mismatch, the results of the uncompressed (green) and compressed (magenta) datasets are overlaid in a single image (b, c; overlap in white). Representative compression levels were chosen at two different multiples of the photon shot noise, at $q=1.6\sigma$ (b) and $q=4.8\sigma$ (c). For all compression levels the segmentation overlap score (Section 4.3.4) was calculated and is plotted in (d) along with the achieved compression ratios.

1 (Figure 4.19).

2 4.3.3 HDF5 integration

- 3 To make our compression method more accessible, we developed a filter plugin for HDF5.
- 4 Because of its versatility, HDF5 has emerged as the de facto standard in the open source
- 5 light sheet microscopy field, and is also the basis for the widely used BigDataViewer
- 6 [151] in Fiji [116]. Starting from version 1.8.11 (May 2013), HDF5 supports dynamically
- 7 loaded filters, and is able to load third party components without having to modify
- 8 any already installed files. When loading a B³D compressed image in an HDF5 enabled
- 9 application, the library automatically calls our filter plugin, decompresses the image on
- 10 the GPU, and copies it back into CPU memory.

4.3 B³D image compression

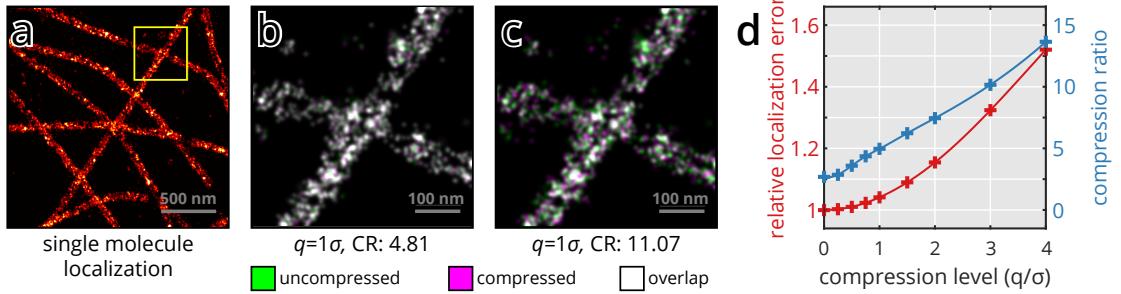


Figure 4.18: Influence of noise dependent lossy compression on single-molecule localization. Microtubules, immunolabeled with Alexa Fluor 647 were imaged by SMLM (a). The raw data was compressed at increasingly higher compression levels, and localized using the same settings as the uncompressed data. To visualize localization mismatch, the results of the uncompressed (green) and compressed (magenta) datasets are overlaid in a single image (b, c; overlap in white). Two representative compression levels were chosen at $q=1\sigma$ (b) and $q=4\sigma$ (c). To assess the effects of compression on localization precision, a simulated dataset with known emitter positions was compressed at various levels. For all compression levels the relative localization error (normalized to the Cramér–Rao lower bound) was calculated and is plotted in (d) along with the achieved compression factors.

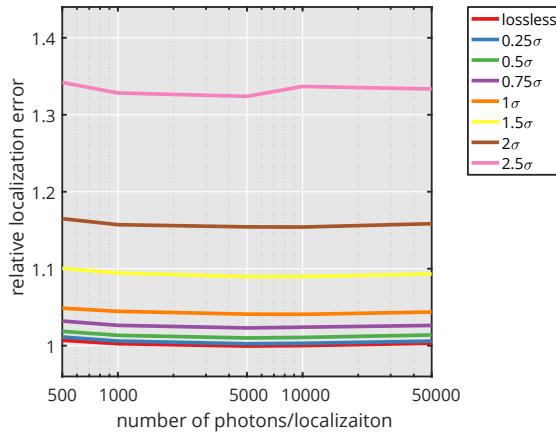


Figure 4.19: Change in localization error only depends on selected quantization step. We simulated multiple datasets (Section 4.3.4) with different average photon numbers per localization. Background was kept at a constant average of 20 photons/pixel. Datasets were compressed at multiple compression levels (see legend), and localization error relative to the Cramér–Rao lower bound was calculated. The relative localization error only depends on the compression level, and not on the signal to background illumination ratio.

1 Since HDF5 is extensively used in many scientific/image analysis software, this plugin
2 format is especially suitable to equip existing software with compression/decompression
3 capabilities. To read compressed files no modification is required, and any software sup-
4 porting HDF5 should be compatible. The following software have been tested with our
5 filter plugin and are able to read B³D compressed files: Fiji (also with BigDataViewer),
6 Imaris 8.4.1, Ilastik 1.2.0, Matlab R2016a, Python 2.7.10 and 3.5.3, LabVIEW 2015,
7 C++.

8 Writing compressed HDF5 files is possible if the user has direct control over the
9 file writing routine, as an additional command is required to set up compression. This
10 functionality has been tested in the following environments: C++, Python 2.7.10 and
11 3.5.3, LabVIEW 2015.

12 4.3.4 Methods

13 Compression benchmarking

14 For all presented benchmarks, TIFF and JPEG2000 performance was measured through
15 MATLAB's imwrite and imread functions, while KLB and B³D performance was mea-
16 sured in C++. All benchmarks were run on a computer featuring 32 processing cores
17 (2×Intel Xeon E5-2620 v4), 128 GB RAM and an NVIDIA GeForce GTX 970 graph-
18 ics processing unit. Read and write measurements were performed in RAM to minimize
19 I/O overhead, and are an average of 5 runs. SMLM datasets were provided by Joran De-
20 schamps (EMBL, Heidelberg), and were originally published in [152] and [153]. Screening
21 datasets were provided by Jean-Karim Hériché (EMBL, Heidelberg), and were originally
22 published in [154]

23 Light-sheet imaging

24 *Drosophila* embryos were imaged in the MuVi-SPIM setup [45] using the electronic con-
25 focal slit detection (eCSD) [75]. Embryos were collected on an agar juice plate, and
26 dechorionated in 50% bleach solution for 1 min. The embryos were then mounted in a
27 shortened glass capillary (Brand 100 µl) filled with 0.8% GelRite (Sigma-Aldrich), and
28 pushed out of the capillary to be supported only by the gel.

29 3D nucleus segmentation

30 3D nucleus segmentation of *Drosophila* embryos was performed using Ilastik [150]. The
31 original dataset was compressed at different quantization levels, then upscaled in z to ob-
32 tain isotropic resolution. To identify the nuclei, we used the pixel classification workflow,
33 and trained it on the uncompressed dataset. This training was then used to segment the
34 compressed datasets as well. Segmentation overlap was calculated in Matlab using the

1 Sørensen–Dice index [155, 156]:

$$QS = 2 |A \cap B| / (|A| + |B|) \quad (4.9)$$

2 where the sets A and B represent the pixels included in two different segmentations.

3 **3D membrane segmentation**

4 Raw MuVi-SPIM recordings of *Phallusia mammillata* embryos expressing PH-citrine
5 membrane marker were kindly provided by Ulla-Maj Fiuzza (EMBL, Heidelberg). Each
6 recording consisted of 4 views at 90 degree rotations. The views were fused using an
7 image based registration algorithm followed by a sigmoidal blending of the 4 views. The
8 fused stack was then segmented using the MARS algorithm [157] with an hmin parameter
9 of 10. The raw data (all 4 views) was compressed at different levels, and segmented using
10 the same pipeline. Segmentation results were then processed in Matlab to calculate the
11 overlap score for the membranes using the Sørensen–Dice index.

12 **Single-molecule localization imaging**

13 In order to visualize microtubules, U2OS cells were treated as in [152] and imaged in a
14 dSTORM buffer [158]. In brief, the cells were permeabilized and fixed with glutaralde-
15 hyde, washed, then incubated with primary tubulin antibodies and finally stained with
16 Alexa Fluor 647 coupled secondary antibodies. The images were recorded on a home-built
17 microscope previously described [152], in its 2D single-channel mode.

18 **Single-molecule localization data analysis**

19 Analysis of single-molecule localization data was performed on a custom-written MAT-
20 LAB software as in [153]. Pixel values were converted to photon counts according to
21 measured offset and calibrated gain of the camera (EMCCD iXon, Andor). The back-
22 ground was estimated with a wavelet filter [159], background-subtracted images were
23 thresholded and local maxima were detected on the same images. 7-pixel ROIs around
24 the detected local maxima were extracted from the raw images and fitted with a GPU
25 based MLE fitter [160]. Drift correction was performed based on cross-correlation. Fi-
26 nally, images were reconstructed by filtering out localizations with a high uncertainty
27 (>30 nm and large PSF (>150 nm) and Gaussian rendering.

28 **Simulation of single-molecule localization data**

29 Single molecule localization data was simulated in Matlab by generating a grid of pixe-
30 lated Gaussian spots with standard deviation of 1 pixel. With a pixel size of a 100 nm,

1 this corresponds to a FWHM of 235.48 nm. The center of each spot was slightly offset
2 from the pixel grid at 0.1 pixel increments in both x and y directions. To this ground
3 truth image a constant value was added to simulate illumination background, and finally
4 Poisson noise was applied to the image. This process was repeated 10,000 times to obtain
5 enough images for adequate accuracy.

6 **Code availability**

7 Code used for analyzing data, B³D source code and compiled binaries, including a filter
8 plugin for HDF5, is available for download at <https://git.embl.de/balazs/B3D>.

9 **4.4 Conclusions**

10 Our algorithm is implemented in C++, and allows for easy integration through an API
11 with various programming languages. The library was tested on Linux (Ubuntu 16.04)
12 and Windows (10). Additionally, we implemented a filter plugin for HDF5 which enables
13 a seamless integration in all software packages that are supporting the native HDF5
14 library, such as Matlab, Python, Imaris, or Ilastik. Due to B³D's efficient compression
15 ratio and its high decompression speed, loading data is often accelerated: For a state-of-
16 the-art hard drive with 200 MB/s bandwidth, loading a 2 GB uncompressed 3D stack of
17 images takes about 10 seconds. With an average compression ratio of 20 fold in the WNL
18 mode, the loading time is reduced to 0.5 seconds followed by 2 seconds of decompression,
19 which yields a factor of four speed-up. It is also worth to note, that the achieved WNL
20 compression reduces the camera data rate to below 40 MB/s, well below the 1 Gb/s
21 Ethernet standard. This enables to use current network infrastructure to move data to
22 long term storage and even makes the use of cloud services possible. Altogether, B³D, our
23 efficient GPU-based image compression library allows for exceptionally fast compression
24 speed and greatly increases compression ratio with its WNL scheme, offering a versatile
25 tool that can be easily tailored to any high-speed microscopy environment.

¹ **Chapter 5**

² **Discussion**

³ **5.1 New scientific results**

⁴ **Thesis I.** *I have designed and constructed a new light-sheet microscope suitable for*
⁵ *high resolution imaging of delicate samples. A novel arrangement of two high numeri-*
⁶ *cal aperture objectives in 120 degrees combined with a tilted light-sheet allows for near*
⁷ *isotropic resolution while increasing light collection efficiency by a factor of two.*

⁸ Corresponding publications: [J3],[J2], [J1]

⁹ Dual Mouse-SPIM is a novel design for symmetric light-sheet microscopy. The use
¹⁰ of high NA objectives in 120° not only increases volumetric resolution compared to the
¹¹ conventional 90° setup, but due to the larger detection angle, light collection efficiency
¹² is doubled. This is especially beneficial for delicate, light-sensitive specimens, such as
¹³ mouse embryos, since phototoxic effects are reduced while the contrast is preserved.

¹⁴ As part of the microscope I have designed a custom beam splitter unit that allows
¹⁵ the use of a single galvo scanner to generate the light-sheet for both objectives. I have
¹⁶ also designed a custom detection merging unit that allows the use of a single camera for
¹⁷ both detection views.

¹⁸ I have characterized the optical properties of the microscope, measured the illumina-
¹⁹ tion profile and point spread function. With a 3.6 µm thick light-sheet, a 95 µm field of
²⁰ view is evenly illuminated. Dual view imaging of bead samples revealed a lateral resolu-
²¹ tion of 314 nm, and axial resolution of 496 nm. This is a 2.67× improvement compared
²² to the axial resolution of a single lens. I have also demonstrated the imaging capabilities
²³ of the microscope on *Drosophila* embryos and mouse zygotes.

²⁴ **Thesis II.** *I have developed a GPU-based image processing pipeline for multi-view*
²⁵ *light-sheet microscopy that enables real time fusion of opposing views.*

²⁶ Corresponding publications: [C1], [C2], [C3]

I have developed a GPU-based image preprocessing pipeline, which integrates directly to our universal microscope control software in LabVIEW. The pipeline currently supports background subtraction and background masking, furthermore it is capable of fusing opposing views of the same plane faster than real-time. I have shown that it is possible to reduce the registration of opposing camera views from a 3D alignment to a 2D alignment without any negative effects in image quality and resolution. This massively reduces the necessary computing resources, and allows the use of CUDA textures for faster than real-time image fusion. Processing speed of this implementation is 138 fps, a $18.3\times$ increase compared to a single threaded CPU implementation.

Thesis III. *I have developed a new image compression algorithm that enables noise dependent lossy compression of light microscopy images, and can reach a compression ratio of 100 fold while preserving the results of downstream data analysis steps. A fast CUDA implementation allows for real-time image compression of high-speed microscopy images.*

Corresponding publications: [J4], [C1], [C2], [C3]

Since many high-speed microscopy methods generate immense amounts of data, easily reaching terabytes per experiment, image compression is especially important to efficiently deal with such datasets. Existing compression methods suitable for microscopy images are not able to deal with the high data rate of modern sCMOS cameras ($\sim 800 \text{ MB/s}$).

I developed a GPU-based parallel image compression algorithm called B³D, capable of over 1 GB/s throughput, allowing live image compression. To further reduce the data size, I developed a noise dependent lossy compression that only modifies the data in a deterministic manner. The allowed differences for each pixel can be specified as a proportion of the inherent image noise, accounting for photon shot noise and camera readout noise. Due to the use of pixel prediction, the subjective image quality is higher than for other methods that simply quantize the square root of the images.

Thesis IV. *I have shown that within noise level compression does not significantly affect the results of most commonly used image processing tasks, and it allows a $3.32\times$ average increase in compression ratio compared to lossless mode.*

Corresponding publications: [J4], [C1], [C2], [C3]

As data integrity in microscopy is paramount for drawing the right conclusions from the experiments, using a lossy compression algorithm might be controversial. I have shown that the within noise level (WNL) mode of B³D does not significantly affect the results of several commonly used image analysis tasks. For light-sheet microscopy data I have shown that WNL compression introduces less variation to the image than the photon shot noise. When segmenting nuclei of *Drosophila* embryos and membranes of *Phallusia*

1 embryos, the overlap of the segmented regions of uncompressed and WNL compressed
2 datasets were 99.6% and 94.5% respectively, while compression ratios were 19.83 for
3 *Drosophila* and 40.01 for *Phallusia* embryos. For single molecule localization microscopy
4 data I have shown that WNL compression only introduces 4% increase in localization
5 uncertainty, while the average compression ratio is increased from 1.44 (lossless) to 4.96
6 (WNL). I have also shown that change in localization error due to the compression does
7 not depend on the SNR of the input images.

8 5.2 Application of the results

9 Both the new Dual Mouse-SPIM microscope and the GPU-based image processing and
10 compression pipeline have direct applications in light-sheet imaging of embryonic devel-
11 opment.

12 Multiple potential collaborators indicated their interest in using the Dual Mouse-
13 SPIM for their studies in mouse embryonic development. The Hiiragi group, focusing
14 on symmetry breaking events in the pre-implantation and early post-implantation stages
15 would like to use this system for imaging larger specimens from multiple direction, which
16 is not possible on their current microscopes, and could allow them to observe previously
17 unknown mechanisms. The Ellenberg group is interested in investigating chromosome
18 missesgregation mechanisms in the first few divisions during embryonic development. The
19 increased axial resolution of this system will allow to track each individual chromosome
20 during the division process, which was not possible on their current setup due to the
21 insufficient axial resolution.

22 The GPU-based image processing pipeline, especially the 2D fusion of opposing
23 views is already being used on our lab's workhorse microscope, the MuVi-SPIM. Being
24 able to fuse the two views of the opposing objectives during imaging not only results in
25 considerable storage space savings, but significantly speeds up the data analysis as well.

26 The image compression algorithm, B³D, although was developed with light-sheet
27 microscopy in mind, has a more wide-spread use-case. Any kind of high-speed, high-
28 throughput light-microscopy experiment can benefit form the massive data reduction
29 offered by the within noise level mode. Since the compression can also be done imme-
30 diately during imaging, not only the storage requirements, but the data bandwidth is
31 reduced as well, which renders the use of high performance RAID arrays and 10 Gbit
32 networks unnecessary, further reducing costs. Due to the similarly high decompression
33 speed, reading the data is also accelerated, which can be beneficial for data browsing
34 and 3D rendering applications. Several companies of different fields already expressed
35 their interest in the compression library, including Bitplane AG (3D data analysis and
36 visualisation), Luxendo GmbH (light-sheet microscopy), and Hamamatsu Photonics K.K

5.2 Application of the results

¹ (camera and sensor manufacturing).

¹ Appendix

² A Bill of materials

³ Optical components

- ⁴ • Lenses

- ⁵ – 2×Nikon CFI75 Apo LWD 25x/1.10w water dipping objectives
- ⁶ – 2×Nikon ITL200 200 mm tube lens
- ⁷ – 2×200 mm x 25 mm Dia. achromatic lens (Edmunds Optics, #47-645)
- ⁸ – 2×400 mm x 40 mm Dia. achromatic lens (Edmunds Optics, #49-281)
- ⁹ – 3×75 mm x 25 mm Dia. achromatic lens (Edmunds Optics, #47-639)
- ¹⁰ – SILL 112751 1:2 beam expander

- ¹¹ • Filters

- ¹² – 2×BrightLine quad-edge dichroic beam splitter (Semrock, Di03-R405/488/561/635-t3-25x36)
- ¹³ – EdgeBasic 488 nm long pass filter (Semrock, BLP01-488R-25)
- ¹⁴ – BrightLine 525/50 band pass filter (Semrock, FF03-525/50-25)
- ¹⁵ – EdgeBasic 561 nm long pass filter (Semrock, BLP02-561R-25)
- ¹⁶ – RazorEdge 647 nm long pass filter (Semrock, LP02-647RU-25)

- ¹⁷ • Mirrors

- ¹⁹ – 6×1” Broadband Dielectric Elliptical Mirror (Thorlabs, BBE1-E03)
- ²⁰ – 2×30 mm Broadband 1/10λ Mirror (OptoSigma, TFMS-30C05-4/11)
- ²¹ – 10 Pack of 1” Protected Silver Mirrors (Thorlabs, PF10-03-P01-10)
- ²² – Knife-Edge Right-Angle Prism Dielectric Mirror (Thorlabs, MRAK25-E02)

²³ Mechanical components

- ²⁴ • 40 mm travel range pneumatic cylinder (Airtac, HM-10-040)
- ²⁵ • 5/2-way electric valve (Airtac, M-20-510-HN)
- ²⁶ • 2×25 mm extended contact bearing steel stage (OptoSigma, TSDH-251C)
- ²⁷ • 30x90 mm stainless steel slide (OptoSigma, IPWS-F3090)
- ²⁸ • close proximity gimbal mirror mount (Thorlabs, GMB1/M)
- ²⁹ • 30 mm cage elliptical mirror mount (Thorlabs, KCB1E)
- ³⁰ • Melles Griot Performance Plus Optical Breadboard
- ³¹ • 4×Newport Stabilizer, High Performance laminar Flow Isolator, I-2000 Series

1 Custom parts

2 All parts are (anodized) aluminium, unless stated otherwise.

- 3 • 2×mirror holder block**
- 4 • Front plate for objective, chamber and mirror mounting**
- 5 • Imaging chamber (PEEK)**
- 6 • Wedge ring and matching threaded ring to fasten objectives**
- 7 • Camera bridge**
- 8 • Illumination splitter unit**
- 9 • adapter plates to mount stages**

10 Electronics

- 11 • Embedded system (National Instruments, cRIO-9068) equipped with:**
 - 12 – 2×C series digital I/O card (NI 9401)**
 - 13 – 1×C Series 100 kS/s 4-channel Voltage Output Module (NI 9263)**
 - 14 – 1×C Series 25 kS/s 16-channel Voltage Output Module (NI 9264)**
- 15 • Omicron SOLE-3 laser combiner, with 488, 561 and 638 nm laser lines**
- 16 • Andor Zyla 4.2 sCMOS Camera**
- 17 • Galvanometric scanner mirror (Cambridge Technology, 6210B)**
- 18 • 6 position filter wheel (Ludl Electronic Products, 96A361)**
- 19 • Filter wheel controller unit (Ludl Electronic Products, MAC5000)**
- 20 • 2 piezoelectric stages (Nanos Instruments, LPS-30-30-1-V2_61-S-N)**
- 21 • 2 stage controller boards (Nanos Instruments, BMC101)**

B Supplementary Tables

¹ B Supplementary Tables

Table B1: Data sizes in microscopy. Typical devices used for confocal microscopy, high-content screening, single-molecule localization microscopy and light-sheet microscopy and their data production characteristics. Data visualized on Figure 4.1

	imaging device	image size	frame rate	data rate	data size
SPIM	2x sCMOS camera (e.g. Hamamatsu ORCA Flash4.0)	2048x2048	50/s	800 MB/s	10 TB
SMLM	2x EMCCD camera (e.g. Andor iXon Ultra 897)	512x512	56/s	56 MB/s	500 GB
screening	CCD camera (e.g. Hamamatsu ORCA-R2)	1344x1024	8.5s/	22 MB/s	5 TB
confocal	Zeiss LSM 880, 10 channels	512x512	5/s	12.5 MB/s	50 GB

Table B2: Lossless compression performance. B³D is compared with various popular lossless image compression methods regarding write speed, read speed and compression ratio (original size / compressed size). Data visualized on Figure 4.13.

	write speed	read speed	CR	file size
B³D	1,115.08 MB/s	928.97 MB/s	9.861	100%
KLB	283.19 MB/s	619.95 MB/s	10.571	93.28%
JPEG2000	31.94 MB/s	26.38 MB/s	11.782	83.69%
TIFF uncompressed	202.32 MB/s	161.08 MB/s	1.00	986.1%
TIFF + LZW	40.85 MB/s	102.37 MB/s	5.822	169.37%

B Supplementary Tables

Table B3: Datasets used for benchmarking compression performance.

Dataset name	Imaging modality	Description	Size (MB)
drosophila	SPIM	dataset acquired in MuVi-SPIM of a <i>Drosophila melanogaster</i> embryo expressing H2Av-mCherry nuclear marker	494.53
zebrafish	SPIM	dataset acquired in MuVi-SPIM of a zebrafish embryo expressing b-actin::GCaMP6f calcium sensor	2,408.00
phallusia	SPIM	dataset acquired in MuVi-SPIM of a <i>Phallusia mammillata</i> embryo expressing PH-citrine membrane marker	1,323.88
simulation	SMLM	MT0.N1.LD-2D simulated dataset of microtubules labeled with Alexa Fluor 647 from SMLMS 2016 challenge	156.22
microtubules	SMLM	microtubules immuno-labeled with Alexa Fluor 674-bound antibodies in U2OS cells	1,643.86
lifeact	SMLM	actin network labeled with LifeAct-tdEOS in U2OS cells	3,316.15
dapi	screening	wide field fluorescence images of DAPI stained HeLa Kyoto cells [154]	1,005.38
vsvg	screening	wide field fluorescence images of CFP-tsO45G proteins in HeLa Kyoto cells [154]	1,005.38
membrane	screening	wide field fluorescence images of membrane localized CFP-tsO45G proteins labeled with AlexaFluor647 in HeLa Kyoto cells [154]	1,005.38

¹ C Light collection efficiency of an objective

² Let's define light collection efficiency η as the ratio of collected photons and all emitted
³ photons:

$$\eta = \frac{N_{collected}}{N_{emitted}}$$

⁴ Since we can assume that the direction of photons emitted from a fluorescent molecule
⁵ are random, the light collection efficiency will correspond to the solid angle subtended
⁶ by the objective front lens at the focal point. To calculate this, let's consider the unit
⁷ sphere centered at the focal point, and calculate the surface area of the spherical cap
⁸ corresponding to the objective acceptance angle α (Fig. C1a). The area of the cap can
⁹ be expressed as a function of the angle:

$$A_{cap} = 2\pi r^2(1 - \cos \alpha)$$

¹⁰ The surface area of the full sphere is calculated as:

$$A_{sph} = 4\pi r^2$$

¹¹ For both equations r is the radius of the sphere. From here, the light collection efficiency
¹² can be calculated as:

$$\eta = \frac{N_{collected}}{N_{emitted}} = \frac{A_{cap}}{A_{sph}} = \frac{1 - \cos \alpha}{2}$$

¹³ As most objectives are characterized by the numerical aperture, we also plot η as a
¹⁴ function of the NA on Figure C1b.

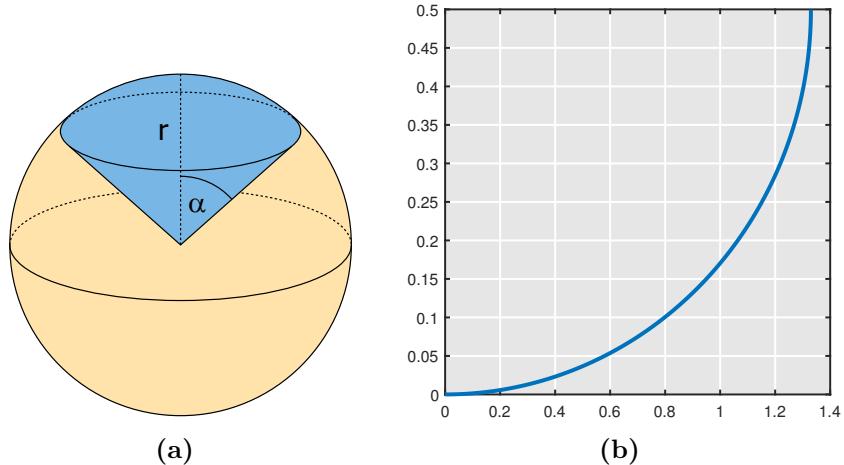


Figure C1: Light collection efficiency of an objective. (a) Light collection efficiency is the ratio of photons collected by the objective and all emitted photons. If the fluorophores are emitted randomly in all directions, it will be the surface ratio of the conical section (blue) to the whole sphere. (b) Light collection efficiency (η) as a function of the numerical aperture (NA).

1 D 3D model of Dual Mouse-SPIM

**2 To view the 3D figure on the next page, Adobe Reader is required. Click on the figure
3 to activate the 3D view.**

4 Navigation:

- 5 • zoom: mouse wheel / right click and drag vertically**
- 6 • rotate: left click and drag**
- 7 • pan: left + right click and drag / Ctrl + click and drag**

Interactive 3D figure
Click to activate

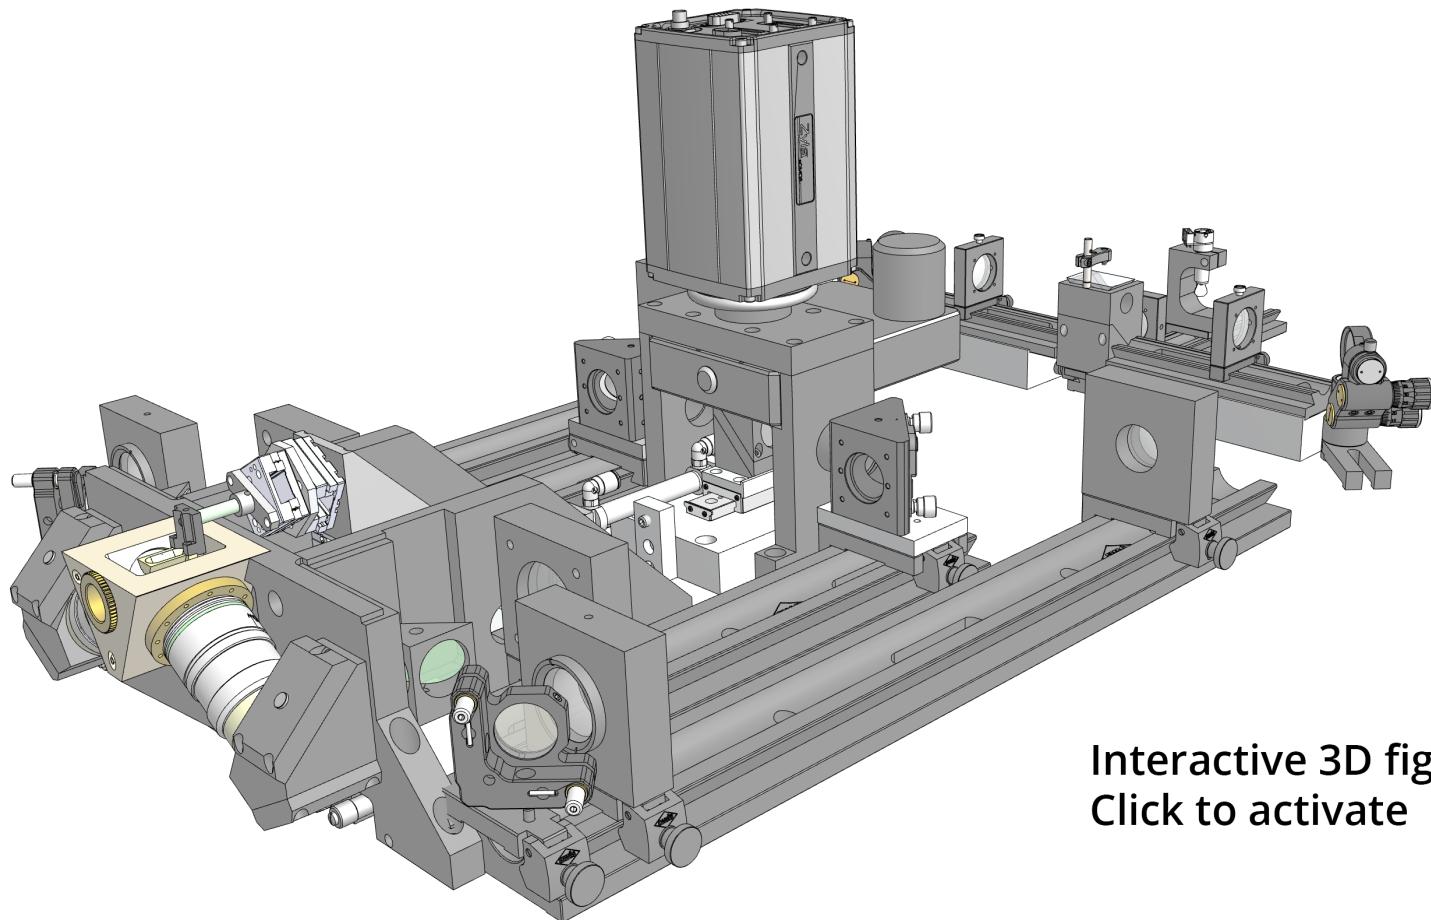


Figure D1: 3D model of DualMouse-SPIM.

¹ References

² The author's publications

- ³ [J1] Patrick Hoyer, Gustavo de Medeiros, Bálint Balázs, Nils Norlin, Christina Be-
⁴ sir, Janina Hanne, Hans-Georg Kräusslich, Johann Engelhardt, Steffen J. Sahl,
⁵ Stefan W. Hell, and Lars Hufnagel. “Breaking the diffraction limit of light-sheet
⁶ fluorescence microscopy by RESOLFT”. *Proceedings of the National Academy of
⁷ Sciences* 113.13 (Mar. 2016), pp. 3442–3446. DOI: [10.1073/pnas.1522292113](https://doi.org/10.1073/pnas.1522292113)
⁸ (cit. on pp. 14, 84).
- ⁹ [J2] Petr Strnad, Stefan Gunther, Judith Reichmann, Uros Krzic, Balint Balazs, Gus-
¹⁰ tavo de Medeiros, Nils Norlin, Takashi Hiragi, Lars Hufnagel, and Jan Ellenberg.
¹¹ “Inverted light-sheet microscope for imaging mouse pre-implantation develop-
¹² ment”. *Nature Methods* 13.2 (Feb. 2016), pp. 139–142. DOI: [10.1038/nmeth.3690](https://doi.org/10.1038/nmeth.3690)
¹³ (cit. on pp. 13, 14, 20, 21, 35, 84).
- ¹⁴ [J3] Gustavo de Medeiros, Bálint Balázs, and Lars Hufnagel. “Light-sheet imaging
¹⁵ of mammalian development”. *Seminars in Cell & Developmental Biology*. Mam-
¹⁶ malian development 55 (July 2016), pp. 148–155. DOI: [10.1016/j.semcdb.2015.11.001](https://doi.org/10.1016/j.semcdb.2015.11.001) (cit. on pp. 13, 84).
- ¹⁸ [J4] Balint Balazs, Joran Deschamps, Marvin Albert, Jonas Ries, and Lars Hufnagel.
¹⁹ “A real-time compression library for microscopy images”. *bioRxiv* (July 2017),
²⁰ p. 164624. DOI: [10.1101/164624](https://doi.org/10.1101/164624) (cit. on p. 85).

²¹ The author's others publications

- ²² [J5] Zoltán Jakus, Edina Simon, Bálint Balázs, and Attila Mócsai. “Genetic deficiency
²³ of Syk protects mice from autoantibody-induced arthritis”. *Arthritis and Rheuma-
²⁴ tism* 62.7 (July 2010), pp. 1899–1910. DOI: [10.1002/art.27438](https://doi.org/10.1002/art.27438).

-
- 1 [J6] Balázs Győrffy, Zsombor Benke, András Lánczky, Bálint Balázs, Zoltán Szállási,
2 József Timár, and Reinhold Schäfer. “RecurrenceOnline: an online analysis tool to
3 determine breast cancer recurrence and hormone receptor status using microarray
4 data”. *Breast Cancer Research and Treatment* (July 2011). DOI: 10.1007/s10549-
5 011-1676-y.
- 6 [J7] Weiwei Shi, Balint Balazs, Balazs Györffy, Tingting Jiang, W. Fraser Symmans,
7 Christos Hatzis, and Lajos Pusztai. “Combined analysis of gene expression, DNA
8 copy number, and mutation profiling data to display biological process anomalies
9 in individual breast cancers”. *Breast Cancer Research and Treatment* 144.3 (Mar.
10 2014), pp. 561–568. DOI: 10.1007/s10549-014-2904-z.

11 **The author’s conference presentations**

- 12 [C1] Bálint Balázs, Marvin Albert, and Lars Hufnagel. “GPU-based image processing
13 for multiview microscopy data”. *Light Sheet Fluorescence Microscopy International
14 Conference*. Sheffield, UK, Sept. 2016 (cit. on pp. 84, 85).
- 15 [C2] Bálint Balázs, Marvin Albert, and Lars Hufnagel. “GPU-based image processing
16 for multi-view microscopy data”. *Focus on Microscopy*. Taipei, Taiwan, Mar. 2016
17 (cit. on pp. 84, 85).
- 18 [C3] Bálint Balázs, Marvin Albert, and Lars Hufnagel. “GPU-based image processing
19 for multi-view microscopy data”. *Focus on Microscopy*. Bordeaux, France, Apr.
20 2017 (cit. on pp. 84, 85).

1 **References cited in the thesis**

- 2 [1] Robert Hooke. *Micrographia: or Some Physiological Descriptions of Minute Bodies Made by Magnifying Glasses. With Observations and Inquiries Thereupon.* London: J. Martyn and J. Allestry, 1665 (cit. on p. x). 53
- 3 [2] Philipp J Keller and Ernst HK Stelzer. “Quantitative in vivo imaging of entire embryos with Digital Scanned Laser Light Sheet Fluorescence Microscopy”. *Current Opinion in Neurobiology* 18.6 (Dec. 2008). review, pp. 624–632. DOI: 10.1016/j.conb.2009.03.008 (cit. on p. x). 58
- 4 [3] Jan Huisken and Didier Y. R. Stainier. “Selective plane illumination microscopy techniques in developmental biology”. *Development* 136.12 (June 2009), pp. 1963–1975. DOI: 10.1242/dev.022426 (cit. on pp. x, 13). 63
- 5 [4] Michael Weber and Jan Huisken. “Light sheet microscopy for real-time developmental biology”. *Current Opinion in Genetics & Development* 21.5 (2011), pp. 566–572. DOI: 10.1016/j.gde.2011.09.009 (cit. on p. x). 69
- 6 [5] Raju Tomer, Khaled Khairy, and Philipp J Keller. “Shedding light on the system: studying embryonic development with light sheet microscopy”. *Current Opinion in Genetics & Development*. Developmental mechanisms, patterning and evolution 21.5 (Oct. 2011). Review from 2011, pp. 558–565. DOI: 10.1016/j.gde.2011.07.003 (cit. on p. x). 74
- 7 [6] Hans-Ulrich Dodt, Ulrich Leischner, Anja Schierloh, Nina Jährling, Christoph Peter Mauch, Katrin Deininger, Jan Michael Deussing, Matthias Eder, Walter Zieglgänsberger, and Klaus Becker. “Ultramicroscopy: three-dimensional visualization of neuronal networks in the whole mouse brain”. *Nature Methods* 4.4 (Mar. 2007), pp. 331–336. DOI: 10.1038/nmeth1036 (cit. on pp. x, 13, 24). 90
- 8 [7] Bi-Chang Chen et al. “Lattice light-sheet microscopy: Imaging molecules to embryos at high spatiotemporal resolution”. *Science* 346.6208 (Oct. 2014), p. 1257998. DOI: 10.1126/science.1257998 (cit. on pp. x, 14, 60). 95
- 9 [8] P. Philippe Laissie, Rana A. Alghamdi, Pavol Tomancak, Emmanuel G. Reynaud, and Hari Shroff. “Assessing phototoxicity in live fluorescence imaging”. *Nature Methods* 14.7 (July 2017), pp. 657–661. DOI: 10.1038/nmeth.4344 (cit. on pp. 1, 37). 101
- 10 [9] Jeff W. Lichtman and José-Angel Conchello. “Fluorescence microscopy”. *Nature Methods* 2.12 (Dec. 2005), pp. 910–919. DOI: 10.1038/nmeth817 (cit. on p. 2).
- 11 [10] Alberto Diaspro. *Optical Fluorescence Microscopy: From the Spectral to the Nano Dimension*. 1st ed. Springer-Verlag Berlin Heidelberg, 2011 (cit. on p. 2).
- 12 [11] G. G. Stokes. “On the Change of Refrangi-bility of Light”. *Philosophical Transactions of the Royal Society of London* 142 (Jan. 1852), pp. 463–562. DOI: 10.1098/rstl.1852.0022 (cit. on p. 2).
- 13 [12] *Spectra Viewer*. URL: <https://www.chroma.com/spectra-viewer> (visited on 09/11/2017) (cit. on p. 2).
- 14 [13] Robert Bacallao, Morgane Bomsel, Ernst H. K. Stelzer, and Jan De Mey. “Guiding Principles of Specimen Preservation for Confocal Fluorescence Microscopy”. *Handbook of Biological Confocal Microscopy*. DOI: 10.1007/978-1-4615-7133-9_18. Springer, Boston, MA, 1990, pp. 197–205 (cit. on p. 3).
- 15 [14] O. Shimomura, F. H. Johnson, and Y. Saiga. “Extraction, purification and properties of aequorin, a bioluminescent protein from the luminous hydromedusan, Aequorea”. *Journal of Cellular and Comparative Physiology* 59 (June 1962). first purification of GFP from jellyfish, pp. 223–239 (cit. on p. 3).
- 16 [15] Douglas C. Prasher, Virginia K. Eckenrode, William W. Ward, Frank G. Prendergast, and Milton J. Cormier. “Primary structure of the Aequorea victoria green-fluorescent protein”. *Gene* 111.2 (Feb. 1992). cloning GFP cDNA, pp. 229–233. DOI: 10.1016/0378-1119(92)90691-H (cit. on p. 3).
- 17 [16] M. Chalfie, Y. Tu, G. Euskirchen, W. W. Ward, and D. C. Prasher. “Green fluorescent protein as a marker for gene expression”. *Science* 263.5148 (Feb. 1994). GFP in *c. elegans* / nematodes, pp. 802–805. DOI: 10.1126/science.8303295 (cit. on p. 3).
- 18 [17] Adam Amsterdam, Shuo Lin, and Nancy Hopkins. “The Aequorea victoria Green Fluorescent Protein Can Be Used as a Reporter in Live Zebrafish Embryos”. *Developmental Biology* 171.1 (Sept. 1995). first GFP zebrafish, pp. 123–129. DOI: 10.1006/dbio.1995.1265 (cit. on p. 3).

References cited in the thesis

- 1 [18] Masaru Okabe, Masahito Ikawa, Katsuy⁴⁸
2 Kominami, Tomoko Nakanishi, and Yoshitake⁴⁹
3 Nishimune. “‘Green mice’ as a source of ubiquitous⁵⁰
4 green cells”. *FEBS Letters* 407.3 (May⁵¹
5 1997). first EGFP mouse, pp. 313–319. DOI:⁵²
6 10.1016/S0014-5793(97)00313-X (cit. on⁵³
7 p. 3).
8 [19] R Heim, D C Prasher, and R Y Tsien. “Wave-⁵⁵
9 length mutations and posttranslational autox-⁵⁶
10 idation of green fluorescent protein.” *Proceed-⁵⁷
11 ings of the National Academy of Sciences of the⁵⁸
12 United States of America* 91.26 (Dec. 1994),⁵⁹
13 pp. 12501–12504 (cit. on p. 3).
14 [20] Roger Heim and Roger Y Tsien. “Engineering⁶⁰
15 green fluorescent protein for improved bright-⁶¹
16 ness, longer wavelengths and fluorescence res-⁶²
17 onance energy transfer”. *Current Biology* 6.2
18 (Feb. 1996), pp. 178–182. DOI: 10.1016/S0960-
19 9822(02)00450-5 (cit. on p. 3).
20 [21] Brendan P. Cormack, Raphael H. Valdivia,⁶³
21 and Stanley Falkow. “FACS-optimized mu-⁶⁴
22 tants of the green fluorescent protein (GFP)⁶⁵.
23 *Gene. Flourescent Proteins and Applications*⁶⁶
24 173.1 (1996), pp. 33–38. DOI: 10.1016/0378-
25 1119(95)00685-0 (cit. on p. 3).
26 [22] Robert F. Service. “Three Scientists Bask in⁶⁷
27 Prize’s Fluorescent Glow”. *Science* 322.5900
28 (Oct. 2008), pp. 361–361. DOI: 10.1126/
29 science.322.5900.361 (cit. on p. 3).
30 [23] E. Abbe. “Beiträge zur Theorie des Mikroskop⁶⁸
31 und der mikroskopischen Wahrnehmung⁶⁹.
32 *Archiv für mikroskopische Anatomie*⁷⁰
33 (1873), pp. 413–418. DOI: 10.1007/BF02956173
34 (cit. on p. 5).
35 [24] Max Born and Emil Wolf. *Principles of Optics: Electromagnetic Theory of Propagation, Interference and Diffraction of Light*. Elsevier,⁸⁵
36 June 2013 (cit. on pp. 6, 59).
37 [25] C. J. R. Sheppard and H. J. Matthews. “Imag-⁸⁹
38 ing in high-aperture optical systems”. *JOSA A*⁹⁰
39 4.8 (Aug. 1987), pp. 1354–1360. DOI: 10.1364/
40 JOSAA.4.001354 (cit. on p. 6).
41 [26] Lord Rayleigh F.R.S. “XXXI. Investigation⁹¹
42 in optics, with special reference to the⁹²
43 spectroscope”. *Philosophical Magazine* 8.40
44 (Oct. 1879), pp. 261–274. DOI: 10.1080/
45 14786447908639684 (cit. on p. 6).
46 [27] Jim Swoger, Jan Huisken, and Ernst H. K.
47 Stelzer. “Multiple imaging axis microscopy
48 improves resolution for thick-sample applica-
49 tions”. *Optics Letters* 28.18 (Sept. 2003),
50 p. 1654. DOI: 10.1364/OL.28.001654 (cit. on
51 p. 9).
52 [28] Jim Swoger, Peter Verveer, Klaus Greger, Jan
53 Huisken, and Ernst H. K. Stelzer. “Multi-
54 view image fusion improves resolution in three-
55 dimensional microscopy”. *Optics Express* 15.13
56 (2007), p. 8029. DOI: 10.1364/OE.15.008029
57 (cit. on pp. 9, 36).
58 [29] Marvin Minsky. “Microscopy apparatus”.
59 US3013467 A. U.S. Classification 356/432,
60 359/389, 348/79, 250/215; International
61 Classification G02B21/00; Cooperative
62 Classification G02B21/0024, G02B21/002;
63 European Classification G02B21/00M4A,
64 G02B21/00M4. Dec. 1961 (cit. on p. 9).
65 [30] Paul Davidovits and M. David Egger. “Scan-
66 ning Laser Microscope”. *Nature* 223.5208 (Aug.
67 1969), pp. 831–831. DOI: 10.1038/223831a0
68 (cit. on p. 9).
69 [31] Ernst H.K. Stelzer and Steffen Lindek. “Fun-
70 damental reduction of the observation vol-
71 ume in far-field light microscopy by detec-
72 tion orthogonal to the illumination axis: con-
73 focal theta microscopy”. *Optics Communica-
74 tions* 111.5–6 (Oct. 1994), pp. 536–547. DOI:
75 10.1016/0030-4018(94)90533-9 (cit. on
76 p. 11).
77 [32] Silvia Aldaz, Luis M. Escudero, and Matthew
78 Freeman. “Live Imaging of Drosophila Imaginal
79 Disc Development”. *Proceedings of the
80 National Academy of Sciences* 107.32 (Aug.
81 2010), pp. 14217–14222. DOI: 10.1073/pnas.
82 1008623107 (cit. on p. 12).
83 [33] Jean-Léon Maître, Hervé Turlier, Rukshala
84 Illukkumbura, Björn Eismann, Ritsuya Ni-
85 wayama, François Nédélec, and Takashi Hi-
86 iragi. “Asymmetric division of contractile do-
87 mains couples cell positioning and fate specifi-
88 cation”. *Nature* 536.7616 (Aug. 2016), pp. 344–
89 348. DOI: 10.1038/nature18958 (cit. on pp. 12,
90 20).
91 [34] Emmanuel G. Reynaud, Uroš Kržič, Klaus
92 Greger, and Ernst H.K. Stelzer. “Light sheet-
93 based fluorescence microscopy: more dimen-
94 sions, more photons, and less photodamage”.
95 *HFSP Journal* 2.5 (Oct. 2008), pp. 266–275.
96 DOI: 10.2976/1.2974980 (cit. on p. 12).

- 1 [35] Stelzer. “Contrast, resolution, pixelation, dynamic range and signal-to-noise ratio: fundamental limits to resolution in fluorescence light microscopy”. *Journal of Microscopy* 189.1 (Jan. 1998). This is also the reason why it is sufficient to store the square root of the count rate. That number will contain all the available information., pp. 15–24. DOI: 10.1046/j.1365-2818.1998.00290.x (cit. on p. 12). 60
- 10 [36] H. Siedentopf and R. Zsigmondy. “Über Sichtbare barmachung und Größenbestimmung ultramikroskopischer Teilchen, mit besonderer Anwendung auf Goldrubiingläser”. *Annalen der Physik* 315.1 (1902), pp. 1–39. DOI: 10.1002/andp.19023150102 (cit. on p. 13). 66
- 16 [37] A H Voie, D H Burns, and F A Spelman. “Orthogonal-plane fluorescence optical sectioning: three-dimensional imaging of macroscopic biological specimens”. *Journal of Microscopy* 170.Pt 3 (June 1993), pp. 229–36. DOI: 8371260 (cit. on p. 13). 72
- 22 [38] Arne H. Voie and Francis A. Spelman. “Three-dimensional reconstruction of the cochlea from two-dimensional images of optical sections”. *Computerized Medical Imaging and Graphics* 19.5 (Sept. 1995), pp. 377–384. DOI: 10.1016/0895-6111(95)00034-8 (cit. on p. 13). 78
- 28 [39] Eran Fuchs, Jules S. Jaffe, Richard A. Long, and Farooq Azam. “Thin laser light sheet microscope for microbial oceanography”. *Optics Express* 10.2 (Jan. 2002), pp. 145–154. DOI: 10.1364/OE.10.000145 (cit. on p. 13). 82
- 33 [40] Jan Huisken, Jim Swoger, Filippo Del Bene, Joachim Wittbrodt, and Ernst H. K. Stelzer. “Optical Sectioning Deep Inside Live Embryos by Selective Plane Illumination Microscopy”. *Science* 305.5686 (2004), pp. 1007–1009 (cit. on pp. 13, 14, 16). 88
- 39 [41] Jérémie Capoulade, Malte Wachsmuth, Lars Hufnagel, and Michael Knop. “Quantitative fluorescence imaging of protein diffusion and interaction in living cells”. *Nature Biotechnology* 29.9 (Sept. 2011), pp. 835–839. DOI: 10.1038/nbt.1928 (cit. on p. 14). 94
- 45 [42] Yicong Wu, Alireza Ghitani, Ryan Christensen, Anthony Santella, Zhuo Du, Gary Roodeau, Zhirong Bao, Daniel Colón-Ramos, and Hari Shroff. “Inverted selective plane illumination microscopy (iSPIM) enables coupled cell identity lineage and neurodevelopmental imaging in *Caenorhabditis elegans*”. *Proceedings of the National Academy of Sciences* 108.43 (Oct. 2011). iSPIM, tracking *C. elegans* nuclei, pp. 17708–17713. DOI: 10.1073/pnas.1108494108 (cit. on pp. 13, 14). 100
- [43] Yicong Wu et al. “Spatially isotropic four-dimensional imaging with dual-view plane illumination microscopy”. *Nature Biotechnology* 31.11 (Nov. 2013), pp. 1032–1038. DOI: 10.1038/nbt.2713 (cit. on pp. 14, 36).
- [44] Jan Huisken and Didier Y. R. Stainier. “Even fluorescence excitation by multidirectional selective plane illumination microscopy (mSPIM)”. *Optics Letters* 32.17 (2007), pp. 2608–2610. DOI: 10.1364/OL.32.002608 (cit. on pp. 14, 18).
- [45] Uros Krzic, Stefan Gunther, Timothy E. Saunders, Sebastian J. Streichan, and Lars Hufnagel. “Multiview light-sheet microscope for rapid *in toto* imaging”. *Nature Methods* 9.7 (July 2012). MuVi-SPIM, pp. 730–733. DOI: 10.1038/nmeth.2064 (cit. on pp. 14, 61–63, 68, 79, 81).
- [46] Raju Tomer, Khaled Khairy, Fernando Amat, and Philipp J. Keller. “Quantitative high-speed imaging of entire developing embryos with simultaneous multiview light-sheet microscopy”. *Nature Methods* 9.7 (July 2012). SimView, pp. 755–763. DOI: 10.1038/nmeth.2062 (cit. on p. 14).
- [47] Benjamin Schmid, Gopi Shah, Nico Scherf, Michael Weber, Konstantin Thierbach, Cíatlali Pérez Campos, Ingo Roeder, Pia Aanstad, and Jan Huisken. “High-speed panoramic light-sheet microscopy reveals global endodermal cell dynamics”. *Nature Communications* 4 (July 2013). zebrafish sphere projection + FEP tube. DOI: 10.1038/ncomms3207 (cit. on p. 14).
- [48] Raghav K. Chhetri, Fernando Amat, Yinan Wan, Burkhard Höckendorf, William C. Lemon, and Philipp J. Keller. “Whole-animal functional and developmental imaging with isotropic spatial resolution”. *Nature Methods* 12.12 (Dec. 2015), pp. 1171–1178. DOI: 10.1038/nmeth.3632 (cit. on p. 14).
- [49] Philipp J. Keller, Annette D. Schmidt, Joachim Wittbrodt, and Ernst H. K. Stelzer. “Reconstruction of Zebrafish Early Embryonic Development by Scanned Light Sheet Microscopy”. *Science* 322.5904 (Nov. 2008), pp. 1065–1069. DOI: 10.1126/science.1162493 (cit. on pp. 13, 16, 18, 63).

References cited in the thesis

- 1 [50] Takehiko Ichikawa, Kenichi Nakazato, Philipp
2 J. Keller, Hiroko Kajiura-Kobayashi, Ernst
3 H. K. Stelzer, Atsushi Mochizuki, and
4 Shigenori Nonaka. "Live Imaging of Whole
5 Mouse Embryos during Gastrulation: Migrat-
6 tion Analyses of Epiblast and Mesodermal
7 Cells". *PLoS ONE* 8.7 (July 2013). post im-
8 plantation, e64506. DOI: 10.1371/journal.
9 pone.0064506 (cit. on pp. 13, 22, 23). 60
- 10 [51] Ryan S. Udan, Victor G. Piazza, Chih-wei Hsu,
11 Anna-Katerina Hadjantonakis, and Mary E.
12 Dickinson. "Quantitative imaging of cell dy-
13 namics in mouse embryos using light-sheet mi-
14 croscopy". *Development* (Oct. 2014). post im-
15 plantation, dev.111021. DOI: 10.1242/dev.
16 111021 (cit. on pp. 13, 23). 66
- 17 [52] Abhishek Kumar et al. "Dual-view plane il-
18 lumination microscopy for rapid and spatially
19 isotropic imaging". *Nature Protocols* 9.11 (Nov.
20 2014). diSPIM, pp. 2555–2573. DOI: 10.1038/
21 nprot.2014.172 (cit. on p. 14). 71
- 22 [53] Francesca Cella Zanacchi, Zeno Lavagnino,
23 Michela Perrone Donnorso, Alessio Del Bue,
24 Laura Furia, Mario Faretta, and Alberto Di-
25 aspro. "Live-cell 3D super-resolution imaging
26 in thick biological samples". *Nature Methods*
27 8.12 (Dec. 2011), pp. 1047–1049. DOI: 10.1038/
28 nmeth.1744 (cit. on p. 14). 78
- 29 [54] Mike Friedrich, Qiang Gan, Vladimir Ermo-
30 layev, and Gregory S. Harms. "STED-SPIM:
31 Stimulated Emission Depletion Improves Sheet
32 Illumination Microscopy Resolution". *Biophys-
33 ical Journal* 100.8 (Apr. 2011), pp. L43–L45.
34 DOI: 10.1016/j.bpj.2010.12.3748 (cit. 84
35 p. 14). 85
- 36 [55] Philipp J. Keller, Annette D. Schmidt, An-
37 thony Santella, Khaled Khairy, Zhirong Ba,
38 Joachim Wittbrodt, and Ernst H. K. Stelzer.
39 "Fast, high-contrast imaging of animal de-
40 velopment with scanned light sheet-based
41 structured-illumination microscopy". *Nature
42 Methods* 7.8 (Aug. 2010), pp. 637–642. DOI:
43 10.1038/nmeth.1476 (cit. on pp. 14, 60). 93
- 44 [56] Bo-Jui Chang, Victor Didier Perez Meza, and
45 Ernst H. K. Stelzer. "csiLSFM combines light-
46 sheet fluorescence microscopy and coher-
47 ent structured illumination for a lateral resol-
48 ution below 100 nm". *Proceedings of the Na-
49 tional Academy of Sciences* 114.19 (May 2017)
50 pp. 4869–4874. DOI: 10.1073/pnas.1609278114
51 (cit. on pp. 14, 60). 101
- [57] K. Greger, J. Swoger, and E. H. K. Stelzer.
"Basic building units and properties of a fluo-
rescence single plane illumination microscope".
Review of Scientific Instruments 78.2 (Feb.
2007), pp. 023705–023705–7. DOI: doi : 10.
1063/1.2428277 (cit. on p. 16).
- [58] Bahaa E. A. Saleh and Malvin Carl Teich. *Fund-
amentals of Photonics*. John Wiley & Sons,
Mar. 2007 (cit. on p. 16).
- [59] David M. Shotton. "Confocal scanning optical
microscopy and its applications for biological
specimens". *Journal of Cell Science* 94.2 (Oct.
1989), pp. 175–206 (cit. on p. 20).
- [60] Ralph Gräf, Jens Rietdorf, and Timo Zimmer-
mann. "Live Cell Spinning Disk Microscopy".
*Microscopy Techniques. Advances in Bio-
chemical Engineering*. DOI: 10.1007/b102210.
Springer, Berlin, Heidelberg, 2005, pp. 57–75
(cit. on p. 20).
- [61] James Jonkman and Claire M. Brown. "Any
Way You Slice It—A Comparison of Confocal
Microscopy Techniques". *Journal of Biomole-
cular Techniques : JBT* 26.2 (July 2015),
pp. 54–65. DOI: 10.7171/jbt.15–2602–003
(cit. on p. 20).
- [62] G. S. Kino. "Intermediate Optics in Nip-
kow Disk Microscopes". *Handbook of Biologi-
cal Confocal Microscopy*. DOI: 10.1007/978-1-
4615-7133-9_10. Springer, Boston, MA, 1990,
pp. 105–111 (cit. on p. 20).
- [63] Akihiko Nakano. "Spinning-disk Confocal Mi-
croscopy — A Cutting-Edge Tool for Imag-
ing of Membrane Traffic". *Cell Structure and
Function* 27.5 (2002), pp. 349–355. DOI: 10.
1247/csf.27.349 (cit. on p. 20).
- [64] Ekaterina Korotkevich, Ritsuya Niwayama,
Aurélien Courtois, Stefanie Friese, Nicolas
Berger, Frank Buchholz, and Takashi Hiiragi.
"The Apical Domain Is Required and Suf-
ficient for the First Lineage Segregation in
the Mouse Embryo". *Developmental Cell* 40.3
(2017), 235–247.e7. DOI: http://dx.doi.org/
10.1016/j.devcel.2017.01.006 (cit. on
p. 20).
- [65] Jean-Léon Maître, Ritsuya Niwayama, Hervé
Turlier, François Nédélec, and Takashi Hiiragi.
"Pulsatile cell-autonomous contractility drives
compaction in the mouse embryo". *Nature Cell
Biology* 17.7 (July 2015), pp. 849–855. DOI: 10.
1038/ncb3185 (cit. on p. 20).

- 1 [66] Jens-Erik Dietrich, Laura Panavaite, Stefan Gunther, Sebastian Wennekamp, Anna Groner, Anton Pigge, Stefanie Salvenmoser, Didier Trono, Lars Hufnagel, and Takashi Hiragi. “Venus trap in the mouse embryo reveals distinct molecular dynamics underlying specification of first embryonic lineages”. *EMB Reports* 16.8 (Aug. 2015), pp. 1005–1021. DOI: 10.1525/embr.201540162 (cit. on p. 20). 60
- 10 [67] Sonja Nowotschin, Anna Ferrer-Vaquer, and Anna-Katerina Hadjantonakis. “Chapter - Imaging Mouse Development with Confocal Time-Lapse Microscopy”. *Methods in Embryology*. Ed. by Paul M. Wassarman and Philippe M. Soriano. Vol. 476. Guide to Techniques in Mouse Development, Part A: Mice, Embryos, and Cells, 2nd Edition. Academic Press, 2010, pp. 351–377 (cit. on p. 20). 69
- 19 [68] Lewis Wolpert. *Principles of Development*. OUP Oxford, Jan. 2011 (cit. on p. 20). 71
- 21 [69] Adam S. Doherty and Richard M. Schultz. “Culture of Preimplantation Mouse Embryos”. *Developmental Biology Protocols*. Methods in Molecular Biology™. DOI: 10.1385/1-59259-685-1:47. Humana Press, 2000, pp. 47–52 (cit. on p. 20). 72
- 27 [70] Jens-Erik Dietrich and Takashi Hiragi. “Stochastic patterning in the mouse pre-implantation embryo”. *Development* 134.23 (Dec. 2007), pp. 4219–4231. DOI: 10.1242/dev.003798 (cit. on p. 21). 83
- 32 [71] W. Denk, J. H. Strickler, and W. W. Webb. “Two-photon laser scanning fluorescence microscopy”. *Science* 248.4951 (Apr. 1990), pp. 73–76. DOI: 10.1126/science.2321027 (cit. on p. 21). 88
- 37 [72] Jayne M. Squirrell, David L. Wokosin, John G. White, and Barry D. Bavister. “Long-term two-photon fluorescence imaging of mammalian embryos without compromising viability”. *Nature Biotechnology* 17.8 (Aug. 1999), pp. 763–767. DOI: 10.1038/11698 (cit. on p. 21). 96
- 45 [73] Katie McDole, Yuan Xiong, Pablo A. Iglesias, and Yixian Zheng. “Lineage mapping of the pre-implantation mouse embryo by two-photon microscopy, new insights into the segregation of cell fates”. *Developmental Biology* 355.2 (July 2011), pp. 239–249. DOI: 10.1016/j.ydbio.2011.04.024 (cit. on p. 21). 103
- [74] Kazuo Yamagata, Rinako Suetsugu, and Teruhiko Wakayama. “Long-Term, Six-Dimensional Live-Cell Imaging for the Mouse Preimplantation Embryo That Does Not Affect Full-Term Development”. *Journal of Reproduction and Development* 55.3 (2009), pp. 343–350. DOI: 10.1262/jrd.20166 (cit. on p. 21).
- [75] Gustavo de Medeiros, Nils Norlin, Stefan Gunther, Marvin Albert, Laura Panavaite, Ulla-Maj Fiuzza, Francesca Peri, Takashi Hiragi, Uros Krzic, and Lars Hufnagel. “Confocal multiview light-sheet microscopy”. *Nature Communications* 6 (Nov. 2015), p. 8881. DOI: 10.1038/ncomms9881 (cit. on pp. 23, 24, 63, 65, 73, 81).
- [76] Laura Panavaite, Balint Balazs, Tristan Rodriguez, Shankar Srinivas, Jerome Collignon, Lars Hufnagel, and Takashi Hiragi. “3D-geec: a method for studying mouse peri-implantation development”. *Mechanisms of Development*. 18th International Congress of Developmental Biology 18–22 June, University Cultural Centre, National University of Singapore 145. Supplement (July 2017), S78–S79. DOI: 10.1016/j.mod.2017.04.189 (cit. on p. 22).
- [77] Yu-Chih Hsu. “In vitro development of individually cultured whole mouse embryos from blastocyst to early somite stage”. *Developmental Biology* 68.2 (Feb. 1979). post-implantation culture, pp. 453–461. DOI: 10.1016/0012-1606(79)90217-3 (cit. on p. 22).
- [78] Fu-Jen Huang, Tsung-Chieh J. Wu, and Meng-Yin Tsai. “Effect of retinoic acid on implantation and post-implantation development of mouse embryos in vitro”. *Human Reproduction* 16.10 (Oct. 2001). post-implantation culture, pp. 2171–2176. DOI: 10.1093/humrep/16.10.2171 (cit. on p. 22).
- [79] Sonja Nowotschin and Anna-Katerina Hadjantonakis. “Cellular dynamics in the early mouse embryo: from axis formation to gastrulation”. *Current Opinion in Genetics & Development*. Developmental mechanisms, patterning and evolution 20.4 (Aug. 2010), pp. 420–427. DOI: 10.1016/j.gde.2010.05.008 (cit. on p. 22).
- [80] Monica D. Garcia, Ryan S. Udan, Anna-Katerina Hadjantonakis, and Mary E. Dickinson. “Live Imaging of Mouse Embryos”. *Cold Spring Harbor Protocols* 2011.4 (Apr. 2011),

References cited in the thesis

- [81] Alessandro Bria and Giulio Iannelli. “TeraStitcher - A tool for fast automatic 3D stitching of teravoxel-sized microscopy images”. *BMC Bioinformatics* 13 (Nov. 2012), p. 316. doi: 10.1186/1471-2105-13-316 (cit. on p. 24). 51
52

[82] Gergely Katona, Gergely Szalay, Pál Maák, Attila Kaszás, Máté Veress, Dániel Hillier, Balázs Chiovini, E. Sylvester Vizi, Botond Roska, and Balázs Rózsa. “Fast two-photon ⁵⁹₆₀ vivo imaging with three-dimensional random access scanning in large tissue volumes”. *Nature Methods* 9.2 (Feb. 2012), pp. 201–208. doi: 10.1038/nmeth.1851 (cit. on p. 25). 61
62
63
64
65
66
67

[83] Hiroshi Hama, Hiroshi Kurokawa, Hiroyuki Kawano, Ryoko Ando, Tomomi Shimogori, Hisayori Noda, Kiyoko Fukami, Asako Sakaue-Sawano, and Atsushi Miyawaki. “Scale: a chemical approach for fluorescence imaging and reconstruction of transparent mouse brain”. *Nature Neuroscience* 14.11 (Nov. 2011), pp. 1481–1488. doi: 10.1038/nn.2928 (cit. on p. 25). 68
69
70
71
72
73
74
75
76

[84] Ali Ertürk, Klaus Becker, Nina Jährling, Christoph P. Mauch, Caroline D. Hojer, Jackson G. Egen, Farida Hellal, Frank Bradke, Morgan Sheng, and Hans-Ulrich Dodt. “Three-dimensional imaging of solvent-cleared organs using 3DISCO”. *Nature Protocols* 7.11 (Nov. 2012), pp. 1983–1995. doi: 10.1038/nprot.2012.119 (cit. on p. 25). 77
78
79
80
81
82
83
84

[85] Ali Ertürk et al. “Three-dimensional imaging of the unsectioned adult spinal cord to assess axon regeneration and glial responses after injury”. *Nature Medicine* 18.1 (Jan. 2012), pp. 166–171. doi: 10.1038/nm.2600 (cit. on p. 25). 85
86
87
88
89
90
91

[86] Meng-Tsen Ke, Satoshi Fujimoto, and Takeshi Imai. “SeeDB: a simple and morphology-preserving optical clearing agent for neuronal circuit reconstruction”. *Nature Neuroscience* 16.8 (Aug. 2013), pp. 1154–1161. doi: 10.1038/nrn.3447 (cit. on p. 25). 92
93
94
95
96
97

[87] Kwanghun Chung and Karl Deisseroth. “CLARITY for mapping the nervous system”. *Nature Methods* 10.6 (June 2013), pp. 508–510. doi: 10.1038/nmeth.2481 (cit. on p. 25). 98
99
100

[88] Etsuo A. Susaki et al. “Whole-Brain Imaging with Single-Cell Resolution Using Chemical Cocktails and Computational Analysis”. *Cell* 157.3 (Apr. 2014), pp. 726–739. doi: 10.1016/j.cell.2014.03.042 (cit. on p. 25). 101
102
103
104
105
106
107
108
109
110
111
112
113
114
115
116
117
118
119
120
121
122
123
124
125
126
127
128
129
130
131
132
133
134
135
136
137
138
139
140
141
142
143
144
145
146
147
148
149
150
151
152
153
154
155
156
157
158
159
160
161
162
163
164
165
166
167
168
169
170
171
172
173
174
175
176
177
178
179
180
181
182
183
184
185
186
187
188
189
190
191
192
193
194
195
196
197
198
199
200
201
202
203
204
205
206
207
208
209
210
211
212
213
214
215
216
217
218
219
220
221
222
223
224
225
226
227
228
229
230
231
232
233
234
235
236
237
238
239
240
241
242
243
244
245
246
247
248
249
250
251
252
253
254
255
256
257
258
259
260
261
262
263
264
265
266
267
268
269
270
271
272
273
274
275
276
277
278
279
280
281
282
283
284
285
286
287
288
289
290
291
292
293
294
295
296
297
298
299
300
301
302
303
304
305
306
307
308
309
310
311
312
313
314
315
316
317
318
319
320
321
322
323
324
325
326
327
328
329
330
331
332
333
334
335
336
337
338
339
340
341
342
343
344
345
346
347
348
349
350
351
352
353
354
355
356
357
358
359
360
361
362
363
364
365
366
367
368
369
370
371
372
373
374
375
376
377
378
379
380
381
382
383
384
385
386
387
388
389
390
391
392
393
394
395
396
397
398
399
400
401
402
403
404
405
406
407
408
409
410
411
412
413
414
415
416
417
418
419
420
421
422
423
424
425
426
427
428
429
430
431
432
433
434
435
436
437
438
439
440
441
442
443
444
445
446
447
448
449
450
451
452
453
454
455
456
457
458
459
460
461
462
463
464
465
466
467
468
469
470
471
472
473
474
475
476
477
478
479
480
481
482
483
484
485
486
487
488
489
490
491
492
493
494
495
496
497
498
499
500
501
502
503
504
505
506
507
508
509
510
511
512
513
514
515
516
517
518
519
520
521
522
523
524
525
526
527
528
529
530
531
532
533
534
535
536
537
538
539
540
541
542
543
544
545
546
547
548
549
550
551
552
553
554
555
556
557
558
559
5510
5511
5512
5513
5514
5515
5516
5517
5518
5519
5520
5521
5522
5523
5524
5525
5526
5527
5528
5529
5530
5531
5532
5533
5534
5535
5536
5537
5538
5539
5540
5541
5542
5543
5544
5545
5546
5547
5548
5549
5550
5551
5552
5553
5554
5555
5556
5557
5558
5559
55510
55511
55512
55513
55514
55515
55516
55517
55518
55519
55520
55521
55522
55523
55524
55525
55526
55527
55528
55529
55530
55531
55532
55533
55534
55535
55536
55537
55538
55539
55540
55541
55542
55543
55544
55545
55546
55547
55548
55549
55550
55551
55552
55553
55554
55555
55556
55557
55558
55559
55560
55561
55562
55563
55564
55565
55566
55567
55568
55569
55570
55571
55572
55573
55574
55575
55576
55577
55578
55579
55580
55581
55582
55583
55584
55585
55586
55587
55588
55589
55590
55591
55592
55593
55594
55595
55596
55597
55598
55599
555100
555101
555102
555103
555104
555105
555106
555107
555108
555109
555110
555111
555112
555113
555114
555115
555116
555117
555118
555119
555120
555121
555122
555123
555124
555125
555126
555127
555128
555129
555130
555131
555132
555133
555134
555135
555136
555137
555138
555139
555140
555141
555142
555143
555144
555145
555146
555147
555148
555149
555150
555151
555152
555153
555154
555155
555156
555157
555158
555159
555160
555161
555162
555163
555164
555165
555166
555167
555168
555169
555170
555171
555172
555173
555174
555175
555176
555177
555178
555179
555180
555181
555182
555183
555184
555185
555186
555187
555188
555189
555190
555191
555192
555193
555194
555195
555196
555197
555198
555199
555200
555201
555202
555203
555204
555205
555206
555207
555208
555209
555210
555211
555212
555213
555214
555215
555216
555217
555218
555219
555220
555221
555222
555223
555224
555225
555226
555227
555228
555229
555230
555231
555232
555233
555234
555235
555236
555237
555238
555239
555240
555241
555242
555243
555244
555245
555246
555247
555248
555249
555250
555251
555252
555253
555254
555255
555256
555257
555258
555259
555260
555261
555262
555263
555264
555265
555266
555267
555268
555269
555270
555271
555272
555273
555274
555275
555276
555277
555278
555279
555280
555281
555282
555283
555284
555285
555286
555287
555288
555289
555290
555291
555292
555293
555294
555295
555296
555297
555298
555299
555300
555301
555302
555303
555304
555305
555306
555307
555308
555309
555310
555311
555312
555313
555314
555315
555316
555317
555318
555319
555320
555321
555322
555323
555324
555325
555326
555327
555328
555329
555330
555331
555332
555333
555334
555335
555336
555337
555338
555339
555340
555341
555342
555343
555344
555345
555346
555347
555348
555349
555350
555351
555352
555353
555354
555355
555356
555357
555358
555359
555360
555361
555362
555363
555364
555365
555366
555367
555368
555369
555370
555371
555372
555373
555374
555375
555376
555377
555378
555379
555380
555381
555382
555383
555384
555385
555386
555387
555388
555389
555390
555391
555392
555393
555394
555395
555396
555397
555398
555399
555400
555401
555402
555403
555404
555405
555406
555407
555408
555409
555410
555411
555412
555413
555414
555415
555416
555417
555418
555419
555420
555421
555422
555423
555424
555425
555426
555427
555428
555429
555430
555431
555432
555433
555434
555435
555436
555437
555438
555439
555440
555441
555442
555443
555444
555445
555446
555447
555448
555449
555450
555451
555452
555453
555454
555455
555456
555457
555458
555459
555460
555461
555462
555463
555464
555465
555466
555467
555468
555469
555470
555471
555472
555473
555474
555475
555476
555477
555478
555479
555480
555481
555482
555483
555484
555485
555486
555487
555488
555489
555490
555491
555492
555493
555494
555495
555496
555497
555498
555499
555500
555501
555502
555503
555504
555505
555506
555507
555508
555509
555510
555511
555512
555513
555514
555515
555516
555517
555518
555519
555520
555521
555522
555523
555524
555525
555526
555527
555528
555529
555530
555531
555532
555533
555534
555535
555536
555537
555538
555539
555540
555541
555542
555543
555544
555545
555546
555547
555548
555549
555550
555551
555552
555553
555554
555555
555556
555557
555558
555559
555560
555561
555562
555563
555564
555565
555566
555567
555568
555569
555570
555571
555572
555573
555574
555575
555576
555577
555578
555579
555580
555581
555582
555583
555584
555585
555586
555587
555588
555589
555590
555591
555592
555593
555594
555595
555596
555597
555598
555599
5555100
5555101
5555102
5555103
5555104
5555105
5555106
5555107
5555108
5555109
5555110
5555111
5555112
5555113
5555114
5555115
5555116
5555117
5555118
5555119
5555120
5555121
5555122
5555123
5555124
5555125
5555126
5555127
5555128
5555129
5555130
5555131
5555132
5555133
5555134
5555135
5555136
5555137
5555138
5555139
5555140
5555141
5555142
5555143
5555144
5555145
5555146
5555147
5555148
5555149
5555150
5555151
5555152
5555153
5555154
5555155
5555156
5555157
5555158
5555159
5555160
5555161
5555162
5555163
5555164
5555165
5555166
5555167
5555168
5555169
5555170
5555171
5555172
5555173
5555174
5555175
5555176
5555177
5555178
5555179
5555180
5555181
5555182
5555183
5555184
5555185
5555186
5555187
5555188
5555189
5555190
5555191
5555192
5555193
5555194
5555195
5555196
5555197
5555198
5555199
5555200
5555201
5555202
5555203
5555204
5555205
5555206
5555207
5555208
5555209
5555210
5555211
5555212
5555213
5555214
5555215
5555216
5555217
5555218
5555219
5555220
5555221
5555222
5555223
5555224
5555225
5555226
5555227
5555228
5555229
5555230
5555231
5555232
5555233
5555234
5555235
5555236
5555237
5555238
5555239
5555240
5555241
5555242
5555243
5555244
5555245
5555246
5555247
5555248
5555249
5555250
5555251
5555252
5555253
5555254
5555255
5555256
5555257
5555258
5555259
5555260
5555261
5555262
5555263
5555264
5555265
5555266
5555267
5555268
5555269
5555270
5555271
5555272
5555273
5555274
5555275
5555276
5555277
5555278
5555279
5555280
5555281
5555282
5555283
5555284
5555285
5555286
5555287
5555288
5555289
5555290
5555291
5555292
5555293
5555294
5555295
5555296
5555297
5555298
5555299
5555300
5555301
5555302
5555303
5555304
5555305
5555306
5555307
5555308
5555309
5555310
5555311
5555312
5555313
5555314
5555315
5555316
5555317
5555318
5555319
5555320
5555321
5555322
5555323
5555324
5555325
5555326
5555327
5555328
5555329
5555330
5555331
5555332
5555333
5555334
5555335
5555336
5555337
5555338
5555339
5555340
5555341
5555342
5555343
5555344
5555345
5555346
5555347
5555348
5555349
5555350
5555351
5555352
5555353
5555354
5555355
5555356
5555357
5555358
5555359
5555360
5555361
5555362
5555363
5555364
5555365
5555366
5555367
5555368
5555369
5555370
5555371
5555372
5555373
5555374
5555375
5555376
5555377
5555378
5555379
5555380
5555381
5555382
5555383
5555384
5555385
5555386
5555387
5555388
5555389
5555390
5555391
5555392
5555393
5555394
5555395
5555396
5555397
5555398
5555399
5555400
5555401
5555402
5555403
5555404
5555405
5555406
5555407
5555408
5555409
5555410
5555411
5555412
5555413
5555414
5555415
5555416
5555417
5555418
5555419
5555420
5555421
5555422
5555423
5555424
5555425
5555426
5555427
5555428
5555429
5555430
5555431
5555432
5555433
5555434
5555435
5555436
5555437
5555438
5555439
5555440
5555441
5555442
5555443
5555444
5555445
5555446
5555447
5555448
5555449
5555450
5555451
5555452
5555453
5555454
5555455
5555456
5555457
5555458
5555459
5555460
5555461
5555462
5555463
5555464
5555465
5555466
5555467
5555468
5555469
5555470
5555471
5555472
5555473
5555474
5555475
5555476
5555477
5555478
5555479
5555480
5555481
5555482
5555483
5555484
5555485
5555486
5555487
5555488
5555489
5555490
5555491
5555492
5555493
5555494
5555495
5555496
5555497
5555498
5555499
5555500
5555501
5555502
5555503
5555504
5555505
5555506
5555507
5555508
5555509
5555510
5555511
5555512
5555513
5555514
5555515
5555516
5555517
5555518
5555519
5555520
5555521
5555522
5555523
5555524
5555525
5555526
5555527
5555528
5555529
5555530
5555531
5555532
5555533
5555534
5555535
5555536
5555537
5555538
5555539
5555540
5555541
5555542
5555543
5555544
5555545

- 1 [97] Claude E. Shannon. "A mathematical theory
2 of communication". *The Bell System Technical Journal* 27.3 (July 1948), pp. 379–423. DOI
3 10.1002/j.1538-7305.1948.tb01338.x (cit.
4 on p. 26). 56
- 6 [98] Claude E. Shannon. "Prediction and entropy of
7 printed English". *Bell Labs Technical Journal*
8 30.1 (1951), pp. 50–64 (cit. on p. 26). 57
9 [99] J. Rissanen and G. Langdon. "Universal modeling
10 and coding". *IEEE Transactions on Information Theory* 27.1 (Jan. 1981), pp. 12–23. DOI:
11 10.1109/TIT.1981.1056282 (cit. on p. 27). 58
12 [100] David A. Huffman. "A Method for the Construction
13 of Minimum-Redundancy Codes". *Proceedings of the IRE* 40.9 (Sept. 1952),
14 pp. 1098–1101. DOI: 10.1109/JRPROC.1952.
15 273898 (cit. on p. 28). 59
- 16 [101] N. Ahmed, T. Natarajan, and K. R. Rao. "Discrete
17 Cosine Transform". *IEEE Transactions on Computers* C-23.1 (Jan. 1974), pp. 90–93.
18 DOI: 10.1109/TC.1974.223784 (cit. on p. 31). 60
- 19 [102] Stephane G. Mallat. "A theory for multiresolution signal decomposition : the wavelet representation". *IEEE Transaction on Pattern Analysis and Machine Intelligence* (1989) (cit. on p. 32). 61
- 20 [103] Arne Jensen and Anders la Cour-Harbo. *Ripples in Mathematics*. DOI: 10.1007/978-3-642-
21 56702-5. Berlin, Heidelberg: Springer Berlin
22 Heidelberg, 2001 (cit. on p. 32). 62
- 23 [104] William B. Pennebaker and Joan L. Mitchell. *JPEG: Still Image Data Compression Standard*. Springer Science & Business Media, Dec. 1992 (cit. on pp. 33, 72). 63
- 24 [105] M.J. Weinberger, G. Seroussi, and G. Sapiro. "The LOCO-I lossless image compression algorithm: principles and standardization into JPEG-LS". *IEEE Transactions on Image Processing* 9.8 (Aug. 2000), pp. 1309–1324. DOI:
25 10.1109/83.855427 (cit. on pp. 33, 34, 72, 74). 64
- 26 [106] X. Wu and N. Memon. "Context-based, adaptive, lossless image coding". *IEEE Transactions on Communications* 45.4 (Apr. 1997), pp. 437–444. DOI: 10.1109/26.585919 (cit. on p. 33). 65
- 27 [107] Roman Starosolski. "Simple fast and adaptive lossless image compression algorithm". *Software: Practice and Experience* 37.1 (Jan. 2007), pp. 65–91. DOI: 10.1002/spe.746 (cit. on pp. 33, 72). 66
- [108] Z. Wang, M. Klaiber, Y. Gera, S. Simon, and T. Richter. "Fast lossless image compression with 2D Golomb parameter adaptation based on JPEG-LS". *Signal Processing Conference (EUSIPCO), 2012 Proceedings of the 20th European*. Aug. 2012, pp. 1920–1924 (cit. on pp. 33, 72). 67
- [109] Nazeeh Aranki, Didier Keymeulen, Alireza Bakhshi, and Matthew Klimesh. "Hardware Implementation of Lossless Adaptive and Scalable Hyperspectral Data Compression for Space". *Proceedings of the 2009 NASA/ESA Conference on Adaptive Hardware and Systems*. AHS '09. Washington, DC, USA: IEEE Computer Society, 2009, pp. 315–322. DOI: 10.1109/AHS.2009.66 (cit. on p. 33). 68
- [110] Scott F. Gilbert. *Developmental Biology*. 10th. Sinauer Associates, 2013 (cit. on p. 35). 69
- [111] M. Temerinac-Ott, O. Ronneberger, P. Ochs, W. Driever, T. Brox, and H. Burkhardt. "Multiview Deblurring for 3-D Images from Light-Sheet-Based Fluorescence Microscopy". *IEEE Transactions on Image Processing* 21.4 (Apr. 2012), pp. 1863–1873. DOI: 10.1109/TIP.2011.2181528 (cit. on p. 36). 70
- [112] Stephan Preibisch, Fernando Amat, Evangelia Stamataki, Mihail Sarov, Robert H. Singer, Eugene Myers, and Pavel Tomancak. "Efficient Bayesian-based multiview deconvolution". *Nature Methods* 11.6 (June 2014), pp. 645–648. DOI: 10.1038/nmeth.2929 (cit. on pp. 36, 57, 59). 71
- [113] Bálint Balázs. "Development of a symmetric single-plane illumination microscope". Master's Thesis. Hungary: Pázmány Péter Catholic University, 2013 (cit. on pp. 36, 48). 72
- [114] Sarah Frisken Gibson and Frederick Lanni. "Experimental test of an analytical model of aberration in an oil-immersion objective lens used in three-dimensional light microscopy". *JOSA A* 9.1 (Jan. 1992), pp. 154–166. DOI: 10.1364/JOSAA.9.000154 (cit. on p. 54). 73
- [115] Jizhou Li, Feng Xue, and Thierry Blu. "Fast and accurate three-dimensional point spread function computation for fluorescence microscopy". *JOSA A* 34.6 (June 2017), pp. 1029–1034. DOI: 10.1364/JOSAA.34.001029 (cit. on p. 54). 74

- 1 [116] Johannes Schindelin et al. “Fiji: an open¹⁰
2 source platform for biological-image analysis¹¹
3 *Nature Methods* 9.7 (July 2012), pp. 676–682.
4 doi: 10.1038/nmeth.2019 (cit. on pp. 55, 59,
5 79). 54
- 6 [117] Janick Cardinale. *An ImageJ Plugin to Measure 3D Point Spread Functions*. 2010. UR¹⁵
7 http://mosaic.mpi-cbg.de/Downloads/PSF_16
8 measurement_3D.pdf (visited on 10/04/2016)
9 (cit. on p. 55). 59
- 11 [118] Daniel Sage, Lauréne Donati, Ferréol Soule²⁰
12 Denis Fortun, Guillaume Schmit, Arne Seitz²¹
13 Romain Guiet, Cédric Vonesch, and Michael²²
14 Unser. “DeconvolutionLab2: An open-source²³
15 software for deconvolution microscopy”. *Metho²⁴*
16 ods. Image Processing for Biologists 115 (Feb.
17 2017), pp. 28–41. doi: 10.1016/j.ymeth.2016²⁵
18 12.015 (cit. on p. 56). 66
19 [119] Pierre Gönczy. “Towards a molecular archi²⁶
20 tecture of centriole assembly”. *Nature Reviews 27*
21 *Molecular Cell Biology* 13 (2012). doi: 10.1038/nrm3373 (cit. on p. 56). 71
22
23 [120] Stephan Preibisch, Stephan Saalfeld, Johannes²⁸
24 Schindelin, and Pavel Tomancak. “Software for²⁹
25 bead-based registration of selective plane illumi³⁰
26 nation microscopy data”. *Nature Methods* 7.6 (June 2010), pp. 418–419. doi: 10.1038/nmeth0610-418 (cit. on pp. 59, 64). 77
27
28
29 [121] H. Kirshner, D. Sage, and M. Unser. “3D PSF Models for Fluorescence Microscopy in ImageJ”. *Proceedings of the Twelfth International Conference on Methods and Applications of Fluorescence Spectroscopy, Imaging and Probes (MAF'11)*. ImageJ PSF generator. Strasbourg, French Republic, Sept. 2011. p. 154 (cit. on p. 59). 78
30
31
32
33
34
35
36
37 [122] M. Rauzi. “Probing tissue interaction with laser-based cauterization in the early developing Drosophila embryo”. *Methods in Cell Biology*. Cell Polarity and Morphogenesis 139 (Jan. 2017), pp. 153–165. doi: 10.1016/bs.mcb.2016.11.003 (cit. on p. 60). 90
38
39
40
41
42
43 [123] Kevin M. Dean, Philippe Roudot, Carlos Reis, Erik S. Welf, Marcel Mettlen, and Reto Fiolka. “Diagonally Scanned Light-Sheet Microscopy for Fast Volumetric Imaging of Adherent Cells”. *Biophysical Journal* 110.6 (Mar. 2016), pp. 1456–1465. doi: 10.1016/j.bpj.2016.01.029 (cit. on p. 60). 97
- [124] Anne E. Carpenter and David M. Sabatini. “Systematic genome-wide screens of gene function”. *Nature Reviews Genetics* 5.1 (Jan. 2004), pp. 11–22. doi: 10.1038/nrg1248 (cit. on p. 61).
- [125] Christophe J. Echeverri and Norbert Perrimon. “High-throughput RNAi screening in cultured cells: a user’s guide”. *Nature Reviews Genetics* 7.5 (May 2006), pp. 373–384. doi: 10.1038/nrg1836 (cit. on p. 61).
- [126] Rainer Pepperkok and Jan Ellenberg. “High-throughput fluorescence microscopy for systems biology”. *Nature Reviews Molecular Cell Biology* 7.9 (Sept. 2006), pp. 690–696. doi: 10.1038/nrm1979 (cit. on p. 61).
- [127] Eric Betzig, George H. Patterson, Rachid Sougrat, O. Wolf Lindwasser, Scott Olenych, Juan S. Bonifacino, Michael W. Davidson, Jennifer Lippincott-Schwartz, and Harald F. Hess. “Imaging Intracellular Fluorescent Proteins at Nanometer Resolution”. *Science* 313.5793 (Sept. 2006), pp. 1642–1645. doi: 10.1126/science.1127344 (cit. on p. 61).
- [128] Samuel T. Hess, Thanu P. K. Girirajan, and Michael D. Mason. “Ultra-High Resolution Imaging by Fluorescence Photoactivation Localization Microscopy”. *Biophysical Journal* 91.11 (Dec. 2006), pp. 4258–4272. doi: 10.1529/biophysj.106.091116 (cit. on p. 61).
- [129] Michael J. Rust, Mark Bates, and Xiaowei Zhuang. “Sub-diffraction-limit imaging by stochastic optical reconstruction microscopy (STORM)”. *Nature Methods* 3.10 (Oct. 2006), pp. 793–796. doi: 10.1038/nmeth929 (cit. on p. 61).
- [130] Roy Wollman and Nico Stuurman. “High throughput microscopy: from raw images to discoveries”. *Journal of Cell Science* 120.21 (Nov. 2007), pp. 3715–3722. doi: 10.1242/jcs.013623 (cit. on p. 61).
- [131] Emmanuel G. Reynaud, Jan Peychl, Jan Huisken, and Pavel Tomancak. “Guide to light-sheet microscopy for adventurous biologists”. *Nature Methods* 12.1 (Jan. 2015), pp. 30–34. doi: 10.1038/nmeth.3222 (cit. on p. 61).
- [132] Jeffrey M. Perkel. “The struggle with image glut”. *Nature* 533.7601 (Apr. 2016), pp. 131–132. doi: 10.1038/533131a (cit. on p. 61).

- 1 [133] John Nickolls, Ian Buck, Michael Garland, and
2 Kevin Skadron. “Scalable Parallel Program
3 ming with CUDA”. *Queue* 6.2 (Mar. 2008),
4 pp. 40–53. DOI: 10.1145/1365490.1365500 (cit.
5 on p. 61). 56
- 6 [134] Gustavo Q. G. de Medeiros. “Deep tissue
7 light-sheet microscopy”. PhD thesis. Germany:
8 Ruperto-Carola University of Heidelberg, 2016
9 (cit. on p. 62). 57
- 10 [135] Eugen Baumgart and Ulrich Kubitschek.
11 “Scanned light sheet microscopy with confo-
12 cal slit detection”. *Optics Express* 20.19 (2012),
13 pp. 21805–21814. DOI: 10.1364/OE.20.021805
14 (cit. on p. 63). 60
- 15 [136] Uroš Kržič. “Multiple-view microscopy with
16 light-sheet based fluorescence microscope”.
17 PhD thesis. Germany: Ruperto-Carola Univer-
18 sity of Heidelberg, 2009 (cit. on p. 64). 65
- 19 [137] Stephan Preibisch, Stephan Saalfeld, Torsten
20 Rohlfing, and Pavel Tomancak. “Bead-based
21 mosaicing of single plane illumination mi-
22 croscopy images using geometric local descrip-
23 tor matching”. Ed. by Josien P. W. Pluim and
24 Benoit M. Dawant. Feb. 2009, 72592S. DOI: 10.
25 1117/12.812612 (cit. on p. 64). 69
- 26 [138] The HDF Group. *Hierarchical Data Format*,
27 version 5. 1997 (cit. on p. 67). 76
- 28 [139] Fernando Amat, Burkhard Höckendorf, Yinan
29 Wan, William C. Lemon, Katie McDole, and
30 Philipp J. Keller. “Efficient processing and
31 analysis of large-scale light-sheet microscopy
32 data”. *Nature Protocols* 10.11 (Nov. 2015),
33 pp. 1679–1696. DOI: 10.1038/nprot.2015.138
34 (cit. on pp. 67, 76). 77
- 35 [140] G. W. Zack, W. E. Rogers, and S. A. Latt. “Au-
36 tomatic measurement of sister chromatid ex-
37 change frequency”. *The Journal of Histochem-
38 istry and Cytochemistry: Official Journal of
39 the Histochemistry Society* 25.7 (July 1977),
40 pp. 741–753. DOI: 10.1177/25.7.70454 (cit.
41 p. 67). 84
- 42 [141] Loïc A. Royer, William C. Lemon, Raghav K.
43 Chhetri, Yinan Wan, Michael Coleman, Ed
44 gene W. Myers, and Philipp J. Keller. “Adap-
45 tive light-sheet microscopy for long-term, high-
46 resolution imaging in living organisms”. *Nature
47 Biotechnology* 34.12 (Dec. 2016), pp. 1267–
48 1278. DOI: 10.1038/nbt.3708 (cit. on p. 70). 95
- 49 [142] Michael D. Adams. *The JPEG-2000 still im-
50 age compression standard*. 2001 (cit. on pp.
51 72). 100
- [143] International Telecommunications Union. *H.265 : High efficiency video coding*. Dec. 2016. URL: <http://www.itu.int/rec/T-REC-H.265-201612-1/en> (visited on 10/02/2017) (cit. on p. 71).
- [144] *x265 HEVC Encoder / H.265 Video Codec*. URL: <http://x265.org/> (visited on 10/11/2017) (cit. on p. 71).
- [145] Marc Treib, Florian Reichl, Stefan Auer, and
Rüdiger Westermann. “Interactive Editing of
GigaSample Terrain Fields”. *Computer Graphics Forum* 31.2pt2 (May 2012), pp. 383–392.
DOI: 10.1111/j.1467-8659.2012.03017.x (cit.
on pp. 72, 73). 62
- [146] M. Treib, K. Burger, F. Reichl, C. Mene-
veau, A. Szalay, and R. Westermann. “Turbu-
lence Visualization at the Terascale on Desk-
top PCs”. *IEEE Transactions on Visualization
and Computer Graphics* 18.12 (Dec. 2012),
pp. 2169–2177. DOI: 10.1109/TVCG.2012.274
(cit. on p. 73). 63
- [147] Robert A. Gowen and Alan Smith. “Square
root data compression”. *Review of Scientific
Instruments* 74.8 (Aug. 2003), pp. 3853–3861.
DOI: 10.1063/1.1593811 (cit. on p. 74). 68
- [148] Gary M. Bernstein, Chris Bebek, Jason
Rhodes, Chris Stoughton, R. Ali Vanderveld,
and Penshu Yeh. “Noise and bias in square-
root compression schemes”. *Publications of the
Astronomical Society of the Pacific* 122.889
(Mar. 2010). arXiv: 0910.4571, pp. 336–346.
DOI: 10.1086/651281 (cit. on p. 74). 69
- [149] R. M. Gray and D. L. Neuhoff. “Quantiza-
tion”. *IEEE Transactions on Information The-
ory* 44.6 (Oct. 1998), pp. 2325–2383. DOI: 10.
1109/18.720541 (cit. on p. 75). 70
- [150] C. Sommer, C. Straehle, U. Köthe, and F. A.
Hamprecht. “Ilastik: Interactive learning and
segmentation toolkit”. *2011 IEEE Interna-
tional Symposium on Biomedical Imaging: From
Nano to Macro*. Mar. 2011, pp. 230–
233. DOI: 10.1109/ISBI.2011.5872394 (cit.
on pp. 78, 81). 71
- [151] Tobias Pietzsch, Stephan Saalfeld, Stephan
Preibisch, and Pavel Tomancak. “Big-
DataViewer: visualization and processing for
large image data sets”. *Nature Methods* 12.6
(June 2015), pp. 481–483. DOI: 10.1038/nmeth.
3392 (cit. on p. 79). 72

-
- 1 [152] Joran Deschamps, Markus Mund, and Jonas Ries. “3D superresolution microscopy by sequential percritical angle detection”. *Optics Express* 22.23 (Nov. 2014), pp. 29081–29091 (cit. on pp. 81, 82). 32
2
3
4
5
6 [153] Joran Deschamps, Andreas Rowald, and Jonas Ries. “Efficient homogeneous illumination and optical sectioning for quantitative single molecule localization microscopy”. *Optics Express* 24.24 (Nov. 2016), pp. 28080–28090. DOI: 10.1364/OE.24.028080 (cit. on pp. 81, 82). 39
7
8
9
10
11
12 [154] Jeremy C. Simpson et al. “Genome-wide RNAi screening identifies human proteins with a regulatory function in the early secretory pathway”. *Nature Cell Biology* 14.7 (July 2012), pp. 764–774. DOI: 10.1038/ncb2510 (cit. on pp. 81, 91). 46
13
14
15
16
17
18 [155] Thorvald Julius Sørensen. *A method of establishing groups of equal amplitude in plant sociology based on similarity of species content and its application to analyses of the vegetation on Danish commons*. København: I kommission hos E. Munksgaard, 1948 (cit. on p. 82). 53
19
20
21
22
23
24 [156] Lee R. Dice. “Measures of the Amount of Ecologic Association Between Species”. *Ecology* 26.3 (July 1945), pp. 297–302. DOI: 10.2307/1932409 (cit. on p. 82). 59
25
26
27
- [157] Romain Fernandez, Pradeep Das, Vincent Mirabet, Eric Moscardi, Jan Traas, Jean-Luc Verdeil, Grégoire Malandain, and Christophe Godin. “Imaging plant growth in 4D: robust tissue reconstruction and lineageing at cell resolution”. *Nature Methods* 7.7 (July 2010), pp. 547–553. DOI: 10.1038/nmeth.1472 (cit. on p. 82).
[158] Mike Heilemann, Sebastian van de Linde, Mark Schüttelz, Robert Kasper, Britta Seefeldt, Anindita Mukherjee, Philip Tinnefeld, and Markus Sauer. “Subdiffraction-Resolution Fluorescence Imaging with Conventional Fluorescent Probes”. *Angewandte Chemie International Edition* 47.33 (Aug. 2008), pp. 6172–6176. DOI: 10.1002/anie.200802376 (cit. on p. 82).
[159] I. Izeddin, J. Boulanger, V. Racine, C. G. Specht, A. Kechkar, D. Nair, A. Triller, D. Choquet, M. Dahan, and J. B. Sibarita. “Wavelet analysis for single molecule localization microscopy”. *Optics Express* 20.3 (Jan. 2012), pp. 2081–2095 (cit. on p. 82).
[160] Carlas S. Smith, Nikolai Joseph, Bernd Rieger, and Keith A. Lidke. “Fast, single-molecule localization that achieves theoretically minimum uncertainty”. *Nature Methods* 7.5 (May 2010), pp. 373–375. DOI: 10.1038/nmeth.1449 (cit. on p. 82).

¹ Acknowledgements

- ² The work presented in this thesis has been carried out in the Hufnagel group at the
³ European Molecular Biology Laboratory (EMBL) in Heidelberg, Germany. I would like
⁴ to thank Lars Hufnagel for this unique opportunity to work in the field of microscopy,
⁵ and for his continuous support through the project.
- ⁶ I am very grateful to the members of my thesis advisory committee: Jonas Ries, Takashi
⁷ Hiiragi and Balázs Rózsa; thank you for the support and the fruitful discussions.
- ⁸ I would also like to thank Prof. Péter Szolgay for the opportunity to be part of the
⁹ Roska Tamás Doctoral School of Sciences and Technology at Pázmány Péter Catholic
¹⁰ University.
- ¹¹ I would like to thank Gustavo Quintas Glasner de Medeiros and Nils Norlin for the
¹² microscope building and debugging sessions, and for sharing all their experience and
¹³ knowledge. A big thank you to Marvin Albert and Joran Deschamps for their help with
¹⁴ the compression algorithm, and also for sharing the ups and downs of EMBL PhD life.
- ¹⁵ Many thanks to all friends and colleagues who helped me throughout my four years:
¹⁶ Dimitri Kromm, Ulla-Maj Fiuza, Li-Ling Yang, Stefan Günther, Lucía Durrieu, Patrick
¹⁷ Hoyer, Laura Panavaite, Uroš Kržič, Petr Strnad, Sebastian Streichan, Aldona Nowicka,
¹⁸ Christina Besir, Tatjana Schneidt, Judith Reichmann, Yu Lin, Nils Florian Wagner,
¹⁹ Christian Tischer; it has been a truly memorable time.
- ²⁰ Development of the microscope would not have been possible without the expert help of
²¹ Alfons Riedinger, Alejandro Gil Ortiz, Leo Burger, Sascha Blättel, Tim Hettinger and
²² all other members of the EMBL electronic and mechanical workshops.
- ²³ Special thanks goes to Judit Tóth, István Gärtner and Attila Mócsai for introducing me
²⁴ to the world of natural sciences, and Prof. Szabad János for showing me EMBL for the
²⁵ first time.
- ²⁶ I am eternally grateful to my parents and my first scientific advisors, Béla Balázs and
²⁷ Ilona Fige, and my sister, Eszter for their unconditional support.
- ²⁸ Finally, Melánia: Thank you for your infinite patience, support and love.