

# Portable Visible Spectrophotometer for Glucose Microdroplet Measurements in Digital Microfluidics System

Alzana Armaniar Farhani\*, Balkan Khilmi Assakandari<sup>†</sup>, Anindhita Nayazirly<sup>‡</sup>,  
Akhmadi Surawijaya<sup>§</sup>, Muhammad Ogin Hasanuddin<sup>¶</sup>

*Department of Electrical Engineering  
School of Electrical Engineering and Informatics  
Institut Teknologi Bandung  
Bandung, Indonesia*

\*farhanialzana@gmail.com, <sup>†</sup>balkankhilmi@gmail.com, <sup>‡</sup>zirlisukarno@gmail.com, <sup>§</sup>asurawijaya@itb.ac.id, <sup>¶</sup>moginh@itb.ac.id

**Abstract**—Instrumen yang telah dikembangkan kelompok Tugas Akhir Teknik Elektro sebelumnya adalah sebuah spektrofotometer portabel yang dapat bekerja pada spektrum gelombang ultraviolet dan cahaya tampak, atau umumnya disebut spektrofotometer UV-Vis. Spektrofotometer yang dibuat hanya dapat melakukan perhitungan intensitas cahaya secara relatif terhadap nilai intensitas tertinggi yang terukur, tidak dilakukan kalibrasi skala panjang gelombang dan tuning fungsi konversi citra. Hal ini menunjukkan bahwa pengukuran yang dilakukan masih bersifat kualitatif. Spektrofotometer yang telah dikembangkan kelompok Tugas Akhir Teknik Elektro belum memiliki kapabilitas untuk

**Index Terms**—UV-VIS Spectrophotometry

## I. INTRODUCTION

Currently, various methods detect and measure glucose concentrations in food matrices. These methods can be broadly grouped into two main categories: enzymatic approaches, such as spectrophotometric assays; and non-enzymatic instrumentation, such as HPLC systems. While the first group is glucose specific, the latter is broadly adaptable and can be used to detect not only glucose but a wide variety of other carbohydrates as well. However, the spectrophotometric test is becoming a more commonly used method for glucose detection because of its ability to detect in a shorter time and at a lower cost. Spectrophotometric tests utilize the light transmitted or reflected by a sample to perform qualitative and quantitative analysis. For qualitative analysis, the light transmitted by a sample has a unique spectrum based on the atoms or molecules contained in the sample.

Meanwhile, for quantitative analysis, the absorbance level of the sample for a specific wavelength is directly proportional to the concentration of the sample. Glucose spectrophotometry test includes colorimetric measurement methods, namely measurements that involve changing the color of the sample to measure quantities such as absorbance and sample concentration. Various colorimetric methods involving reactions with different enzymes for glucose measurement are the object of research being developed to obtain colorimetric

methods that are accurate, sensitive, selective, and inexpensive. Several approaches were studied to develop a colorimetric glucose biosensor by using glucose oxidase (GOx) to oxidize glucose to gluconic acid and hydrogen peroxide (H<sub>2</sub>O<sub>2</sub>). In colorimetric assays, studies revealed that the Horseradish Peroxidase (HRP) enzyme could catalyze the reaction of H<sub>2</sub>O<sub>2</sub> and organic substrates such as 3,3',5,5'-tetramethylbenzidine (TMB) to produce visible colors [?].

Microfluidics offer several advantages for glucose analysis, such as reduced sample and reagent consumption, faster analysis, portability, and high compatibility with multiplexing detection means. One application called digital microfluidics (DMF) has a promising potential to operate microdroplets in portable analytical systems. The platform is based on the droplet manipulation using electrowetting-on-dielectric (EWOD) principle which applies electric potential to the control electrodes coated with a hydrophobic dielectric [?]. The DMF system mainly consists of a fluid layer located between the top and bottom plates. Nowadays, DMF technology is commonly used for various processes which include sample preparation and diagnostics [?]. Droplet mixing allows all chemical reactions to be done on chip. An optical detection system needs to be developed in order to measure the absorbance and concentration of a glucose droplet on the DMF chip.

In this study, we present the development of a portable visible spectrophotometer, which is detachable to DMF platforms. It allows the integration with a DMF platform and can be removed if the DMF is needed for other purposes. A light will be emitted through the droplet located on the DMF chip and an array of photodetectors will collect the intensity of incident light. A program is uploaded to the system to compute the absorbance and the concentration of the sample droplet. Users can interact with the system using four input buttons and an LCD which displays the result of the measurements.

The current version of the spectrophotometer has some features as follows:

- Concentration measurement of microdroplet samples

- Absorbance measurement of samples based on wavelength characteristic
- Able to work in visible spectrum (400 nm to 700 nm)
- Able to be integrated with a digital microfluidic platform
- The measurement results can be displayed on an LCD and stored
- Portable (12cm x 13cm x 20cm)

## II. METHODS

### A. System Overview

The proposed system consists of five subsystems which are light source, light sensor, control, user interface, and power subsystem. Its data flow diagram (DFD) is shown in Fig. ???. The light sensor subsystem is composed of a slit, a monochromator, and an array of photodetector. The source light, which is emitted by a polychromatic light source, will be passed through the sample droplet located on an electrode of a DMF platform. The light which is not absorbed by the droplet will pass through the slit then to a monochromator. The monochromator decomposes the light into monochromatic light to be detected by the photodetector array. Each detector in the array measures the light intensity for a specific wavelength. The measurement readings will be sent to the control subsystem to be computed into absorbance values.

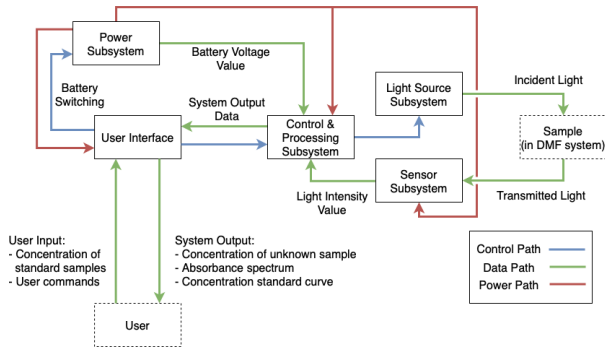


Fig. 1. Level-1 Data Flow Diagram (DFD) of the system

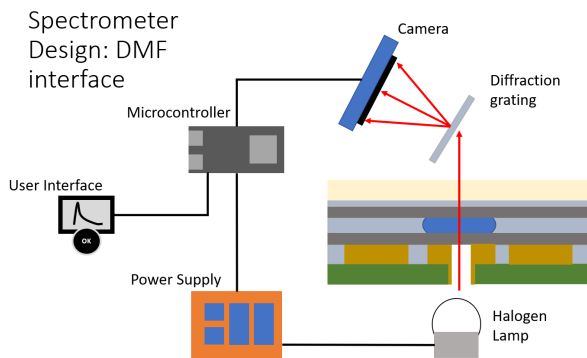


Fig. 2. The main components of the proposed device

### B. Light Source Subsystem

The light source subsystem functions to produce polychromatic light as the primary variable to be manipulated and measured by the instrument. This subsystem includes 2 modules, namely switching circuits and light sources. The process in this subsystem begins with receiving a control signal from the control subsystem to the switching circuit. The switching circuit then flows the source voltage to the lamp so that it can be lit. The polychromatic light source will illuminate and produce light with all UV-Vis frequencies within the specification. This light is then passed on to the sample for a certain period.

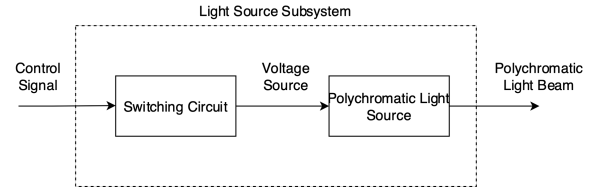


Fig. 3. DFD of the light source subsystem

### C. Light Sensor Subsystem

The light sensor subsystem functions as a spectrometer that receives polychromatic light beam and outputs light intensities of discrete wavelengths in the form of digital data. Polychromatic light beam enters the sensor subsystem through a hole and gets diffracted by a transmissive diffraction grating as to spatially separate light by its wavelengths. The grating has a groove density of 1200 lines/mm, and the first order of diffraction is used to separate the visible spectrum. The resulting ray is then recorded by a CMOS image sensor (Arducam MT9M001 Monochrome Camera Module). Different pixel of the image sensor captures the intensity of different wavelengths ranging from 400 nanometer to 700 nanometer formatted into 10-bit unsigned integer. The light sensor subsystem outputs, at maximum, 400 16-bit unsigned integer values, each value representing the light intensity of wavelengths in the visible spectrum range.

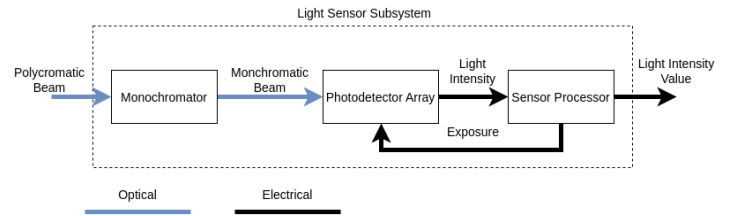


Fig. 4. DFD of the light sensor subsystem

### D. Control and Processing Subsystem

The control and processing subsystem consists of control and data processing unit. Other subsystems in the spectrophotometer are controlled by a ESP32-S3-DevkitC-1 microcontroller board (Espressif Systems, China). The task of the

control unit is to execute the main workflow of the spectrophotometer by a FSM. The control subsystem synchronizes other subsystems, such as the light source with the light sensor when measuring light intensities. The processing of data signals for measurement processes and results is a responsibility of the data processing unit. It converts the sensor's intensity data into an absorbance spectrum (spectrum mode) and performs linear regression to calculate the sample concentration according to the standard samples.

C++ programming was used to create the control subsystem program, and the PlatformIO IDE for Microsoft Visual Studio Code was used (VSCode). The primary responsibility of the control unit is to execute the spectrophotometer's processes based on the designed Finite State Machine (FSM), as shown in Fig. ??.

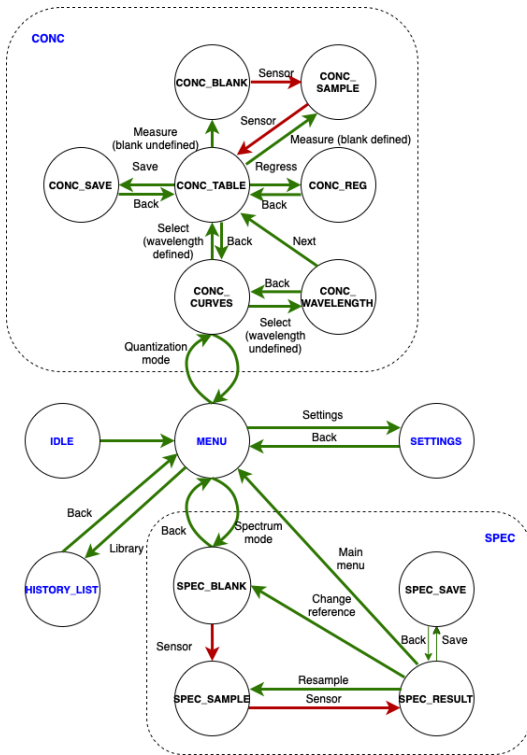


Fig. 5. FSM diagram of the portable visible spectrophotometer

The measurement data are stored on an external SD card that is part of the data processing device. The data for the absorbance spectrum and the calibration curves for the quantization mode are tabulated in a CSV-file format. The interface between the micro-SD card and the control system is provided by a microSD click module (MikroElektronika, Serbia). In order to store calibration values for absorbance measurement and quantization-mode calibration curves, the microcontroller also utilizes its non-volatile memory storage (NVS).

### E. User Interface Subsystem

The user interface subsystem plays a role in connecting the system and the users. This can be done by interpreting the

commands given by users through the input interface devices and process it into control signals that will be sent to the control subsystem. The subsystem also has a function to display measurement data which include sample concentration values, sample absorbance spectrum, regression curves, menus, and settings. Fig. ?? shows the data flow diagram of the user interface subsystem.

Four push buttons and a power switch are used as the input interface devices. For the display, a 3.5-inch non-touchscreen TFT LCD with ILI9488 driver is used. The configuration of buttons and non-touchscreen LCD is chosen because it fits the users who use the spectrophotometer using laboratory gloves.

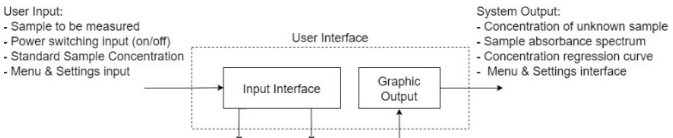


Fig. 6. DFD of the user interface subsystem

### F. Power Subsystem

The power subsystem enables the system to be activated by supplying power from the battery to the entire electrical circuit. The battery can be recharged easily whenever the battery voltage is insufficient. The power subsystem also provides information about the battery voltage value to be displayed to the user.

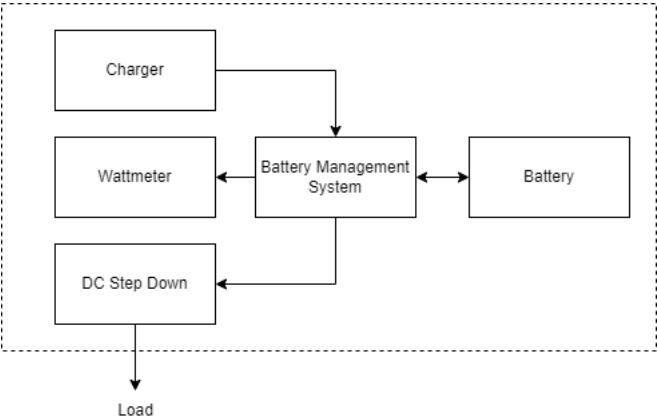


Fig. 7. DFD of the power subsystem

The power subsystem is activated when the user presses the power button for the first time—allowing the power to flow to the microcontroller. The microcontroller will supply power to certain sub-blocks according to user input by adjusting the whether the battery voltage is sufficient based on a specified threshold. If the battery voltage value is below the threshold or the user presses the power button again, the power supply to the entire circuit will be cut off, and the system will be disabled.



### G. Hardware Assembly

Using Autodesk Fusion 360 software, the body and individual parts of the portable visible spectrophotometer were created and 3D printed. The primary body, the optical light path, Fig. 1, and the control board, Fig. 2, are shown. The body of the device is made of 3D printed plastic and the control board is a custom PCB.

A. A

A

Aldr

60  $\mu$

betw

the 1

Fi

expe

Man

a vo

samp

at 5

Absc

the 6

conc

obse

nake

As

with

were

0.03

were

The

stretc

drop

and

M

as sl

lengt

peak

in ac

term

Accu

due

spon

B. R

C. V

### D. Resolution

Resolution testing is carried out by calculating the resolution of the measurement results stored on an external SD card in the form of a CSV file. The number of pixels needed for the absorbance spectrum measurement, which is obtained from

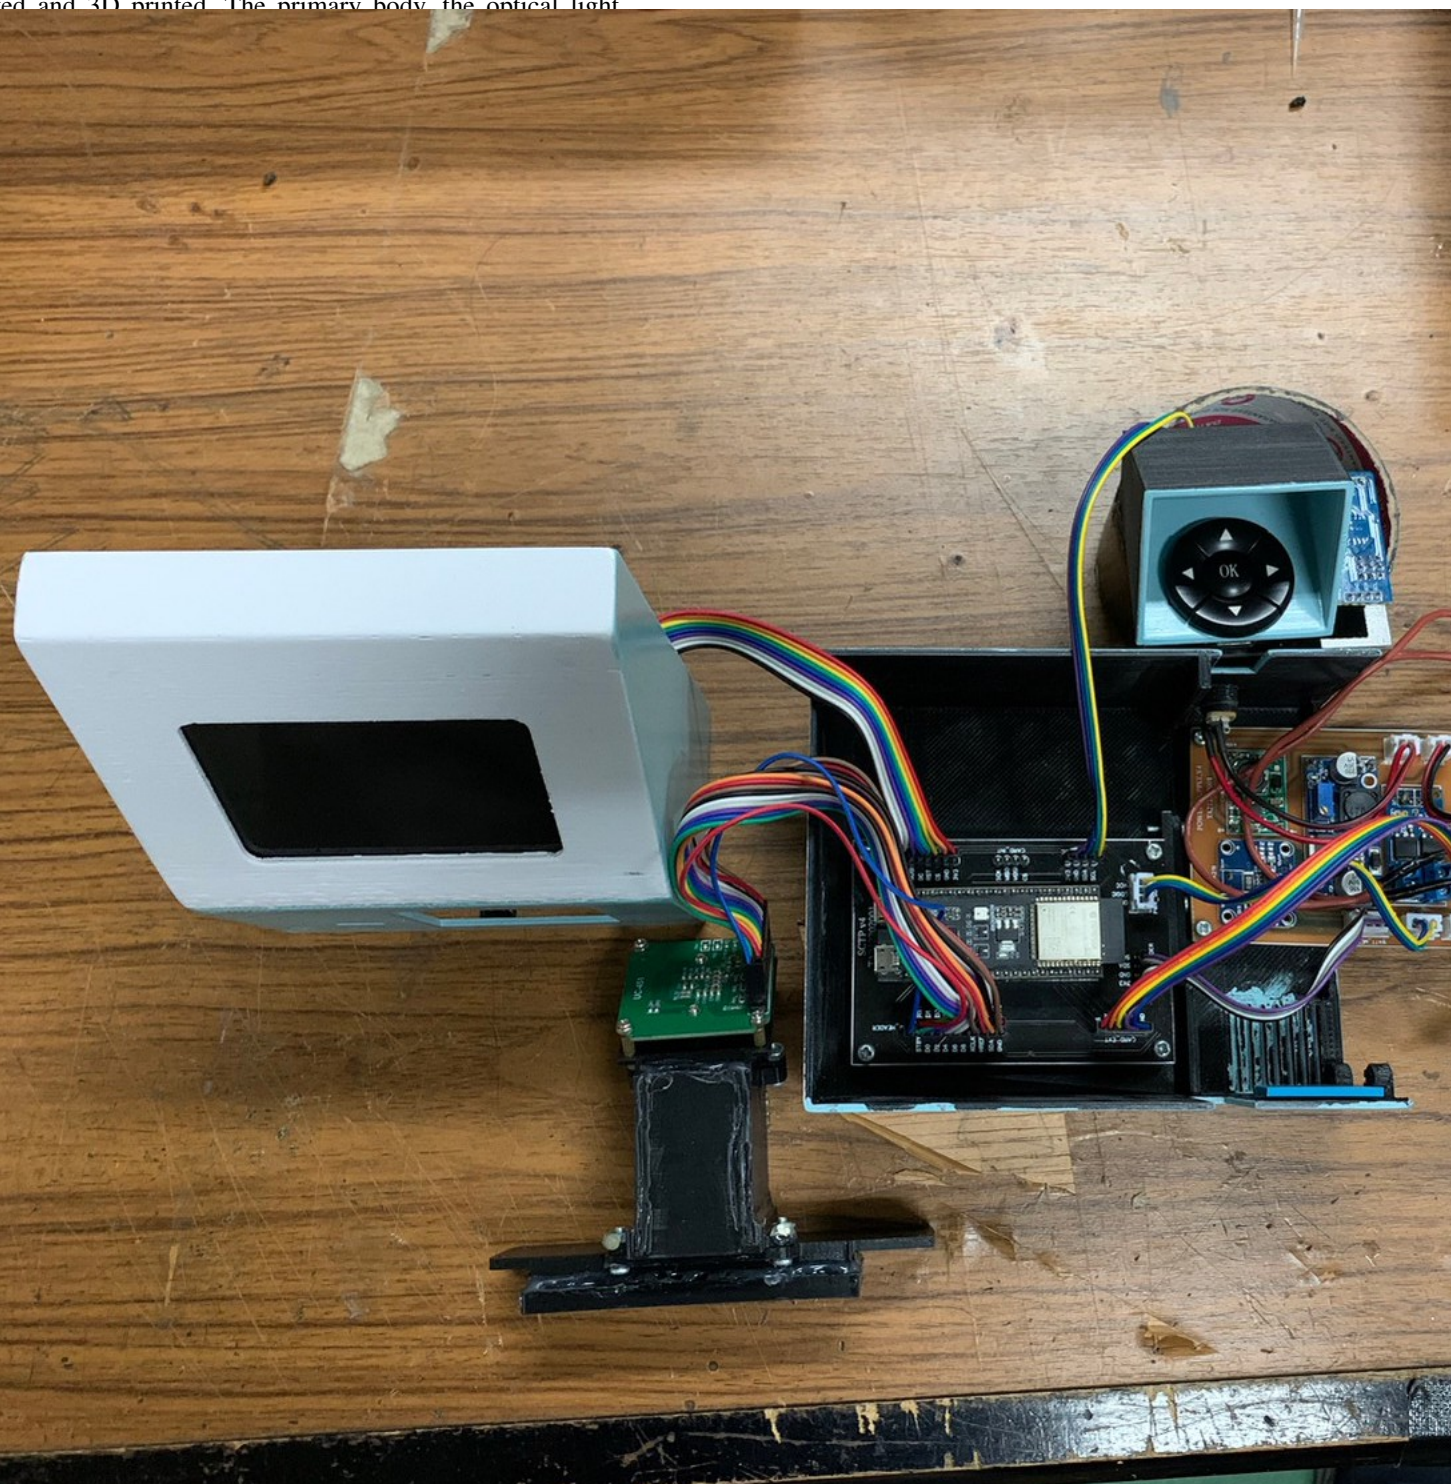


Fig. 8. Overview of the device's internal components

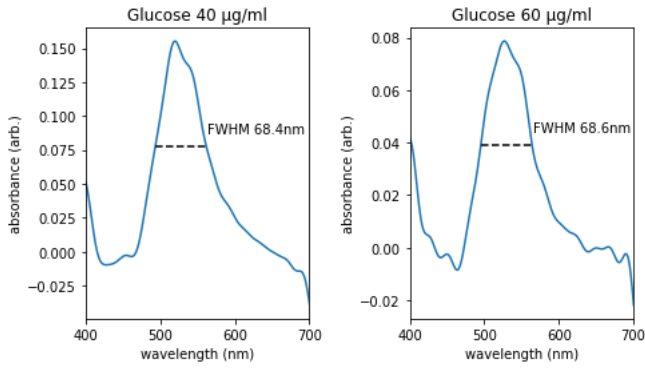


Fig. 9. Glucose absorbance spectrum measurement result, baseline corrected

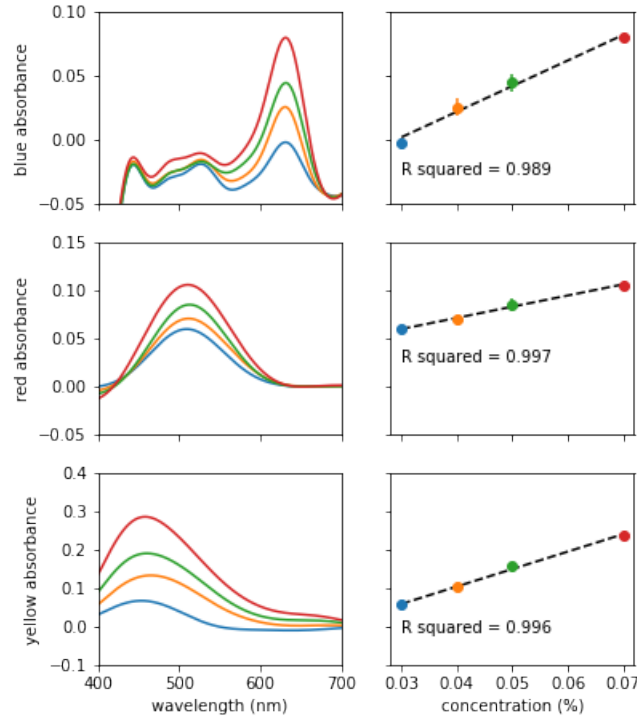


Fig. 10. Dye measurement results

the calibration results, was 297. The absorbance measurement results are stored on an external SD card with a resolution that can be calculated using Equation (??).

$$resolution = \frac{\lambda_{max} - \lambda_{min}}{n_{pixels}} = \frac{(700 - 400)nm}{393} \approx 0.77nm \quad (1)$$

#### E. Device and DMF Cartridge Distance

#### F. Weight and Size

Weight measurement is done by placing the product on a digital scale. Fig. ?? shows that the product's weight is 0.832 kilograms.

The dimension produced are 120 mm x 131 x 207 mm, as shown in Fig. ?? Product dimensions are affected by the

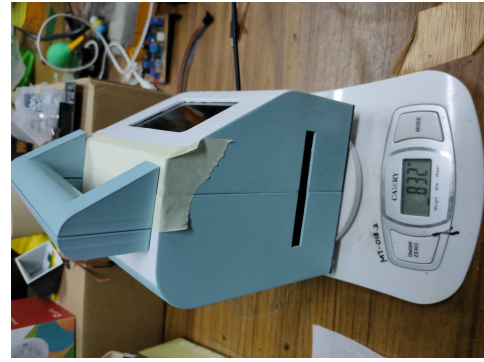


Fig. 11. Device's weight measurement

number of components used in the system and the optical configuration used. The sensor's location, diffraction grating, and light source mainly influence the product's height. The battery has a size of 70 x 42 x 21 mm, which significantly affects the determination of the minimum area of the product base. In addition, the button component with a diagonal position uses a large enough area but leaves quite a lot of remaining space.




Fig. 12. Device's dimensions

#### G. User Interface

The first page of the spectrum-mode measurement instructs the user to insert the blank reference sample into the DMF system. The sample input page, which resembles the blank input page, will be on the next page. A result page with the peak wavelength and absorbance results will show up after the other subsystems have finished measuring absorbance. The user has the option to save the result, return to the main menu, or view the entire spectrum of the absorbance measurement. Fig. ?? illustrates how the spectrum page of the absorbance measurement is shown.

	Conc	A
4	0.400	4.00
5	0.500	5.00
6	0.600	6.00
7	0.080	0.80
<div> <div>BACK</div> <div>SAVE</div> <div>REGRESS</div> </div>		

Fig. 13. The display of the spectrum page of a spectrum-mode measurement



Quantization-mode measurement starts with a page that displays the list of saved curves. Users have the option of using, removing, or adding new curves. The user will get a table page if they select an existing curve. The table consists of concentration and absorbance values of standard samples, as shown in Fig. ?? . By moving the pointer to the desired absorbance (A) cell and clicking the OK physical button, an absorbance measurement for each concentration value should be made. The user will be directed to the blank and sample input page. The user should click the REGRESS button to calculate the concentration of the unknown sample and view the standard curve plot.



Fig. 14. The display of the table page of a quantization-mode curve

#### IV. CONCLUSIONS

To support the study of spectrophotometry analysis in DMF platform, we describe the assembly of a portable spectrophotometer that can be integrated with a particular DMF system. The portability makes on-the-go research processes easier. Data acquisition, storage, and user experience is made simpler by our developed portable visible spectrophotometer and a user-friendly interface. Measurement's accuracy of red, yellow, and blue food dyes and its repeatability demonstrated good performances in experimental validation versus commercial spectrophotometer (Evolution 220). The colorimetric glucose assay (maximum of absorbance at 540 nm) measurements were comparable but quite inferior; these issues could be resolved by retesting the colorimetric reactions more thoroughly. Future work will focus on designing a better voltage regulation and heat insulation for the lamp, as well as designing reducing movable parts from the light path configuration.

#### REFERENCES

#### REFERENCES

- [1] H. V. Tran et al., "Silver nanoparticles-decorated reduced graphene oxide: A novel peroxidase-like activity nanomaterial for development of a colorimetric glucose biosensor," *Arabian Journal of Chemistry*, vol. 13, no. 7, pp. 6084–6091, Jul. 2020, doi: 10.1016/j.arabjc.2020.05.008.
- [2] Z. Gu, M. L. Wu, B. Y. Yan, H. F. Wang, and C. Kong, "Integrated Digital Microfluidic Platform for Colorimetric Sensing of Nitrite," *ACS Omega*, vol. 5, no. 19, pp. 11196–11201, May 2020, doi: 10.1021/acsomega.0c01274.
- [3] S. Huang and R. B. Fair, "Quantitative measurements of inorganic analytes on a digital microfluidics platform," *SN Applied Sciences*, vol. 1, no. 12, Dec. 2019, doi: 10.1007/s42452-019-1693-8.