


Input to Real ICD Device



Therapy Decision Match

Input to Device Model

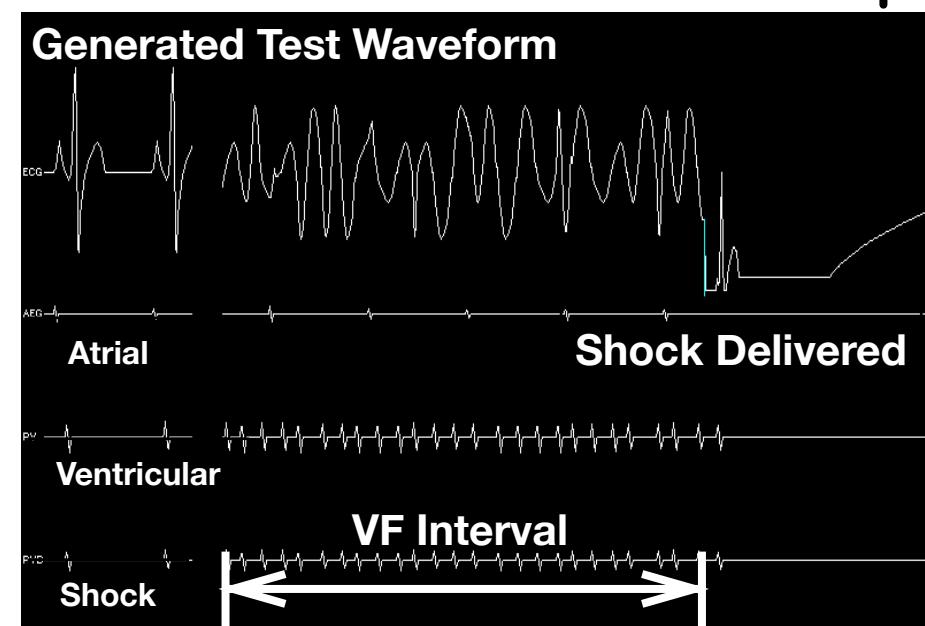