Supplement of: A Simple Method for Helium Step Heat Experiments at High Water or Sulfur Fugacity

Ben J. Thyer[1], Jonathan Treffkorn[1], and Ken A. Farley[1]

[1]Division of Geological and Planetary Sciences, California Institute of Technology, Pasadena, CA 91125, USA

Correspondence: Ben J. Thyer (bthyer@caltech.edu)

S1 Ampoules and Analytical Details

Heating steps and isotopic measurements for all samples were automated using custom LabView routines with the exception of the tank helium-soaked empty tube experiment on the Helix-MC-Plus^{10K} multi-collector mass spectrometer after the 7th measurement. For all other ampoules, a Watlow temperature controller held the ampoule at the temperature set point for a pre-programmed duration, after which the ampoule was allowed to cool while the evolved gas was prepared for measurement for about 25 minutes. After the first 7 measurements, the empty tube experiment on the Helix-MC-Plus^{10K} was instead set to an elevated temperature manually while the evolved gas was allowed to accumulate continuously in an attempt to mitigate uncertainties related to frequently changing temperatures (supplementary Eq. (S38); Fig. S9) and continued permeation at room temperature during gas cleanup and measurement. The accumulated gas was measured every 40-120 minutes. For this experiment, the temperature was changed either during the 1 minute pump-out of the lamp cell after inletting gas into the mass spectrometer, or during a period of helium accumulation for measurement. When the temperature was changed during an accumulation period, no permeability was calculated for that step, and the measured abundances of those steps were used only to track the helium contents of the tube.

Helium isotope measurements of evolved gases from step heats of one empty silica glass ampoule and glass-encapsulated sulfur and water ampoules equilibrated with 2-20 torr of high purity tank helium ($R \approx 0.15\ R_a$) were acquired at Caltech on a Thermo Fisher Helix-MC-Plus^{10K} mass spectrometer in peak hopping mode. Helium was purified by exposing evolved gases to a charcoal trap held in liquid nitrogen, a titanium sponge getter, then a SAES NP10 getter before freely expanding into the Helix-MC-Plus^{10K}.

Helium-4 evolved during the step heat of the silica glass-encapsulated Durango apatite was quantified using isotope dilution with a high purity 3He spike on a Pfeiffer Prisma QMS 200 quadrupole mass spectrometer. Evolved gas from the ampoule in the lamp heating cell was allowed to mix with the 3He spike and the mixture was frozen on charcoal held at 14 K within a cryostat, then helium was selectively released to the mass spectrometer by raising the temperature to 36 K.

Standard gasses were routinely measured to monitor drift in the sensitivities of 3He and 4He. Blanks are approximately 5 pccSTP ^{4}He, which is very small compared to all interpreted ^{4}He measurements. Further analytical details are given by Thyer (2026).

Table S1. Silica Glass tubes that were the subject of helium step heat experiments in this work. The ampoule labeled "Quad" had evolved 4He quantified by isotope dilution using a Pfeiffer Prisma QMS 200 quadrupole mass spectrometer, whereas ampoules labeled "MC" had both evolved 3He and 4He quantified using a Helix-MC-Plus^{10K} multi-collector mass spectrometer. Where 3He was measured, the ampoule was soaked in tank helium with an isotope ratio of ~0.15 Ra.

Ampoule Contents	Mass Spec.	Inner Diameter μm	Outer Diameter μm	Geometric factor *G* cm^{-2}	Volume Ratio $\left(\frac{V_{glass}}{V_{gas}}\right)$	Content Mass	Helium Source
Empty	MC	747	1159	3264	1.41	—	Tank He
Sulfur	MC	529–550	835–872	5992	1.5	~0.2 mg	Tank He
Water	MC	487–515	734–776	7789	1.27	~0.5 mg	Tank He
Durango Apatite	Quad	850	1350	2394	1.52	3.18 mg	Radiogenic

S2 Relating the Rate Constant to Glass Permeability and Ampoule Geometry

Helium permeation through fused silica in diffusive steady state is a first order process that can be described with the simple differential equation:

$$\frac{dn}{dt} = -GKnRT \tag{S1}$$

Where *n* is the number of helium atoms, *t* is the time, *G* is the geometric parameter in units of cm^{-2}, which is a function only of the geometry of the glass membrane, *K* is the permeation constant for helium in fused silica, which follows the Arrhenius law: $\left(K(T) = K_0 e^{-\frac{E_a}{RT}}\right)$ and has been repeatedly measured for fused silica (Norton, 1953; Altemose, 1961; Swets et al., 1961; Masaryk, 1968), *R* is the gas constant, and *T* is the temperature in Kelvin. Equation (S1) is identical to the permeation equation used in early studies (Norton, 1953; Altemose, 1961; Swets et al., 1961; Studt, 1962; Masaryk, 1968), except that it is formulated in terms of absolute atomic abundances instead of helium gas pressure by the ideal gas law. It is easily integrated by separation of variables to yield $n_t = n_0 e^{-GKRTt}$ (see Sect. S3 for details). Comparison with main-text Eq. (2) gives $\lambda = KGRT$.

The geometric factor *G* for a cylindrical membrane with negligible permeation through the top or bottom is determined using the effective area of permeation given by Masaryk (1968):

$$G = \frac{2}{a^2 \ln\left(\frac{b}{a}\right)} \tag{S2}$$

where *a* is the cylinder's internal radius, and *b* is the external radius. There is no dependence on the cylinder length when permeation through the top and bottom is negligible. This geometric constant will vary according to the experimental design and therefore must be measured by the experimentalist.

S3 A Fick's Law Formulation Describing Helium Migration Across Semi-Permeable Membranes

We derive the relevant equations describing helium permeation through glass by beginning with Fick's Law, similarly to previous works (Rogers et al., 1954; Altemose, 1961).

$$J = -D\frac{d\varphi}{dx} \tag{S3}$$

Where *J* is the area-normalized Fickian diffusive flux in units of $\frac{atoms}{s \times cm^2}$, *D* is the diffusivity (of helium in glass) in units of $\frac{cm^2}{s}$, and $\frac{d\varphi}{dx}$ is the concentration gradient, in units of $\frac{\left(\frac{atoms}{cm^3}\right)}{cm}$ or $\frac{atoms}{cm^4}$.

For steady state permeation across a planar membrane, the concentration gradient is constant. If we take *l* to be the glass thickness and we rewrite the Fickian flux *J* as $\frac{F}{A}$, where F is the absolute atom flux in units of $\frac{atoms}{s}$, and A is simply the membrane area, we can rewrite Fick's law as:

$$F = -DA\frac{\Delta\varphi}{l} \tag{S4}$$

Finally, we assume that the concentration of helium within the glass membrane is Henrian, i.e. proportional to the gas pressure in contact with the membrane. Experimental work has shown that helium permeation through silica glass is Henrian at pressures of several hundred bars and lower (Shelby, 1976), well above the experimental helium partial pressures for this work. We define this proportionality factor as the solubility, *S*, in units of $\frac{atoms}{atm \times cm^3}$. Now we may write the expression in terms of the gas pressure gradient, or the difference of helium partial pressures on each side of the membrane.

$$F = -DA\frac{S\Delta P}{l} \tag{S5}$$

Diffusivity and solubility are material properties that are functions of temperature following the Arrhenius equation, and therefore their mathematical product (permeability, *K*) also follows an Arrhenius relation with temperature (Rogers et al., 1954; Swets et al., 1961). Now, recognizing that K = DS, we may express the equation in terms of permeability $\frac{atoms}{s \times cm \times atm}$.

$$F = -\frac{KA\Delta P}{l} \tag{S6}$$

Studt (1962) and Masaryk (1968) also use this equation to describe helium permeation through silica glass, taken from Darcy's Law for gas flow through semi-permeable membranes (Carman, 1956). This ordinary, first-order differential equation is well suited for describing permeation through a silica membrane when the permeate pressures on each side of the membrane

are constant (Norton, 1953; Altemose, 1961; Swets et al., 1961). Cases where permeate partial pressure changes during the experiment (such as this work) require solving the first order ODE above to relate the abundance of an analyzed permeate to the abundance of unanalyzed permeate remaining in the depleting reservoir.

Recalling that F is an atomic flux in units of $\frac{atoms}{s}$ that could be notated as $\frac{dn}{dt}$:

$$\frac{dn}{dt} = -\frac{KA\Delta P}{l} \tag{S7}$$

We assume that the helium partial pressure in the ultra-high vacuum (UHV) heating cell surrounding the ampoule is 0, so that the pressure gradient equals the partial pressure within the ampoule ($\Delta P = P$). This is a valid assumption for this work because the heating cell is 4-5 orders of magnitude more voluminous than the glass ampoule. The assumption therefore is only appreciably violated for the trivial case in which effectively all the helium present within the tube is permeated out and the helium partial pressures within and outside of the ampoule are equal. In this case, net helium flux goes to zero even though the ampoule is not entirely evacuated. Relative to the amount of helium within the ampoule at time 0 (n_0), the amount of helium remaining in the ampoule after infinite time *(n_{eqm})* will be set by the volume ratio of the ampoule and the lamp cell.

$$\frac{n_{eqm}}{n_0 - n_{eqm}} \approx \frac{n_{eqm}}{n_0} = \frac{V_{ampoule}}{V_{lamp\ cell}} \approx 10^{-4}$$

For this experimental setup, only 1 part in 10000 helium atoms will remain in the ampoule after infinite time in the closed heating cell.

Before integrating Eq. (S7), it is useful to experimentalists working with mass spectrometry to express the pressure term *P* in terms of atoms *n*, the atomic abundance of helium within the ampoule. Helium is well-approximated as an ideal gas at experimental conditions, so the ideal gas law (PV = nRT) relates the pressure, *P*, to the atomic abundance, *n*, yielding Eq. (S8):

$$\frac{dn}{dt} = -\frac{AKnRT}{lV} \tag{S8}$$

Where *R* is the gas constant $\left(1.36 \times 10^{-22} \frac{cm^3 atm}{K\ atoms}\right)$, *T* is the temperature in Kelvin, and *V* is the volume in cm^3. It is now obvious that the helium atoms in the gas phase (*n*) decrease over time. Because Eq. (S8) assumes a steady state helium concentration profile in the glass walls of the ampoule in equilibrium with the helium partial pressure inside the ampoule, one must make another essential assumption to continue: that the permeation timescale be small with respect to the diffusive timescale so that the helium concentration profile of the glass effectively remains in an equilibrium with the helium atoms in the gas phase (*n*). If the inner gas volume is small relative to the volume of the ampoule glass, then $\frac{dn}{dt}$ will be relatively large and the helium atoms in the gas phase (*n*) will decrease faster than diffusion's ability to maintain an equilibrium concentration profile in the glass, violating the assumption of a steady state concentration profile in equilibrium with the inner gas phase. Then, Eq. (S8) and all equations derived from it will be invalid. In other words, the timescale of diffusion must be much smaller than the timescale of permeation ($\tau_D \ll \tau_P$) for Eq. (S8) and all derived equations to apply. A more thorough analysis of this assumption is presented in §S4.

Eq. (S8) can be simplified by defining a geometric factor (G) in units of cm^{-2} that incorporates the spatial parameters for area, volume, and length of the experimental glass ampoule:

$$\frac{dn}{dt} = -GKnRT \tag{S9}$$

Eq. (S9) can be integrated using a straightforward separation of variables to get a useful general equation describing helium reservoirs depleting via permeation.

$$n_t = n_0 e^{-KGRTt} \tag{S10}$$

Where n_t is the amount of helium atoms within the reservoir after time t in seconds, and n_0 is the amount of helium atoms within the reservoir at time t = 0.

Eq. (S10) can equivalently be expressed in terms of the fraction of the initial helium reservoir that has permeated during time t, which is often a more intuitive quantity when relating this equation to a measured amount of helium. Defining the fractional permeation yield ${}^{He}F \equiv \frac{m}{n_0}$, where $m \equiv n_0 - n_t$ is the amount of helium permeated and available to be measured during time t, Eq. (S10) can be recast as:

$${}^{He}F = \frac{m}{n_0} = 1 - e^{-KGRTt} \tag{S11}$$

Eq. (S10) can be solved for permeability (K) for use in experimentally determining permeability for experiments in which the permeating helium source is significantly depleted during the experiment, yielding Eq. (S12):

$$K = -\frac{\ln(n_t) - \ln(n_0)}{GRTt} \tag{S12}$$

In typical experimental measurements of helium permeability through glass, permeation rates are measured in real time, and the pressure gradient is constant throughout the measurement, so an equation like Eq. (S6) is used to solve for permeability instead (Norton, 1953; Swets et al., 1961; Altemose, 1961).

S3.1 Permeation Through Cylindrical Membranes

For non-planar membranes, the effective area of permeation, A, is not straightforward to evaluate because the surface area on each side of the membrane differs. Masaryk (1968) gives the effective area of permeation for a cylinder (such as for this experiment) as:

$$A = \frac{2\pi hl}{\ln\left(\frac{b}{a}\right)} \tag{S13}$$

Where a is the cylinder's internal radius, b is the cylinder's external radius, and h is its length. This effective area of permeation (Eq. (S13)) can be used with the equation for the internal volume of the cylinder: $V = h\pi a^2$ to evaluate the geometric factor G (Eq. (S9)) for a cylinder in terms of the ampoule geometry. Reducing yields Eq. (S14):

$$G = \frac{2}{a^2 \ln\left(\frac{b}{a}\right)} \tag{S14}$$

Interestingly, h cancels so that the permeation rate has no dependence on the ampoule length when permeation through the top and bottom is negligible. Eq. (S14) displays the intuitive behavior that thinner walls and narrower tubes lead to more efficient permeation. Where G is used elsewhere in this work, it refers to the cylindrical geometric factor given in Eq. (S14). Most silica ampoules sealed at Caltech for helium step heat experiments were 0.6-1.2 mm wide with 150-300 μm thick glass, translating to values of G between 2000-7000 cm^{-2}. In this work, if no value of G is specified, then a typical 200 μm thick ampoule with an outer diameter of 1 mm is assumed, corresponding to a = 0.03 cm, b = 0.05 cm and G = 4350.26 cm^{-2}.

S4 Diffusive Steady State Concentration Profiles in Cylindrical Membranes

To establish a steady state concentration profile, the diffusive timescale must be much faster than the permeation timescale, otherwise the helium concentration profile within the glass will respond too slowly to maintain equilibrium with the rapidly depleting internal gas phase (Fig. S1). The ratio of the permeation timescale and diffusive timescale is a strong function of the ratio of the ampoule's glass and internal gas volumes with a very minor dependence on temperature (Fig. S2 below). An ampoule with a glass/gas volume ratio of 2 has a diffusive timescale that is ~5.6% of the permeation timescale (Eq. (S18) below). Numerical diffusion-permeation simulations show that Eq. (S12) accrues less than 1% error due to deviation from the idealized helium concentration profile (Figs. S3 and S4 below). Smaller glass/gas volume ratios are better: the ampoules in the main text have glass/gas volume ratios ~1.25-1.5. Numerical simulations show that this error is determined nearly entirely by the volume ratio of the ampoule glass and gas and is otherwise insensitive to ampoule geometry (Figs. S5 and S6 below).

The derivation for Eq. (S12) always assumes an equilibrium steady state helium concentration profile across the ampoule. The most important corollary of this assumption is that the timescale of permeation must be much larger than the diffusive timescale ($\tau_D \ll \tau_P$) for Eq. (S12) and all derived equations to apply. An analysis is presented here exploring the ampoule geometries that permit the use of the analytical solutions for helium permeation through silica glass.

The diffusive timescale is the timescale at which diffusion is generally expected to establish a steady state concentration profile between two (effectively) constant reservoirs. For a diffusive domain size L, the timescale is given as:

$$\tau_D = \frac{L^2}{D} \tag{S15}$$

The permeation timescale is analogous to an "e-folding time" or "mean life" in radioactive decay, the time after which point the original abundance of something decaying by a first order process following the form $\frac{dn}{dt} = -\lambda n$ would have decreased

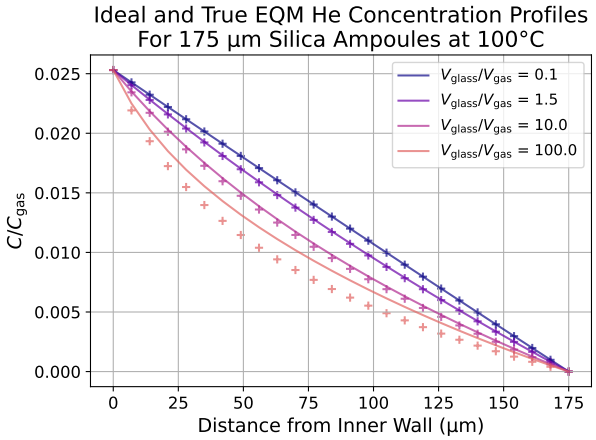


Figure S1. Ideal diffusive steady state concentration profiles (demarcated by the '+' symbols) are contrasted with the numerically calculated "effective" steady state concentration profile, represented by the solid lines. These effective concentration profiles are not strictly in steady state, but they are effectively in equilibrium with a rapidly decreasing internal helium reservoir. These profiles are retrieved by numerically simulating a model ampoule permeating helium for at least one diffusive timescale. At low glass/gas volume ratios, the idealized and true concentration profiles are indistinguishable. Ideal steady state concentration profiles for cylindrical membranes are strongly curved at high glass/gas volume ratios and become linear as the glass/gas volume ratio approaches 0. For closed ampoules where internal pressure is not constant, but instead decreases due to permeation, the internal pressure decreases faster than the glass concentration profile can respond to the new internal helium pressure, so the concentrations are higher (and less curved) than the ideal profile, because of memory of higher internal helium pressures. 4He diffusivities and solubilities are taken from Swets et al. (1961).

by a factor of Euler's number ($1/e$). After one permeation timescale has passed, more than half of the original helium has permeated through the ampoule walls, leading to the intuition that the dimensionless timescale ratio must satisfy $\frac{\tau_D}{\tau_P} \ll 1$ in order for Eq. (S12) and Eq. (S10) to apply, because only vanishingly small changes in the total helium are allowed within one diffusive timescale in order for an equilibrium helium concentration profile to be stabilized and maintained.

$$\tau_P = \frac{1}{\lambda} = \frac{1}{GRTK} \tag{S16}$$

The ratio of these two timescales is a weak function of temperature and a strong function of the ratio of ampoule glass and internal gas volumes $\left(\frac{V_{glass}}{V_{gas}}\right)$ (Fig. S2). By the equation for the volume of cylinders:

$$V_{\frac{glass}{gas}} = \frac{h\pi\left(b^2 - a^2\right)}{h\pi a^2} = \frac{\left(b^2 - a^2\right)}{a^2} \tag{S17}$$

$\frac{\tau_D}{\tau_P}$ can be expanded and recast to be a function of only temperature and $V_{\frac{glass}{gas}}$. Recall that L = b-a and K = SD, and the identity of G for cylinders from Eq. (S14):

$$\frac{\tau_D}{\tau_P} = \frac{L^2}{D} GRTK = \frac{(b-a)^2}{D} \frac{2}{a^2 \ln\left(\frac{b}{a}\right)} RTSD$$

Factoring $\left(b^2 - a^2\right) = (b-a)(b+a)$, substituting, and simplifying:

$$\frac{\tau_D}{\tau_P} = V_{\frac{glass}{gas}} \bullet \frac{(b-a)}{(b+a)} \frac{2}{\ln\left(\frac{b}{a}\right)} RTS$$

Now using Eq. (S17) to relate the terms containing a and b to $V_{glass/gas}$, all spatial terms can be expressed in terms of this ratio.

$$\left(\frac{b}{a}\right) = \sqrt{V_{\frac{glass}{gas}} + 1}$$

For example:

$$b = a\sqrt{V_{\frac{glass}{gas}} + 1}$$

$$(b-a) = a\left(-1 + \sqrt{V_{\frac{glass}{gas}} + 1}\right)$$

$$(b+a) = a\left(1 + \sqrt{V_{\frac{glass}{gas}} + 1}\right)$$

$$\frac{\tau_D}{\tau_P} = S(T) \bullet RT \bullet V_{\frac{glass}{gas}} \bullet \frac{-1 + \sqrt{V_{\frac{glass}{gas}} + 1}}{1 + \sqrt{V_{\frac{glass}{gas}} + 1}} \bullet \frac{2}{\ln\left(\sqrt{V_{\frac{glass}{gas}} + 1}\right)} \tag{S18}$$

Eq. (S18) is plotted for three temperatures as a function of glass/gas volume ratio in Fig. S2. $\frac{\tau_D}{\tau_P}$ increases monotonically and nearly linearly in log-log space with the glass/gas volume ratio of ampoules, whereas temperature plays only a minor role. Ampoules with high glass/gas volume ratios and $\frac{\tau_D}{\tau_P}$ ratios can be considered "glass dominated". For these glass-dominated ampoules, the relative difference in surface area between the inner and outer surfaces is large, resulting in a more profoundly curved ideal concentration profile (Fig. S1 above, Eq. (S23)). For glass dominated ampoules, this ideal curved concentration profile is only realized if the internal pressure is held constant, otherwise, this internal helium partial pressure decays rapidly due to permeation relative to the rate of diffusion within the glass, thereby stabilizing a helium concentration profile in the glass that will be less curved and higher than the idealized steady state of Eq. (S23) (Fig. S1 above). When normalized to the

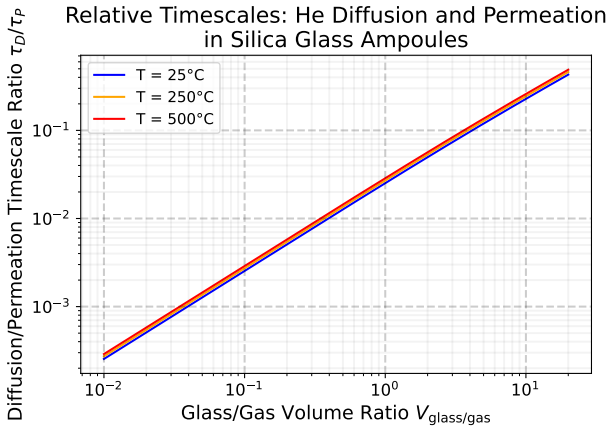


Figure S2. The accuracy of Eq. (S10) and equations derived from it is dependent on a steady state concentration profile in equilibrium with the helium gas concentration inside the ampoule. If the timescale of permeation is comparable to or lower than the timescale of diffusion for the ampoule, then the gas concentration inside the ampoule will change faster than the response of the concentration profile within the glass, and these equations will become inaccurate. In other words, these equations are only accurate when $\tau_D/\tau_P \ll 1$. For helium permeation in silica glass ampoules, the ratio of the diffusive and permeation timescales is a strong function of the ratio of glass and gas volume, and a weak function of temperature. τ_D/τ_P is nearly linear with V_{glass}/V_{gas} in log-log space, forming subtly-offset parallel arrays at different temperatures. 4He solubilities are taken from Swets et al. (1961).

concentration, quantity, or pressure of helium within the gas phase of the ampoule, this quasi-steady state concentration profile is reached within one diffusive timescale and remains constant as diffusion and permeation proceed, regardless of the ratio of glass and gas volumes (this property was tested by varying the permeation time between one and ten diffusive timescales, which had no effect on the concentration profile normalized to the concentration, abundance, or partial pressure of helium in the gas phase). Indeed, all model ampoule calculations from Figs. S3–S5 were initialized to have this effective steady state concentration profile, which is done by allowing the model ampoule to permeate and diffuse for one diffusive timescale, after which the concentration profile is multiplied by the simulated $\frac{n_0}{n_t}$ to renormalize it to the original helium contents of the ampoule. The helium content of the gas is then recalculated using the relation $n_{gas} = n_0 - n_{glass}$, and the permeated helium outside of the ampoule is reset to 0. Numerical simulations of model ampoules with glass/gas volume ratios above ~ 0.1 that were initialized to the ideal steady state of Eq. (S23) recorded an early spike in relative error with Eq. (S12) that was maximized before one diffusive timescale because of an incorrect initial steady state assumption. This artifact vanished completely when the true steady state profile was used.

Numerical simulations of model ampoules of varying dimensions, thicknesses, and geometric factors show that the only geometric parameter that directly affects the accuracy of the analytical solutions, e.g. Eq. (S12), is the glass/gas volume ratio of the ampoules (Figs. S3–S5). This geometric dependence is much more important than subtle effects of temperature (Figs. S2; S5). Ampoules from this work have glass/gas volume ratios between 1.2 and 1.6, for which Eq. (S12) is accurate to within 1%

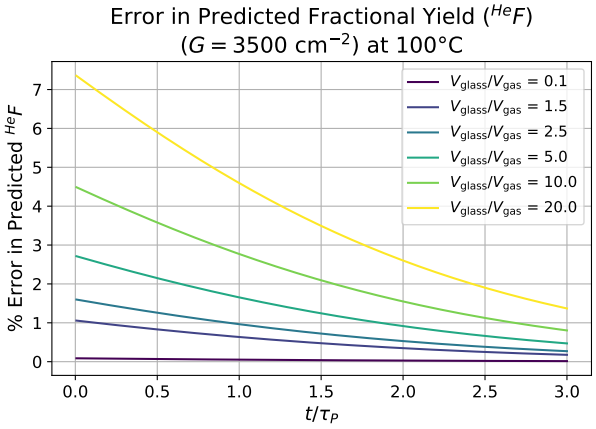


Figure S3. Numerical simulations confirm that Eq. (S12) is accurate for ampoules with low glass/gas volume ratios. For ampoules with higher glass/gas volume ratios, the relative error is not constant but depends on the duration of the step. The relative error reaches a maximum at a step shorter than the permeation timescale (τ_P) for ampoules with glass/gas volume ratios higher than 1, then decreases as steps continue and most of the original gas within the ampoule has been permeated. 4He diffusivities, solubilities, and permeabilities are taken from Swets et al. (1961).

for temperatures less than 500°C (Fig. S4). For more precise handling, odd thermal schedules, or for ampoules with higher glass/gas volume ratios, permeation fractions would need to be numerically solved to achieve sufficient accuracy to use a permeation measurement to constrain the helium contents of an ampoule.

To understand the steady state helium concentration profile in the glass, it is necessary to model the radial diffusion through a symmetrical, hollow cylinder. Carslaw and Jaeger (1959) give the equation for the change in concentration by diffusion in a cylinder (eqn. 5, page 17, second edition), expressed here in terms of concentration and diffusivity.

$$\frac{dC}{dt} = D\left[\frac{\partial^2 C}{\partial r^2} + \frac{1}{r}\frac{\partial C}{\partial r} + \frac{1}{r^2}\frac{\partial^2 C}{\partial \theta^2} + \frac{\partial^2 C}{\partial z^2}\right] \tag{S19}$$

For typical ampoules used in this work, the surface area of the top and bottom together is about 5-10% of the surface area of the walls, but they are neglected here for simplicity. Assuming that the concentration profiles are radially symmetrical and uniform with height (z), Eq. (S19) is reduced to:

$$\frac{dC}{dt} = D\left[\frac{\partial^2 C}{\partial r^2} + \frac{1}{r}\frac{\partial C}{\partial r}\right] \tag{S20}$$

At steady state, $\frac{dC}{dt} = 0$, so

$$\frac{\partial^2 C}{\partial r^2} + \frac{1}{r}\frac{\partial C}{\partial r} = 0$$

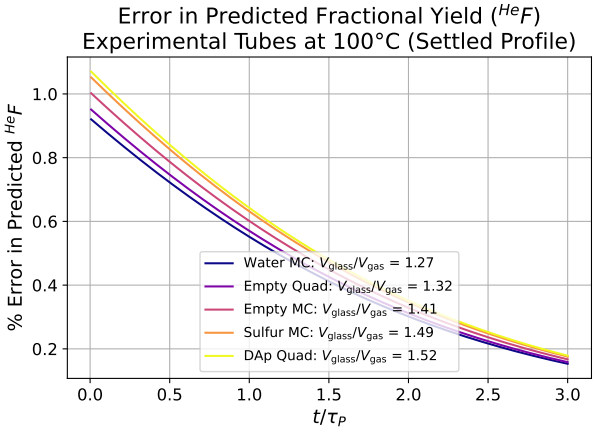


Figure S4. Numerical experiments of this work show that these equations will be accurate to within 1% for ampoule glass/gas volume ratios less than 2 for temperatures less than 500°C, which corresponds to $\tau_D/\tau_P < 0.056$. Experimental ampoules at Caltech have glass/gas volume ratios generally between 1.25 and 1.5, and thus Eq. (S12) is accurate to within 1% for ampoules with concentration profiles in steady state. 4He diffusivities, solubilities, and permeabilities are taken from Swets et al. (1961).

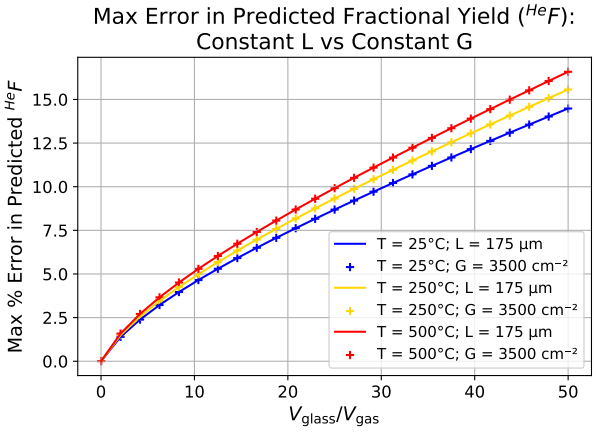


Figure S5. Numerical simulations of two suites of model ampoules with varying glass/gas volume ratios and a constant thickness (L) or permeation geometric factor (G) show that the only factors that determine the applicability of Eq. (S12) for helium permeation of closed ampoules are glass/gas volume ratio (primarily) and temperature (secondarily). These two suites have different geometries and permeation rates, yet the deviation of the numerical model from Eq. (S12) is the same for different ampoules with the same glass/gas volume ratio at the same temperature. This is clear evidence that the ratio of diffusive and permeation timescales is the primary control on the accuracy of Eq. (S12). 4He diffusivities, solubilities, and permeabilities are taken from Swets et al. (1961).

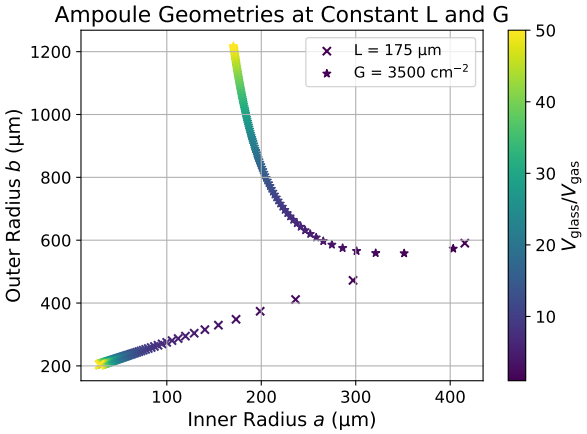


Figure S6. Model ampoules with uniformly distributed glass/gas volume ratios between 0.01 and 50 and one other constraint (either constant thickness or constant geometric permeation factor *G*, Eq. (S14)) have defined inner and outer radii. These are the same suites of ampoules for which helium permeation was numerically simulated in Fig. S5.

Which, by the product rule, can be expressed as:

$$\frac{1}{r}\frac{\partial}{\partial r}\left(r\frac{\partial C}{\partial r}\right) = 0$$

Now, the $\frac{1}{r}$ term can be dropped, and both sides can be integrated with respect to r to yield:

$$r\frac{\partial C}{\partial r} = A$$

Where A is a constant of integration. Now both sides are integrated again with respect to r, leaving the equation describing the geometry of the diffusive steady state concentration profile of a cylinder (Eq. (S21)):

$$\frac{\partial C}{\partial r} = \frac{A}{r}$$

$$C(r) = \int \frac{A}{r} dr$$

$$C(r) = Aln(r) + B \tag{S21}$$

Where B is another constant of integration. Constants *A* and *B* can be solved for once the boundary conditions are defined, that is, the helium concentrations at the inner and outer walls of the glass ampoule. The concentration of helium at the outer wall is effectively 0 because the high vacuum heating cell is essentially an infinite volume compared to the glass ampoule. At the inner wall, the concentration is governed by the solubility and helium partial pressure of the encapsulated volume. Letting *a* be the radius of the ampoule inner wall, *b* be the radius of the outer wall, and P_{He}^{gas} be the partial pressure of helium in the encapsulated gas of the ampoule, the following boundary conditions are enforced:

$$C(r = b) = 0$$

$$C(r = a) = S(T) \bullet P_{He}^{gas}$$

Now a system of equations can be formulated so that *A* can be solved first, then *B*.

$$0 = Aln(b) + B$$

$$S(T) \bullet P_{He}^{gas} = Aln(a) + B$$

$$S(T) \bullet P_{He}^{gas} = Aln(a) - Aln(b)$$

$$S(T) \bullet P_{He}^{gas} = A\, ln\left(\frac{a}{b}\right)$$

$$A = \frac{S(T) \bullet P_{He}^{gas}}{ln\left(\frac{a}{b}\right)}$$

$$B = -\frac{S(T) \bullet P_{He}^{gas}}{\ln\left(\frac{a}{b}\right)} ln(b)$$

Substituting *A* and *B* back into Eq. (S21):

$$C(r) = \frac{S(T) \bullet P_{He}^{gas}}{\ln\left(\frac{a}{b}\right)} \ln(r) - \frac{S(T) \bullet P_{He}^{gas}}{\ln\left(\frac{a}{b}\right)} \ln(b)$$

$$C(r) = S(T) \bullet P_{He}^{gas} \bullet \frac{\ln\left(\frac{r}{b}\right)}{\ln\left(\frac{a}{b}\right)} \tag{S22}$$

Using the ideal gas law and the volume for the cylinder, the partial pressure of helium within the ampoule can be related to the geometry of the ampoule and the abundance of helium atoms within the ampoule:

$$P_{He}^{gas} = \frac{n_{He}^{gas} RT}{V_{gas}}$$

$$V_{gas} = \pi a^2 h$$

$$P_{He}^{gas} = \frac{n_{He}^{gas} RT}{\pi a^2 h}$$

$$C(r) = S(T) \bullet \frac{n_{He}^{gas} RT}{\pi a^2 h} \bullet \frac{\ln\left(\frac{r}{b}\right)}{\ln\left(\frac{a}{b}\right)} \tag{S23}$$

Where *h* is the length of the ampoule.

Because the concentration profile of the ampoule is radially symmetrical, Eq. (S23) can be expressed as a radial density of helium atoms instead to eliminate the dependence on *h*. The concentration ($C(r)\frac{atoms}{cm^3}$) can be converted into a radial density ($\epsilon(r)\frac{atoms}{cm}$) by multiplying by the circumference of a circle with radius *r* and the cylinder height *h*.

$$\epsilon(r) = C(r) * 2\pi r h \tag{S24}$$

Substituting in $C(r)$ from Eq. (S23) and the geometric constant of permeation *G* from Eq. (S14) $\left(G = \frac{2}{a^2 \ln\left(\frac{b}{a}\right)} = -\frac{2}{a^2 \ln\left(\frac{a}{b}\right)}\right)$:

$$\epsilon(r) = S(T) \bullet \frac{2 n_{He}^{gas} r RT}{a^2} \bullet \frac{\ln\left(\frac{r}{b}\right)}{\ln\left(\frac{a}{b}\right)}$$

$$\epsilon(r) = -S(T) \bullet n_{He}^{gas} GRTr \ln\left(\frac{r}{b}\right) \tag{S25}$$

To find the proportion of helium within the glass at steady state, the radial density is integrated from *r* = *a* to *r* = *b*.

$$n_{He}^{glass} = \int_a^b \epsilon(r) dr = \int_a^b -S(T) \bullet n_{He}^{gas} GRTr \ln\left(\frac{r}{b}\right) dr$$

$$n_{He}^{glass} = -S(T) \bullet n_{He}^{gas} GRT \bullet \int_a^b [rln(r) - rln(b)]\, dr$$

Applying the sum rule, then integration by parts to one term yields the indefinite integral:

$$\int [rln(r) - rln(b)]\, dr = \frac{1}{2} r^2 \ln(r) - \frac{r^2}{4} - \frac{1}{2} r^2 \ln(b) + C$$

Evaluating the definite integral from the bounds of $r = a$ to $r = b$ yields:

$$\int_a^b [rln(r) - rln(b)]\, dr = \frac{1}{2} b^2 \ln(b) - \frac{b^2}{4} - \frac{1}{2} b^2 \ln(b) - \frac{1}{2} a^2 \ln(a) + \frac{a^2}{4} + \frac{1}{2} a^2 \ln(b)$$

Reducing and simplifying:

$$\int_a^b [rln(r) - rln(b)]\, dr = \frac{1}{2} a^2 \left(\ln\left(\frac{b}{a}\right) + \frac{1}{2} \right) - \frac{b^2}{4}$$

$$n_{He}^{glass} = -S(T) \bullet n_{He}^{gas} GRT \bullet \left(\frac{1}{2} a^2 \left(\ln\left(\frac{b}{a}\right) + \frac{1}{2} \right) - \frac{b^2}{4} \right) \tag{S26}$$

Eq. (S26) can be easily expressed in terms of total helium in the ampoule by substituting for the relationship $n_{He}^{gas} = n_0 - n_{He}^{glass}$

$$n_{He}^{glass} = -S(T) \bullet \left(n_0 - n_{He}^{glass} \right) GRT \bullet \left(\frac{1}{2} a^2 \left(\ln\left(\frac{b}{a}\right) + \frac{1}{2} \right) - \frac{b^2}{4} \right)$$

$$\frac{\left(n_0 - n_{He}^{glass} \right)}{n_{He}^{glass}} = \left[-S(T) \bullet GRT \bullet \left(\frac{1}{2} a^2 \left(\ln\left(\frac{b}{a}\right) + \frac{1}{2} \right) - \frac{b^2}{4} \right) \right]^{-1}$$

$$\frac{n_0}{n_{He}^{glass}} = 1 + \left[-S(T) \bullet GRT \bullet \left(\frac{1}{2} a^2 \left(\ln\left(\frac{b}{a}\right) + \frac{1}{2} \right) - \frac{b^2}{4} \right) \right]^{-1} \tag{S27}$$

S4.1 A Numerical Model for Diffusive Permeation of Helium Through Silica Glass Ampoules

Most of the permeation measurements performed on the Helix-MC-Plus^{10K} mass spectrometer were complicated by additional permeation occurring at variable temperature during long cooling times following high temperature experimental steps. Such a complication can be effectively avoided by limiting the duration of time for which the diffusion cell is opened to the rest of the vacuum line, or by keeping the sample at-temperature during this equilibration time. To address this, a numerical diffusive permeation model is used to calculate the ampoule's expected permeation fraction (n_t/n_0) for each step with a complex thermal history.

A numerical model to estimate diffusive permeation is invaluable, as it provides a flexible way to estimate the permeation fraction $\left(\frac{m}{n_0}\right)$ even when the required assumptions for the analytical solutions are not met. For example, a numerical approach can calculate the expected permeation fraction for a non-isothermal time-temperature history, and it needn't obey the assumption that the helium concentration profile in the glass is in diffusive equilibrium with the partial pressure of helium in the encapsulated gas phase. As will be investigated below, the equilibrium concentration profile assumption is ephemerally broken when temperatures are changed, and for ampoules with high glass/gas ratios it is never true.

We numerically solve the radial diffusion equation for cylinders (Eq. (S20)) using the Forward-Time Central-Space (FTCS) Finite Difference Method (FDM) along a radial transect of a model ampoule of arbitrary geometry for small, discrete time intervals. The system is spatially discretized into 100 cells along a radial transect, and numerical stability was ensured by solving for the time interval of a single step, Δt, such that $\frac{D\Delta t}{\Delta x^2} = 0.5$, satisfying the Courant-Friedrichs-Lewy (CFL) condition.

Helium concentrations along the transect (except for the boundaries, where r = a and r = b) are updated according to the following equation, an FTCS discretization of the radially symmetric diffusion equation for a cylinder (Eq. (S20)):

$$\frac{dC_r}{dt} = D\left[\frac{\partial^2 C}{\partial r^2} + \frac{1}{r}\frac{\partial C}{\partial r}\right]$$

$$\Delta C_r \approx \Delta t \bullet D\left[\frac{C_{r-\Delta r} - 2C_r + C_{r+\Delta r}}{\Delta r^2} + \frac{1}{r}\frac{C_{r+\Delta r} - C_{r-\Delta r}}{2\Delta r}\right] \tag{S28}$$

Dirichlet boundary conditions were enforced at the inner and outer boundaries. The concentration at the model ampoule's outer boundary (where r = b) was held at 0, while the concentration at the inner boundary (where r = a) was calculated at each discrete step by multiplying the solubility (in units of $\frac{atoms}{atm \times cm^3}$) by the helium partial pressure within the ampoule, according to Eq. (S29) or (S30).

$$C_{He}^{glass} = S(T) \bullet P_{He}^{gas} \tag{S29}$$

Eq. (S29) can be related to the atomic abundance of helium in the gas phase using the ideal gas law and the formula for the volume of a cylinder:

$$P_{He}^{gas} = \frac{n_{gas} RT}{V_{gas}}$$

$$V_{gas} = \pi a^2 h$$

$$C_{He}^{glass} = S(T) \bullet \frac{n_{gas} RT}{\pi a^2 h} \tag{S30}$$

For simulations where the internal pressure is not constant, n_{gas} changes after every step and Eq. (S29) is reapplied to the inner boundary cell where r = a. While the helium concentrations in the glass and in the encapsulated gas phase are both dependent on the length of the ampoule (*h*), they compensate for one another such that the absolute atom flux into and out of the ampoule is not a function of *h*. Within the numerical model, *h* was varied by orders of magnitude and the results of the simulations did not change, confirming this property.

It is sometimes useful to normalize the helium concentration of the glass to the concentration of helium in the gas. To do this, the internal helium partial pressure is related to an atomic or molar concentration using the ideal gas law:

$$C_{He}^{gas} = \frac{n}{V} = \frac{P_{He}^{gas}}{RT}$$

The pressure term vanishes in the ratio of the two concentrations and depends only on temperature:

$$C_{He}^{glass/gas} = \frac{C_{He}^{glass}}{C_{He}^{gas}} = S(T) \bullet RT \tag{S31}$$

Eq. (S31) is plotted in Fig. S7. It shows that this partitioning ratio strongly favors the gas and is only a weak function of temperature, varying between 2.5 and 2.8% between 0 and 300°C. This implies that departures from the equilibrium steady state assumption due to temperature changes will be small and perhaps negligible, which is confirmed in Fig. S9.

In order to simulate permeation, the atomic abundances of helium within the gas phases both outside the ampoule (at high vacuum) and inside the ampoule must be tracked, as must the fluxes between the glass and these two gas phases. These fluxes were calculated simply as the diffusive flux in $\frac{atoms}{s \bullet cm^2}$ as is given by Fick's law (Eq. (S3)). For spatially discrete cells throughout the ampoule at any radius except for the boundaries, the diffusive flux can be approximated with the finite difference:

$$J_r = -D\frac{\partial C_r}{\partial r} \approx -D\frac{C_{r+\Delta r} - C_{r-\Delta r}}{2\Delta r} \tag{S32}$$

However, Eq. (S32) cannot be applied at the ampoule's inner wall when r = a or outer wall when r = b because there is no remaining glass on one side of the cell. In that case, second order terms from Taylor expansions centered at $a + \Delta r$ and $b - \Delta r$ can be used to better approximate the $\frac{\partial C_a}{\partial r}$ and $\frac{\partial C_b}{\partial r}$ terms. Letting $f(r) = \frac{\partial C_r}{\partial r}$ and $f'(r) = \frac{\partial^2 C_r}{\partial r^2}$:

$$J_a = -D\frac{\partial C_a}{\partial r} \approx -D\left(\frac{\partial C_{a+\Delta r}}{\partial r} + \frac{\partial^2 C_{a+\Delta r}}{\partial r^2}\Delta r\right) \approx -D\left(\frac{C_{a+2\Delta r} - C_a}{2\Delta r} + \frac{C_a - 2C_{a+\Delta r} + C_{a+2\Delta r}}{2\Delta r^2}\Delta r\right) \tag{S33}$$

$$J_b = -D\frac{\partial C_b}{\partial r} \approx -D\left(\frac{\partial C_{b-\Delta r}}{\partial r} - \frac{\partial^2 C_{b-\Delta r}}{\partial r^2}\Delta r\right) \approx -D\left(\frac{C_b - C_{b-2\Delta r}}{2\Delta r} - \frac{C_b - 2C_{b-\Delta r} + C_{b-2\Delta r}}{2\Delta r^2}\Delta r\right) \tag{S34}$$

The helium contents in the measurable (external, high vacuum) reservoir and the inner encapsulated gas phase are updated every step using fluxes determined from Eq. (S34) and (S33) respectively. To convert these area-normalized fluxes into absolute atomic abundances, these fluxes are multiplied by the time increment (Δt) and the surface area of the cylinder at the outer and inner walls respectively.

S4.1.1 Modeling permeation for ampoules that experienced complex thermal histories

In order to compare the experimental results for ampoules that experienced complex cooling histories with the expectations of the first order permeation model developed in this work, the numerical model developed above was used. The model predicts the relative helium permeation for the three experiments on the Helix-MC-Plus^{10K} multi-collector mass spectrometer for both 4He and 3He by simulating helium permeation of a model ampoule with the same dimensions and thermal history of the real experiment. For ampoules with multiple measurements of the geometric dimensions, the smaller set of measurements is used for the numerical model.

To simulate permeation during cooling of an ampoule, the temperature is decreased at every step following a parabolic rate law determined using the Watlow temperature records of the cooling ampoule. A parabolic function is fit to cooling rates evaluated as a function of temperature. Cooling rates were algorithmically calculated for discrete time intervals using the Watlow temperature files of the relevant ampoule in Python. Temperatures were taken to be the mid-point between the maximum and minimum temperatures of the interval over which the temperature change was evaluated. The quadratic functions fit to these data were forced to have a single root at T = 24°C so that the simulated ampoules would cool to a final temperature of 24°C, a common room temperature of the Noble Gas Laboratory at Caltech.

The model ampoules were initially assigned an arbitrary and unitless amount of helium, and the permeation predictions were output as step fractional yields $\left(\frac{n_t}{n_0}\right)$, where n_0 was the amount of helium in the ampoule at the beginning of the step. Before the first heating step was simulated, the ampoule was assumed to be in diffusive steady state at 24°C. Afterwards, the ampoule was not assumed to be in diffusive equilibrium except for isothermal steps at times longer than the diffusive timescale at that temperature, so that the concentration profile of the model ampoule was tracked throughout the entire heating history. For steps above room temperature, the ampoule was simulated to immediately transition to the target temperature, then the helium concentration profile, influx, and outflux of the glass were tracked for the nominal (programmed) heating times

for times smaller than the diffusive timescale at that temperature. After a heated step, an equilibrium concentration profile was reinitialized at that temperature only if the equilibrium equation (Eq. (S12)) was used for permeation timescales longer than the diffusive timescale, then the temperature of the ampoule was cooled continuously according to the quadratic rate law determined from the experimental ampoule's thermal history while helium diffusion and permeation were continuously simulated.

S4.2 Errors related to violation of the steady state concentration profile assumption due to temperature change

The equilibrium concentration profile is always a function of temperature because the partitioning of helium between the gas phase and the glass at the ampoule's inner boundary is temperature dependent (Shackelford et al., 1972). A new steady-state helium concentration profile must be established every time the temperature is changed. Because of this behavior, it is advantageous to characterize the timescales necessary to achieve a steady state diffusive profile at different temperatures, as well as the magnitude of the uncertainties that result from applying Eq. (S12) immediately after a temperature change, when the diffusive steady state concentration profile is violated.

A new steady state concentration profile must first be established when the temperature is changed for Eq. (S12) to strictly apply. It is possible to design experiments where permeation measurements are taken only after a diffusive steady state concentration profile is established within the ampoule, which is further discussed below.

It may unduly inconvenience the experimentalist to experimentally enforce the diffusive steady state condition when the uncertainties introduced by violating the assumption are small. In Fig. S7, Eq. (S31) is plotted for relevant experimental temperatures using the solubilities reported by Swets et al. (1961). Fig. S7 shows that the helium volume density of glass at the ampoule's inner boundary will be between 2.5 and 3% of the volume density of equilibrated gaseous helium. The overall variation in helium partitioning is small ($\leq$12%) across temperatures relevant to step heat experiments on encapsulated goethite (0-300°C). There will be excess helium within the glass when changing from a higher temperature experimental step ($\geq$175°C) to a lower temperature permeation step ($\leq$120°C) that would result in a slightly higher measured value than what would be predicted by Eq. (S10). Other temperature shifts could also result in a deficit of dissolved helium instead of an excess (e.g. when shifting temperatures from 70°C to 25°C: Figs. S8, S9).

$$Disequilibrium\ Excess = n_{He}^{glass}\ (T_1) - n_{He}^{glass}(T_2) \tag{S35}$$

The disequilibrium excess of Eq. (S35) can be made into a relative error by dividing by the ideal amount of permeated helium measured in a permeation step from Eq. (S10).

$$Relative\ Disequilibrium\ Error\ = \frac{n_{He}^{glass}\ (T_1) - n_{He}^{glass}(T_2)}{n_0(1 - e^{-\lambda(T_2)t})} \tag{S36}$$

To evaluate Eq. (S35) and (S36), n_{He}^{glass} must be calculated. An upper bound can be obtained by assuming a steady state diffusion profile and an ideal open tube geometry (with small tops and bottoms neglected for simplicity), assuming that the

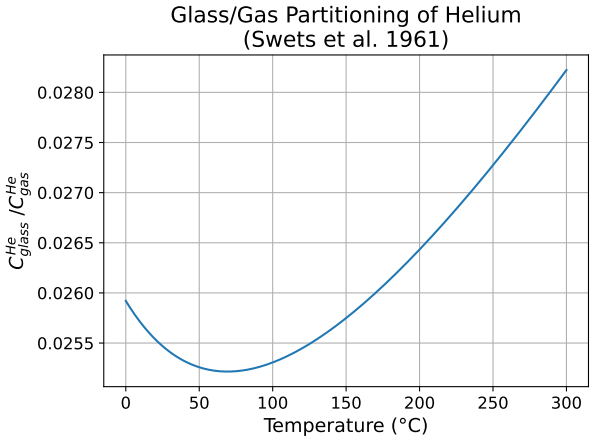


Figure S7. Helium preferentially partitions into the gas phase over silica glass. Eq. (S31) is plotted here: $\frac{C^{glass}_{He}}{C^{gas}_{He}} = S \cdot RT$. It is the ratio of concentrations (in units of atoms/mL) for helium in silica glass over gas at equilibrium using solubility values of 4He from Swets et al. (1961). This partitioning is only a weak function of temperature, so the concentration ratio is between 2.5% and 2.9% for temperatures between 0 and 300°C.

helium partial pressure outside of the ampoule is 0 and defining the abundance of helium within the gas phase as n^{gas}_{He} . The radial concentration profile at diffusive steady state as a function of radius and temperature is given in Eq. (S25). Radially integrated, the total amount of helium dissolved within the glass is given in Eq. (S27), which can be solved for n^{glass}_{He} , yielding Eq. (S37).

$$n^{glass}_{He} = \frac{n_0}{1 + \left[-S(T) \bullet GRT \bullet \left(\frac{1}{2}a^2\left(\ln\left(\frac{b}{a}\right) + \frac{1}{2}\right) - \frac{b^2}{4}\right)\right]^{-1}} \tag{S37}$$

Where *a* is the radius of the ampoule's inner wall and *b* is the radius of the ampoule's outer wall. For legibility, the terms that are not a function of temperature are grouped as the parameter *H*.

$$H = -GR \bullet \left(\frac{1}{2}a^2\left(\ln\left(\frac{b}{a}\right) + \frac{1}{2}\right) - \frac{b^2}{4}\right)$$

Now Eq. (S37) can be expressed as:

$$n^{glass}_{He} = \frac{n_0}{\left(\frac{1}{HTS} + 1\right)}$$

$\frac{n^{glass}_{He}}{n_0}$, the fraction of helium atoms within the ampoule dissolved within glass, is a function only of temperature for a given ampoule. This quantity is evaluated using Eq. (S37) for several tubes of varying glass/gas volume ratios that share a geometric

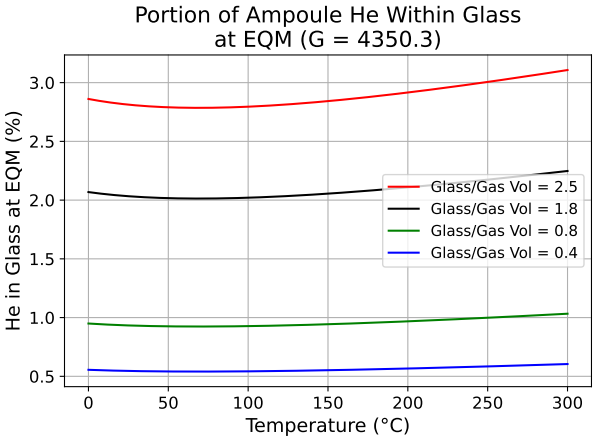


Figure S8. Most helium trapped within the ampoules of this work resides in the gas phase. Permeation from ampoules with more glass relative to gas will deviate more strongly from the expected permeation at diffusive steady state (Eq. (S10)) after thermal perturbation. At diffusive equilibrium, the concentration of helium at the ampoule's inner wall is defined by the equilibrium concentration ratio with the gas phase plotted in Fig. S7. The concentration at the outer wall is effectively 0. The concentration profile at any point along a transect through the tube is defined by Eq. (S25). Eq. (S26) integrates this concentration profile along the radius to calculate the total amount of helium within the glass, and this value is divided by the total amount of helium within the gas to show the relative distribution of helium between glass and gas for ampoules as a function of inner and outer radii and temperature. It is solved here using solubilities of 4He from Swets et al. (1961) for several tubes with varying glass/gas volume ratios that share the same geometric constant of permeation G. Red, black, green, and blue lines correspond to inner radii a of 270, 300, 400, and 500 microns and outer radii of 507, 500, 533, and 601 microns respectively. The black line follows the "standard ampoule" of this work.

385 factor for permeation of G = 4350 cm^{-2} and plotted in Fig. S8. Although these model tubes would all permeate helium at the same rate in diffusive steady state, they have different sizes, thicknesses, and relative internal (gas) and glass volumes, which affect how long they would need to achieve a steady state diffusive concentration profile after thermal perturbation and how severely diffusive disequilibrium would cause the amount of permeated helium to vary from the predicted amount from Eq. (S9). Fig. S8 gives the intuitive result that ampoules containing more glass relative to gas will produce larger helium
390 excesses/deficits when permeating immediately after thermal perturbation.

Now that the amount of helium atoms dissolved in the glass is defined as a function of temperature, Eq. (S37) evaluated at the old and new temperatures (T_1 and T_2 respectively) can be substituted into Eq. (S36) to estimate the relative measured helium excess caused by thermal perturbation as a function of time. Considering that the predicted value of n_0 is proportional to the measured amount of helium in a permeation step according to Eq. (S9), the *Relative Disequilibrium Excess* defined
395 below applies to both the measured value of helium atoms m and to the calculated value of helium within the ampoule at the beginning of the permeation step n_0.

$$Relative\ Disequilibrium\ Excess = \frac{\left(\frac{n_0}{\left(\frac{1}{HT_1S_1}+1\right)} - \frac{n_0}{\left(\frac{1}{HT_2S_2}+1\right)}\right)}{n_0(1-e^{-KGRT_2t})}$$

Upon factoring and simplifying, n_0 cancels out, removing the dependence of this error estimation on knowledge of the true initial helium content of the ampoule.

$$Relative\ Disequilibrium\ Excess = \frac{\left(\frac{1}{\left(\frac{1}{HT_1S_1}+1\right)} - \frac{1}{\left(\frac{1}{HT_2S_2}+1\right)}\right)}{1-e^{-KGRT_2t}} \tag{S38}$$

The relative excess helium that would be measured in a permeation step following a high-temperature experimental step is plotted in percent in Fig. S9 as a function of permeation time according to Eq. (S38) for several initial experimental temperatures and permeation temperatures. This relative error decreases as the new equilibrium concentration profile is established, approaching the permeation behavior expected from Eq. (S9). These excesses assume an instantaneous transition from experimental step to permeation step and therefore are upper bounds. These excesses are dependent also on the ampoule dimension; in Fig. S9, a standard ampoule (a = 0.03 cm, b = 0.05 cm) is assumed. Thicker ampoules will produce higher magnitudes of excesses (or deficits) for the same heating schedules. Within the temperature range 0-300°C the maximum excess helium that could be introduced into a permeation step measurement due to diffusive disequilibrium would be for an 80°C permeation step following an experimental step at 300°C. Even for those circumstances, the maximum relative error would be $\leq$2% for a 3-hour permeation step (Fig. S9). It is important to recognize, however, that this error estimation does not account for non-instantaneous cooling, although fast thermal response for similar experiments and the exponential temperature dependence of diffusion and permeation typically permit experimentalists to neglect fast but non-instantaneous heating and cooling (Farley et al., 1999). These calculations show that, at least for ampoules of similar dimensions to those sealed at Caltech, the error in Eq. (S10) resulting from violating the diffusive steady state assumption of Eq. (S12) is small.

For cases where more precise determinations of n_0 and n_t from the application of Eq. (S10) on a permeation step are desired, it is possible to experimentally ensure compliance with the diffusive steady state concentration assumption. For example, the ampoule could be programmed to be held at the target permeation temperature (for example, 80°C) immediately after a high temperature experimental step instead of completely cooling (to ~25°C) while evolved gases are processed and helium is purified from the high temperature experimental step. To do this, one must be aware of the timescale necessary to reach diffusive equilibrium at a given temperature. At Caltech, helium purification after heating steps typically takes 30 minutes, which is only enough time to establish steady state concentration profiles for ampoules <175 μm thick at 100°C (main text Fig. S17). For larger ampoules or cooler permeation step temperatures, an additional delay may need to be programmed in order to experimentally enforce the diffusive steady state assumption. Alternatively, expected permeation fractions for any arbitrary thermal schedule can be numerically solved, provided that the solubility and diffusivity are each known for the experimental temperature range.

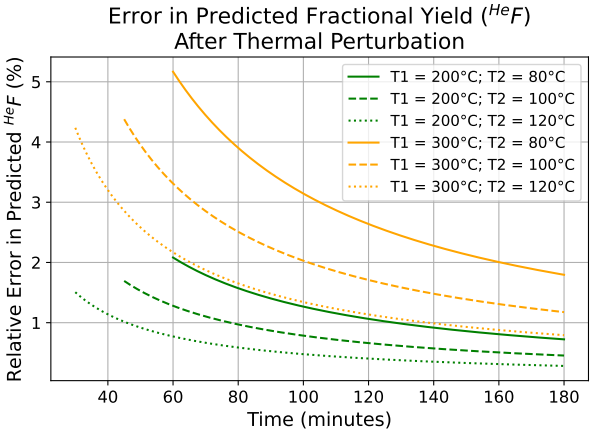


Figure S9. When changing temperatures, the inner boundary condition and diffusive steady state concentration profile of helium within a silica glass ampoule change, so the amount permeated will be different from the expected permeate amount of Eq. (S10) that assumes a diffusive steady state profile has already been established at the new temperature. This difference is calculated here as the difference of helium dissolved within the tube at the starting and final temperature (neglecting the change in helium abundance in the gas phase) and is normalized to the expected permeation amount at the final temperature as a function of time for several temperature jumps, using Eq. (S26) and solubilities of 4He from Swets et al. (1961) for a standard ampoule (with inner and outer radii of a = 300 microns and b = 500 microns respectively). Generally, larger temperature jumps produce larger relative errors. For a standard ampoule, the error of Eq. (S10) will be less than 2% for any permeation step 3 hours or longer following a 300°C experimental step.

The Fourier number can be used to determine the time necessary to establish diffusive equilibrium of the helium concentration profile within the ampoule. The Fourier number is a dimensionless number that describes the extent of diffusive equilibration or homogenization of a system by heat or mass transfer given a characteristic length scale and time (Ostrogorsky and Glicksman, 2015). It is the time divided by the diffusive timescale:

$$Fo = \frac{Dt}{L^2} = \frac{t}{\tau} \tag{S39}$$

Where t is time and L is the diffusive length scale. For the purposes of helium permeation through silica glass ampoules, L is the glass thickness of the ampoule. When $Fo > 1$, a system is generally said to be effectively homogenized or at equilibrium with respect to diffusion, but it is somewhat arbitrary to define a specific Fourier number at which one can confidently say that diffusion has effectively re-established an equilibrium concentration profile (Ostrogorsky and Glicksman, 2015). To test the value of $Fo = 1$ as the relevant minimum value, we use the numerical diffusive permeation model described above for a characteristic ampoule where a = 300 μm and b = 500 μm. Dirichlet boundary conditions are imposed at the ampoule's inner and outer boundaries, where r = a and r = b, holding $C_{r=b}^{Glass} = 0$ and $C_{r=a}^{Glass} = C_{He}^{Gas} \bullet \frac{C_{He}^{Glass}}{C_{He}^{Gas}}_{EQM}$ as calculated in Eq. (S31) and plotted in Fig. S7. For the analysis of the Fourier number during the approach to the diffusive equilibrium concentration

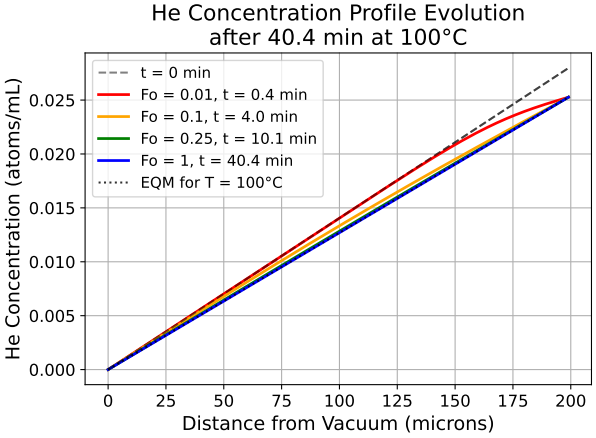


Figure S10. A numerical simulation of the evolution of 4He concentration profiles in silica glass ampoules from steady state at 300°C to steady state at 100°C. The steady state concentration profile is only subtly different for different temperatures. The diffusive timescale $\tau = L^2/D$ corresponding to a Fourier number of 1 is effectively sufficient to reestablish a steady state concentration profile at the new temperature. The concentration is arbitrary and is normalized to the concentration of helium in the gas phase of the ampoule, which is held constant for this simulation (therefore the ideal steady state of Eq. (S25) applies regardless of the glass/gas volume ratio). The inner boundary condition is determined as a function of temperature using the values of Eq. (S31), plotted in Fig. S7. The ampoule simulated here is a standard ampoule with an outer radius of 500 microns and inner radius of 300 microns.

profile in Figs. S10 and S11, C_{He}^{Gas} is arbitrary and held constant, so plotted concentrations are normalized to C_{He}^{Gas}. A steady state concentration profile (Eq. (S23)) is taken as the initial condition. The absolute concentration is technically dependent on the ampoule height, but this dependence on h vanishes when normalizing the glass concentration to the gas concentration. The results of these calculations are plotted in Figs. S10 and S11, where Fig. S10 shows the transition from an equilibrium concentration profile at 300°C to 100°C, and Fig. S11 shows the more dramatic establishment of an equilibrium concentration profile at 100°C from an initial helium concentration of 0 throughout, such as could be expected after suddenly introducing helium into an ampoule that previously contained no helium. Both figures show that an equilibrium concentration profile is well-established for Fourier number *Fo = 1,* and Fig. S10 in particular shows that the difference in concentration profiles is small and nearly reestablished even when the Fourier number *Fo = 0.1*. We conclude that the timescale associated with *Fo = 1* is the relevant time needed to hold the ampoule to ensure that Eq. (S10) strictly applies without errors due to thermally-forced disequilibrium in the helium concentration profile. The diffusive timescales associated with *Fo = 1* for permeability values taken from Swets et al. (1961) are plotted in main text Fig. S17 for a few different thickness values (L) as a function of temperature for typical permeation step temperatures used in this study.

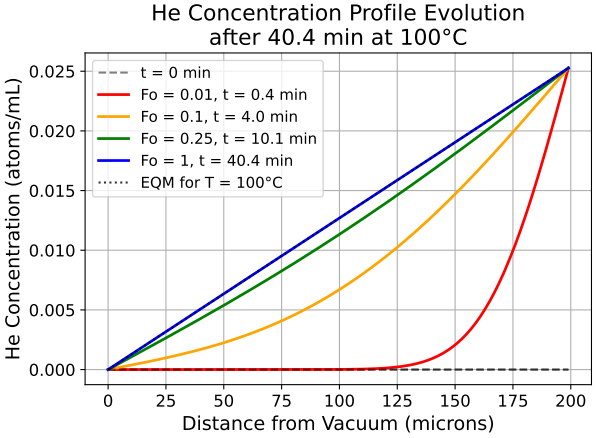


Figure S11. Similar to Fig. S10, but starting from a helium concentration of 0 throughout the ampoule. This is most useful to visualize the incomplete establishment of a steady state concentration profile for timescales corresponding to Fourier numbers up to 0.25. When the Fourier number is 1, the concentration profile is in diffusive steady state.

S5 Estimating permeation lag uncertainty for uncorrected, long heating steps

The uncertainty of the helium evolution of the encapsulated natural material during a heating step (ω) due to permeation lag correction can be estimated by calculating the maximum possible helium residing in the tube between steps, i.e. for the values for n_0 and n_t: n_0^{UB} and n_t^{UB}. From the permeation lag equation (main text Eq. (1)), upper bound estimates for n_0 and n_t bound the encapsulated material contribution ω within:

$$m - n_0^{UB} \leq \omega \leq m + n_t^{UB} \tag{S40}$$

Upper bounds for n_t for a given high temperature experimental step can be calculated if step heats are long enough to assume steady state permeation, assuming G and K are known or can be conservatively estimated. To proceed, one must make the generally conservative assumption that the production rate of helium within the ampoule due to degassing of the encapsulated natural sample ($\Omega = \frac{\omega}{t}$) is constant over time at a given temperature. In reality, Ω will decrease over time for helium loss governed by first order processes (Yakubovich et al., 2010; Wilson and Bisson, 1973) or diffusion (except for the case of initially inhomogeneous distributions, the memory of which is often erased early in any diffusion experiment: Shuster et al., 2004). Eq. (S42), given below, shows that the amount of helium trapped in the tube (n_t) is proportional to the rate of helium outgassing from the natural encapsulated sample (Ω), so the approximation that this rate is constant will overestimate the amount of unanalyzed helium remaining in the ampoule after a high temperature experimental step. The rate of helium degassing over time will decrease for degassing controlled by second-order volume diffusion *except* for the minor case of the alpha-ejection effect at low He-release fractions (Farley et al., 1996; Ketcham et al., 2011) or for the more serious effects of

radiation damage annealing (Goldsmith et al., 2020) and mineral decomposition (Farley et al., 2024). In any case, sequential isothermal steps immediately reveal when $\frac{\omega}{t}$ increases over time.

A new first order differential equation like Eq. (S9) is formulated, now incorporating a constant source term (Ω) to conservatively approximate the helium influx into the ampoule from the degassing natural sample.

$$\frac{dn}{dt} = \Omega - \lambda n \tag{S41}$$

Where $\Omega = \frac{\omega}{t}$ and $\lambda = KGRT$. Immediately, the steady state quantity of helium atoms (n_{ss}) present in the ampoule can be found by solving Eq. (S41) for the steady state condition where $\frac{dn}{dt} = 0$.

$$n_{ss} = \frac{\Omega}{\lambda} = \frac{\omega}{\lambda t} \tag{S42}$$

Additionally, the helium concentration within the ampoule during the approach to the steady state concentration can be solved for by integrating Eq. (S41) with respect to *t*. First, the integrating factor for Eq. (S41) is identified: $I = e^{\lambda t}$, which is multiplied to both sides to yield Eq. (S43).

$$e^{\lambda t}\frac{dn}{dt} + e^{\lambda t}\lambda n = e^{\lambda t}\Omega \tag{S43}$$

Then both sides are integrated with respect to *t:*

$$\int \left(e^{\lambda t}\frac{dn}{dt} + e^{\lambda t}\lambda n \right) dt = \int e^{\lambda t}\Omega dt$$

Because $\frac{d}{dt}(ne^{\lambda t}) = e^{\lambda t}\frac{dn}{dt} + e^{\lambda t}\lambda n$ by the product rule Eq. (S43) reduces to:

$$n_t e^{\lambda t} = \frac{\Omega}{\lambda}e^{\lambda t} + C \tag{S44}$$

Where *C* is an unknown constant introduced by indefinite integration. This expression becomes more intuitive when both sides are divided by the integrating factor and by substituting the steady state concentration from Eq. (S42).

$$n_t = n_{ss} + Ce^{-\lambda t} \tag{S45}$$

The integration constant *C* can be solved by enforcing the condition that $n_t(t = 0) = n_0$, leading to:

$$n_0 = n_{ss} + C \tag{S46}$$

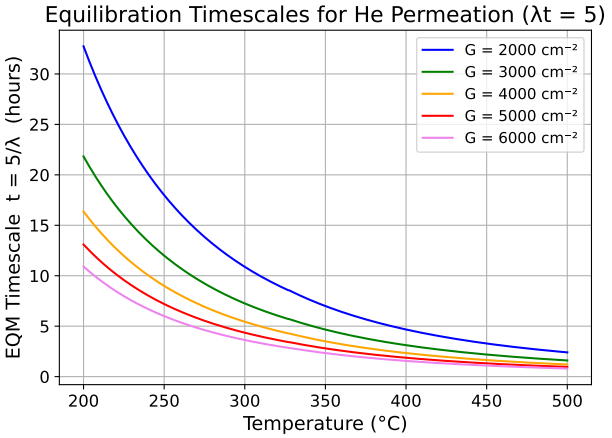


Figure S12. The upper limit of helium contents within the ampoule between high temperature experimental steps can be reasonably estimated without further measurement, provided permeative equilibrium has been reached. For typical ampoules with geometric factors between 3000 and 4000 cm^{-2}, this criterion is generally met for steps longer than 24 hours, or within 5 hours at 350°C or higher.

Solving Eq. (S46) for *C* and substituting into Eq. (S45) yields Eq. (S47). Now an inequality is assigned to the equation to reflect the initial assumption that the isothermal helium outgassing rate (Ω) is constant *or decreasing*.

$$n_t \leq n_{ss} + (n_0 - n_{ss})\, e^{-\lambda t} \tag{S47}$$

For long timescales (i.e. when $e^{-\lambda t} \approx 0$), Eq. (S47) reduces to $n_t \leq n_{ss}$. This is effectively true for steps long enough such that $t \geq \frac{5}{\lambda}$, for which $e^{-\lambda t} \leq 0.007$. It is advisable to only consider the bounding method for steps of sufficiently long duration such that $t \geq \frac{5}{\lambda}$ so that the estimation for n_t can be reduced to simply the steady state value and not be dependent upon the estimation for n_0 or its uncertainties. The timescales required to reach permeation equilibrium are plotted as a function of temperature in Fig. S12 below for some select values of *G*, the geometric factor.

To estimate the upper bound on the permeation lag (n_t^{UB}), one must consider the circumstances that would produce the highest possible value for n_t. In addition, the constraint that $t \geq \frac{5}{\lambda}$ is enforced so that previous heating steps are not significant, simplifying the problem significantly. Because n_t scales with ω by Eq. (S42), the upper bound estimate n_t^{UB} must assume the upper bound estimate for ω, which is given in Eq. (S40) as $m + n_t^{UB}$. Substituting $\omega^{UB} = m + n_t^{UB}$ into Eq. (S42) to express n_t^{UB} in terms of the measured value *m*:

$$n_t^{UB} = n_{ss}(\omega^{UB} = m + n_t^{UB}) = \frac{m + n_t^{UB}}{\lambda t}$$

Solving for n_t^{UB} yields Eq. (S48):

$$n_t^{UB} = \frac{m}{\lambda t - 1} \tag{S48}$$

The upper bound amount of helium-4 within the ampoule normalized to the measured value in percent at steady state permeation is plotted in main text Fig. S18 using Eq. (S48) $\left(\frac{n_t^{UB}}{m} = \frac{1}{\lambda t - 1}\right)$, assuming a standard tube where G = 4350.26 cm^{-2} and the permeability values given in Swets et al. (1961). Main text Fig. S18 shows that, in order to push this uncertainty to be less than 5%, even very hot steps require long step durations. For a 5% uncertainty using this method, a 10-hour step duration is required even at 400°C. Much longer durations are required for the same precision at lower temperatures: at 250°C, a step duration of 35 hours is required to push the uncertainty beneath 5%.

S6 Comparison to Literature Permeability Values

Predicted and measured fractional yields for all permeation steps in ampoules besides the encapsulated water experiment agree well (within 1σ: Figs. S19, S14) with the predictive equations presented in this work and with the permeabilities reported by Swets et al. (1961) and Jones (1953) for all studied temperatures (24-300°C; Fig. S13) and step fractional yields (up to ~80%). One outlier measurement on the empty tube experiment on the Helix-MC-Plus^{10K} multi-collector mass spectrometer was excluded from Figs. S19 and S14.

Permeation ratios for 3He and 4He measured in the empty tube experiment on the Helix-MC-Plus^{10K} multi-collector mass spectrometer are plotted in Fig. S15. These data present significant scatter, but generally agree with the reported results of Jones (1953), except for measurements at room temperature, which cluster tightly at a permeation ratio of 1:1 for the two isotopes. Additionally, fields corresponding to the ratios of apparent permeabilities for the water-filled and sulfur-filled experiments are plotted for the temperature ranges of those experiments. Results for those experiments are plotted as fields because each step integrated permeation behavior over a complex (non-isothermal) cooling history. These experiments also agree with the results of Jones (1953) and the empty ampoule experiment. The qualitative result of Jones (1953) that silica glass is only slightly more permeable for 3He than 4He is supported by these data, which are in marked contrast to the reported extreme differences in 3He and 4He diffusivity in silica glass of McMurtry et al. (2019), who report instantaneous isotopic fractionations up to a factor of 1000.

S7 Additional Analytical Corrections for the Empty Ampoule Calibration Experiments

S7.1 Anomalous Signal Recalculation for the Tank Helium-Soaked Empty Ampoule

The last high temperature step of the empty ampoule experiment on the Helix-MC-Plus^{10K} multi-collector mass spectrometer had an unusual and non-linear signal evolution at the beginning of the measurement for both 3He and 4He. For this measurement, 4He was recalculated using a linear regression on the last three of six measurement cycles with an R^2 of 0.985 to regress to the 4He content at time 0. Typically, the signal evolution for a measurement like this would have a negative slope because the

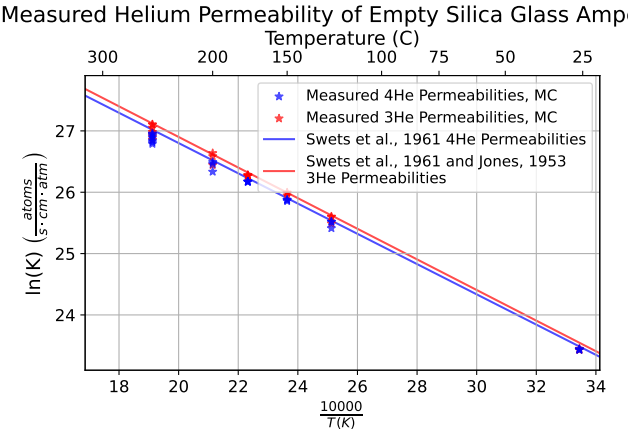


Figure S13. Helium permeabilities measured in an empty silica glass ampoule at Caltech on a Helix-MC-Plus^{10K} multi-collector mass spectrometer (both 3He and 4He) are compared to literature values. Permeabilities of 3He and 4He are very similar, but 3He permeates slightly faster. The final measurement on the Helix-MC-Plus^{10K} mass spectrometer is an outlier and is excluded from the plot, as it is most sensitive to the value of the total yield remaining in the ampoule. This experiment on an empty tube at Caltech shows excellent agreement with the literature values with allowance for some scatter. This result shows that existing understanding of helium permeability in glass can be reasonably leveraged for use in helium step heats of silica glass encapsulated geological samples. Literature 4He permeabilities are taken from Swets et al. (1961); whereas 3He permeabilities from the literature are calculated by multiplying the 3He/4He permeability ratios of Jones (1953) with the 4He permeabilities of Swets et al. (1961).

helium in the mass spectrometer is consumed as it is ionized and measured, but the slope for this measurement was positive. 3He from this measurement was calculated based on the recalculated 4He and an assumed isotope ratio for the measurement of 0.07 Ra. Three more measurements were taken over the next few days to ensure complete degassing of the ampoule. Two of these measurements yielded helium above blank, but were small compared to the final high temperature step. The yields of these steps were all considered in the calculation of the experiment's total yield.

S7.2 Independent Verification of the Encapsulated Durango Apatite Mass

The total yield for the encapsulated Durango apatite experiment (main text, §3.3) is estimated from the precisely-measured mass of the encapsulated apatite (3.18 mg) and a helium concentration of 194.2 nccSTP/mg (Farley, 2000). This concentration is independently supported by the measurement of 8 different >0.5 mg aliquots of the same Durango apatite sample in-lab, which yield a concentration of 194 ± 9 nccSTP/mg.

S8 Additional Figures and Tables Referenced in the Main Text

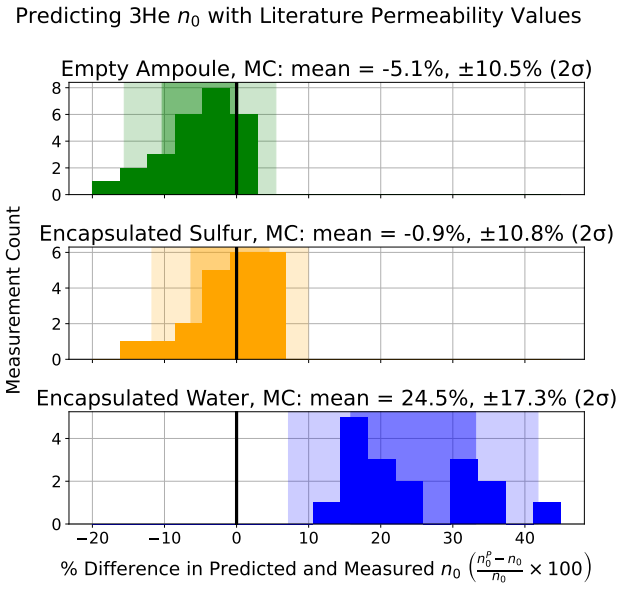


Figure S14. Similar to Fig. S19, but with 3He permeabilities taken from Jones (1953) and Swets et al. (1961). Shaded regions behind the histograms correspond to 1 and 2 sigma (σ) from the average relative difference between the predicted and measured values. The 3He permeation model and literature permeability values apply well to empty and sulfur-filled ampoules, and such models can be used to reliably recover 3He contents of permeating ampoules for use in permeation lag corrections. On the other hand, measured and predicted values of 3He n_0 for water-filled ampoules are well resolved beyond 2σ, suggesting that their permeability differs strongly from the literature values. Internal reproducibilities (1σ) of a gas standard repeatedly analyzed during these experiments were better than 3% for 3He, requiring that much of the scatter in these data be related to factors outside of analytical precision such as long/inconsistent ramp times during heating or uncertainties or rounding of heating times.

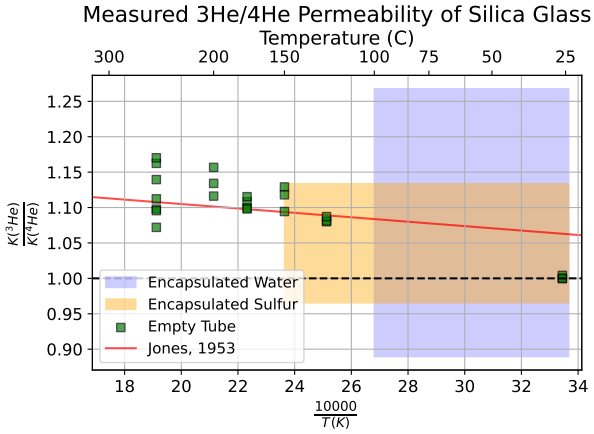


Figure S15. Ratios of calculated permeabilities from step heat experiments on silica glass ampoules on the Helix-MC-Plus^{10K} mass spectrometer at Caltech. The last measurement on the empty tube experiment is an outlier and was excluded from the plot. Experiments on encapsulated water and encapsulated sulfur were allowed to cool before isotopic measurements. Because of slow cooling rates, simple corrections could not be applied to these two experiments, which effectively queried permeabilities at a range of temperatures within a single step. Therefore, the ratios of their apparent permeabilities are plotted as a field with 2σ standard deviation across the experimental temperature range. These three experiments show general, albeit imprecise, agreement with the results of Jones (1953), except for the measurements at room temperature. Jones (1953) was likely able to measure the relative permeabilities of 4He and 3He with much higher precision because his experimental vessel was charged with 3He at a partial pressure of around 0.5 atmospheres, over one billion times higher than the 3He partial pressure within the fused silica ampoule used in this work. Interestingly, three room-temperature measurements of helium permeation of an empty tube at Caltech yielded essentially identical permeability of 3He and 4He.

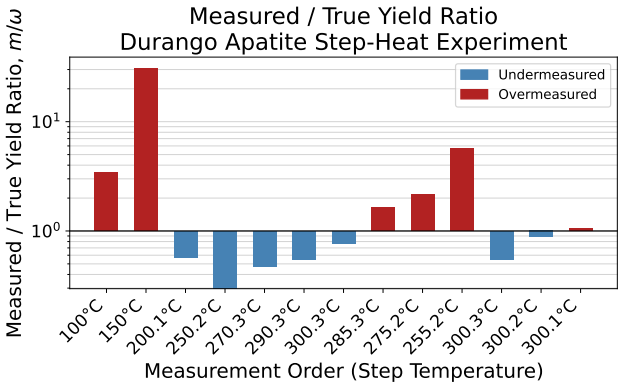


Figure S16. Measured-to-true yield ratio, m/ω, for the first 13 experimental steps (through the isothermal 300°C triplicate) of the real encapsulated Durango apatite step heat experiment described above (§3) and tabulated in full in Table S3, plotted in measurement order and labeled by nominal step temperature. Here m is the raw measured helium yield for a step and ω is its permeation lag-corrected yield; bars are anchored at a ratio of 1 (no anomaly) on a logarithmic axis, so a doubling and a halving of the ratio are given equal visual weight. Steps taken while ramping to higher temperatures are generally undermeasured (blue), as some of the sample's evolved helium has not yet fully permeated out of the tube at the time of measurement, while steps taken while ramping to lower temperatures are generally overmeasured (red), as helium retained in the tube from earlier, hotter steps continues to permeate out. The first two steps (100-150°C) are strongly overmeasured despite being on the heating ramp because little helium had yet evolved from the apatite, so measured yield there is dominated by pre-existing atmospheric helium draining from the tube rather than fresh sample degassing.

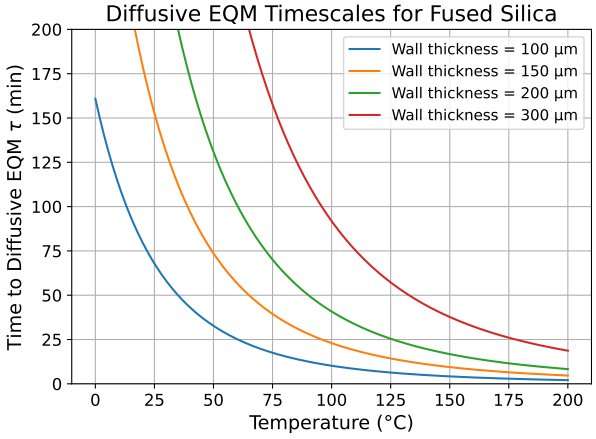


Figure S17. Timescales as a function of temperature to reestablish a steady state diffusive concentration profile for different glass thicknesses. These curves correspond to the timescales at which the Fourier number equals 1. 4He diffusivities are taken from Swets et al. (1961).

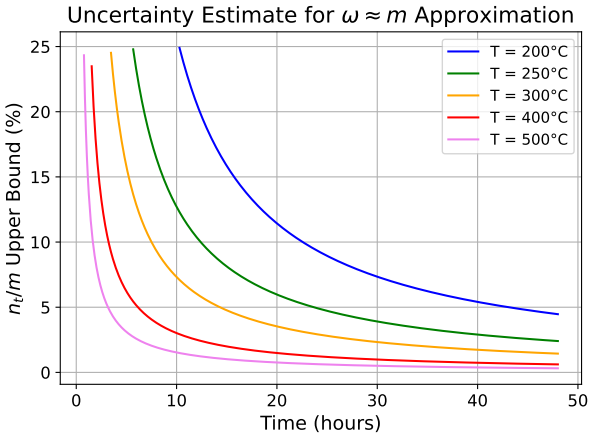


Figure S18. For long steps and high temperatures, the abundance of helium within the ampoule will reach a steady state and will be constant as the measurable helium outside the ampoule in the lamp cell increases. As the step gets longer, this amount becomes small relative to the amount of measurable helium, and the measurable helium can be used to approximate the total amount of degassed helium with only minor inaccuracy. Eq. (7) is plotted here to show the upper bound relative amount of helium trapped within the ampoule normalized to the measurable amount. The geometric factor for these calculations is 4350 cm^{-2}, corresponding to an ampoule with an inner and outer diameter of 0.6 and 1 mm respectively. Permeability values (K) are for 4He in silica glass and are taken from Swets et al. (1961).

Table S2. In-situ permeation rate constants of the empty ampoule, fit to consecutive isothermal permeation steps with Eq. (6) (written in mass-balance form). The first steps of the 125 and 200 °C runs are excluded (see main text and Fig. S20), leaving exactly determined two-step fits. The last two 250 °C accumulations (steps 28–29), which permeate anomalously fast in both isotopes just before the anomalous final measurement, are also excluded. n_0 (true) is known independently from the experiment's total yield and is not used in the fits. λ_{pred} is predicted from the measured ampoule geometry and literature permeabilities (Swets et al., 1961; Jones, 1953) and is shown only as a check. Uncertainties are 1σ from the fit covariance.

Isotope	T (°C)	Steps	λ (10^{-5} s^{-1})	$\lambda/\lambda_{\mathrm{pred}}$	n_0 fit / true	λt_{cum}	$\lambda(^3\mathrm{He})/\lambda(^4\mathrm{He})$
^{4}He	125	2 (8–9)	2.063 ± 0.235	0.945	1.036	0.13	
^{3}He	125	2 (8–9)	2.075 ± 0.472	0.873	1.110	0.13	1.006 ± 0.256
^{4}He	150	3 (11–13)	3.110 ± 0.074	0.930	1.033	0.40	
^{3}He	150	3 (11–13)	3.525 ± 0.139	0.964	1.014	0.45	1.133 ± 0.052
^{4}He	175	4 (14–17)	4.662 ± 0.040	0.951	0.999	0.59	
^{3}He	175	4 (14–17)	5.273 ± 0.108	0.980	0.981	0.67	1.131 ± 0.025
^{4}He	200	2 (20–21)	5.825 ± 0.063	0.841	1.122	0.44	
^{3}He	200	2 (20–21)	6.277 ± 0.392	0.823	1.167	0.48	1.078 ± 0.068
^{4}He	250	6 (22–27)	12.216 ± 0.013	0.969	0.996	2.33	
^{3}He	250	6 (22–27)	14.233 ± 0.137	1.020	0.986	2.72	1.165 ± 0.011

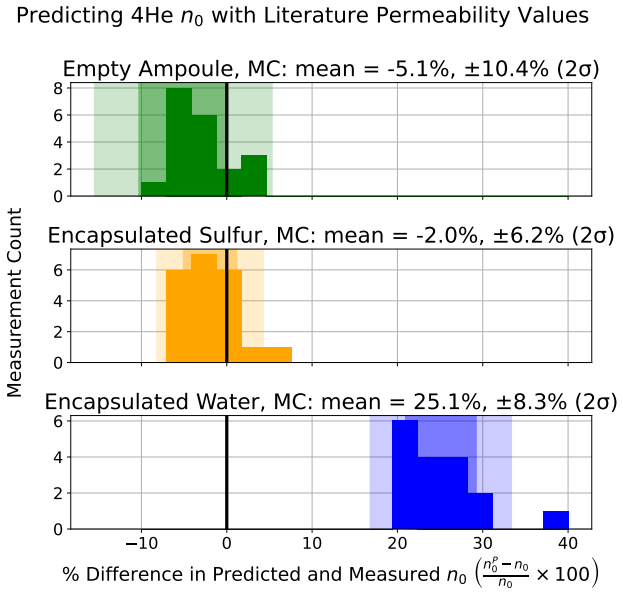
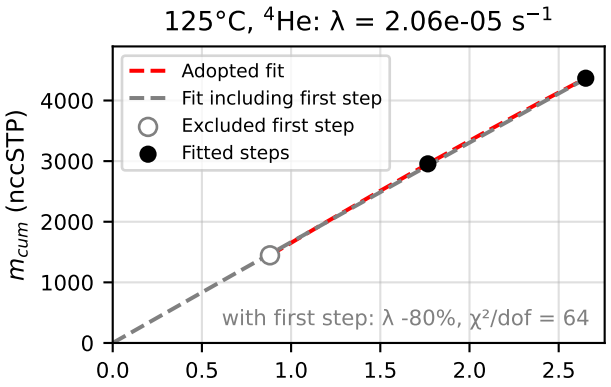
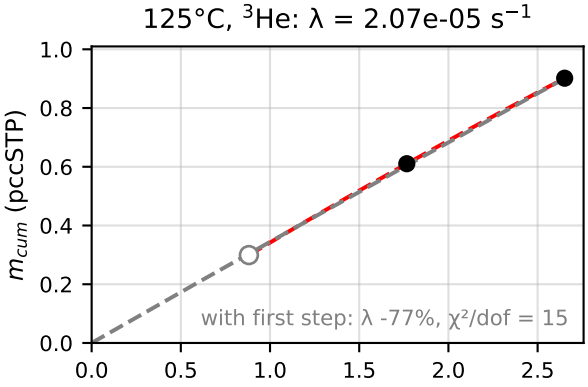
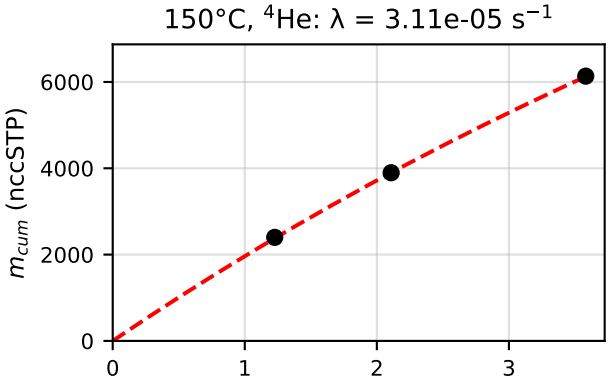
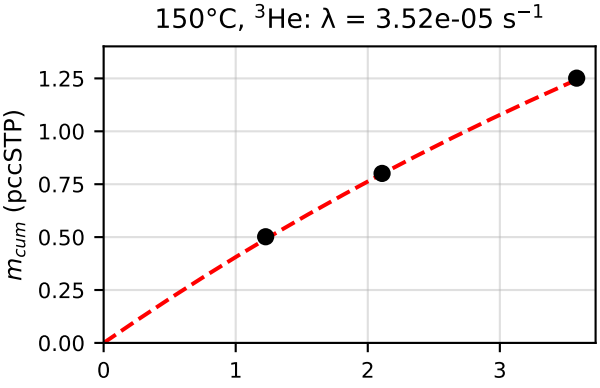



Figure S19. Histograms showing the accuracy of 4He n_0 predictions using permeabilities of Swets et al. (1961) from either Eq. (S12) or a numerical diffusion model from the measured value, with shaded regions behind the histograms corresponding to 1 and 2 sigma (σ) from the average relative difference between measured and predicted values. The measured n_0 values of the empty and sulfur-filled ampoules are within 1σ of the predicted values, suggesting that the permeation model and literature values apply well to those systems, and such models can be used to reliably recover helium contents of permeating ampoules for use in permeation lag corrections. On the other hand, measured and predicted 4He n_0 for water-filled ampoules are well resolved beyond 2σ, suggesting that their helium permeability differs strongly from the literature values. Internal reproducibilities (1σ) of a gas standard repeatedly analyzed during these experiments were better than 1% for 4He, requiring that most of the scatter in these data be related to factors outside of analytical precision, such as long/inconsistent ramp times during heating or uncertainties or rounding of heating times.



125°C, ^{4}He: λ = 2.06e-05 s^{-1}
Adopted fit
Fit including first step
Excluded first step
Fitted steps
m_{cum} (nccSTP)
with first step: λ -80%, χ²/dof = 64



125°C, ^{3}He: λ = 2.07e-05 s^{-1}
m_{cum} (pccSTP)
with first step: λ -77%, χ²/dof = 15


150°C, ^{4}He: λ = 3.11e-05 s^{-1}
m_{cum} (nccSTP)


150°C, ^{3}He: λ = 3.52e-05 s^{-1}
m_{cum} (pccSTP)

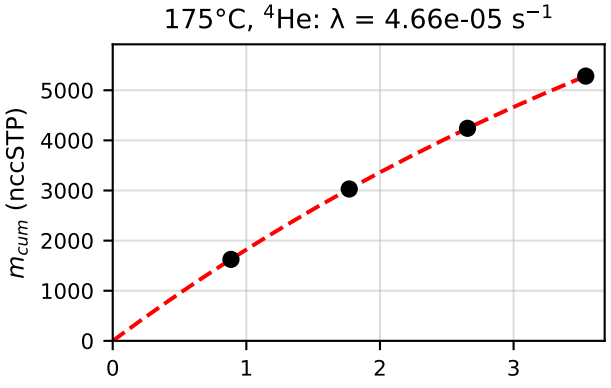
175°C, ^{4}He: λ = 4.66e-05 s^{-1}
m_{cum} (nccSTP)

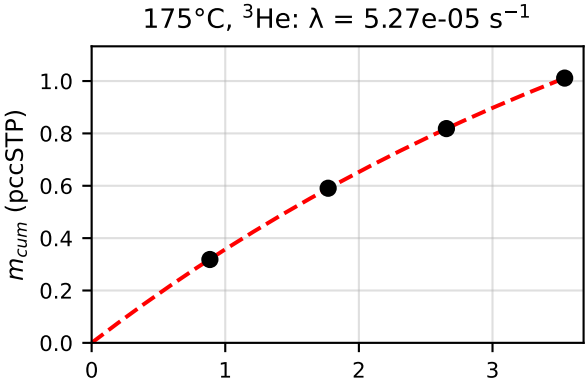
175°C, ^{3}He: λ = 5.27e-05 s^{-1}
m_{cum} (pccSTP)

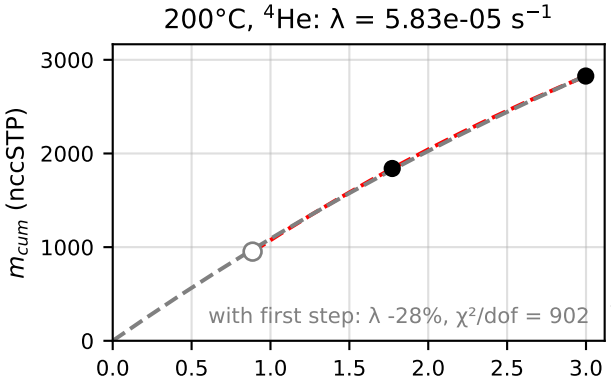
200°C, ^{4}He: λ = 5.83e-05 s^{-1}
m_{cum} (nccSTP)
with first step: λ -28%, χ²/dof = 902

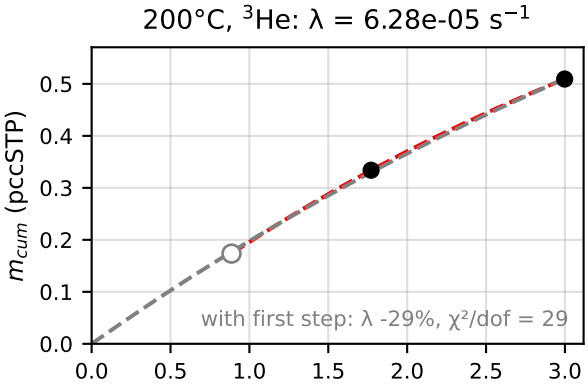

200°C, ^{3}He: λ = 6.28e-05 s^{-1}
m_{cum} (pccSTP)
with first step: λ -29%, χ²/dof = 29

Table S3: Step heat data for the silica glass encapsulated Durango apatite experiment. $^{He}F_{Apatite}$ is the permeation lag-corrected cumulative fractional yield of helium released from the apatite. n_0 values (initial ^{4}He content of the ampoule, Eq. (4)) are shown in **bold** for permeation steps used directly to solve for n_0, and in *italics* for all other steps, where n_0 is instead propagated forward or backward in time from the nearest bolded permeation step using Eq. (1). Blank "Type" entries denote room-temperature measurements preceding the permeation step used to solve for n_0, taken before the diffusive steady state concentration profile was reestablished (see text). Uncertainties are 2σ. Corrected $\ln(D/a^2)$ values shown as "–" correspond to steps where the corrected apatite yield (ω) was within 2σ of 0 and were excluded from the Arrhenius plot (Fig. 3).

Type	Time (min)	Temp. (°C)	m (nccSTP ^{4}He)	n_0 (nccSTP ^{4}He)	ω (nccSTP ^{4}He)	$^{He}F_{Apatite}$	Corrected $\ln(D/a^2)$	Uncorrected $\ln(D/a^2)$
Permeation	15	24.3	0.00704 ± 0.00046	**1.48 ± 0.18**				
Experimental	240	100.0	0.1700 ± 0.0011	*1.47 ± 0.18*	0.05 ± 0.24	0.00803%	–	-28.39
	15	28.0	0.00721 ± 0.00039	*1.35 ± 0.16*				
	15	24.0	0.00639 ± 0.00039	*1.34 ± 0.16*				
Permeation	15	24.0	0.00630 ± 0.00039	**1.34 ± 0.16**				
Experimental	240	150.0	0.3090 ± 0.0023	*1.33 ± 0.16*	0.01 ± 0.21	0.00983%	–	-26.98
	15	28.1	0.00542 ± 0.00039	*1.03 ± 0.13*				
	15	24.3	0.00484 ± 0.00039	*1.03 ± 0.13*				
Permeation	15	24.2	0.00485 ± 0.00039	**1.02 ± 0.13**				
Experimental	240	200.1	0.9416 ± 0.0085	*1.02 ± 0.13*	1.64 ± 0.23	0.276%	-23.80 ± 0.28	-25.02
	15	29.9	0.00947 ± 0.00041	*1.72 ± 0.19*				
	15	23.8	0.00786 ± 0.00040	*1.71 ± 0.19*				
Permeation	15	24.0	0.00804 ± 0.00040	**1.70 ± 0.19**				
Experimental	60	250.2	1.097 ± 0.011	*1.69 ± 0.19*	3.70 ± 0.48	0.874%	-20.21 ± 0.20	-24.01
	15	33.0	0.02653 ± 0.00050	*4.30 ± 0.44*				
	15	23.5	0.02016 ± 0.00046	*4.27 ± 0.44*				
Permeation	15	24.0	0.02003 ± 0.00047	**4.25 ± 0.44**				
Experimental	60	270.3	2.508 ± 0.027	*4.23 ± 0.44*	5.26 ± 0.83	1.73%	-19.04 ± 0.22	-22.51
	15	33.9	0.04414 ± 0.00067	*6.98 ± 0.70*				
Permeation	15	23.6	0.03246 ± 0.00057	**6.93 ± 0.70**				
Experimental	60	290.3	4.979 ± 0.058	*6.90 ± 0.70*	9.0 ± 1.3	3.18%	-17.87 ± 0.20	-21.10
	15	33.6	0.06816 ± 0.00095	*10.9 ± 1.1*				
Permeation	15	23.6	0.05050 ± 0.00078	**10.8 ± 1.1**				
Experimental	60	300.3	7.243 ± 0.091	*10.8 ± 1.1*	9.5 ± 1.7	4.72%	-17.34 ± 0.25	-20.07
	15	34.2	0.0843 ± 0.0012	*13.1 ± 1.3*				

continued on next page

(continued)

Type	Time (min)	Temp. (°C)	m (nccSTP ^{4}He)	n_0 (nccSTP ^{4}He)	ω (nccSTP ^{4}He)	$^{He}F_{Apatite}$	Corrected $\ln(D/a^2)$	Uncorrected $\ln(D/a^2)$
	15	23.5	0.06160 ± 0.00094	*13.0 ± 1.3*				
Permeation	15	24.1	0.06097 ± 0.00095	**12.9 ± 1.3**				
Experimental	60	285.3	5.919 ± 0.080	*12.9 ± 1.3*	3.6 ± 1.7	5.30%	-18.04 ± 0.71	-20.65
	15	36.8	0.0729 ± 0.0011	*10.5 ± 1.1*				
Permeation	15	23.6	0.04846 ± 0.00084	**10.4 ± 1.1**				
Experimental	80	275.2	5.382 ± 0.077	*10.4 ± 1.1*	2.5 ± 1.3	5.71%	-18.6 ± 1.1	-19.80
	15	37.0	0.05243 ± 0.00092	*7.53 ± 0.76*				
Permeation	15	23.6	0.03487 ± 0.00070	**7.48 ± 0.76**				
Experimental	100	255.2	3.382 ± 0.052	*7.44 ± 0.76*	0.60 ± 0.90	5.81%	–	-20.22
	15	37.1	0.03206 ± 0.00069	*4.66 ± 0.48*				
Permeation	15	23.6	0.02147 ± 0.00056	**4.63 ± 0.48**				
Experimental	60	300.3	3.684 ± 0.059	*4.61 ± 0.48*	6.68 ± 0.91	6.89%	-17.17 ± 0.20	-20.76
	15	36.3	0.0518 ± 0.0010	*7.60 ± 0.77*				
Permeation	15	23.6	0.03513 ± 0.00077	**7.55 ± 0.77**				
Experimental	120	300.2	9.78 ± 0.17	*7.51 ± 0.77*	11.1 ± 1.2	8.69%	-17.13 ± 0.22	-19.21
	15	35.7	0.0595 ± 0.0012	*8.85 ± 0.90*				
Permeation	15	23.6	0.04087 ± 0.00089	**8.79 ± 0.90**				
Experimental	180	300.1	14.58 ± 0.27	*8.75 ± 0.90*	13.8 ± 1.2	10.9%	-17.08 ± 0.18	-18.75
	15	35.9	0.0547 ± 0.0012	*7.96 ± 0.81*				
Permeation	15	23.6	0.03782 ± 0.00089	**7.91 ± 0.81**				
Experimental	60	320.3	7.49 ± 0.14	*7.87 ± 0.81*	11.4 ± 1.5	12.8%	-15.96 ± 0.18	-17.94
	15	36.9	0.0813 ± 0.0017	*11.7 ± 1.2*				
Permeation	15	23.5	0.0541 ± 0.0012	**11.7 ± 1.2**				
Experimental	60	330.4	11.18 ± 0.22	*11.6 ± 1.2*	14.5 ± 1.9	15.1%	-15.54 ± 0.21	-18.08
	15	37.4	0.1076 ± 0.0023	*14.9 ± 1.5*				
Permeation	15	23.7	0.0691 ± 0.0016	**14.8 ± 1.5**				
Experimental	60	350.4	19.78 ± 0.41	*14.7 ± 1.5*	28.3 ± 2.8	19.7%	-14.61 ± 0.15	-18.11
	15	37.0	0.1615 ± 0.0035	*23.3 ± 2.4*				
Permeation	15	23.5	0.1071 ± 0.0024	**23.1 ± 2.4**				
Experimental	60	370.4	32.97 ± 0.71	*23.0 ± 2.4*	41.3 ± 4.0	26.4%	-13.90 ± 0.15	-16.15
	15	37.3	0.2207 ± 0.0049	*31.4 ± 3.2*				
Permeation	15	23.5	0.1447 ± 0.0033	**31.1 ± 3.2**				

continued on next page

(continued)

Type	Time (min)	Temp. (°C)	m (nccSTP ^{4}He)	n_0 (nccSTP ^{4}He)	ω (nccSTP ^{4}He)	$^{He}F_{Apatite}$	Corrected $\ln(D/a^2)$	Uncorrected $\ln(D/a^2)$
Experimental	60	385.4	42.32 ± 0.94	*31.0 ± 3.2*	44.8 ± 4.8	33.6%	-13.48 ± 0.17	-15.41
	15	37.8	0.2393 ± 0.0055	*33.5 ± 3.4*				
Permeation	15	23.5	0.1548 ± 0.0037	**33.2 ± 3.4**				
Experimental	60	360.4	27.53 ± 0.64	*33.1 ± 3.4*	15.3 ± 4.1	36.1%	-14.35 ± 0.51	-15.33
	15	39.6	0.1620 ± 0.0039	*20.9 ± 2.1*				
Permeation	15	23.6	0.0963 ± 0.0024	**20.7 ± 2.1**				
Experimental	60	340.4	14.78 ± 0.35	*20.6 ± 2.1*	7.4 ± 2.6	37.3%	-15.00 ± 0.90	-15.63
	15	40.0	0.1029 ± 0.0026	*13.2 ± 1.4*				
Permeation	15	23.5	0.0610 ± 0.0017	**13.1 ± 1.4**				
Experimental	100	325.2	12.37 ± 0.31	*13.1 ± 1.4*	6.8 ± 1.6	38.4%	-15.6 ± 1.1	-13.69
	15	40.1	0.0589 ± 0.0017	*7.50 ± 0.78*				
Permeation	15	24.0	0.0351 ± 0.0011	**7.44 ± 0.78**				
Experimental	240	400.1	101.1 ± 2.7	*7.40 ± 0.78*	110.0 ± 3.2	56.2%	-13.281 ± 0.076	-13.70
	15	34.9	0.1096 ± 0.0031	*16.3 ± 1.7*				
Permeation	15	23.8	0.0757 ± 0.0022	**16.2 ± 1.7**				
Experimental	90	350.3	14.88 ± 0.41	*16.1 ± 1.7*	5.8 ± 1.9	57.2%	-14.92 ± 0.92	-15.42
	15	39.5	0.0567 ± 0.0017	*7.06 ± 0.74*				
Permeation	15	24.0	0.0330 ± 0.0011	**7.00 ± 0.74**				
Experimental	60	400.4	14.21 ± 0.40	*6.97 ± 0.74*	18.1 ± 1.4	60.1%	-13.31 ± 0.31	-15.50
	15	40.4	0.0866 ± 0.0026	*10.9 ± 1.1*				
Permeation	15	24.0	0.0508 ± 0.0016	**10.8 ± 1.1**				
Experimental	120	300.2	7.65 ± 0.22	*10.7 ± 1.1*	0.7 ± 1.2	60.2%	–	-16.50
	15	39.4	0.0291 ± 0.0011	*3.79 ± 0.41*				
Permeation	15	23.7	0.01758 ± 0.00077	**3.76 ± 0.41**				

S9 Supplementary Data Tables

The following tables present the reduced step-by-step helium permeation data underlying the empty-tube, encapsulated-water, and encapsulated-sulfur calibration experiments summarized in Table S1 and the permeability/isotope-ratio comparison figures above. *m* is the measured helium abundance of the step; n_0 and n_t are the helium contents of the ampoule at the beginning and end of the step (Eq. (S10)); n_t/n_0 predicted and measured are the fractional yields expected from the permeability of Swets et al. (1961) (and, for 3He, the isotope ratios of Jones (1953)) and as measured, respectively.

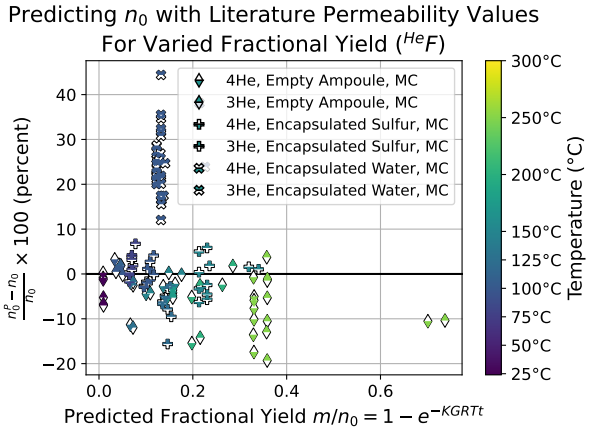


Figure S21. Helium measurements (m) of a permeating ampoule are related to the initial helium contents of the ampoule (n_0) by Eq. (S12), using permeability values taken from Swets et al. (1961) and Jones (1953) (for 3He only). The n_0^P variable is the predicted value of n_0, the true value. For the empty ampoule, except for 3 measurements on the Helix-MC-Plus^{10K}, predicted values (n_0^P) are calculated using Eq. (S10). For the encapsulated sulfur and water ampoules, as well as 3 measurements of the blank ampoule on the Helix-MC-Plus^{10K}, predicted values (n_0^P) were determined by forward modeling diffusion and permeation on ampoules as they were held at high temperature and subsequently allowed to cool (see main text for details). This plot shows that the predicted values are correct to within ~10% for empty and sulfur-filled ampoules regardless of temperature or extent of permeation, whereas n_0^P values for water-filled ampoules are systematically high. The final Helix-MC-Plus^{10K} measurement on the empty ampoule yields an outlier n_0^P that was ~80% high — this measurement is not plotted here.

Table S4. Distilled 3He permeation data for the empty silica glass ampoule equilibrated with high-purity tank helium, measured on the Helix-MC-Plus[10K] multi-collector mass spectrometer ("Empty Tube, Helix MC" in Table S1). Rows marked '–' in the predicted and measured n_t/n_0 and permeability columns are cooling-only intervals for which no isothermal permeability was calculated (see main text).

Temp (°C)	Time (min)	*m* 3He (pccSTP)	$\pm 2\sigma$ (pccSTP)	n_0 3He (pccSTP)	n_t 3He (pccSTP)	n_t/n_0 predicted	n_t/n_0 measured	3He *K* measured ($\frac{atoms}{scm\,atm}$)
26	73.6	0.05159	0.00062	5.787	5.736	0.9902	0.9911	1.53×10^{10}
–	113.3	0.2689	0.0039	5.736	5.467			
26	73.7	0.04801	0.00085	5.467	5.419	0.9902	0.9912	1.50×10^{10}
26	75.3	0.04855	0.00099	5.419	5.370	0.9900	0.9910	1.50×10^{10}
–	112.9	0.2709	0.0057	5.370	5.099			
–	126.6	0.4175	0.0088	5.099	4.682			
125	52.9	0.2993	0.0063	4.682	4.382	0.9275	0.9361	1.18×10^{11}
125	53.1	0.3111	0.0066	4.382	4.071	0.9273	0.9290	1.31×10^{11}
125	53.1	0.2912	0.0062	4.071	3.780	0.9273	0.9285	1.32×10^{11}
–	73.6	0.4224	0.0087	3.780	3.358			
150	73.6	0.5017	0.0086	3.358	2.856	0.8512	0.8506	1.95×10^{11}
150	52.9	0.2993	0.0045	2.856	2.557	0.8907	0.8952	1.86×10^{11}
150	88.4	0.4502	0.0063	2.557	2.107	0.8240	0.8240	1.94×10^{11}
175	53.1	0.3184	0.0046	2.107	1.788	0.8427	0.8489	2.59×10^{11}
175	53.1	0.2722	0.0040	1.788	1.516	0.8427	0.8478	2.61×10^{11}
175	53.1	0.2278	0.0035	1.516	1.288	0.8427	0.8498	2.57×10^{11}
175	53.1	0.1929	0.0032	1.288	1.095	0.8427	0.8504	2.56×10^{11}
–	53.1	0.1635	0.0028	1.095	0.9317			
200	53.2	0.1735	0.0032	0.9317	0.7582	0.7843	0.8139	3.07×10^{11}
200	53.1	0.1604	0.0032	0.7582	0.5978	0.7847	0.7887	3.55×10^{11}
200	73.6	0.1754	0.0038	0.5978	0.4224	0.7146	0.7070	3.75×10^{11}
250	53.2	0.1521	0.0039	0.4224	0.2704	0.6410	0.6406	6.02×10^{11}
250	53.1	0.0977	0.0030	0.2704	0.1727	0.6413	0.6396	6.06×10^{11}
250	53.1	0.0607	0.0021	0.1727	0.1119	0.6413	0.6499	5.85×10^{11}
250	53.1	0.0379	0.0016	0.1119	0.07407	0.6414	0.6639	5.58×10^{11}
250	52.9	0.0249	0.0011	0.07407	0.04914	0.6427	0.6634	5.57×10^{11}
250	53.1	0.01599	0.00077	0.04914	0.03315	0.6415	0.6746	5.32×10^{11}
250	159.9	0.0260	0.0013	0.03315	0.007191	0.2625	0.2169	6.86×10^{11}

Temp (°C)	Time (min)	*m* 3He (pccSTP)	$\pm 2\sigma$ (pccSTP)	n_0 3He (pccSTP)	n_t 3He (pccSTP)	n_t/n_0 predicted	n_t/n_0 measured	3He *K* measured ($\frac{atoms}{s\,cm\,atm}$)
250	52.9	0.00494	0.00025	0.007191	0.002250	0.6424	0.3129	1.58×10^{12}
High T	52.2	0.00225		0.002250	0			

Table S5: Distilled 4He permeation data for the same empty silica glass ampoule experiment as Table S4. K_3/K_4 is the ratio of the measured 3He to 4He permeability coefficients for each step; 3He/4He measured (Ra) is the measured 3He/4He ratio of the step, normalized to the atmospheric ratio.

Temp	Time	*m* 4He	$\pm 2\sigma$	n_0 4He	n_t 4He	n_t/n_0 predicted	n_t/n_0 measured	4He *K* measured	K_3/K_4	3He/4He measured (Ra)
(°C)	(min)	(nccSTP)	(nccSTP)	(nccSTP)	(nccSTP)			$(\frac{atoms}{s\,cm\,atm})$		
26	73.6	263.7	1.3	29670	29410	0.9908	0.9911	1.52×10^{10}	1.0031	0.1408
–	113.3	1282.4	8.0	29410	28130					0.1509
26	73.7	247.4	2.0	28130	27880	0.9908	0.9912	1.51×10^{10}	0.9984	0.1396
26	75.3	250.0	2.3	27880	27630	0.9905	0.9910	1.50×10^{10}	0.9990	0.1397
–	112.9	1322	13	27630	26310					0.1475
–	126.6	1971	20	26310	24340					0.1524
125	52.9	1446	15	24340	22890	0.9332	0.9406	1.09×10^{11}	1.0786	0.1489
125	53.1	1509	16	22890	21380	0.9330	0.9341	1.21×10^{11}	1.0795	0.1483
125	53.1	1413	15	21380	19970	0.9330	0.9339	1.21×10^{11}	1.0856	0.1483
–	73.6	2032	21	19970	17940					0.1495
150	73.6	2399	22	17940	15540	0.8630	0.8663	1.73×10^{11}	1.1271	0.1505
150	52.9	1498	13	15540	14040	0.8996	0.9036	1.70×10^{11}	1.0922	0.1438
150	88.4	2238	17	14040	11800	0.8377	0.8406	1.74×10^{11}	1.1155	0.1447
175	53.1	1626	11	11800	10170	0.8556	0.8622	2.34×10^{11}	1.1053	0.1409
175	53.1	1404.1	8.5	10170	8771	0.8556	0.8620	2.34×10^{11}	1.1121	0.1395
175	53.1	1210.8	6.3	8771	7560	0.8556	0.8619	2.34×10^{11}	1.0959	0.1353
175	53.1	1041.8	4.8	7560	6518	0.8556	0.8622	2.34×10^{11}	1.0939	0.1332
–	53.1	895.4	3.7	6518	5623					0.1314
200	53.2	952.2	3.4	5623	4670	0.8020	0.8306	2.77×10^{11}	1.1107	0.1311
200	53.1	887.5	3.0	4670	3783	0.8023	0.8100	3.15×10^{11}	1.1275	0.1300
200	73.6	987.1	3.3	3783	2796	0.7370	0.7391	3.26×10^{11}	1.1485	0.1278
250	53.2	898.0	3.0	2796	1898	0.6693	0.6788	5.23×10^{11}	1.1520	0.1218
250	53.1	609.8	2.1	1898	1288	0.6696	0.6787	5.24×10^{11}	1.1569	0.1153
250	53.1	412.2	1.4	1288	875.7	0.6696	0.6799	5.21×10^{11}	1.1231	0.1059
250	53.1	278.75	1.00	875.7	596.9	0.6697	0.6817	5.18×10^{11}	1.0778	0.0978
250	52.9	187.74	0.69	596.9	409.2	0.6709	0.6855	5.13×10^{11}	1.0868	0.0955
250	53.1	128.81	0.49	409.2	280.4	0.6697	0.6852	5.11×10^{11}	1.0411	0.0893
250	159.9	215.41	0.95	280.4	64.98	0.2990	0.2318	6.56×10^{11}	1.0452	0.0867

continued on next page

(continued)

Temp (°C)	Time (min)	*m* 4He (nccSTP)	$\pm 2\sigma$ (nccSTP)	n_0 4He (nccSTP)	n_t 4He (nccSTP)	n_t/n_0 predicted	n_t/n_0 measured	4He *K* measured ($\frac{atoms}{s\,cm\,atm}$)	K_3/K_4	3He/4He measured (Ra)
250	52.9	41.86	0.20	64.98	23.12	0.6706	0.3558	1.40×10^{12}	1.1246	0.0849
High T	52.2	23.12		23.12	0					0.0700

Table S6. Distilled 3He isothermal permeation data for the silica glass ampoule containing distilled water, equilibrated with high-purity tank helium, measured on the Helix-MC-Plus^{10K} multi-collector mass spectrometer ("Encapsulated Water, Helix MC" in Table S1). Predicted n_t/n_0 values marked '–' correspond to steps for which the ampoule had not yet reached a diffusive steady state concentration profile (see main text).

Temp (°C)	Hot Time (min)	Cold Time (min)	*m* 3He (pccSTP)	$\pm 2\sigma$ (pccSTP)	n_0 3He (pccSTP)	n_t 3He (pccSTP)	n_t/n_0 predicted	n_t/n_0 measured
100	60	26	0.1158	0.0012	0.6447	0.5289	–	0.8204
100	60	25.1	0.0942	0.0010	0.5289	0.4347	0.8677	0.8219
100	60	25	0.07568	0.00081	0.4347	0.3590	0.8678	0.8259
100	60	25.1	0.05784	0.00062	0.3590	0.3012	0.8678	0.8389
100	60	53.5	0.05298	0.00057	0.3012	0.2482	0.8589	0.8241
100	60	25.2	0.03824	0.00043	0.2482	0.2100	0.8678	0.8459
100	60	25.1	0.03368	0.00041	0.2100	0.1763	0.8678	0.8396
100	60	795.6	0.04934	0.00025	0.1763	0.1270	0.7741	0.7201
100	60	28.1	0.019725	0.000094	0.1270	0.1072	0.8666	0.8446
100	60	43.7	0.017349	0.000084	0.1072	0.08988	0.8622	0.8382
100	60	24.9	0.013779	0.000070	0.08988	0.07610	0.8673	0.8467
100	60	24.9	0.013153	0.000076	0.07610	0.06295	0.8678	0.8272
100	60	25	0.009771	0.000063	0.06295	0.05318	0.8678	0.8448
100	60	25.1	0.009520	0.000064	0.05318	0.04366	0.8679	0.8210
100	60	25.1	0.007641	0.000052	0.04366	0.03602	0.8678	0.8250
100	60	25	0.005717	0.000039	0.03602	0.03030	0.8678	0.8413
100	60	25	0.005784	0.000039	0.03030	0.02451	0.8678	0.8091
100	60	25.1	0.003629	0.000024	0.02451	0.02089	0.8679	0.8520
REST			0.02089	0.00014	0.02089	0		

Table S7: Distilled 4He isothermal permeation data for the same encapsulated-water ampoule experiment as Table S6.

Temp (°C)	Hot Time (min)	Cold Time (min)	m 4He (nccSTP)	$\pm 2\sigma$ (nccSTP)	n_0 4He (nccSTP)	n_t 4He (nccSTP)	n_t/n_0 predicted	n_t/n_0 measured	3He/4He measured (Ra)
100	60	26	604.0	1.8	3871	3267	–	0.8440	0.1379
100	60	25.1	515.5	1.5	3267	2751	0.8772	0.8422	0.1315
100	60	25	434.8	1.3	2751	2317	0.8772	0.8420	0.1252
100	60	25.1	361.9	1.1	2317	1955	0.8772	0.8438	0.1150
100	60	53.5	325.43	0.96	1955	1629	0.8688	0.8335	0.1171
100	60	25.2	251.31	0.74	1629	1378	0.8772	0.8458	0.1095
100	60	25.1	212.62	0.63	1378	1165	0.8772	0.8457	0.1140
100	60	795.6	344.78	0.80	1165	820.7	0.7858	0.7042	0.1029
100	60	28.1	127.20	0.28	820.7	693.5	0.8761	0.8450	0.1116
100	60	43.7	111.27	0.22	693.5	582.2	0.8719	0.8395	0.1122
100	60	24.9	88.54	0.17	582.2	493.7	0.8768	0.8479	0.1120
100	60	24.9	74.96	0.12	493.7	418.7	0.8773	0.8481	0.1262
100	60	25	62.687	0.088	418.7	356.0	0.8772	0.8503	0.1121
100	60	25.1	53.284	0.072	356.0	302.7	0.8773	0.8503	0.1285
100	60	25.1	45.452	0.061	302.7	257.3	0.8772	0.8499	0.1209
100	60	25	38.407	0.053	257.3	218.9	0.8773	0.8507	0.1071
100	60	25	32.416	0.048	218.9	186.4	0.8772	0.8519	0.1284
100	60	25.1	27.465	0.044	186.4	159.0	0.8773	0.8527	0.0950
REST			158.98	0.26	159.0	0			0.0945

Table S8. Distilled 3He isothermal permeation data for the silica glass ampoule containing fused sulfur, equilibrated with high-purity tank helium, measured on the Helix-MC-Plus^{10K} multi-collector mass spectrometer ("Encapsulated Sulfur, Helix MC" in Table S1).

Temp (°C)	Hot Time (min)	Cold Time (min)	*m* 3He (pccSTP)	$\pm 2\sigma$ (pccSTP)	n_0 3He (pccSTP)	n_t 3He (pccSTP)	n_t/n_0 predicted	n_t/n_0 measured
80	60	25.6	0.699	0.028	9.569	8.870	0.9299	0.9270
80	60	61.3	0.736	0.029	8.870	8.134	0.9222	0.9170
80	60	25.1	0.591	0.022	8.134	7.543	0.9300	0.9274
80	60	25	0.544	0.018	7.543	6.999	0.9301	0.9279
80	60	25	0.494	0.016	6.999	6.505	0.9301	0.9294
100	60	91.8	0.759	0.024	6.505	5.746	0.8831	0.8834
100	60	25.9	0.601	0.020	5.746	5.145	0.8966	0.8955
100	60	52.0	0.575	0.021	5.145	4.570	0.8912	0.8882
100	60	26	0.463	0.017	4.570	4.108	0.8966	0.8988
100	60	89.9	0.498	0.020	4.108	3.609	0.8834	0.8787
120	60	24.8	0.510	0.023	3.609	3.099	0.8537	0.8586
120	60	52.8	0.457	0.022	3.099	2.641	0.8481	0.8524
120	60	24.9	0.356	0.018	2.641	2.286	0.8537	0.8653
120	60	61.3	0.318	0.016	2.286	1.967	0.8460	0.8607
120	60	25.1	0.243	0.012	1.967	1.724	0.8537	0.8766
150	60	25.0	0.420	0.020	1.724	1.304	0.7695	0.7562
150	60	25.0	0.283	0.013	1.304	1.021	0.7696	0.7828
150	60	690.8	0.351	0.010	1.021	0.6699	0.6598	0.6563
150	60	25	0.1472	0.0040	0.6699	0.5226	0.7696	0.7802
150	60	53.3	0.125	0.003	0.5226	0.3972	0.7643	0.7601
150	60	25.0	0.0893	0.0024	0.3972	0.3080	0.7695	0.7752
remainder			0.3080	0.0085				

Table S9: Distilled 4He isothermal permeation data for the same encapsulated-sulfur ampoule experiment as Table S8.

Temp (°C)	Hot Time (min)	Cold Time (min)	m 4He (nccSTP)	$\pm 2\sigma$ (nccSTP)	n_0 4He (nccSTP)	n_t 4He (nccSTP)	n_t/n_0 predicted	n_t/n_0 measured	3He/4He measured (Ra)
80	60	25.6	3354	11	52330	48980	0.9348	0.9359	0.1499
80	60	61.3	3617	12	48980	45360	0.9276	0.9262	0.1464
80	60	25.1	2949	10	45360	42410	0.9349	0.9350	0.1441
80	60	25	2759.6	9.6	42410	39650	0.9350	0.9349	0.1419
80	60	25	2587.1	9.1	39650	37060	0.9350	0.9348	0.1373
100	60	91.8	3980	15	37060	33080	0.8913	0.8926	0.1371
100	60	25.9	3088	14	33080	30000	0.9041	0.9066	0.1399
100	60	52.0	2978	15	30000	27020	0.8990	0.9007	0.1389
100	60	26	2517	13	27020	24500	0.9041	0.9068	0.1322
100	60	89.9	2687	14	24500	21810	0.8916	0.8903	0.1334
120	60	24.8	2769	15	21810	19040	0.8646	0.8731	0.1327
120	60	52.8	2551	13	19040	16490	0.8592	0.8661	0.1290
120	60	24.9	2097	10	16490	14400	0.8646	0.8728	0.1221
120	60	61.3	1948.5	9.4	14400	12450	0.8572	0.8647	0.1176
120	60	25.1	1573.3	7.4	12450	10870	0.8645	0.8736	0.1110
150	60	25.0	2435	11	10870	8439	0.7868	0.7761	0.1242
150	60	25.0	1806.5	8.2	8439	6633	0.7868	0.7859	0.1128
150	60	690.8	2151.5	8.5	6633	4481	0.6807	0.6756	0.1173
150	60	25	924.6	3.4	4481	3557	0.7868	0.7937	0.1146
150	60	53.3	753.9	2.8	3557	2803	0.7818	0.7880	0.1197
150	60	25.0	560.4	2.1	2803	2242	0.7868	0.8001	0.1146
remainder			2242.4	8.7					0.0988

References

Altemose, V. O. Helium Diffusion through Glass. *Journal of Applied Physics* **32**, 1309–1316 (1961).

Carman, P. C. *Flow of Gases through Porous Media* (Academic Press, New York, 1956).

Carslaw, H. S. & Jaeger, J. C. *Conduction of Heat in Solids*, 2nd edn (Oxford University Press, Oxford, 1959).

Farley, K. A., Wolf, R. A. & Silver, L. T. The effects of long alpha-stopping distances on (U-Th)/He ages. *Geochimica et Cosmochimica Acta* **60**, 4223–4229 (1996).

Farley, K. A., Reiners, P. W. & Nenow, V. An Apparatus for High-Precision Helium Diffusion Measurements from Minerals. *Anal. Chem.* **71**, 2059–2061 (1999).

Farley, K. A., Monteiro, H. B., Vasconcelos, P. M. & Waltenberg, K. Dehydration of goethite during vacuum step-heating and implications for he retentivity characterization. *Chemical Geology* **663**, 122254 (2024).

Farley, K. A. Helium diffusion from apatite: General behavior as illustrated by Durango fluorapatite. *Journal of Geophysical Research: Solid Earth* **105**, 2903–2914 (2000).

Fechtig, H. & Kalbitzer, S. The Diffusion of Argon in Potassium-Bearing Solids. In: *Potassium Argon Dating* (eds Schaeffer, O. A. & Zähringer, J.) 68–107 (Springer, Berlin, Heidelberg, 1966).

Goldsmith, A. S., Ketcham, R. A. & Stockli, D. F. Simulating effects of heterogeneous 4He concentration profiles and radiation damage annealing on whole-grain zircon diffusivity analyses. *Geochimica et Cosmochimica Acta* **284**, 239–253 (2020).

Jones, W. M. Permeability and Solubility of He^3 and He^4 in Vitreous Silica. *J. Am. Chem. Soc.* **75**, 3093–3096 (1953).

Ketcham, R. A., Gautheron, C. & Tassan-Got, L. Accounting for long alpha-particle stopping distances in (U-Th-Sm)/He geochronology: Refinement of the baseline case. *Geochimica et Cosmochimica Acta* **75**, 7779–7791 (2011).

Masaryk, J. S. Permeation in Fused Silica (1968).

McMurtry, G. M., DeLuze, J. R., Hilton, D. R. & Blessing, J. E. Differential Diffusion of Helium Isotopes in Glass, Quantum-tunneling 3He Enrichment, and Portable 3He/4He Monitoring of Mantle Processes. *Sci Rep* **9**, 5213 (2019).

Norton, F. J. Helium Diffusion Through Glass. *Journal of the American Ceramic Society* **36**, 90–96 (1953).

Ostrogorsky, A. G. & Glicksman, M. E. Segregation and Component Distribution. In: *Handbook of Crystal Growth*, 2nd edn, Vol. IIA, Ch. 25 (Elsevier, Amsterdam, 2015).

Rogers, W. A., Buritz, R. S. & Alpert, D. Diffusion Coefficient, Solubility, and Permeability for Helium in Glass. *J. Appl. Phys.* **25**, 868–875 (1954).

Shackelford, J. F., Studt, P. L. & Fulrath, R. M. Solubility of Gases in Glass. II. He, Ne, and H2 in Fused Silica. *Journal of Applied Physics* **43**, 1619–1626 (1972).

Shelby, J. E. Pressure dependence of helium and neon solubility in vitreous silica. *Journal of Applied Physics* **47**, 135–139 (1976).

Shuster, D. L., Farley, K. A., Sisterson, J. M. & Burnett, D. S. Quantifying the diffusion kinetics and spatial distributions of radiogenic 4He in minerals containing proton-induced 3He. *Earth and Planetary Science Letters* **217**, 19–32 (2004).

Studt, P. L. Mechanism of Gaseous Permeation through Glass, Single-Crystal Silicon, and Germanium; and Stress-Enhanced Gaseous Permeation through Alumina Bodies. https://escholarship.org/uc/item/9pj1h2x1 (1962).

Swets, D. E., Lee, R. W. & Frank, R. C. Diffusion Coefficients of Helium in Fused Quartz. *The Journal of Chemical Physics* **34**, 17–22 (1961).

Wilson, W. D. & Bisson, C. L. Atomistics of helium diffusion in copper and tungsten. *Radiation Effects* **19**, 53–58 (1973).

Yakubovich, O. V., Shukolyukov, Yu. A., Kotov, A. B., Yakovleva, S. Z. & Sal'nikova, E. B. Geothermochronology based on noble gases: II. Stability of the (U-Th)/He isotope system in zircon. *Petrology* **18**, 555–570 (2010).