

THE HANDYMAN'S GUIDE TO OSCILLOSCOPES (Part 1 of 2)

by Paul Harden, NA5N

Getting Acquainted with your Scope and making some measurements

Updated May 2004 with actual oscpe waveforms

Print as .pdf file
5 pages
8½ x 11 or A4

When in the course of human events, it becomes necessary to look at neat signals floating around your radio, you go to a hamfest and buy that \$50 o-scope. Now what? This two part article will attempt to explain basically how an oscilloscope works, operator functions, basic measurements, and some advanced applications. An o-scope is a powerful tool in any shack – even a real "cheapie" with limited bandwidth.

HOW AN OSCILLOSCOPE WORKS

A block diagram of a typical o-scope is shown in **Fig. 1**. The test probe usually plugs into the scope via a BNC connector, then passes through a switch to determine whether the input signal will be dc or ac coupled (to remove any dc component). Often this switch will have a "ground" position for setting the zero-volts reference. Next is the input attenuators. The vertical input amplifier is quite sensitive, designed for 20-50mV of input. For larger input voltages, the signal is applied to attenuators comprised of simple voltage dividers. This is the first area of concern for cheap o-scopes, as the input attenuators may not be very linear or accurate. For example, if you apply a 10Vpp signal on the 10v/division setting, the signal should be 1 division high. Switching to 1v/div., the signal should be 10 divisions (usually full-scale) high. If it is not exactly 10 divisions, the attenuator for that setting needs adjusting. Some scopes have internal adjustments for fine-tuning each attenuator setting.

Following the attenuators, the signal is applied to the first vertical amplifier, which converts the input to a differential signal. This differential signal is amplified up to high voltages for the oscilloscope deflecting plates – moving the beam up and down (in the vertical axis).

The sweep generator is usually a constant current source charging a capacitor to make a sawtooth waveform that eventually deflects the beam in the horizontal axis. The frequency of the sawtooth determines how fast the beam travels from the left to the right side of the tube, and is controlled by the sweep control, usually calibrated in seconds, milli-seconds or micro-seconds per division. This is the second area of concern for an oscilloscope – how linear the sawtooth waveform is generated. For example, a sawtooth with a nonlinear ramp will cause the signal displayed in the central portion of the tube to be expanded or compressed compared to the signal at the ends.

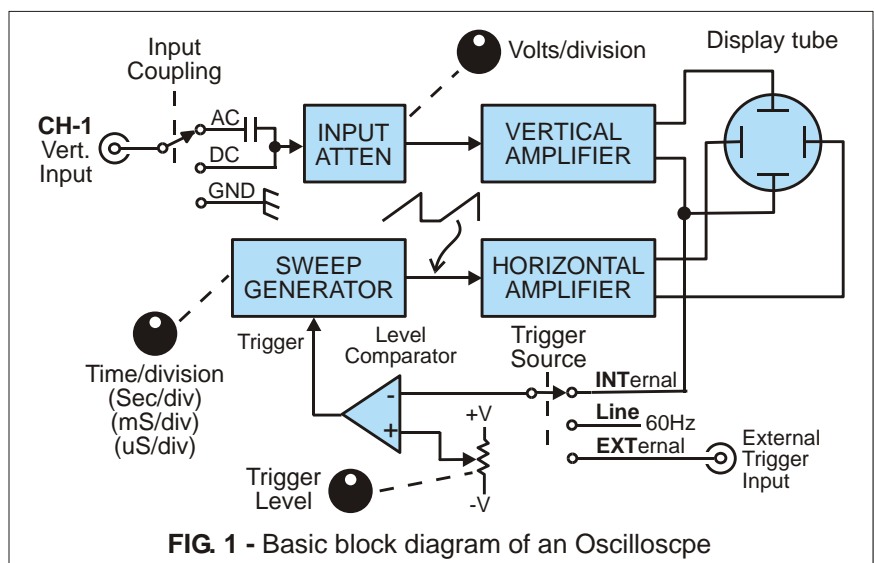


FIG. 1 - Basic block diagram of an Oscilloscope

The sawtooth ramp is amplified to high voltages, applied to the oscope tube, to deflect the beam from left to right. An important task of an oscope is when the horizontal deflection begins. Normally a switch labeled "Trigger Source" determines what initiates the sawtooth ramp. In the "Internal" position, a sample of the input signal (in the vertical amplifiers) is sampled, with a variable resistor setting the level. When the input signal exceeds the "Trigger Level," a pulse is generated to start the sawtooth ramp and hence the horizontal sweep. The purpose of triggering is to keep the input waveform synchronized to the sweep so it appears stationary on each sweep. The trigger source usually has a "Line" position, which simply triggers the sweep off of 60Hz from the power supply. This synchronizes the sweep to the AC power frequency and is useful for checking television signals, which are synchronized to the power mains. Also, an "External" position may be present, which connects an external input signal (via a BNC connector) to trigger the sweep generator.

Other features your oscope may have are two vertical channels for dual trace operation, various modes to display both waveforms (alternate, chopped, A+B added, etc.), delayed sweep features, dual sweep time bases, built in calibrators, etc.

CALIBRATING YOUR OSCILLOSCOPE

The first thing you should do upon acquiring an o-scope is to check its calibration.

The vertical amplifiers can be checked with a known voltage source or 9v transistor radio battery. Measure the output voltage of the battery with an accurate voltmeter. Let's say it just happens to be +9v exactly. Set the input coupling to ground (0v) and move the trace to the bottom division. Switch the input coupling to DC and set the attenuators to 1v/div. The deflection should be 9

divisions. Switching to 10v/div., deflection should be 0.9 divisions. Internal to the oscilloscope (or perhaps accessible from the outside) are adjustments for the vertical amplifier gain. Adjust this for 9 divisions of deflection in the 1v/div. range. Procedure can be repeated with a 1.5v flashlight battery (assuming you know the exact voltage from a DVM).

The horizontal amplifiers should be checked/calibrated using a signal generator. For example, a 1MHz signal has a period of 1μs. Setting the sweep rate to 1.0μs/div., a 1MHz signal should take exactly 1 division per cycle. Set the horizontal width control properly to ensure the beam starts at the first division and ends at the last division. If the sweep rate appears incorrect, an internal adjustment (Sweep gain or similar) can be set for proper display of the test signal.

The main operator controls are:

- **Intensity** - controls the brightness of the beam. **NOTE: Too bright a beam can damage to the CRT tube!**
- **Focus** - adjusts the beam for the thinnest and sharpest display.
- **VERT & HOR Position** - controls the vertical and horizontal position of the display respectively
- **VERT V/div** - controls the vertical sensitivity of the display, i.e., how many volts (or mV) per division.
- **HOR Sweep Speed** - sets the horizontal sensitivity, i.e., how many mS or μs per division.
- **VERT & HOR vernier** - allows the vertical and horizontal sensitivity settings to be varied in small steps.

Other adjustments you may find on your scope are:

Astigmatism - With the scope intensity and focus properly set, this adjustment compensates for the curvature of the CRT tube by making it in-focus across the sweep. If your trace is out-of-focus in certain areas, but in-focus elsewhere, the astigmatism needs to be adjusted. See **Fig. 2**.

Trace Rotation - is a small coil around the CRT that skews the trace to ensure it is perfectly horizontal. On scopes without this adjustment, the trace is leveled by physically rotating the CRT to align the trace to the graticle grid. See **Fig. 2**.

DC BAL (DC Balance) - is a dc offset in the vertical amplifiers that causes a shift in the trace baseline when changing vertical scales. It is most obvious when measuring ac voltages. For example, you are displaying a 10Vpp sine wave, centered on the center graticle, at 2v/div. Changing to 5v/div, the sine wave shifts off the center graticle ... that is, it assumes a dc bias error. The DC BAL is adjusted until the shift no longer occurs when changing vertical scales.

HV ADJ. - is the high voltage that controls the intensity of the trace. Turn up the **Intensity** control to its brightest position, then adjust the HV ADJ for a trace slightly brighter than normal intensity. The **Intensity** control now has the proper range. The HV ADJ might have to be re-adjusted to acquire proper focus.

NOTE: Very bright trace displays can cause permanent damage to the CRT, particularly on a well-used scope.

LET'S MAKE SOME MEASUREMENTS

It is assumed you have your scope relatively calibrated and familiar with the front panel controls. The sample o-scope displays are based on eight vertical and ten horizontal divisions on the CRT screen, typical to most oscilloscopes. Most waveforms are actual displays of the signal cited, photographed from my trusty Tektronix 475 oscilloscope.

First ... a word on TRIGGERING.

Most oscilloscopes have a knob or two for "Triggering." This tells the oscilloscope when to start the sweep. When the **Triggering Slope** is placed in the (+) position, the scope will begin its trace when the *input* signal goes positive. Likewise, when (-) triggering is selected, the trace will begin when the input signal goes negative, as shown in **Fig. 3**. Often there will be the option to choose the **Triggering Source**, such as "CH.1" or "LINE." Line means the scope is triggered off the 60Hz line voltage, and is useful when synchronizing on television signals or looking at 60Hz power supply noise. CH.1 or CH.2 means the scope will trigger off the signal on channel 1 or 2 respectively. **Trigger Level** is at what voltage of the input signal triggering begins. For example, if set high, triggering may not begin until the input signal reaches several volts. When set around zero, it will trigger the moment the signal goes positive (if set for (+) triggering). This setting can be troublesome if noise exists on the signal. Adjust for stable triggering.

Fig. 2 – Effects of Astigmatism & Trace Rotation


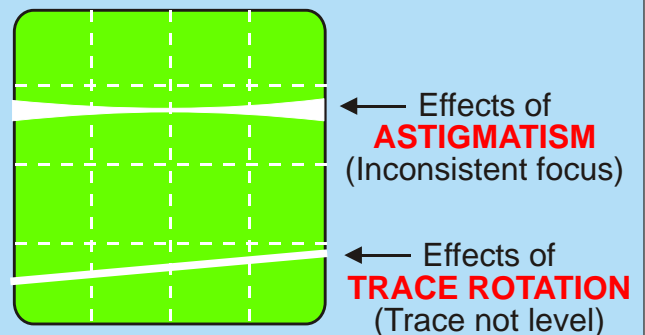


Fig. 3 – Triggering

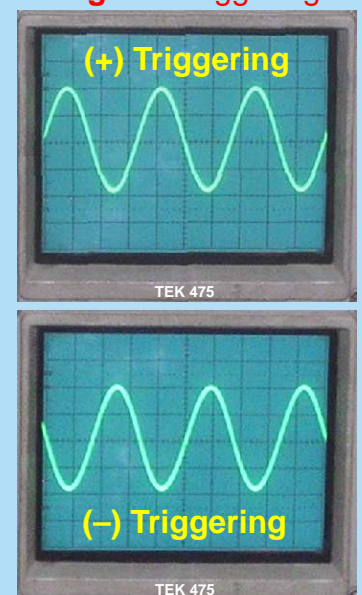

DC Voltages.

Say you want to check the transmit-receiver (T-R) switch in your QRP rig, or other digital signal. See **Fig. 4**. The key line is the input to the HCT240 inverter to form the 0v TX— on key- down and the 0v RX— on key- up. This switches the rig between transmit and receive (T-R Switch). It is a logic function, that is, a voltage to represent ON or OFF.

Place the scope lead on pin 13 at 10v/div. and you should see the waveform like the top trace in **Fig. 4** ... about +6v on key-up and 0v on key down. Move the scope lead to pin 7 and you should see 0v on key-up and about +8v on key-down (bottom trace). If the output does not go "HI" (+8v) on key-down, or does not go to a solid "LO" (<1v) on key-up, the inverter is not working properly. (It's busted). Many shortwave receivers use similar schemes for switching filters or attenuators.

While this test could be done with a DVM, the integration time is slow, requiring long key-downs to get the voltages. A scope will also show you how clean the switching is, or if there is an ac voltage (or RF noise) riding on the T-R voltage.

Scopes are thus good dc voltmeters, with about a 5% reading accuracy.

AC Voltages.

Here is where an oscilloscope pays for itself by making AC voltage (and frequency) measurements. You must remember, AC voltages are displayed on a scope as **peak-to-peak voltages**, while a voltmeter measures in **rms**. RMS voltages are about 1/3 the p-p voltage read on a scope, or specifically:

$$V_{rms} = \frac{1}{2}(.707 \times V_{pp}) = 0.354 \times V_{pp}$$

For example, let's measure the output voltage and frequency from the sidetone oscillator in your QRP rig. Place the scope lead on the audio amplifier output. On key-down, you get the waveform shown in **Fig. 5**. The transmit sidetone audio is 1.9Vpp.

AC Frequency Measurement.

With this waveform, we might as well see what frequency our sidetone or transmit-offset frequency is. Most operators prefer the sidetone to be about 700–750Hz. Trigger the scope for a stable waveform and set the time-base (sweep) to display 2 or 3 cycles, as shown in **Fig. 6**. Center the waveform between two horizontal divisions so zero volts on the waveform is on a graticule line, then move the horizontal position so the first "zero-crossing" is also on a division line.

Measure the time it takes to make one complete sine wave from one zero-crossing to the next. In this example, it is 1.5 divisions, at 1mS per division, or 1.5mS. Frequency is simply the reciprocal of time, such that the sidetone frequency is:

$$f = \frac{1}{t} = \frac{1}{1.5mS} = 667 \text{ Hz}$$

For some, this may be about right. For others, this may be a little low to your liking. To raise it to 700Hz, calculate the time period of 700Hz ($1/700 = 1.4mS$). At 1.0mS/div, you can adjust your sidetone or transmit offset until zero-crossings for a single sinewave is 1.4 divisions. This will be about 700 Hz. (Sidetone may not be adjustable on some rigs).

All frequency measurements are made in this fashion, by measuring the distance between zero-crossings (or from one peak to the next) and converting the time period to frequency. This should emphasize the importance of ensuring your sweep speed is calibrated; as any error in the time base will cause a corresponding error in the accuracy of your time or frequency measurements.




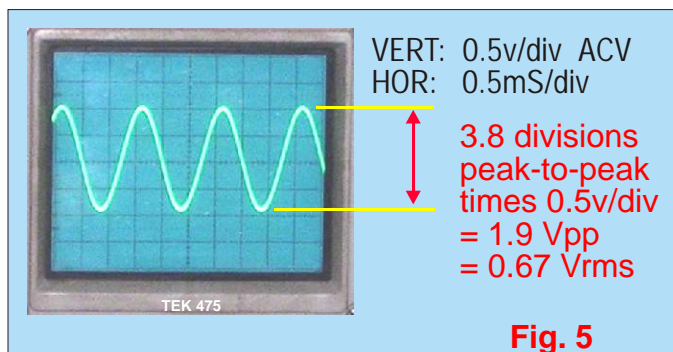


Fig. 6

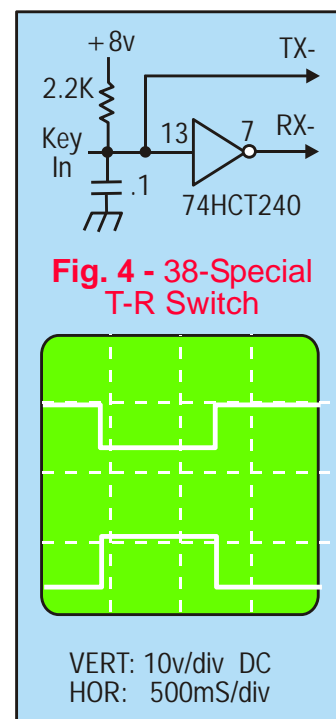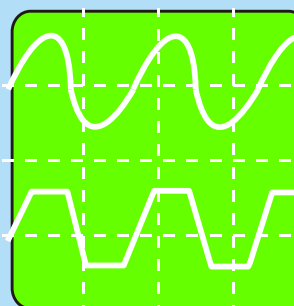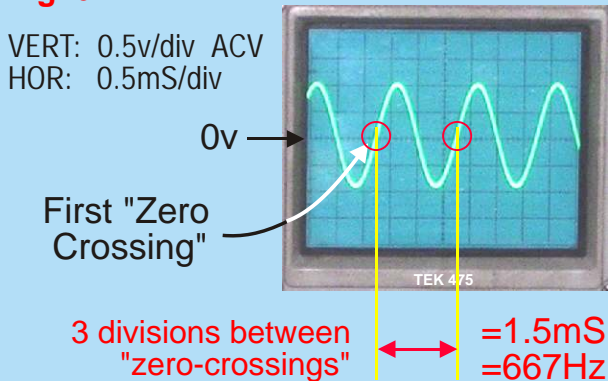

Quality of the waveform is another feature of a scope that is unsurpassed since you are "seeing" the waveform in real time. Two examples of waveform quality are shown in *Fig. 7*.

The top trace shows the sidetone frequency with distortion, perhaps due to improper time-constant on the coupling capacitors or improperly biased audio amplifiers. The bottom trace would be a raspy sounding side tone, due to the amplifier being over-driven and in compression (clipping). The o-scope is an invaluable tool for detecting and diagnosing such impurities in the signal quality.

MORE NIFTY MEASUREMENTS

Amplifier Gain.

The gain of an amplifier can be measured in terms of voltage or decibels (dB). For voltage gain, it is simply V_{out}/V_{in} of the amplifier. For example, if the input is 1Vpp and the output is 4Vpp, then the amplifier has a voltage gain of 4.

Gain in dB is often more useful and is how the gains of amplifiers are usually expressed. With dB's, every-time you double the AC voltage, you add 6dB of gain. It is the **ratio** of output to the input, and this **ratio** is easy to measure on a scope.

It is often easier to start with the output. Set the vertical amplifier gain to display the amplifier **output** as a full-scale signal as shown in *Fig. 8*. Now move the scope probe to the amplifier **input** without disturbing the scope gain. You will of course have a much smaller signal, and the ratio of the input to the output will be the gain in dB. In our example of using eight divisions for full-scale, then four divisions would be 6db, 2 divisions 12dB, etc. as shown in *Fig. 9*. You may want to add your own dB scale along your scope display to remind you of this relationship. Note: this is **voltage gain** ($A_v = 20 \log x V_{out}/V_{in}$). In this example, with 4Vpp output and 1Vpp input ($A_v = 4$), then the gain is $\text{dB} = 20 \log(4) = 20(0.602) = 12\text{dB}$, or as shown directly on the CRT tube. Since this is a relative measurement, the absolute V_{in} or V_{out} voltage does not need to be determined.

Insertion Loss.

In some circuits, such as filters or attenuators, the **loss** in the circuit needs to be measured, and like circuit gain – expressed in dB. The loss through a circuit is called the **insertion loss**. It is determined in the same way as amplifier gain just presented, except start with the input (the highest AC voltage) as the full-scale or reference display, then measure the output AC voltage (the lowest level). **The ratio is the insertion loss in dB.**

For example, with a signal generator connected to your receiver, you want to measure the insertion loss through the IF crystal filter. At the filter input, you can just barely squeek out 2 divisions of input signal on your scope at its most sensitive setting. The output from the crystal filter is 1.5 divisions. The insertion loss would be $20 \log(1.5/2.0 \text{ div.}) = -2.5 \text{ dB}$. If the output were only 1.0 division (50% reduction), the insertion loss would be 6dB.

Measuring Phase Shifts.

Phase relationships between two signals at the same frequency can be measured with 2-5° accuracy with a scope, although more suited for a dual-trace scope. The reference signal is applied to CH. 1 and the signal to be measured to CH. 2. For proper phase measurements, ensure your dual trace display is in the **chopped** mode, not **alternate** mode for proper phased referenced triggering.

There are many methods to do this. One is to stretch out the signal so it takes 4 horizontal divisions, such that each division is 90° of phase, as shown in *Fig. 10*. By measuring from a common point on one signal (zero-crossing or from peak-to-peak) to the next, the phase can be measured. For example, say you are making a phased-array antenna in which one feedline must cause a 90° delay. You calculate the electrical length for a ¼ $[L = (246/f) \times \text{Velocity Factor}]$ and cut the coax to that length. You are now working on blind faith that you have exactly 90°. With a scope, you can measure it fairly accurately by injecting a signal into one end with a signal generator (at the frequency of interest) and a 50 Ω load on the other. Connect the scope CH.1 to the coax (signal) input and CH.2 to the load end and measure the phase. In the *Fig. 10* example, the CH.2 signal is delayed by 1.6 divisions, at 90°/div is 145°. **Your delay line is too long!** Cut off an inch or two at a time until the CH.2 signal is 90° from CH.1 for precise tuning of the delay

FIG. 8 – Full Scale Signal Display

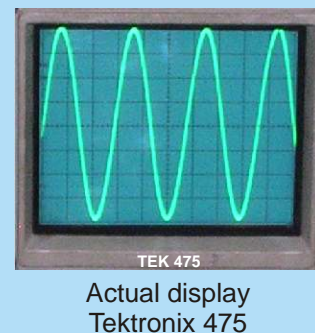


Fig. 9 – Volt. vs. dB relationship



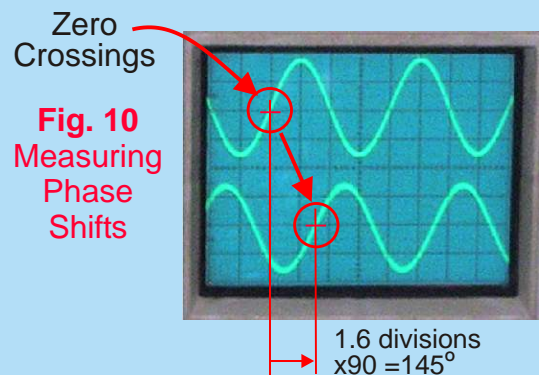


Fig. 11 –Phase Shift by imposition

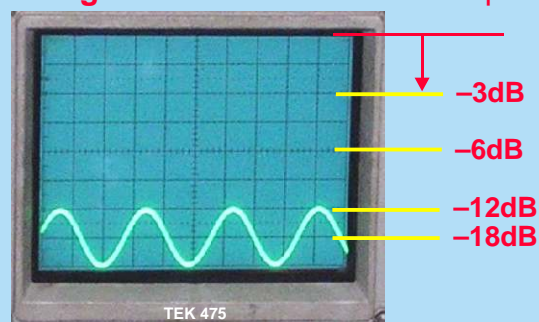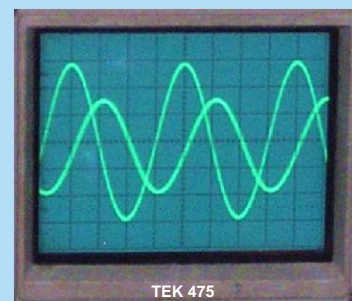

line. (While departing from o-scopes for a moment, the sharp null of a phased array is astounding when exactly 90° delay is achieved. More than 10-15° in error causes a very “mushy” null with little difference over a single vertical antenna. Most errors in achieving exactly 90° by the “measure-and-cut” method are due to uncertainties in the stated velocity factor of the coax).

Another method is to superimpose the two signals on top of each other. Make one signal larger than the other so you know which one is what, as shown in **Fig. 11**. In this example, the smaller signal lags the larger signal by about 100°, estimated by where they cross. For more accurate determination, use the time base to measure the time period of one cycle (T1), then the time period one signal lags (or leads) the other (T2). The phase shift is then $=(T2/T1) \times 360^\circ$.


Phase measurements can be made on a single trace scope as well. First, connect the reference signal, using a BNC “T,” to both the *external trigger* and the normal *vertical input*. Adjust the trigger level so the zero-crossing occurs at the beginning of the trace (left-hand graticule). Remove the reference from the vertical input, but not the *external trigger*, and apply the signal to be tested to the vertical input – without altering the time base or trigger level. The distance of zero-crossing of the test signal is from the left-hand graticule can now be measured to determine the phase, though with slightly less accuracy than using a dual-trace scope.

An interesting experiment is to measure the phase shift of the audio signal at different frequencies as it travels through the stages in a CW, SSB or AM active filter. What is the phase shift of the wanted vs unwanted frequencies?

Measuring Rise and Fall Times.

In digital circuits, it is sometimes important to know the rise and fall times of a signal through a gate. In amateur radio transceivers, this same interest could be applied to how fast the T-R switch switches. On key-down, if the transmitter turns on slightly before the receiver is turned off, it can produce an annoying “thump” in the receiver. Rise and fall times are measured by triggering on the edge of the signal of interest, then increase to a faster sweep speed to measure the time it takes the signal to reach 90% of its final level. The signal to be measured is shown in **Fig. 12** on the top trace, and the expanded version on the bottom. For proper rise times, the signal being measured should be well within the bandwidth of your scope and using a low capacity probe.

For example, in **Fig. 12** (bottom trace), the rise time is about 1/4th of a division. If the sweep speed is 100nS/division, the rise time would then be about 25nS.

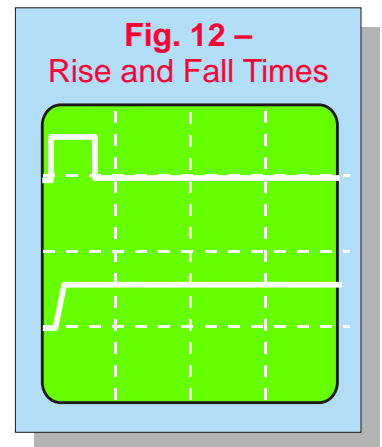

USING LIMITED BANDWIDTH SCOPES

Today's scopes have 200–500MHz bandwidths. Likely your scope is much less than that. A limited bandwidth scope is still very useful to the amateur or homebrewer. Say the bandwidth of your scope is 5MHz. This does not mean you can't see 7MHz signals. It just means the peak-to-peak value has lost meaning, and will likely be very weak, since it is beyond the bandwidth of the scope. (Like other bandwidth measurements in electronics, the “bandwidth” of a scope is usually based on the “3dB bandwidth.” That is, at the maximum bandwidth, you are already at the –3dB point, or a 25% reduction in the peak-to-peak voltage display). You can still resolve individual cycles higher than the cited bandwidth to a certain degree and make gain and phase measurements, since they are based on *ratios*.

Most of the examples in this article explore many regions of a communications receiver or ham transceiver without the benefit of any great bandwidth. Experiment with your scope to learn its limitations. *Use a good scope probe and make measurements with a good ground to get the most out of the bandwidth you have.*

For the homebrewer building circuits in the HF bands, a 50 MHz scope **with good calibration** will yield fairly accurate measurements up to 30 MHz with little concern for accuracy. The old 465 or 475 series of Tektronix scopes, with 100/200 MHz bandwidths, make an excellent oscilloscope for the amateur or experimenter. They can often be found at hamfests today for \$100–150, and tend to maintain a fairly good calibration almost regardless of how much use they have seen.

In Part 2 - we'll probe (bad pun) into some advanced measurement techniques, even with a simple scope ... such as measuring sideband rejection, filter responses, VCO phase noise, etc. (and what it all means).

72, Paul NA5N

na5n@zianet.com
pharden@nrao.edu

Colophon:

Article prepared by NA5N using CorelDraw 11

THE HANDYMAN'S GUIDE TO OSCILLOSCOPES (Part 2 of 2)

by Paul Harden, NA5N

Making some advanced measurements with your Oscilloscope

Print as .pdf file
4 pages
8½ x 11 or A4

In Part 1, oscilloscope operation was covered for making basic voltage, time and frequency measurements. In this part, we'll continue with some more advanced uses of a scope, and in particular, how to use a scope for testing and troubleshooting ham radio QRP transceivers in the homebrewer's workshop.

Receiver Filter Bandwidth.

This procedure uses a scope (a DVM can be used with less accuracy) for determining the overall filter bandwidth (or selectivity) of a receiver. It is basically measured by plotting output voltage vs. audio frequency to construct a picture of the filter response.

Connect scope to the receiver audio output (speaker or phone jack); measurement will be based on peak-to-peak voltages (Vpp) on a scope, or rms voltage (Vrms) on a DVM.

Using a signal generator, set the frequency for the band of interest on your radio. For example, on a general coverage shortwave receiver, you might set it for 10 MHz (top end of the 31M band), or perhaps to 7.040 MHz on a 40M ham radio receiver/transceiver. Tune the receiver to the signal generator signal. If you don't have a signal generator, you can also tune to a steady carrier or station to produce a heterodyne audio "pitch." Tune in the signal to the pitch that causes the maximum peak-to-peak display. Adjust the scope and volume control to produce a 2Vpp display (4 divisions). This is the peak response of the overall filtering stages as shown in **Fig. 13**.

Now determine the audio frequency at this peak response by measuring the time period between cycles and convert to frequency. In the example to the right, the period of one cycle is 1.7mS, which is an audio tone of 750Hz (1/.0017sec). A frequency counter on the output can also be used.

Next, tune the receiver such that the sidetone pitch goes UP in frequency and the peak-to-peak signal will decrease in magnitude. Tune to the point where the signal is exactly 1Vpp on the scope. See **Fig. 12**.

This is the -6dB point of the high end of the filter ($20\log 1v/2v = -6dB$). Determine the frequency of the audio pitch as before. In the example, this is 1100 Hz. Record the data.

From these two data points, the -6dB bandwidth can be estimated. The bandwidth from the filter peak (750 Hz) to the -6dB point (1100 Hz) is 350 Hz. The bandwidth (BW) between the two -6dB points is usually twice this value, or 700 Hz. A filter with a -6dB BW of 700Hz is a mediocre filter for CW reception, and way too narrow for SSB or AM.

Of course you can determine the exact -6dB BW by tuning the receiver back to the 2Vpp peak response, and continue tuning DOWNward in frequency until the audio is again exactly 1Vpp. Determine this frequency and record. In this example, it should occur around 400 Hz if the filter shape is symmetrical.

Plot these three data points on a sheet of graph paper as shown in **Fig. 15** to construct the filter shape. Return to the upper -6dB point (1100Hz in the example) and continue tuning upwards in audio pitch, recording the frequency at 0.5v (-12 dB), 0.25v (-18 dB), 125mV (-24 dB), etc. Everytime you "halve the voltage," it is a 6 dB change. The more points you collect, the more accurate your filter response plot will be.

Fig. 13 – Displaying Filter Peak Response


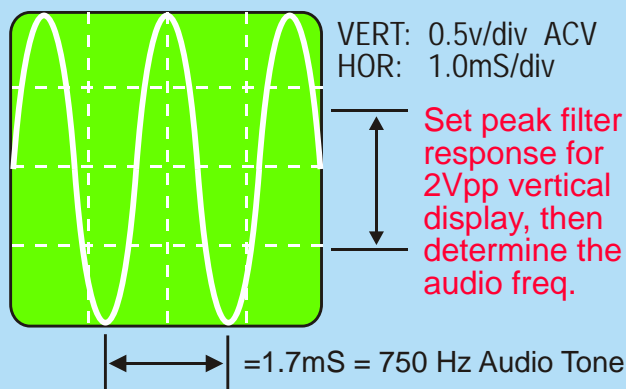


Fig. 14 – Displaying -6dB Frequency

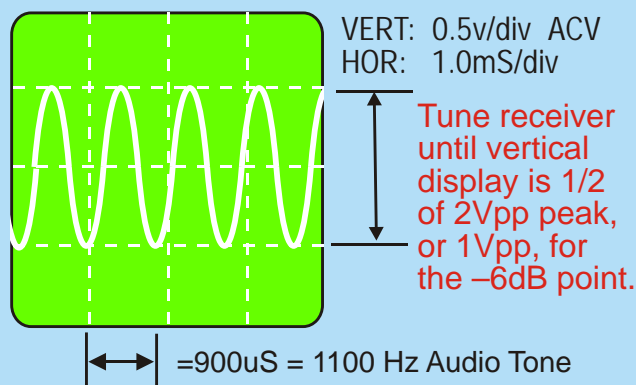

Of interest to proper rig alignment is to repeat the above using the output of the product detector. To maximize the effectiveness of the filtering, the receive offset frequency set by the BFO should be adjusted to the same frequency as the peak frequency response of the audio. In this example, with the peak audio response occurring at 750Hz, if your BFO is set for a sidetone frequency of 700 Hz, you are losing 2–3 dB, since this is in your filter skirt. This is shown on the response plot in **Fig. 15** by the dashed lines. By adjusting your BFO for a sidetone frequency of 750 Hz, you will pick up 3-4dB of overall gain in your receiver, plus increase the selectivity a bit as well. Why? Because nearby stations, such as one at 800–900Hz tone, could actually be louder than the 700Hz tone signal you are trying to copy, since the gain of the receiver is greater at those tones than at 700Hz, as shown in the plot.

Opposite Sideband Rejection

A superhet receiver is supposed to pass just one sideband and reject the other. Poor opposite sideband rejection could indicate the crystals in your IF filter are not well matched or other problems. It is measured almost identical to plotting the filter response just described. First, you tune the receiver to the test signal to find the peak response frequency, or 750Hz in this example. Set the scope display for 2Vpp. Now tune downward in audio pitch, passing zero-beat, and continue tuning and you should hear the test signal, much weaker, now rising again in tone. This is the *opposite sideband*. Measure the peak-to-peak voltage, if you can. For example, say it is 80mVpp, as shown in **Fig. 16**. Calculate the opposite sideband rejection by:

$$\text{rejection} = 20\log \frac{80\text{mV}}{2.0\text{v}} = \frac{80\text{mV}}{2000\text{mV}} = -28\text{dB}$$



If you can't hear the opposite sideband, then obviously you have excellent filter rejection. If you can just barely hear it, you may have to increase the sensitivity of your scope (set vertical gain to 20 or 50 mV/div). In this example, -28dB rejection of the opposite sideband is quite good. A -30dB rejection means the opposite sideband is only 1/1000th of the desired sideband, a very suitable attenuation of the opposite sideband.

These tests are important to perform on your rig for documenting it's current performance, and repeated periodically to detect unfavorable changes or for troubleshooting when a problem is evident. For homebrewing, these tests can allow you to evaluate different circuits or when experimenting with different components or part values.

Oscillator Phase Noise

When homebrewing a basic oscillator circuit, such as a VFO, looking at the oscillator output on a scope can reveal several problems. One is to check for excessive phase noise. Phase noise is small variations of the oscillator frequency that causes power in the close-in sidebands, usually measured on laboratory equipment within 100KHz, or even within 10 KHz.

To check for oscillator phase noise, connect the oscilloscope to the oscillator output, loading the output of the oscillator as little possible. Most scopes have sufficiently high input impedances where this shouldn't be a problem, but some cheaper scopes can load an oscillator circuit. If you suspect your scope is loading the oscillator, couple the scope to the circuit with a small value capacitor, less than 20pF.

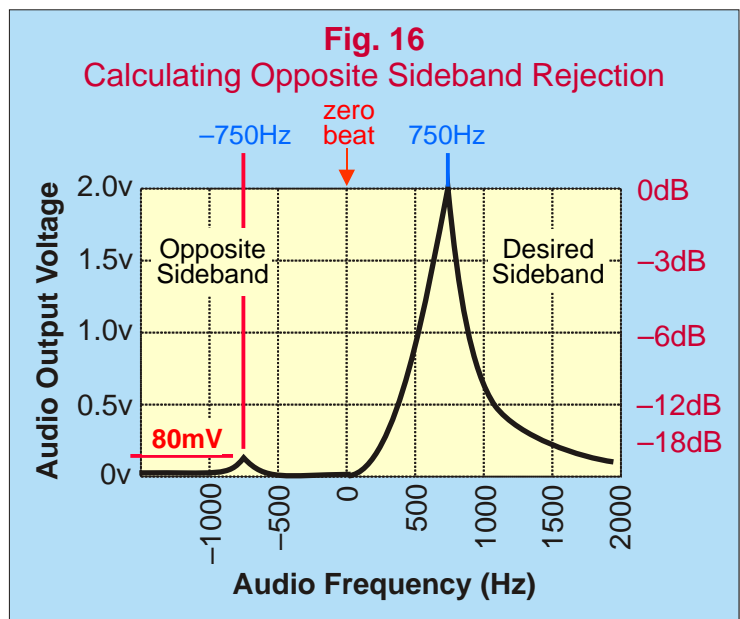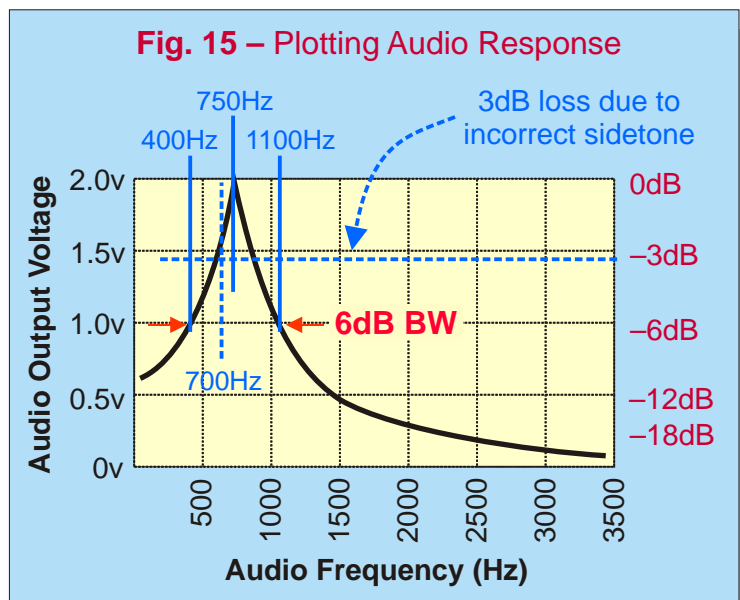

Display 2–3 cycles of the oscillator output as shown on the scope display shown in **Fig. 17**. Properly focus the scope and carefully observe if the waveform appears in focus at the peaks, but slightly out-of-focus at the zero-crossing points, that is, on the rising and falling edges of the sine wave.

If it appears out-of-focus, this is excessive phase noise jittering the signal and “smearing” the waveform along the time (horizontal) axis. Extreme phase noise may show 2-3 sine waves very close to each other, as shown in the exaggerated waveform to the right — assuming you have your scope properly triggered.

Phase noise is random, instantaneous changes in the oscillator

frequency that smears the display. If you can see this on a scope, the phase noise is excessive! If you can’t see it, it doesn’t mean the oscillator has no phase noise (all oscillators have some phase noise), it just means it is not excessive enough to see on a scope. A scope is not a good instrument for checking phase noise, but for homebrew circuits, it is a check to ensure you do not have a serious oscillator problem.

Excessive oscillator phase noise in receivers can cause IMD products and noise in the audio range at the output of the mixer(s), including the product detector. In a transmitter, excessive oscillator phase noise will put power in the close-in sidebands of your carrier, not only wasted power for lower transmitter efficiency, but may produce strange sounds (buzzing or chirping) to the receiving station. A few causes of phase noise are excessive current in the oscillator transistor, low-Q coil(s), high dissipation in the tuning caps or poor power supply filtering at the oscillator frequency.

AM (Amplitude) Noise

Another oscillator problem may be AM noise, or amplitude modulated noise. It is an opposite effect on a scope when displaying the oscillator output — the sine wave appears out-of-focus or thicker at the peaks, and in-focus elsewhere as shown in **Fig. 18**.

If you detect AM noise, slow down the scope’s sweep rate to the audio frequencies or slower to see if you can notice a lower frequency component. A common cause of AM oscillator noise is 60 Hz from the power mains leaking into the circuits. This is particularly true if using a power supply off of 120v 60 Hz, or sometimes it can be due to the AC lighting above your head! If the AM noise seems to be at the same frequency as the audio output tone, it means audio is getting into the Vcc bus, likely due to poor bypass filtering at the audio amplifier stages (particular if using an LM386 or similar).

If you can’t find a low frequency component, the AM noise may be random, which may indicate poor voltage regulation, a noisy voltage regulator, or perhaps a circuit in VHF oscillation. If the

AM noise seems to occur on key-down only on a transmitter, the transmit current may be loading the power supply, the voltage regulator is under-rated, or just simply loading the oscillator. In the case of loading the power supply or regulator(s), perhaps a separate voltage regulator or zener circuit should be used, dedicated for the oscillator(s). In the case of transmit loading, adding a buffer amplifier or emitter follower to isolate the load from the oscillator may help.

Much of this can be diagnosed also with the scope, by looking at the AC ripple on the DC power lines. You should have less than 50mV of any AC component on the 8-12v DC wiring, whether 60Hz, audio or RF. If >50mV, then additional low or high frequency filtering on the DC power is needed.

Monitoring Transmitter RF Output

RF Power (in watts) is E^2/R , where E is in rms and $R=50\Omega$. The voltage displayed on the scope (peak-to-peak) must be converted to rms by $E_{rms}=.707(E_{pp}/2)$. To measure properly, the transmitter should be on a 50W dummy load using the normal hi-Z scope input. If your scope has a selectable “50W” input, it can be the transmitter dummy load directly, providing it can tolerate the 50Vpp input. (Always know what the maximum p-p input voltage your oscilloscope will tolerate. It is often stated on your scope at the vertical channel inputs. 50Vpp to 100Vpp are typical).

Fig. 17 – Checking Oscillator Phase Noise


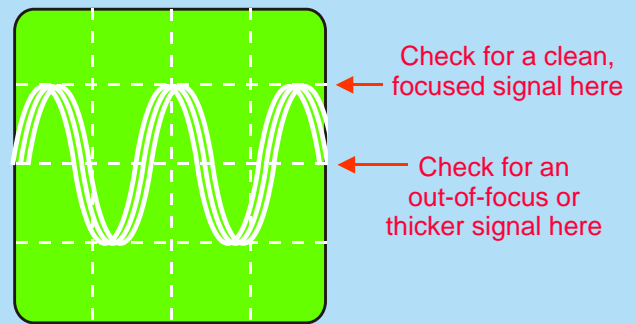


Fig. 18 – Checking for AM Oscillator Noise

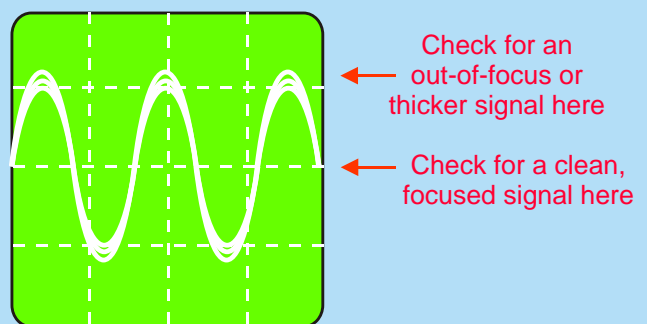

Measuring Transmitter RF Output Power

Figure 19 shows how you can use an oscilloscope to fairly accurately measure output power from a low power transmitter (generally 10W or less with a 1X probe and 20-30W with a 10X probe). Connect transmitter output to a 50W dummy load. Connect the scope lead to the transmitter output (after the low pass filters) or directly to the dummy load. Do not connect the scope leads to the collector or drain of the final PA transistor. The displayed voltage in this case will be erroneous.

In the example, the output transmit voltage across the dummy load measures 24Vpp. Convert this voltage to Vrms, then use the equation (Vrms squared divided by the load resistance) to calculate the power in watts. In the example, 24Vpp, the output power is 1.4 watts. A 5W QRP transmitter should produce about 45Vpp.

The accuracy of your power measurements depend upon the condition of your oscilloscope:

- 1) Ensure your scope's vertical sensitivity (volts/division) is properly calibrated (see Part I)
- 2) Ensure your vertical sensitivity is properly calibrated with the 1X or 10X probe you are using.
- 3) Ensure that the transmitter frequency is well within the bandwidth of your scope. A 100 MHz scope should give reliable readings on all HF bands. A 50 MHz scope should be reliable on all HF bands except slight errors at 28MHz.

Checking Transmitter Purity


Phase Noise of the transmitter is measured identically to the phase noise checks on page 2–3. With the scope properly triggered and focused, you are looking for an out-of-focus “fuzziness” around zero crossing. If it appears phase noise exists, the fault is generally at the beginning of the transmit chain. That is, seldom does the PA transistor add phase noise; it's merely amplifying what it is given. Phase noise on the transmitter output is more likely due to the transmit oscillator, or the transmit mixer if used.

Harmonic Power can also be detected on a scope while looking at the transmitter RF output power. In **Fig. 20**, notice the “dips” or the two “peaks” on the top and bottom of each sine wave. This is caused by excessive 2nd harmonic output power. The rule-of-thumb is – if you can see any 2nd harmonic power (a dip or flattening at the peaks), then you are right at or exceeding the –30dBc FCC harmonic specification. A clean sine wave implies FCC compliance, providing the 2nd harmonic is within your scope's bandwidth. Obviously, a spectrum analyzer should be used for accurate harmonic evaluation, but a scope can be used to indicate if you have a problem. If you build your own transmitter, it is your responsibility to ensure it is compliant. An approximate method of estimating 2nd harmonic attenuation is shown.

–30dBc means the 2nd harmonic power is 1/1000th of the fundamental power. For a 5W transmitter, this means the 2nd harmonic power should be 5mW or less, or about 1Vpp. In displaying a 5W signal on a scope (45Vpp), it would be difficult to resolve much less than a 1Vpp dip or ripple.

Conclusion. This concludes the NA5N “Handiman’s Guide to Oscilloscopes.” Hopefully, it has helped you to understand your oscilloscope to make simple measurements, and with some practice, perform the more advanced measurements discussed. An oscilloscope is a very powerful tool that is invaluable on the homebrewer’s workbench. If there is a particular measurement you feel I omitted, please let me know and I will add it when time permits.


Fig. 19 –Oscilloscope as a Power Meter

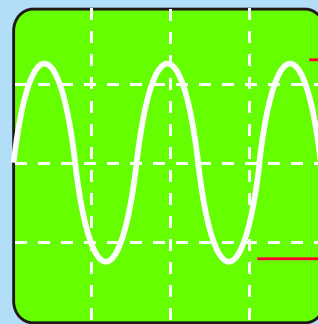

1. Measure output voltage. 24Vpp
2. Convert Vpp to Vrms 8.5Vrms
 $V_{rms} = .707(V_{pp}/2)$
3. Calculate power in watts

$$\frac{V_{rms}^2}{R} = \frac{8.5v^2}{50W} = 1.4W$$

Fig. 20 –Checking 2nd Harmonic Power

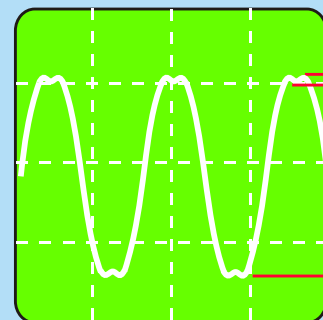

1. Measure output voltage. 24Vpp
2. Measure ripple voltage. 1Vpp
3. Calculate dBc of 2nd harmonic ripple

$$20\log \frac{V_2}{V_1} = 20\log \frac{1v}{24v} = -27.6 \text{ dBc}$$

or, not quite FCC compliant!