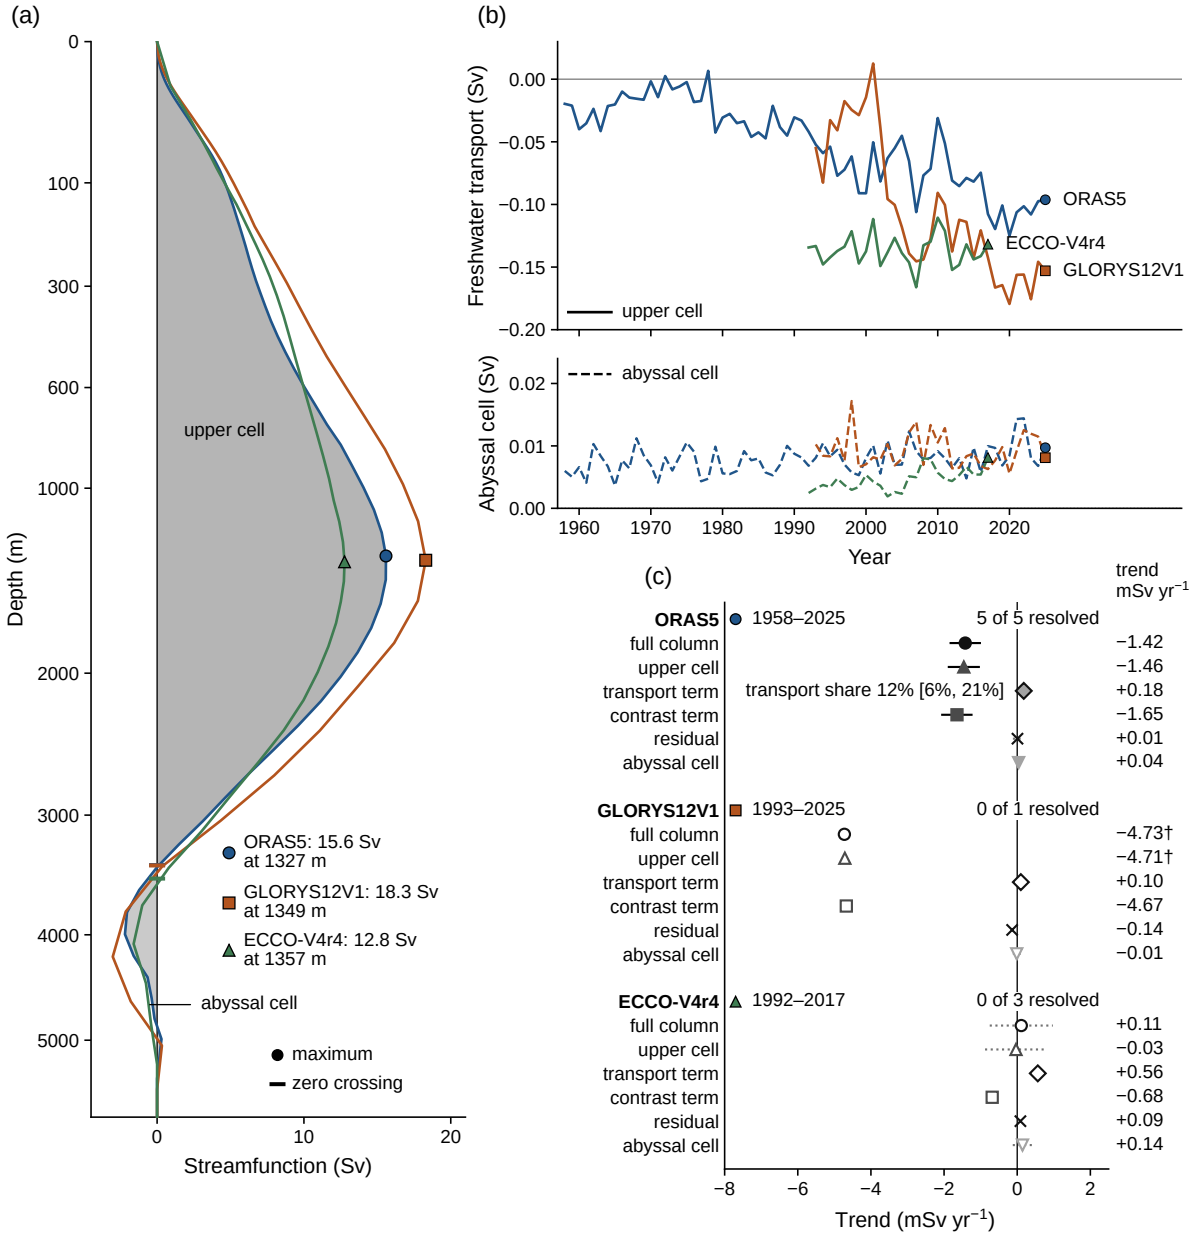

Intervals: totals (full column, upper cell, abyssal cell) use the bias-corrected test interval; the transport and contrast terms and the residual use the ORAS5 sieve interval (10,000 resamples), which GLORYS12V1 and ECCO-V4r4 do not have, so their terms show point estimates only. Filled markers: interval excludes zero (resolved). Dagger: effective sample size at its floor of 3 (uninformative), point values only, not counted.