


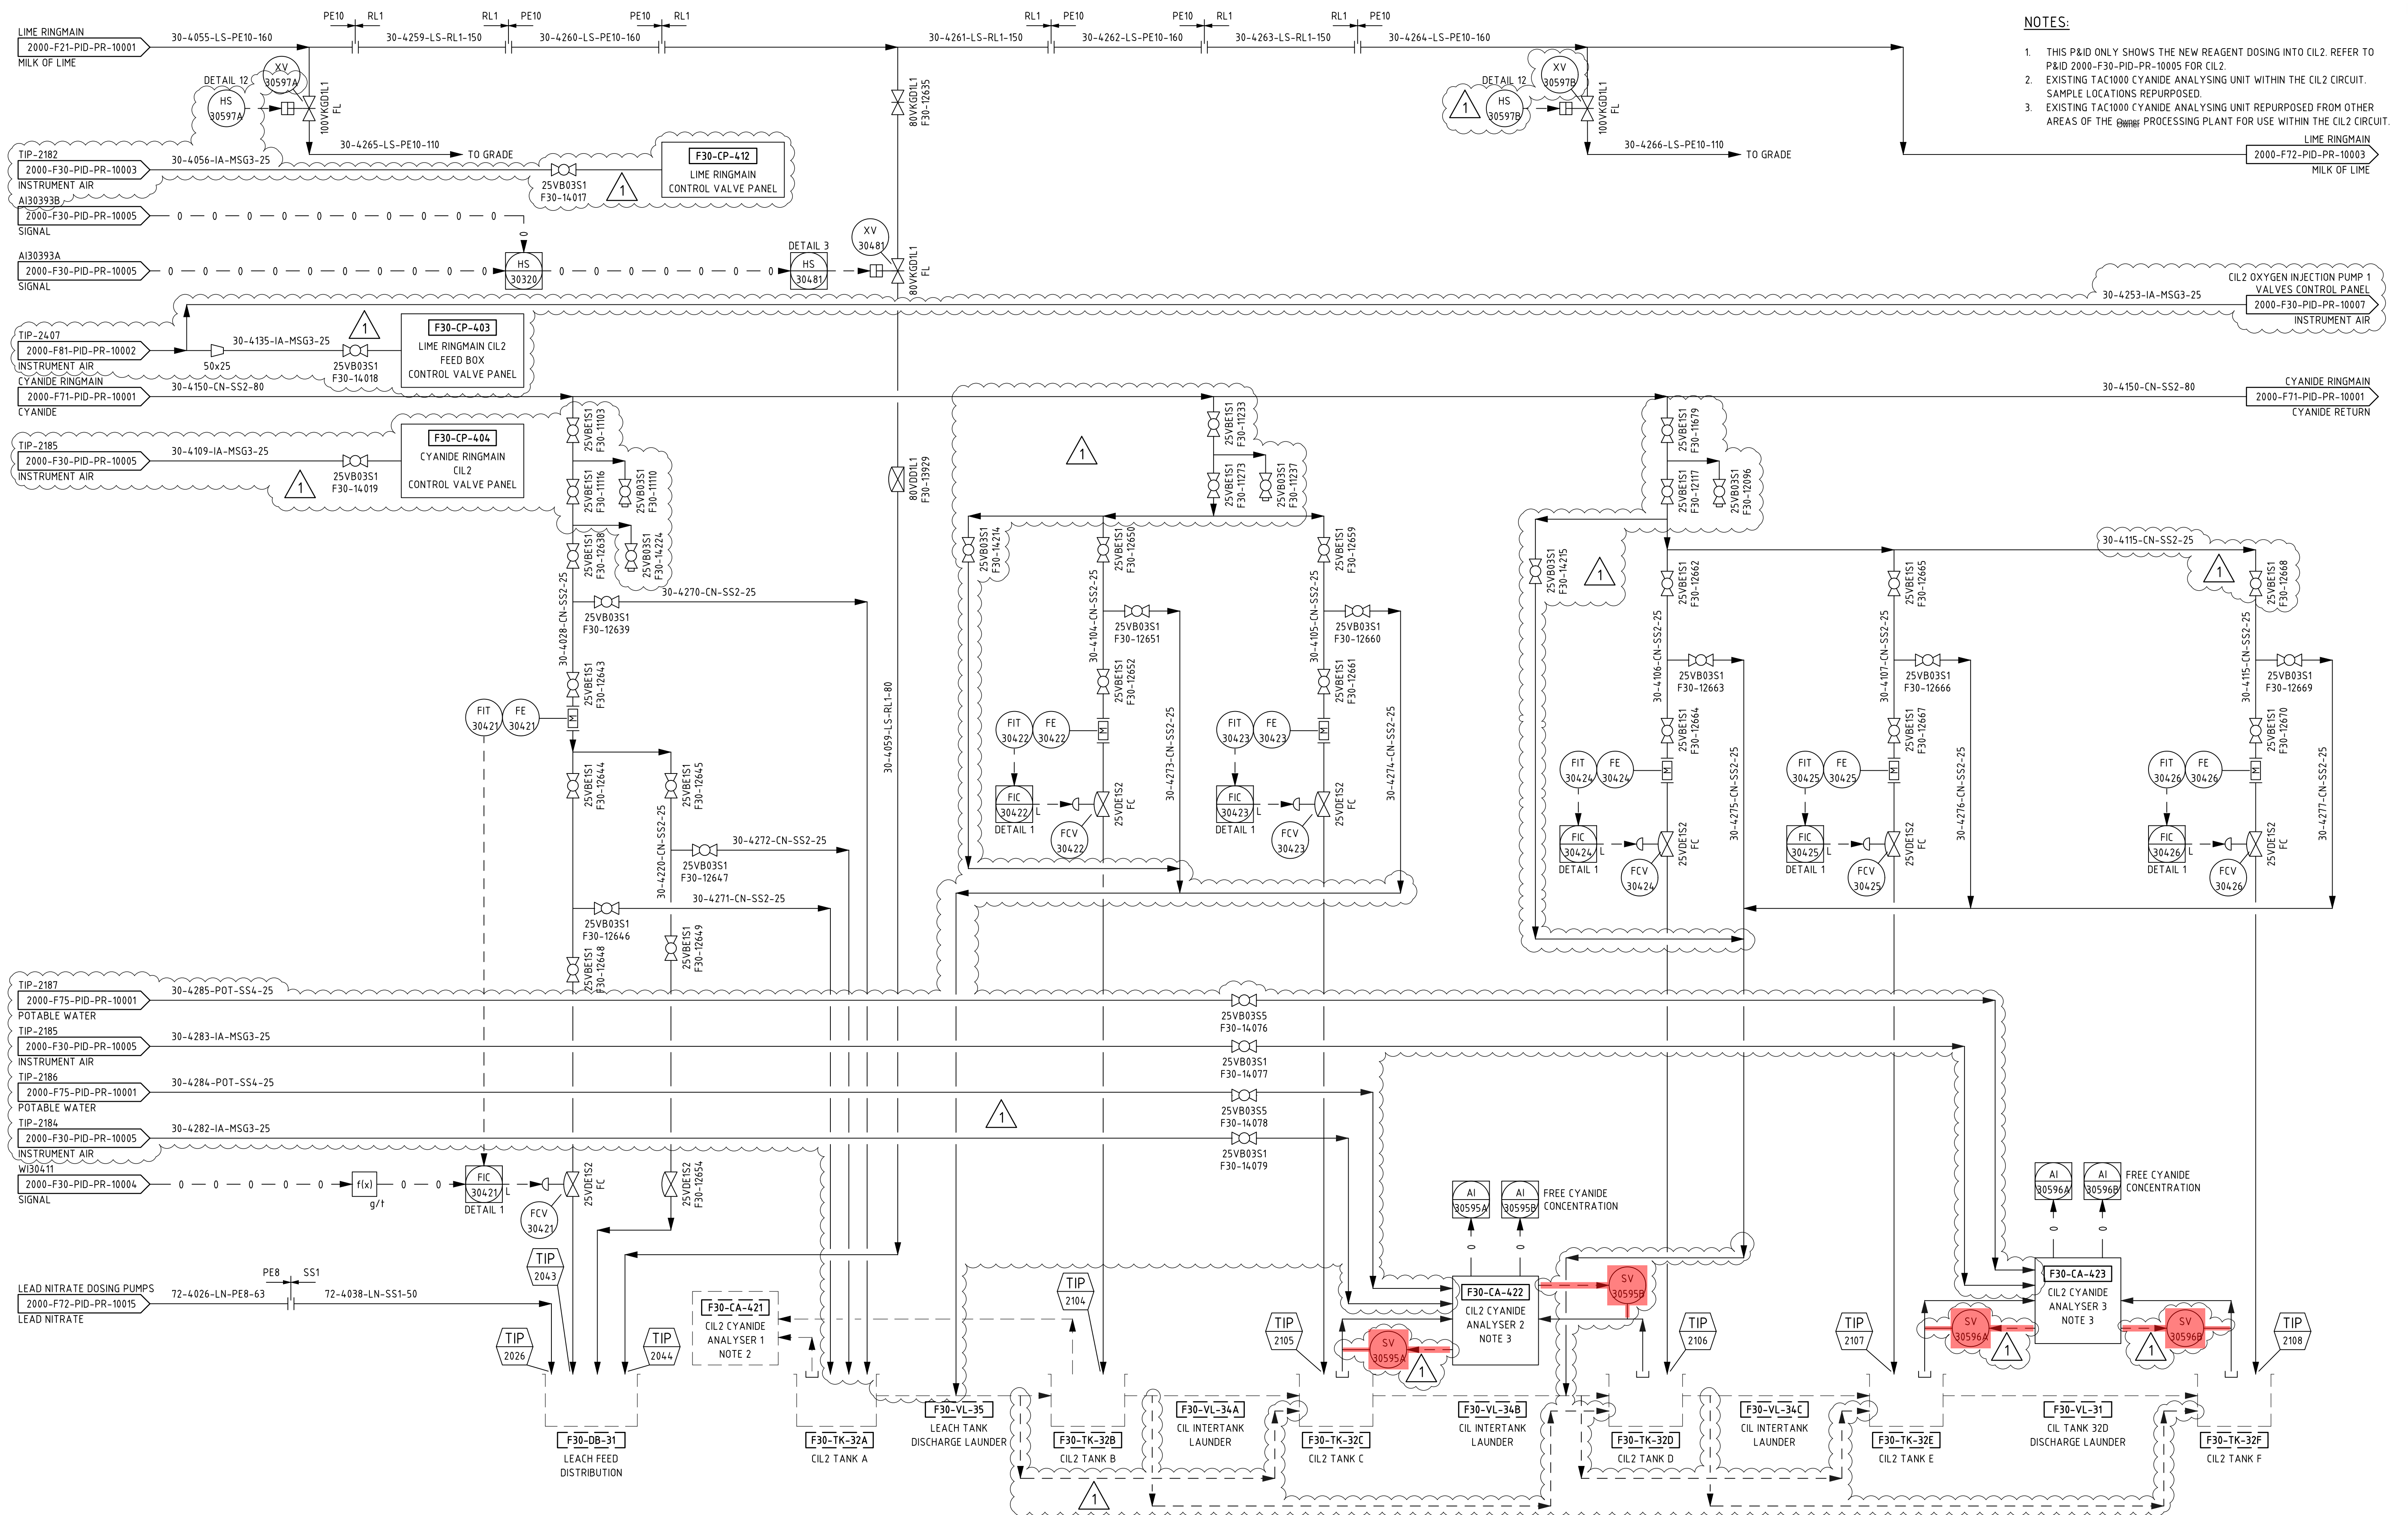

- NOTES:
- THIS P&ID ONLY SHOWS THE NEW REAGENT DOSING INTO CIL2. REFER TO P&ID 2000-F30-PID-PR-10005 FOR CIL2.
 - EXISTING TAC1000 CYANIDE ANALYSING UNIT WITHIN THE CIL2 CIRCUIT. SAMPLE LOCATIONS REPURPOSED.
 - EXISTING TAC1000 CYANIDE ANALYSING UNIT REPURPOSED FROM OTHER AREAS OF THE PLANT FOR USE WITHIN THE CIL2 CIRCUIT.